
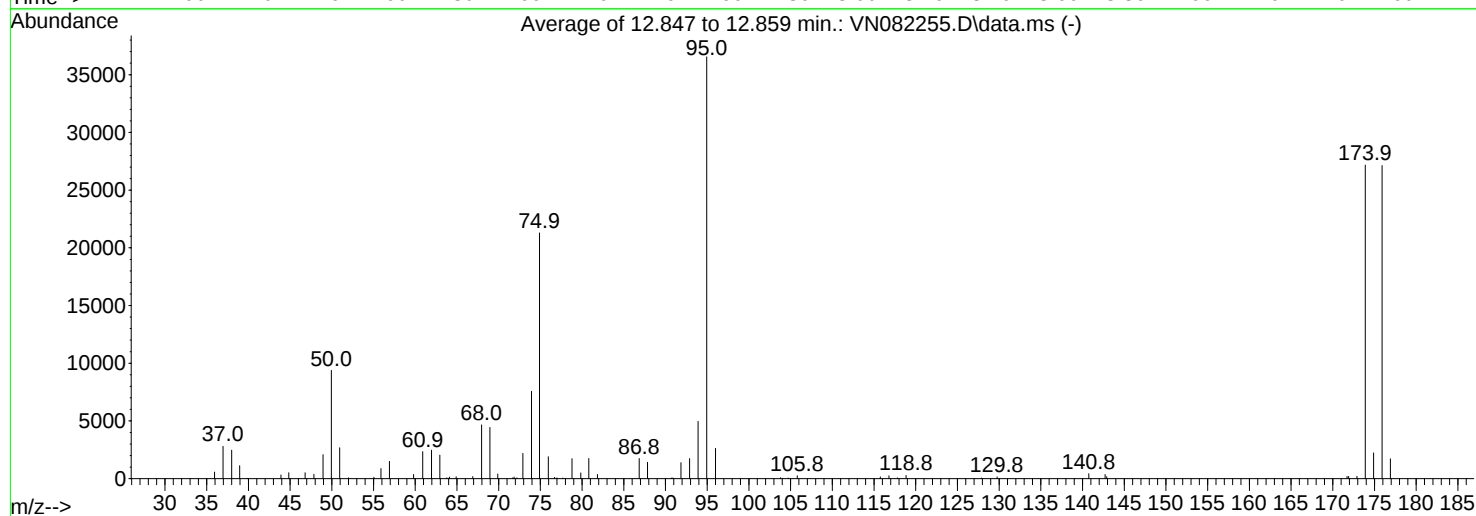


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052124\
Data File : VN082255.D
Acq On : 21 May 2024 21:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

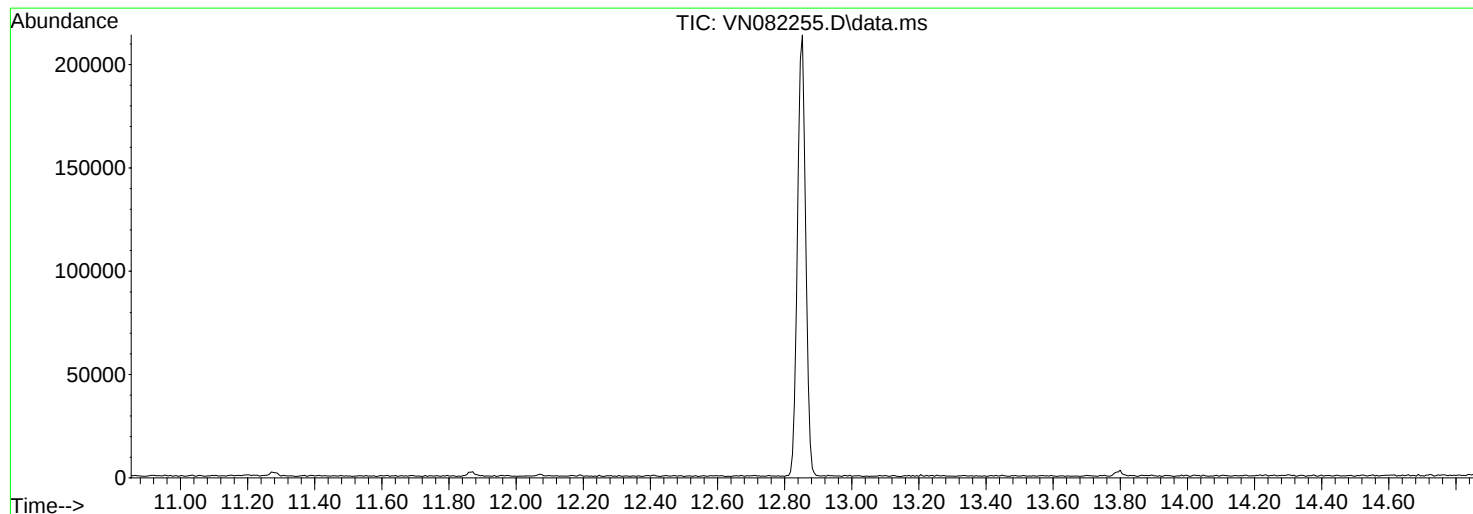

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.7	9380	PASS
75	95	30	60	58.3	21293	PASS
95	95	100	100	100.0	36549	PASS
96	95	5	9	7.2	2617	PASS
173	174	0.00	2	0.8	215	PASS
174	95	50	100	74.3	27171	PASS
175	174	5	9	8.2	2235	PASS
176	174	95	101	99.9	27139	PASS
177	176	5	9	6.3	1716	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	568	50.95	2682	64.90	166	75.95	190
36.95	2805	52.00	64	66.90	182	76.70	10
38.00	2464	55.05	120	67.95	4659	77.00	7
38.95	1120	55.90	879	68.95	4438	77.70	6
39.85	22	56.90	1503	69.90	404	78.80	1738
43.90	318	59.80	363	71.70	65	79.85	505
44.85	517	60.90	2349	71.85	140	80.80	1754
46.80	514	61.95	2469	72.20	67	81.85	362
47.85	370	62.95	2035	72.90	2187	86.85	1755
48.95	2079	63.80	65	73.95	7570	87.85	1418
49.95	9380	64.10	146	74.90	21293	90.70	53

Average of 12.847 to 12.859 min.: VN082255.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
90.90	75	117.80	65	174.90	2235		
91.85	1392	118.85	282	175.90	27139		
92.90	1730	127.90	52	176.90	1716		
93.90	4964	129.75	148				
94.95	36549	140.75	424				
96.00	2617	142.70	367				
103.80	80	142.90	165				
104.70	58	171.70	195				
105.80	248	171.90	194				
115.75	154	172.90	215				
116.80	247	173.90	27171				

Instrument :

MSVOA_N

ClientSampleId :

BFB