

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052125\
 Data File : VN086738.D
 Acq On : 21 May 2025 17:54
 Operator : JC\MD
 Sample : Q2084-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OR-640-COMP-66

Quant Time: May 22 01:28:10 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
 Quant Title : SW846 8260
 QLast Update : Sat May 17 00:46:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.218	168	261016	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.094	114	476055	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	454248	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	195313	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	155981	43.247	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	86.500%
35) Dibromofluoromethane	8.165	113	140836	49.676	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	99.360%
50) Toluene-d8	10.565	98	608052	51.754	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	103.500%
62) 4-Bromofluorobenzene	12.847	95	215193	51.873	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	103.740%
Target Compounds						
					Qvalue	
10) Methyl Iodide	4.583	142	1003	0.294	ug/l #	34
16) Acetone	4.424	43	20034	14.849	ug/l	98
18) Methyl Acetate	5.036	43	5352	1.417	ug/l	97
20) Methylene Chloride	5.277	84	6480	1.820	ug/l #	87
25) 2-Butanone	7.483	43	6806	3.265	ug/l	91
29) Tetrahydrofuran	7.842	42	2100	1.543	ug/l	89
31) Cyclohexane	8.218	56	4820	0.890	ug/l #	1
36) 1,1-Dichloropropene	8.218	75	18705	4.473	ug/l #	50
38) Carbon Tetrachloride	8.218	117	24429	5.929	ug/l #	17
41) Methacrylonitrile	7.842	41	1109	0.486	ug/l #	33
43) Isopropyl Acetate	8.683	43	29123	3.439	ug/l #	90
45) 1,2-Dichloropropane	9.741	63	1292	0.399	ug/l #	42
48) Methyl methacrylate	9.736	41	72875	22.208	ug/l #	35
49) 1,4-Dioxane	9.741	88	54	0.777	ug/l #	1
51) 4-Methyl-2-Pentanone	10.471	43	7247	1.697	ug/l #	33
54) cis-1,3-Dichloropropene	10.353	75	43075	8.272	ug/l #	53
57) 1,3-Dichloropropane	11.200	76	3882	0.712	ug/l #	42
59) 2-Hexanone	11.194	43	64287	20.614	ug/l #	41
67) Ethyl Benzene	11.959	91	10571	0.620	ug/l	99
68) m/p-Xylenes	12.065	106	2049	0.317	ug/l	87
69) o-Xylene	12.394	106	1297	0.202	ug/l	98
74) N-amyl acetate	12.459	43	3301	0.524	ug/l #	41
76) 1,2,3-Trichloropropane	12.847	75	100093	22.660	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	100093	57.186	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.476	105	3375	0.280	ug/l	88
85) sec-Butylbenzene	13.476	105	3375	0.239	ug/l #	56
89) n-Butylbenzene	13.988	91	3023	0.315	ug/l #	40
90) Hexachloroethane	14.318	117	429	0.223	ug/l #	18
95) Naphthalene	15.635	128	435246	47.516	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052125\
Data File : VN086738.D
Acq On : 21 May 2025 17:54
Operator : JC\MD
Sample : Q2084-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66

Quant Time: May 22 01:28:10 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Quant Title : SW846 8260
QLast Update : Sat May 17 00:46:13 2025
Response via : Initial Calibration




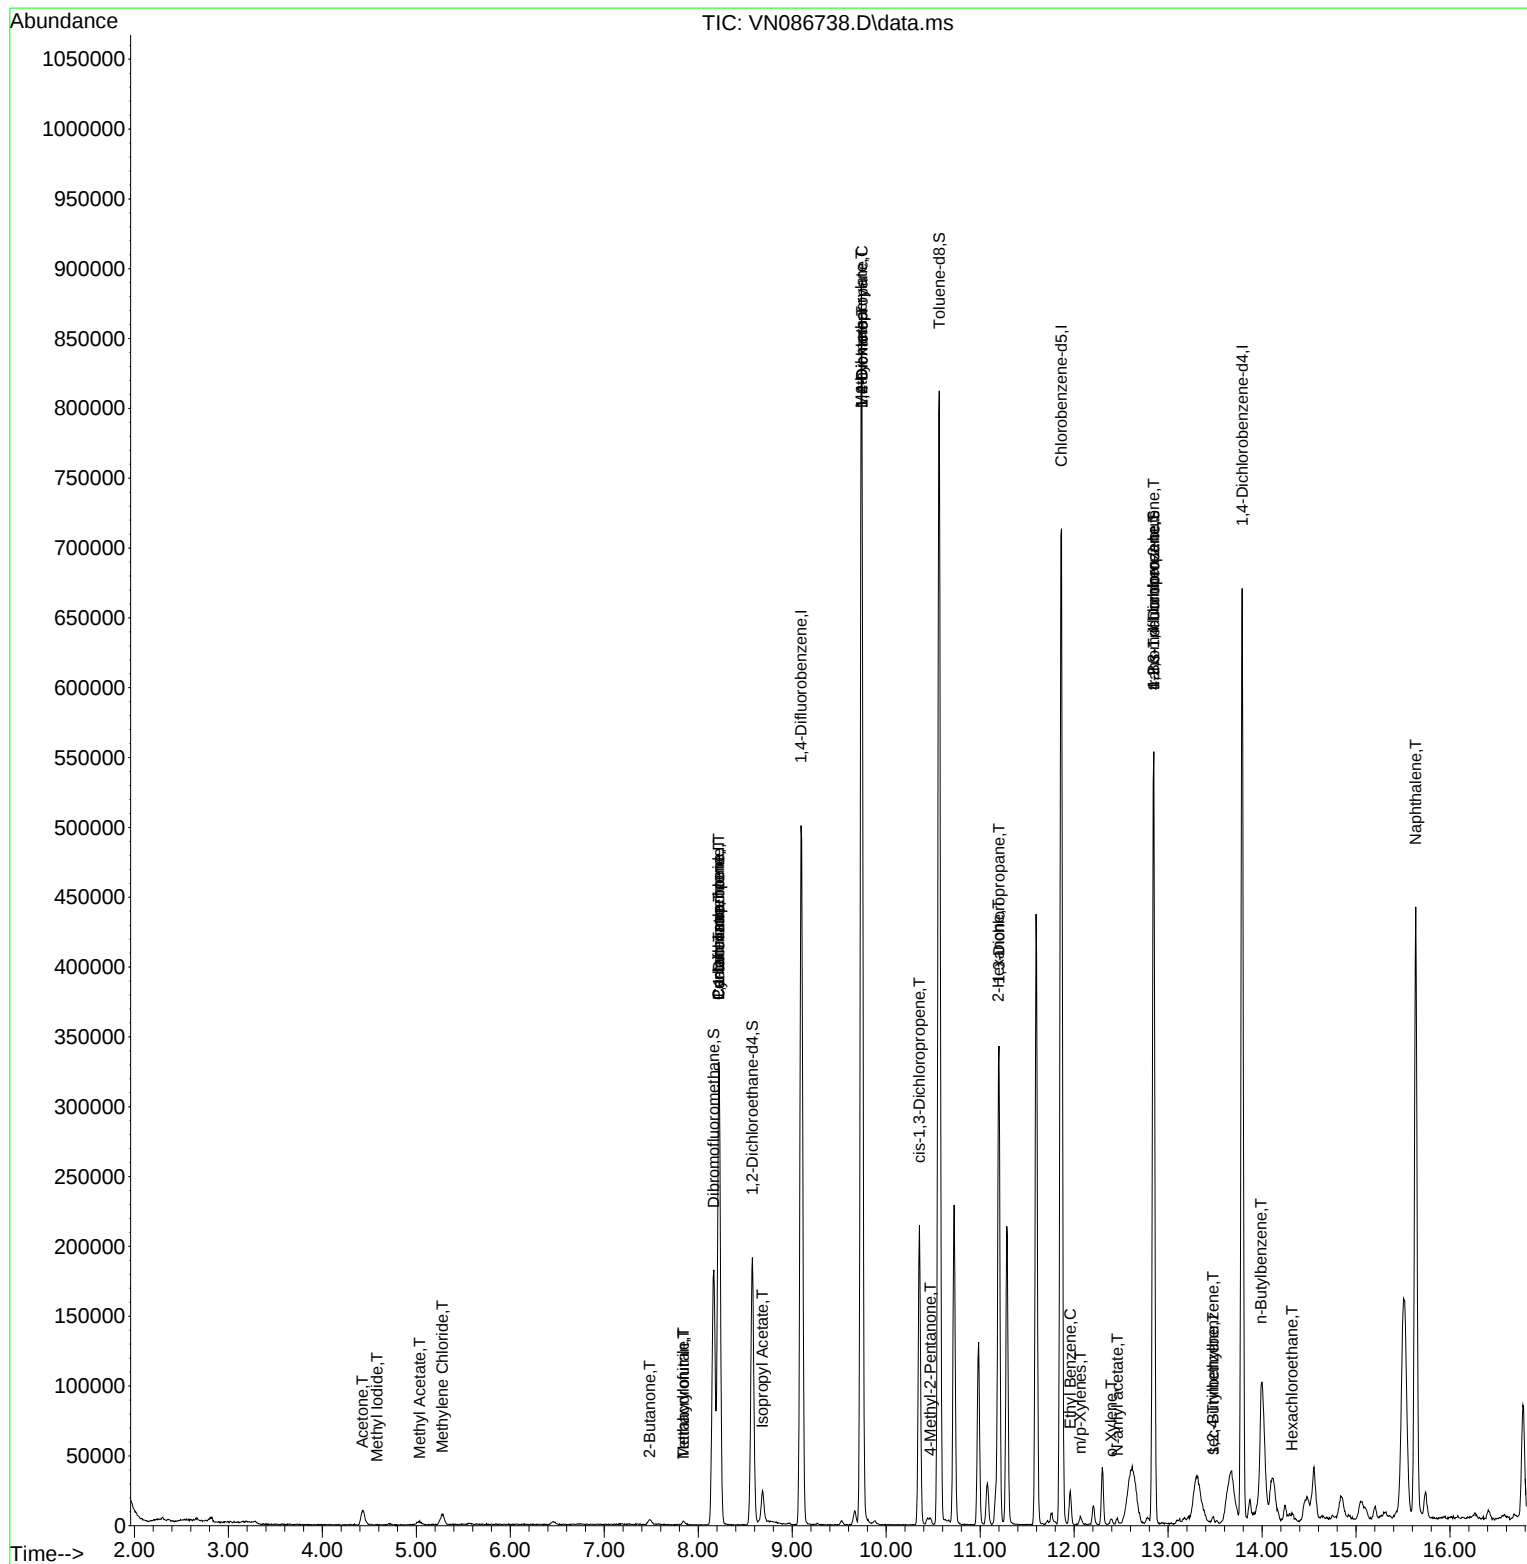


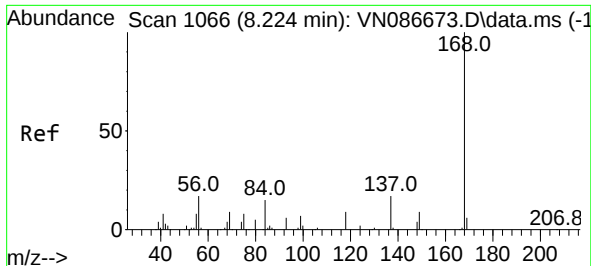

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.006 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion:168 Resp: 261016
Ion Ratio Lower Upper
168 100
99 56.7 47.0 70.4

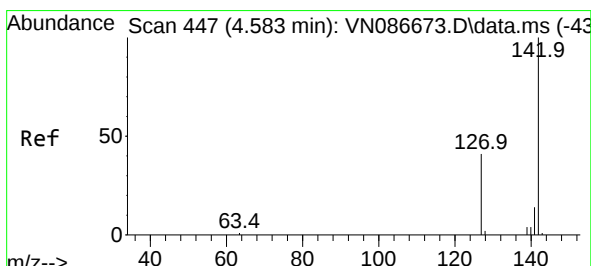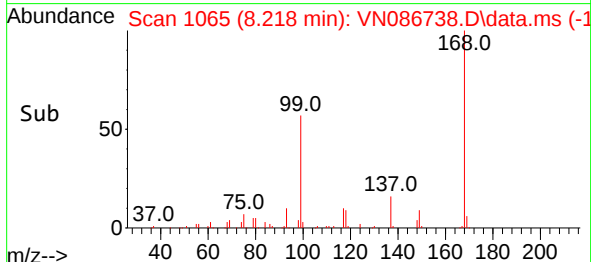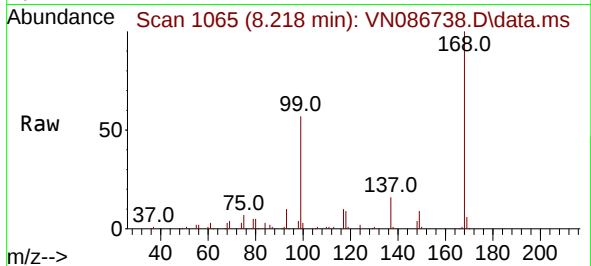

#10
Methyl Iodide
Concen: 0.294 ug/l
RT: 4.583 min Scan# 447
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion:142 Resp: 1003
Ion Ratio Lower Upper
142 100
127 0.0 32.4 48.6#
141 41.6 11.4 17.2#




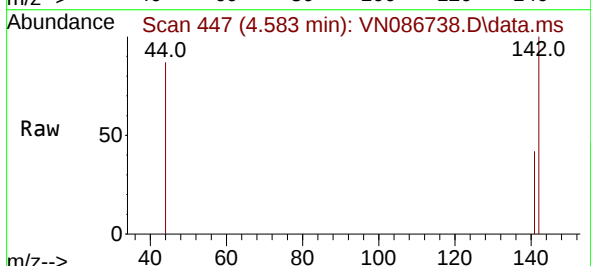


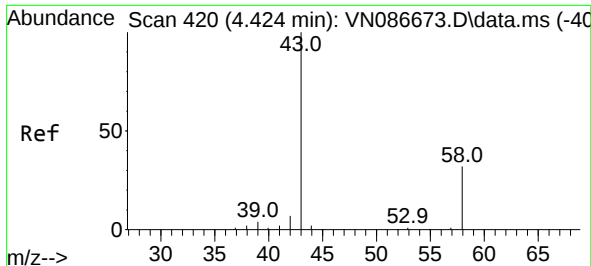

#16
Acetone
Concen: 14.849 ug/l
RT: 4.424 min Scan# 41
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 43 Resp: 20034
Ion Ratio Lower Upper
43 100
58 33.3 25.8 38.6

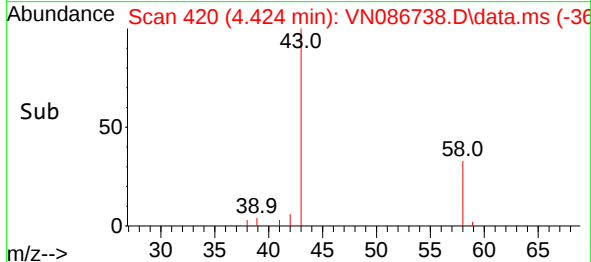

#18
Methyl Acetate
Concen: 1.417 ug/l
RT: 5.036 min Scan# 524
Delta R.T. 0.018 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 43 Resp: 5352
Ion Ratio Lower Upper
43 100
74 27.1 20.5 30.7


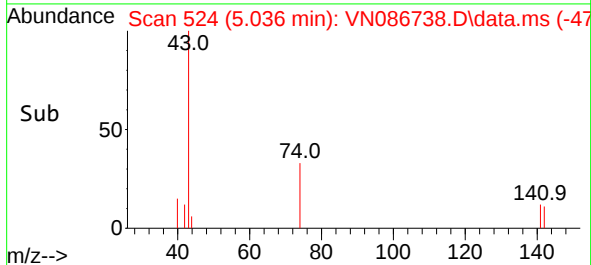

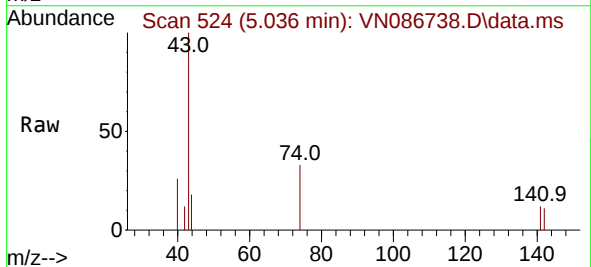


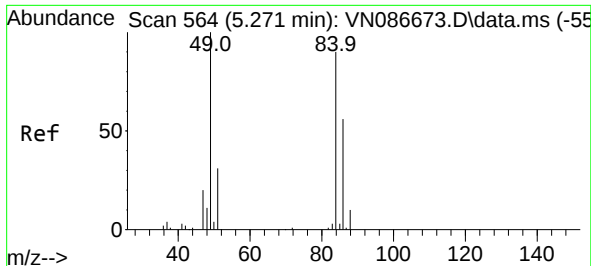

#20
Methylene Chloride
Concen: 1.820 ug/l
RT: 5.277 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion:	84	Resp:	6480
Ion	Ratio	Lower	Upper
84	100		
49	92.2	88.8	133.2
51	26.7	27.8	41.6#
86	65.6	49.8	74.6

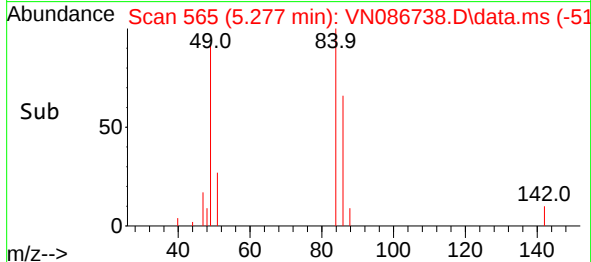

#25
2-Butanone
Concen: 3.265 ug/l
RT: 7.483 min Scan# 940
Delta R.T. 0.006 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion:	43	Resp:	6806
Ion	Ratio	Lower	Upper
43	100		
72	33.9	23.1	34.7

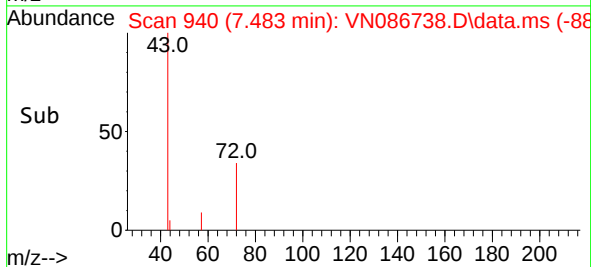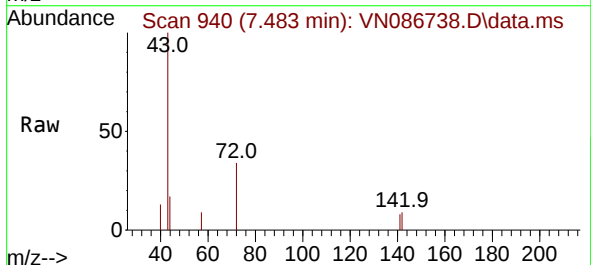

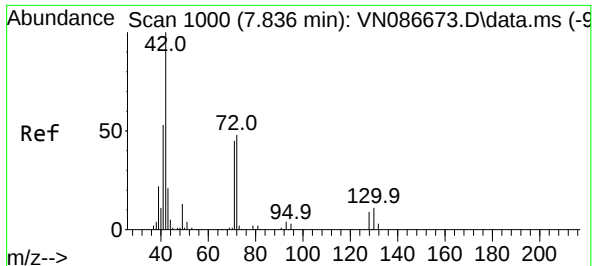

#29

Tetrahydrofuran

Concen: 1.543 ug/l

RT: 7.842 min Scan# 1065

Delta R.T. 0.006 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54





Instrument :

MSVOA_N

ClientSampleId :

OR-640-COMP-66

Tgt Ion:	42	Resp:	2100
Ion	Ratio	Lower	Upper
42	100		
72	39.3	38.7	58.1
71	50.4	36.2	54.4

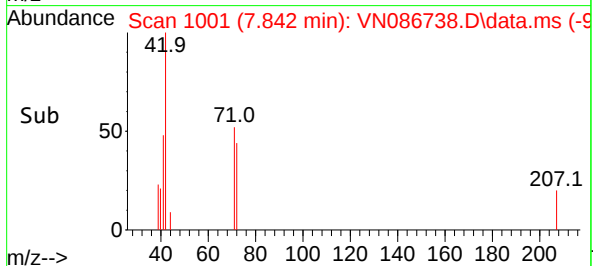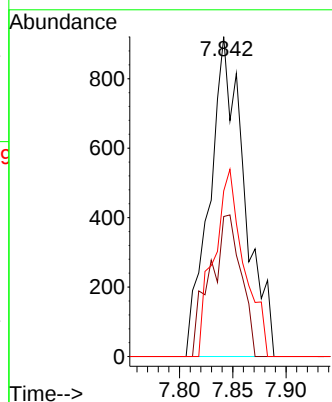

#31

Cyclohexane

Concen: 0.890 ug/l




RT: 8.218 min Scan# 1065


Delta R.T. -0.035 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54

Tgt Ion:	56	Resp:	4820
Ion	Ratio	Lower	Upper
56	100		
69	199.9	25.0	37.6#
84	169.5	71.0	106.4#

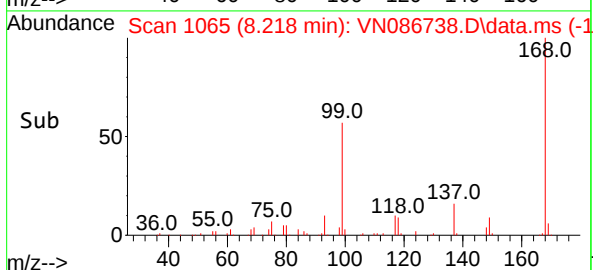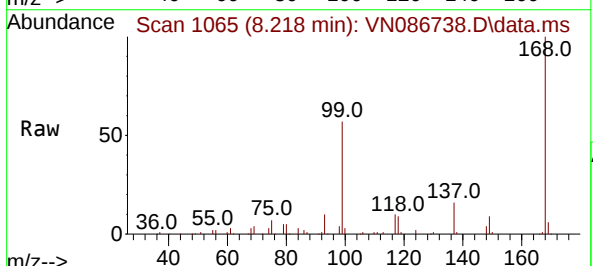



#33

1,2-Dichloroethane-d4

Concen: 43.247 ug/l

RT: 8.577 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54

Instrument :

MSVOA_N

ClientSampleId :





OR-640-COMP-66

Tgt Ion: 65 Resp: 155981

Ion Ratio Lower Upper

65 100

67 53.7 0.0 106.4

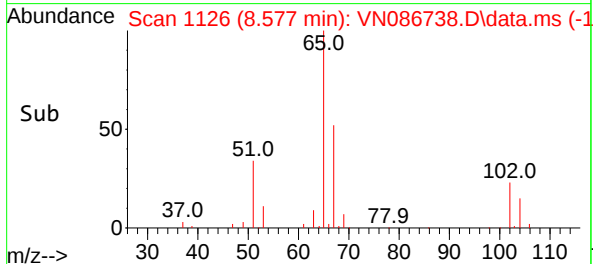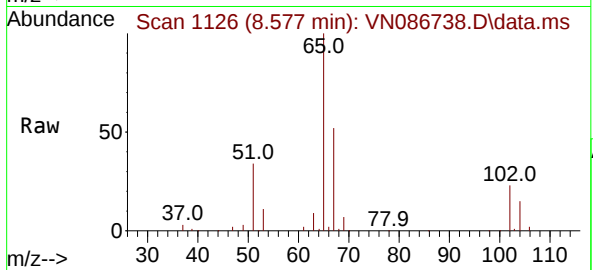

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.094 min Scan# 1214

Delta R.T. -0.006 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54




Tgt Ion: 114 Resp: 476055


Ion Ratio Lower Upper

114 100

63 19.4 0.0 40.2

88 15.7 0.0 31.2

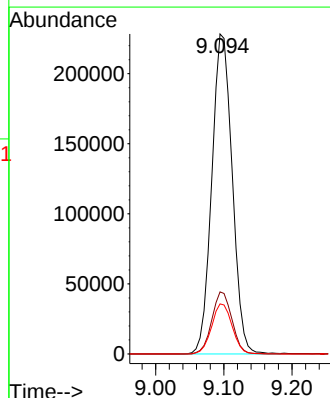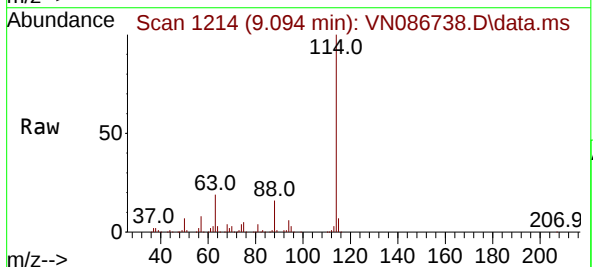

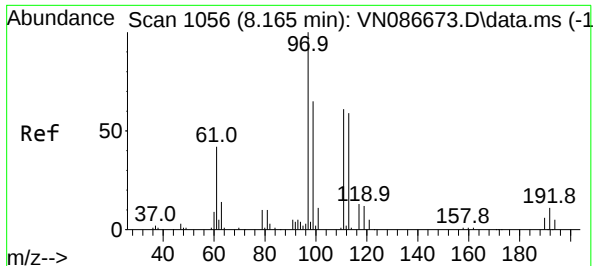

#35

Dibromofluoromethane

Concen: 49.676 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54

Instrument :

MSVOA_N

ClientSampleId :

OR-640-COMP-66





Tgt Ion:113 Resp: 140836

Ion Ratio Lower Upper

113 100

111 103.0 82.2 123.2

192 18.1 13.8 20.8

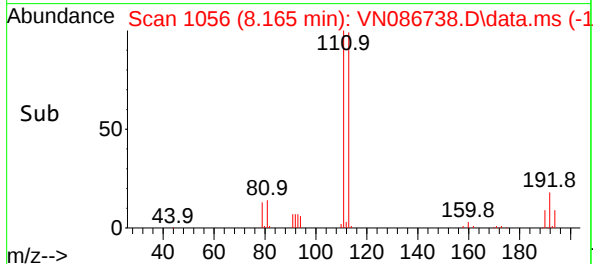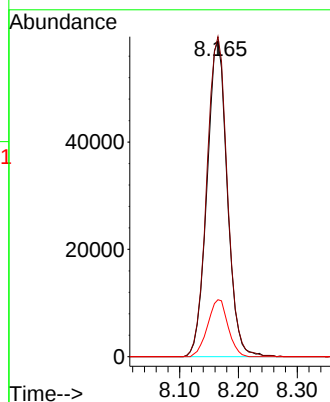

#36

1,1-Dichloropropene

Concen: 4.473 ug/l

RT: 8.218 min Scan# 1065

Delta R.T. -0.147 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54




Tgt Ion: 75 Resp: 18705


Ion Ratio Lower Upper

75 100

110 9.4 17.5 52.5#


77 0.0 25.1 37.7#

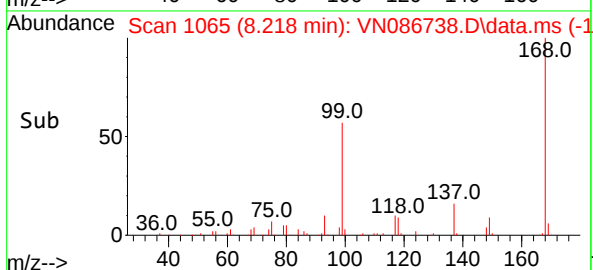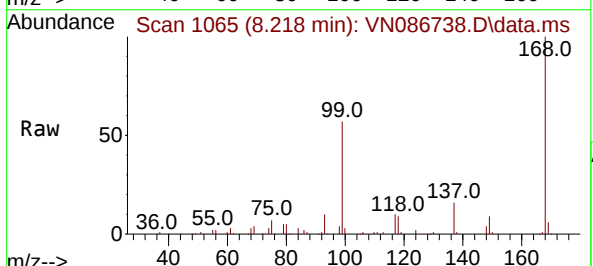



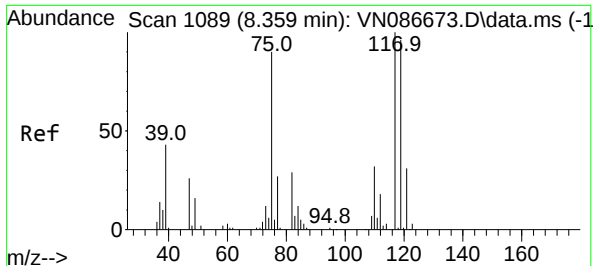


#38
Carbon Tetrachloride
Concen: 5.929 ug/l
RT: 8.218 min Scan# 1001
Delta R.T. -0.141 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66







Tgt Ion:117 Resp: 24429
Ion Ratio Lower Upper
117 100
119 6.1 77.0 115.6#
121 0.0 25.0 37.6#

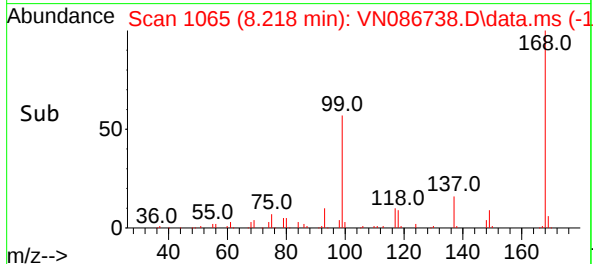

#41
Methacrylonitrile
Concen: 0.486 ug/l
RT: 7.842 min Scan# 1001
Delta R.T. 0.065 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 41 Resp: 1109
Ion Ratio Lower Upper
41 100
39 27.1 44.9 67.3#
67 0.0 63.4 95.0#
52 0.0 24.4 36.6#

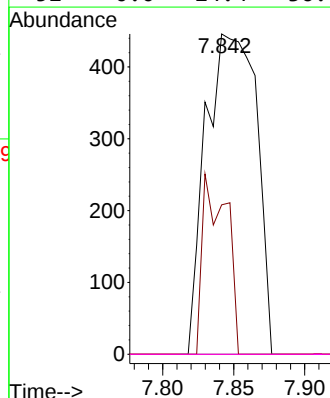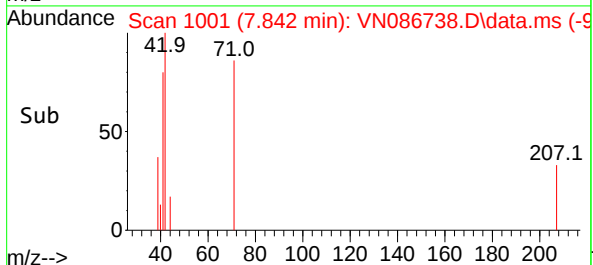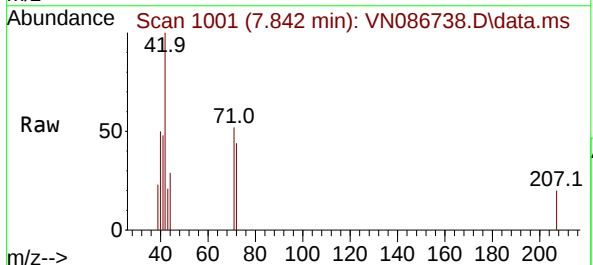

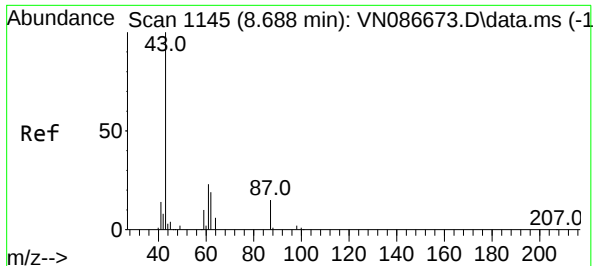

#43

Isopropyl Acetate

Concen: 3.439 ug/l

RT: 8.683 min Scan# 1145

Delta R.T. -0.006 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54

Instrument :

MSVOA_N

ClientSampleId :

OR-640-COMP-66





Tgt Ion: 43 Resp: 29123

Ion Ratio Lower Upper

43 100

61 19.0 21.4 32.2#

87 13.8 11.1 16.7

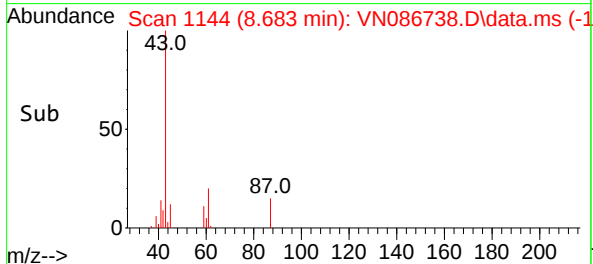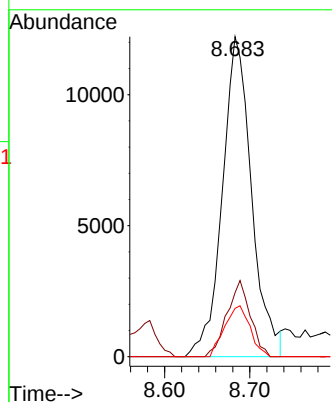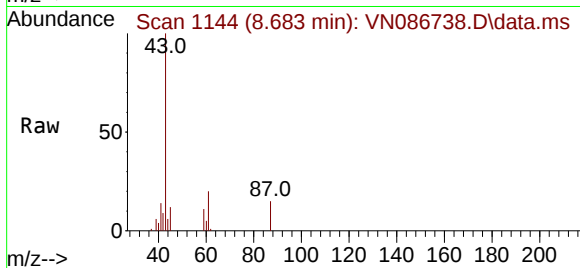

#45

1,2-Dichloropropane

Concen: 0.399 ug/l

RT: 9.741 min Scan# 1324

Delta R.T. 0.124 min

Lab File: VN086738.D




Acq: 21 May 2025 17:54


Tgt Ion: 63 Resp: 1292

Ion Ratio Lower Upper

63 100

65 0.0 25.8 38.6#

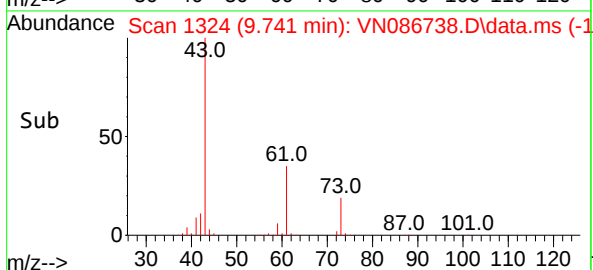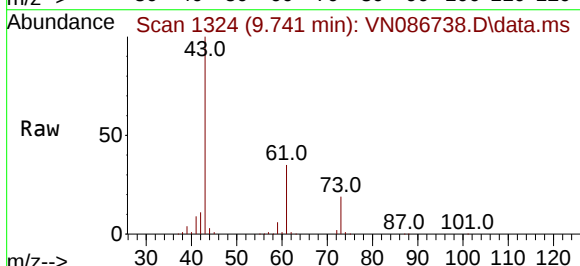

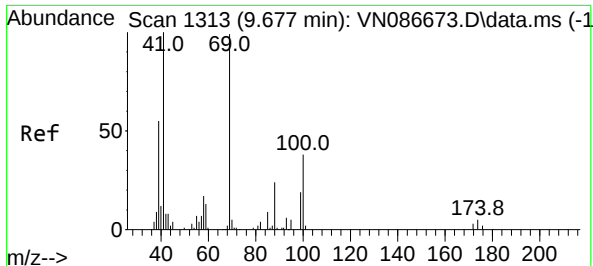

#48

Methyl methacrylate

Concen: 22.208 ug/l

RT: 9.736 min Scan# 1

Delta R.T. 0.059 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54

Instrument :

MSVOA_N

ClientSampleId :

OR-640-COMP-66





Tgt Ion: 41 Resp: 72875

Ion Ratio Lower Upper

41 100

69 0.0 74.1 111.1#

39 46.1 44.1 66.1

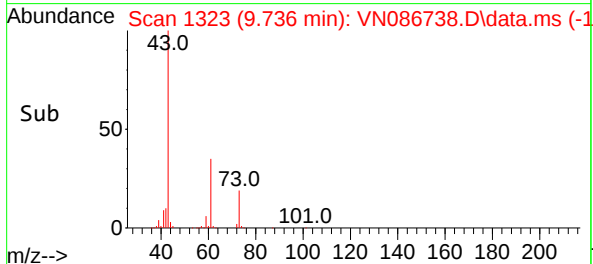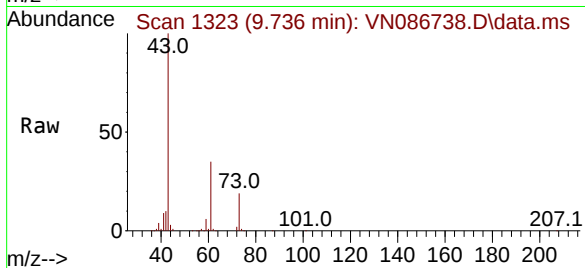

#49

1,4-Dioxane

Concen: 0.777 ug/l

RT: 9.741 min Scan# 1324

Delta R.T. 0.047 min

Lab File: VN086738.D

Acq: 21 May 2025 17:54




Tgt Ion: 88 Resp: 54


Ion Ratio Lower Upper

88 100

43 1547774.1 23.6 35.4#

58 6694.4 55.3 82.9#


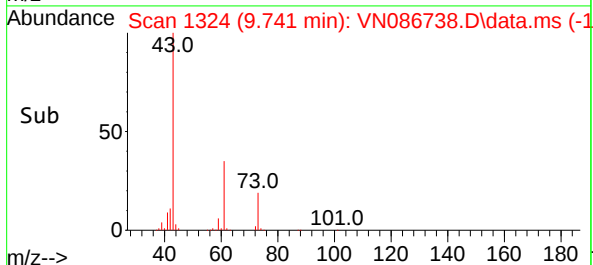
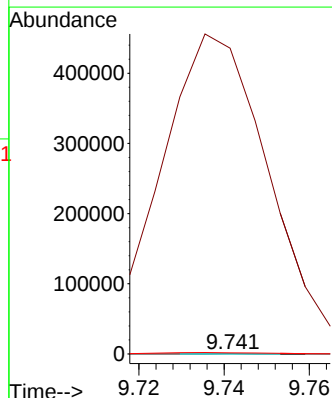
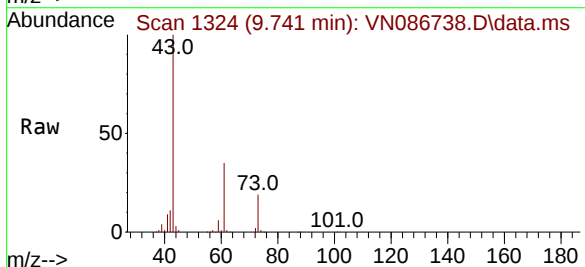


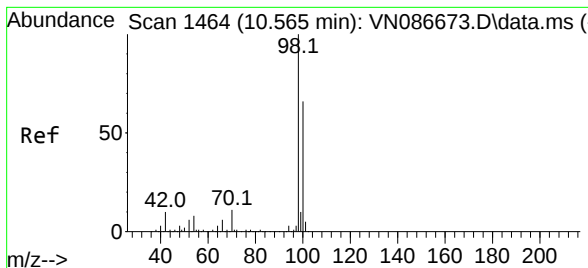

#50
Toluene-d8
Concen: 51.754 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 98 Resp: 608052
Ion Ratio Lower Upper
98 100
100 66.1 52.9 79.3

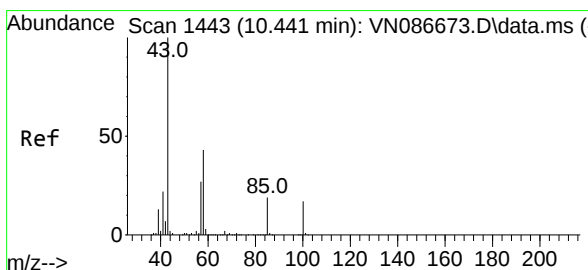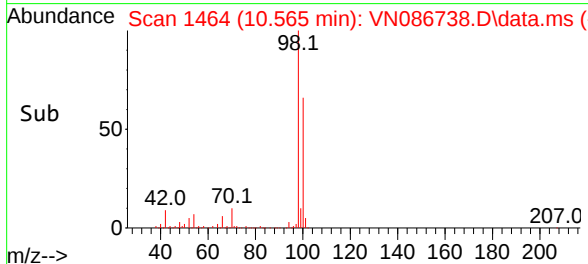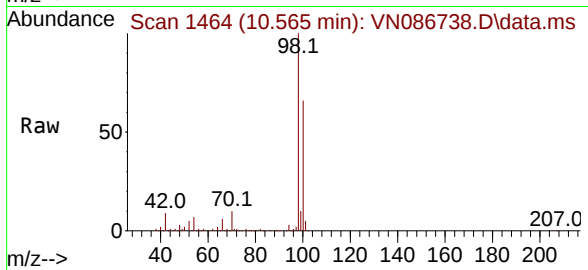

#51
4-Methyl-2-Pentanone
Concen: 1.697 ug/l
RT: 10.471 min Scan# 1448
Delta R.T. 0.029 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 43 Resp: 7247
Ion Ratio Lower Upper
43 100
58 0.0 33.9 50.9#


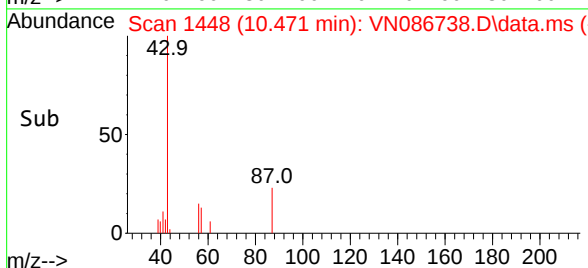

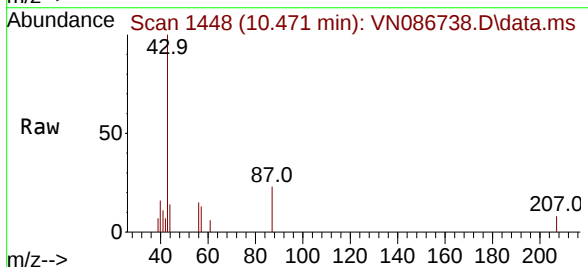


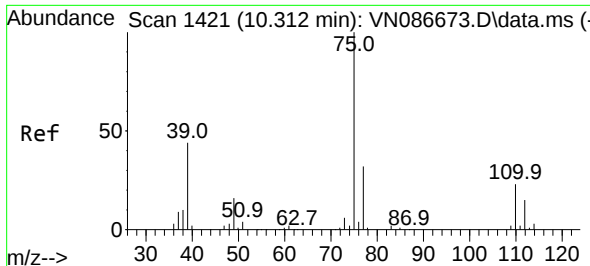

#54
cis-1,3-Dichloropropene
Concen: 8.272 ug/l
RT: 10.353 min Scan# 1428
Delta R.T. 0.041 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 75 Resp: 43075
Ion Ratio Lower Upper
75 100
77 0.0 25.3 37.9#
39 18.8 35.2 52.8#

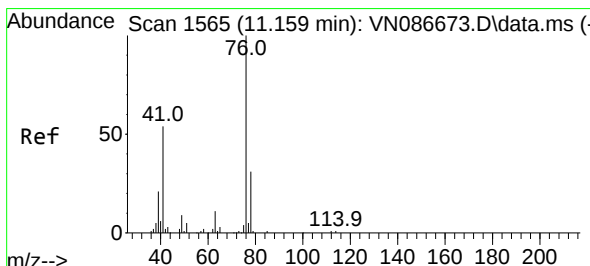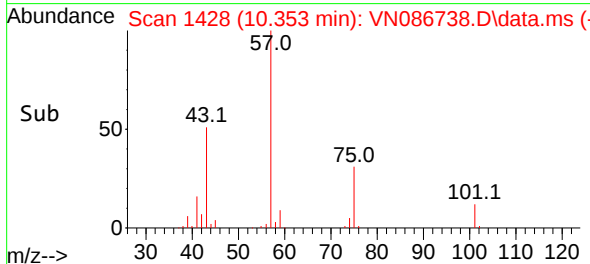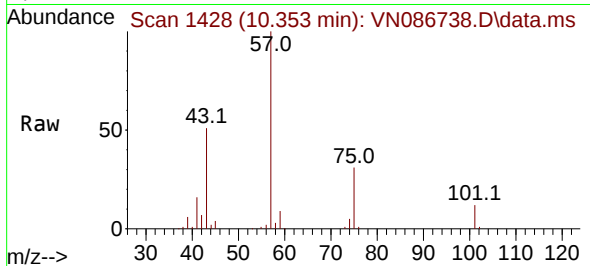

#57
1,3-Dichloropropane
Concen: 0.712 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.041 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 76 Resp: 3882
Ion Ratio Lower Upper
76 100
78 0.0 25.8 38.8#


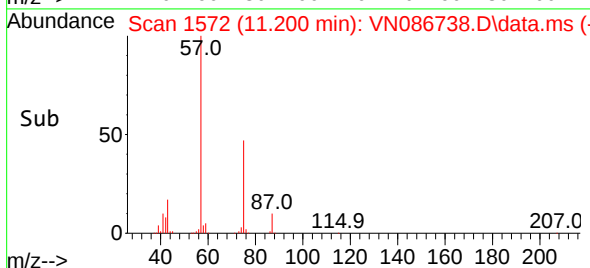

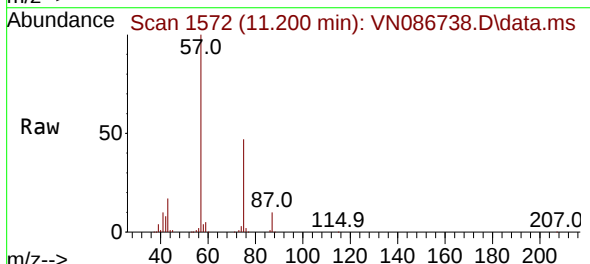


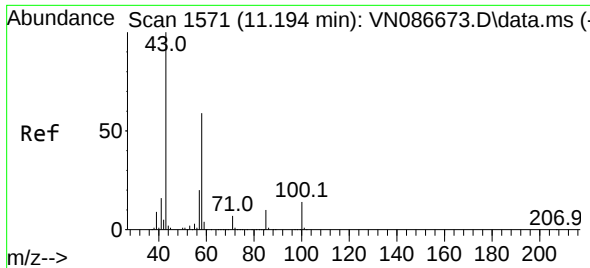

#59
2-Hexanone
Concen: 20.614 ug/l
RT: 11.194 min Scan# 1571
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 43 Resp: 64287
Ion Ratio Lower Upper
43 100
58 15.5 29.8 89.5#

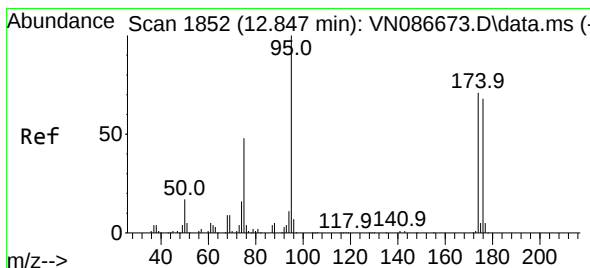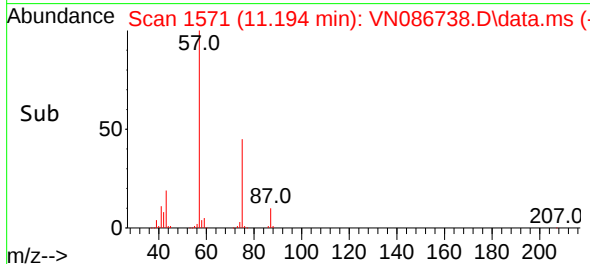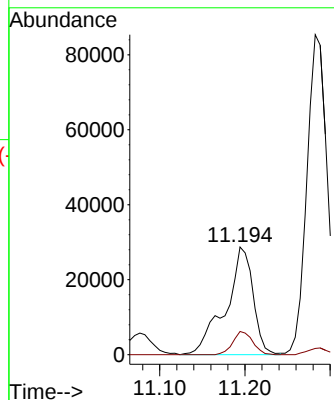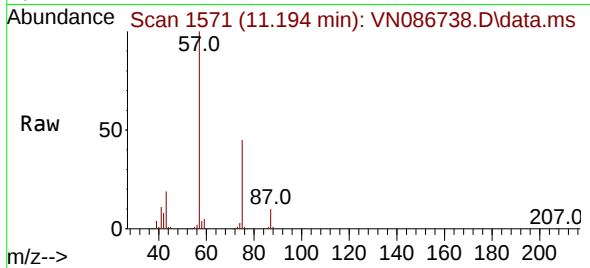

#62
4-Bromofluorobenzene
Concen: 51.873 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 95 Resp: 215193
Ion Ratio Lower Upper
95 100
174 74.7 0.0 145.4
176 71.4 0.0 137.8


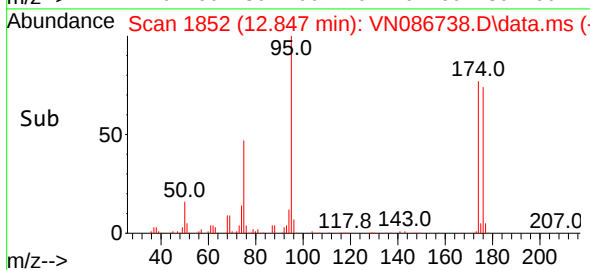
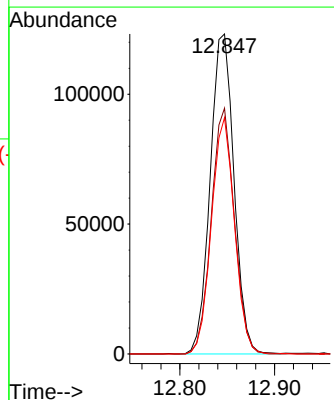
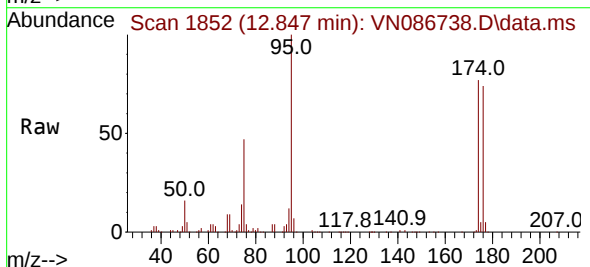


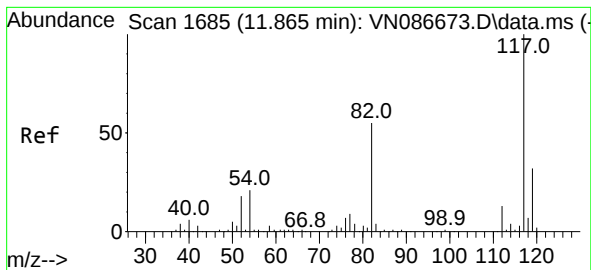

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion:117 Resp: 454248
Ion Ratio Lower Upper
117 100
82 54.4 44.2 66.2
119 32.8 25.4 38.2

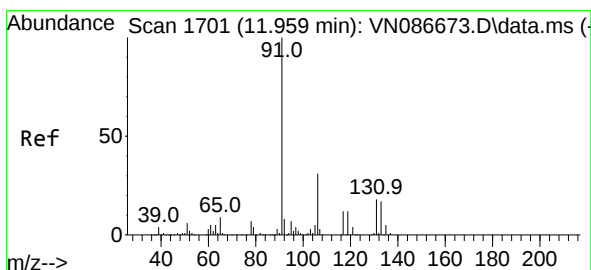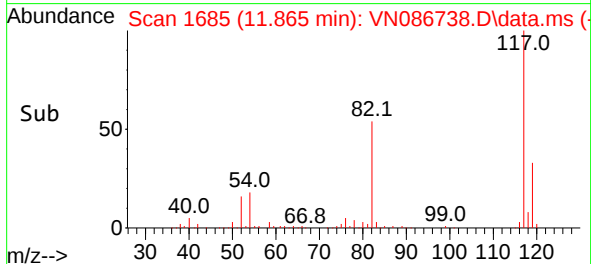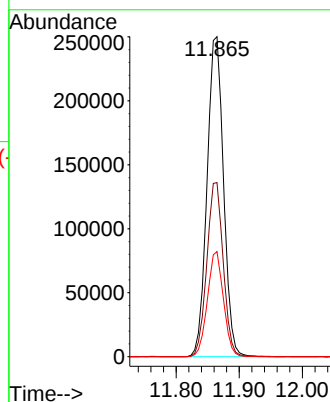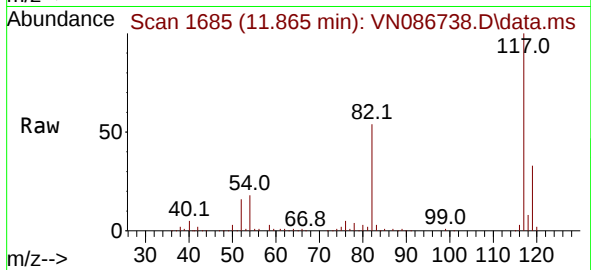

#67
Ethyl Benzene
Concen: 0.620 ug/l
RT: 11.959 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 91 Resp: 10571
Ion Ratio Lower Upper
91 100
106 31.2 24.6 36.8




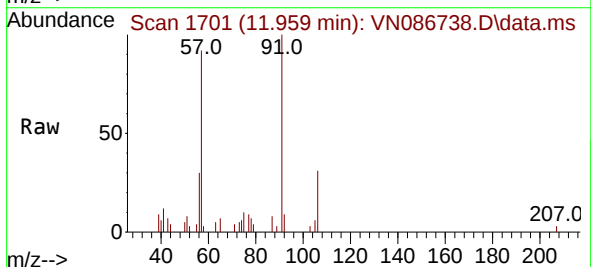


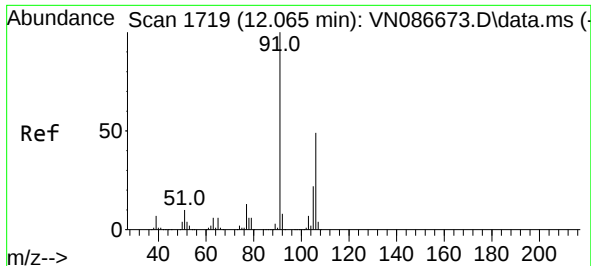

#68
m/p-Xylenes
Concen: 0.317 ug/l
RT: 12.065 min Scan# 1719
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion:106 Resp: 2049
Ion Ratio Lower Upper
106 100
91 222.9 162.4 243.6

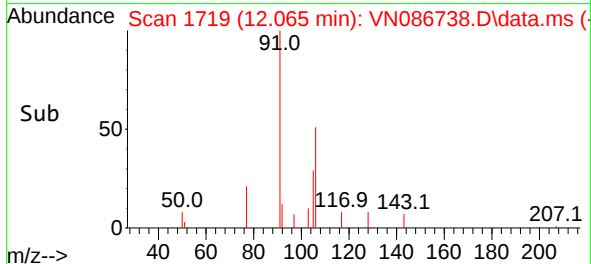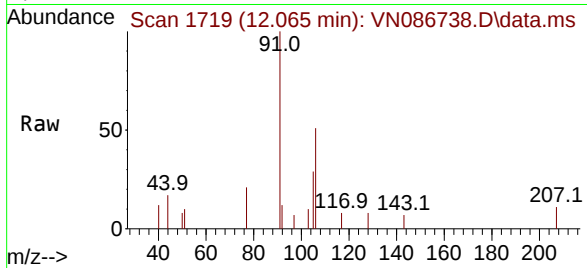

#69
o-Xylene
Concen: 0.202 ug/l
RT: 12.394 min Scan# 1775
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion:106 Resp: 1297
Ion Ratio Lower Upper
106 100
91 206.3 105.1 315.1


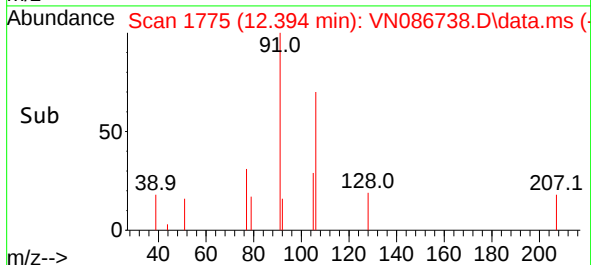
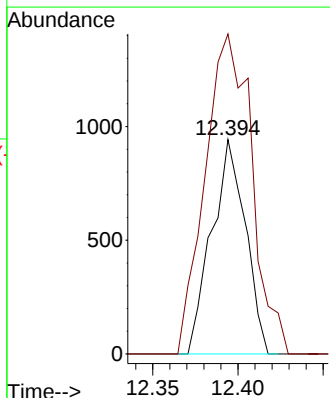
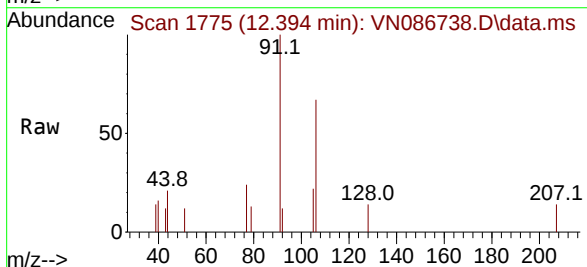


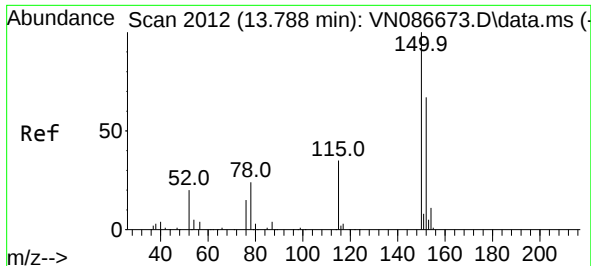

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 2012
 Delta R.T. 0.000 min
 Lab File: VN086738.D
 Acq: 21 May 2025 17:54




Instrument :
 MSVOA_N
 ClientSampleId :
 OR-640-COMP-66


Tgt Ion:152 Resp: 195313
 Ion Ratio Lower Upper
 152 100
 115 58.5 30.0 90.1
 150 155.5 0.0 347.8

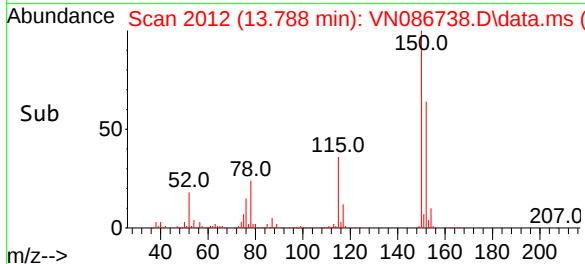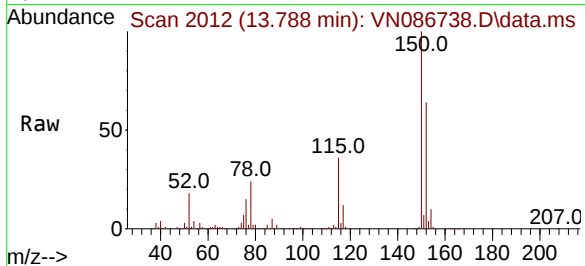

#74
 N-ethyl acetate
 Concen: 0.524 ug/l
 RT: 12.459 min Scan# 1786
 Delta R.T. -0.029 min
 Lab File: VN086738.D
 Acq: 21 May 2025 17:54

Tgt Ion: 43 Resp: 3301
 Ion Ratio Lower Upper
 43 100
 70 0.0 37.9 56.9#
 55 3.9 20.5 30.7#
 61 0.0 21.7 32.5#


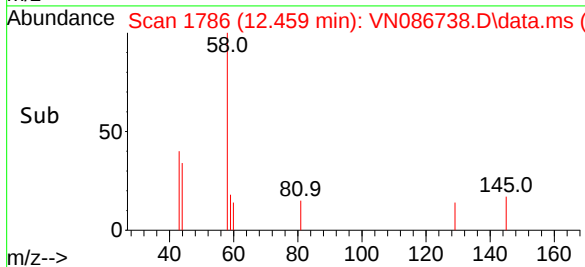

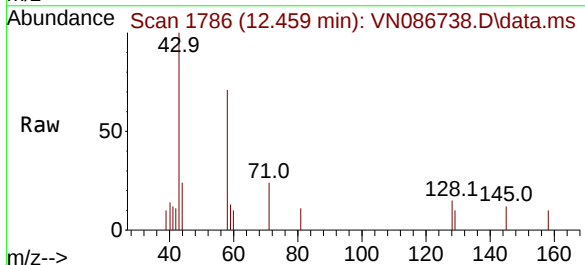


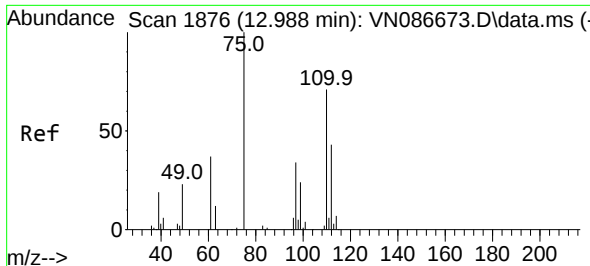

#76
1,2,3-Trichloropropane
Concen: 22.660 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 75 Resp: 100093
Ion Ratio Lower Upper
75 100
77 1.5 96.0 288.1#

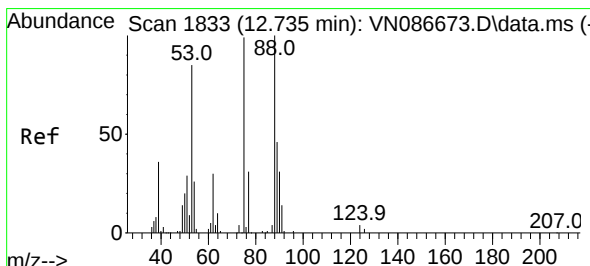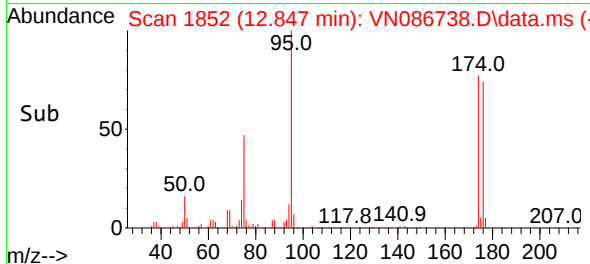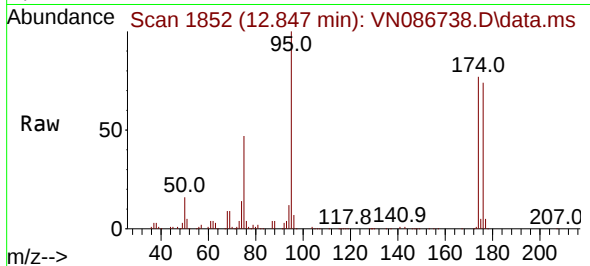

#81
trans-1,4-Dichloro-2-butene
Concen: 57.186 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.112 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 75 Resp: 100093
Ion Ratio Lower Upper
75 100
53 0.0 70.4 105.6#
89 0.0 32.4 48.6#


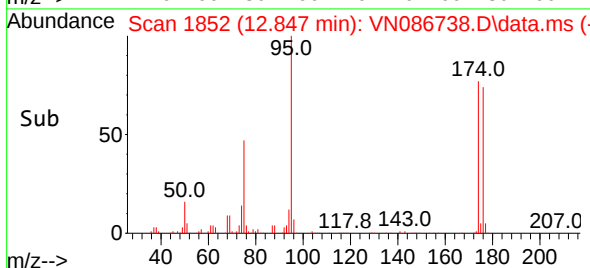
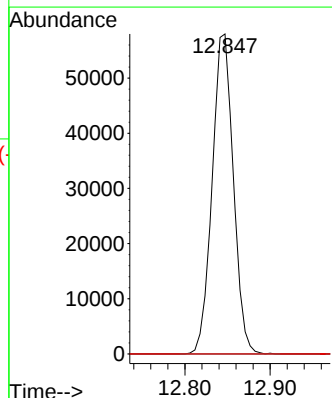
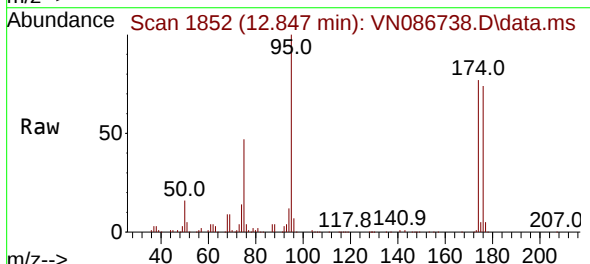


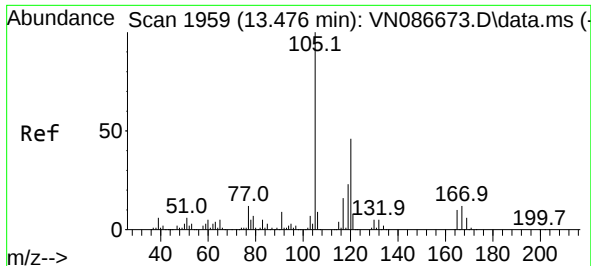

#84
1,2,4-Trimethylbenzene
Concen: 0.280 ug/l
RT: 13.476 min Scan# 1959
Delta R.T. 0.000 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion:105 Resp: 3375
Ion Ratio Lower Upper
105 100
120 38.5 23.2 69.6

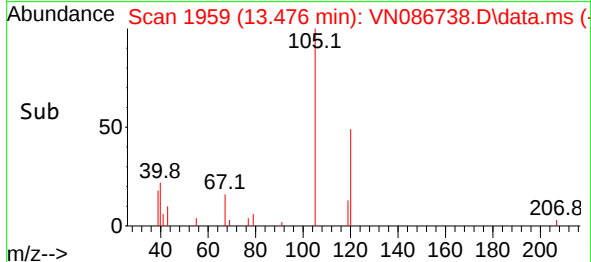

#85
sec-Butylbenzene
Concen: 0.239 ug/l
RT: 13.476 min Scan# 1959
Delta R.T. -0.135 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion:105 Resp: 3375
Ion Ratio Lower Upper
105 100
134 0.0 10.1 30.1#


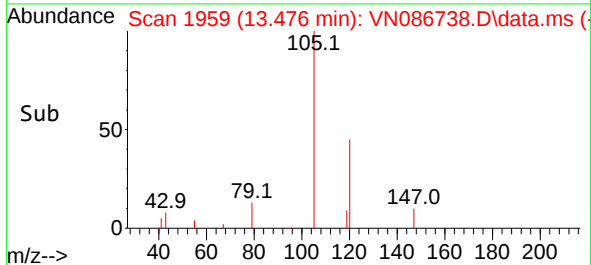

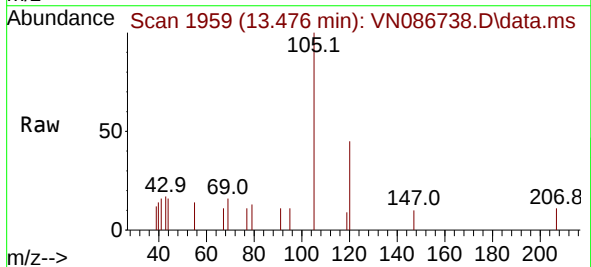


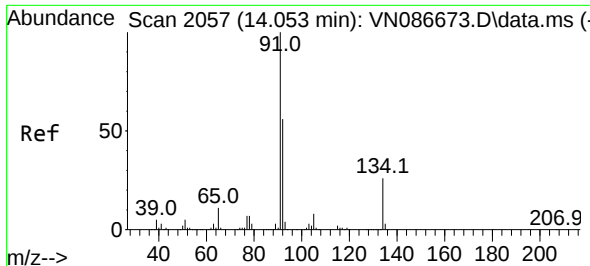

#89
n-Butylbenzene
Concen: 0.315 ug/l
RT: 13.988 min Scan# 2057
Delta R.T. -0.065 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54




Instrument :
MSVOA_N
ClientSampleId :
OR-640-COMP-66


Tgt Ion: 91 Resp: 3023
Ion Ratio Lower Upper
91 100
92 8.1 27.4 82.0#
134 0.0 12.8 38.4#

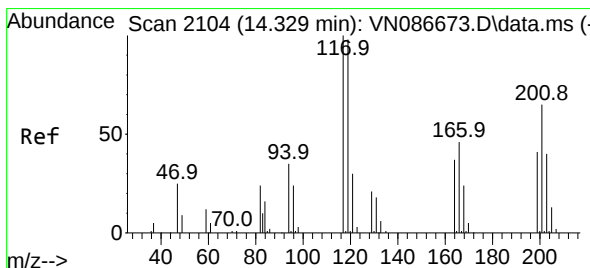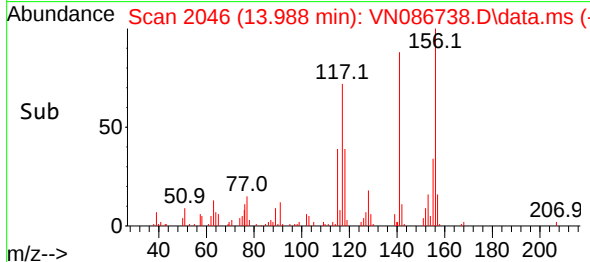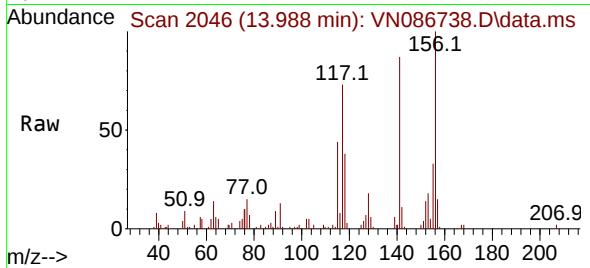

#90
Hexachloroethane
Concen: 0.223 ug/l
RT: 14.318 min Scan# 2102
Delta R.T. -0.012 min
Lab File: VN086738.D
Acq: 21 May 2025 17:54

Tgt Ion: 117 Resp: 429
Ion Ratio Lower Upper
117 100
201 0.0 32.0 96.0#

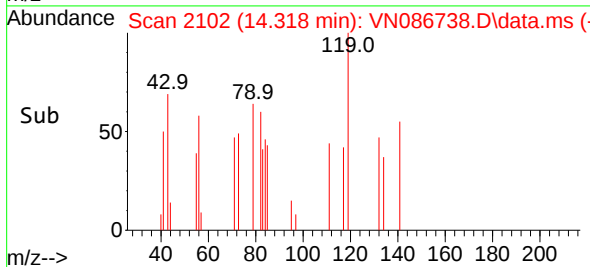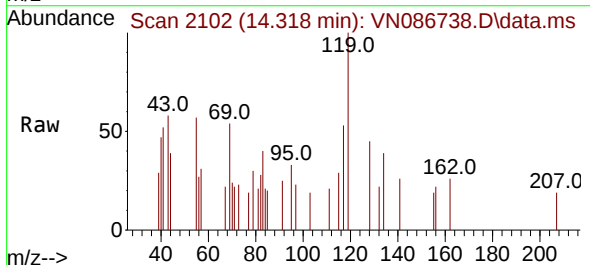



#95

Naphthalene

Concen: 47.516 ug/l

RT: 15.635 min Scan# 21

Delta R.T. 0.000 min

Lab File: VN086738.D


Acq: 21 May 2025 17:54

Instrument :

MSVOA_N

ClientSampleId :

OR-640-COMP-66

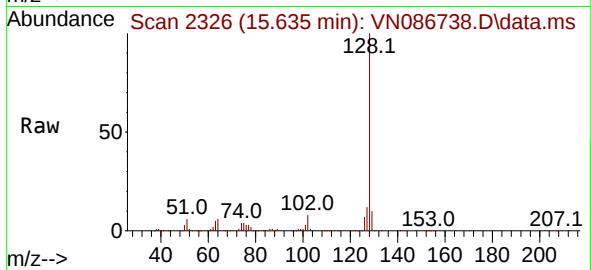

Tgt Ion:128 Resp: 435246

Ion Ratio Lower Upper

128 100

127 12.8 10.1 15.1

129 10.8 8.6 13.0

