


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052125\
Data File : VN086721.D
Acq On : 21 May 2025 10:37
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

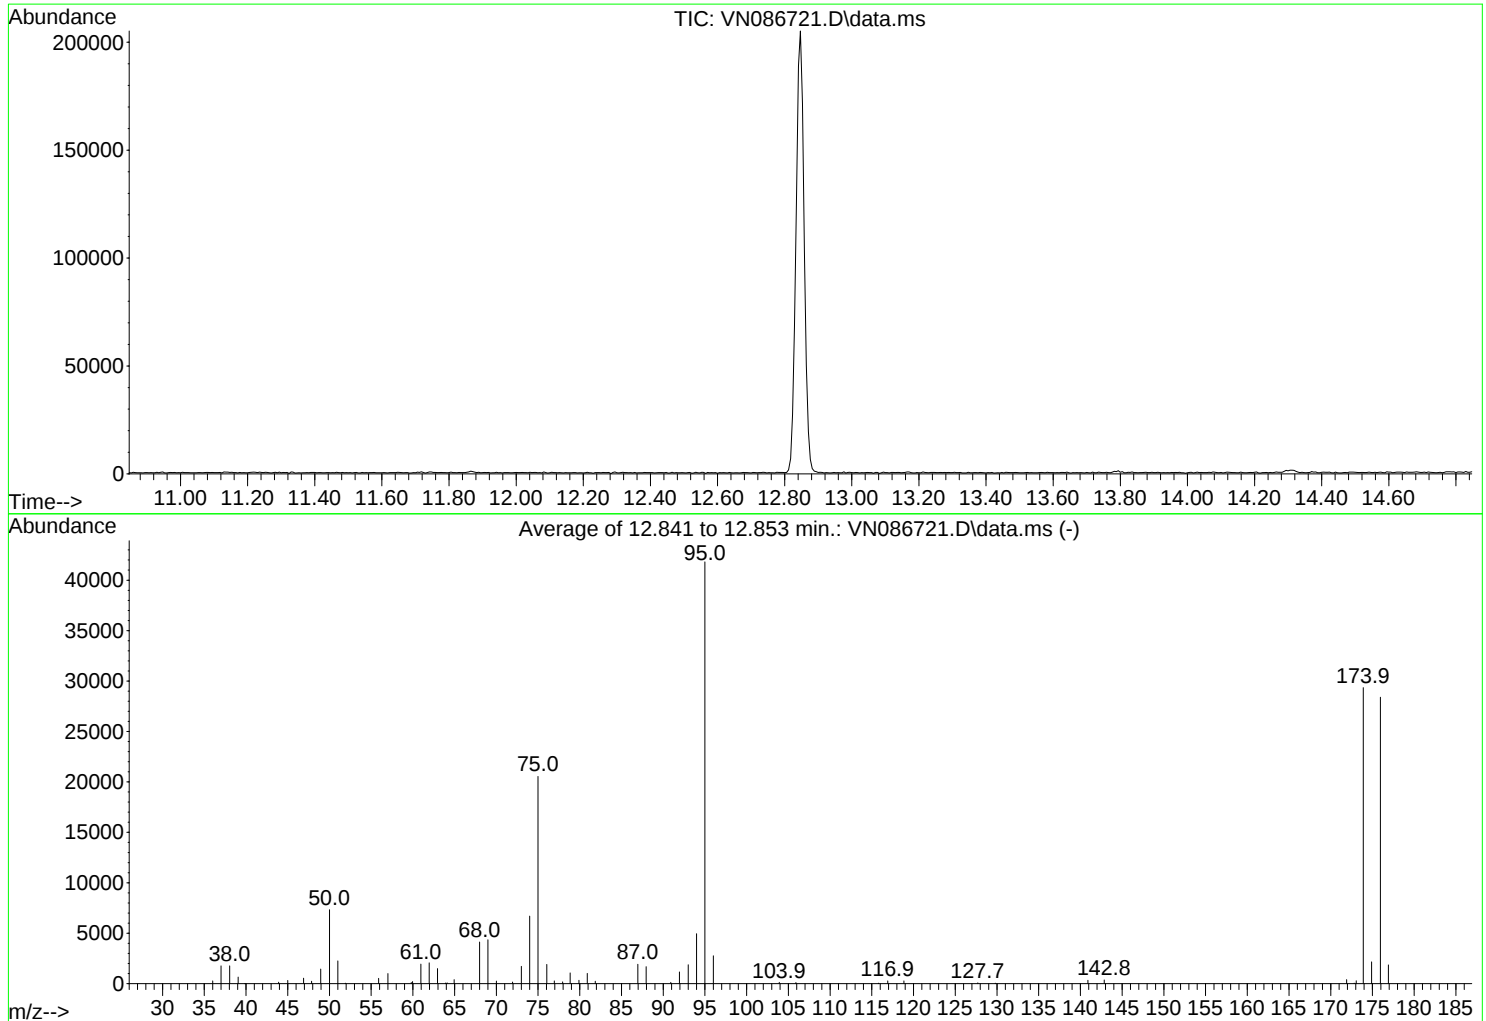

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	7326	PASS
75	95	30	60	49.1	20544	PASS
95	95	100	100	100.0	41819	PASS
96	95	5	9	6.6	2764	PASS
173	174	0.00	2	1.0	289	PASS
174	95	50	100	70.2	29341	PASS
175	174	5	9	7.3	2156	PASS
176	174	95	101	96.8	28400	PASS
177	176	5	9	6.5	1855	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	269	51.00	2252	64.95	401	78.85	106
37.00	1757	51.90	53	68.00	4123	79.90	33
38.05	1766	55.90	529	69.00	4347	80.90	101
39.05	654	57.00	992	70.00	253	81.85	24
39.85	7	59.80	111	71.95	159	86.95	1926
43.90	139	59.95	215	73.00	1716	87.95	1680
45.00	321	60.95	1937	74.00	6692	90.90	130
46.90	536	61.95	2069	75.00	20544	91.95	1152
47.85	234	62.95	1488	76.05	1912	93.00	1875
48.95	1444	63.90	59	76.95	268	94.00	4952
50.00	7326	64.10	77	77.95	169	95.00	41819

Average of 12.841 to 12.853 min.: VN086721.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
96.00	2764	172.80	57				
103.90	122	173.05	289				
105.90	115	173.90	29341				
115.80	52	174.90	2156				
116.90	268	175.95	28400				
118.85	264	176.90	1855				
127.70	78						
129.80	54						
140.90	330						
142.85	362						
171.90	394						

Instrument :

MSVOA_N

ClientSampleId :

BFB