

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052223\
 Data File : VN077783.D
 Acq On : 22 May 2023 12:42
 Operator : JC\MD
 Sample : 02880-03 20X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 RE132D6-20230517

Quant Time: May 23 04:18:54 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	393869	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	696869	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	603892	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	199907	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	257535	43.700	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.400%
35) Dibromofluoromethane	8.171	113	224421	49.386	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.780%
50) Toluene-d8	10.571	98	849528	48.569	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.140%
62) 4-Bromofluorobenzene	12.853	95	269830	43.680	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	87.360%
Target Compounds						Qvalue
3) Chloromethane	2.371	50	1296	Below Cal		90
9) 1,1,2-Trichlorotrifluo...	4.395	101	6382	1.464 ug/l #		61
10) Methyl Iodide	4.606	142	2203	0.424 ug/l #		88
12) 1,1-Dichloroethene	4.353	96	2291	0.553 ug/l #		62
13) Acrolein	4.183	56	309	Below Cal #		63
16) Acetone	4.442	43	1163	0.627 ug/l #		40
20) Methylene Chloride	5.271	84	2050	Below Cal #		70
27) cis-1,2-Dichloroethene	7.494	96	1655	0.297 ug/l		91
31) Cyclohexane	8.236	56	9002	1.124 ug/l #		1
36) 1,1-Dichloropropene	8.230	75	33050	4.972 ug/l #		50
38) Carbon Tetrachloride	8.236	117	43611	6.498 ug/l #		17
39) Methylcyclohexane	9.365	83	5844	0.718 ug/l #		1
44) Trichloroethene	9.359	130	461317	92.887 ug/l		97
45) 1,2-Dichloropropane	9.353	63	1496	0.299 ug/l #		1
51) 4-Methyl-2-Pentanone	10.465	43	1561	0.271 ug/l #		55
58) 2-Chloroethyl Vinyl ether	10.171	63	3722	1.032 ug/l		95
59) 2-Hexanone	11.206	43	1661	0.390 ug/l		98
64) Tetrachloroethene	11.112	164	1458	0.345 ug/l		90
76) 1,2,3-Trichloropropane	12.853	75	140909	28.146 ug/l #		1
77) Bromobenzene	12.982	156	808	0.205 ug/l		87
79) 2-Chlorotoluene	13.223	91	2823	0.233 ug/l		98
81) trans-1,4-Dichloro-2-b...	12.853	75	140909	89.969 ug/l #		15
82) 4-Chlorotoluene	13.223	91	2823	0.234 ug/l		96
87) 1,3-Dichlorobenzene	13.753	146	2802	0.385 ug/l		69
88) 1,4-Dichlorobenzene	13.753	146	2802	0.388 ug/l		71
89) n-Butylbenzene	14.059	91	3440	0.261 ug/l		87
91) 1,2-Dichlorobenzene	14.112	146	2302	0.339 ug/l		85
92) 1,2-Dibromo-3-Chloropr...	14.735	75	341	0.332 ug/l #		27
93) 1,2,4-Trichlorobenzene	15.412	180	2134	0.537 ug/l #		59
95) Naphthalene	15.647	128	8513	0.623 ug/l #		93
96) 1,2,3-Trichlorobenzene	15.841	180	2812	0.723 ug/l		96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052223\
Data File : VN077783.D
Acq On : 22 May 2023 12:42
Operator : JC\MD
Sample : 02880-03 20X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517

Quant Time: May 23 04:18:54 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration




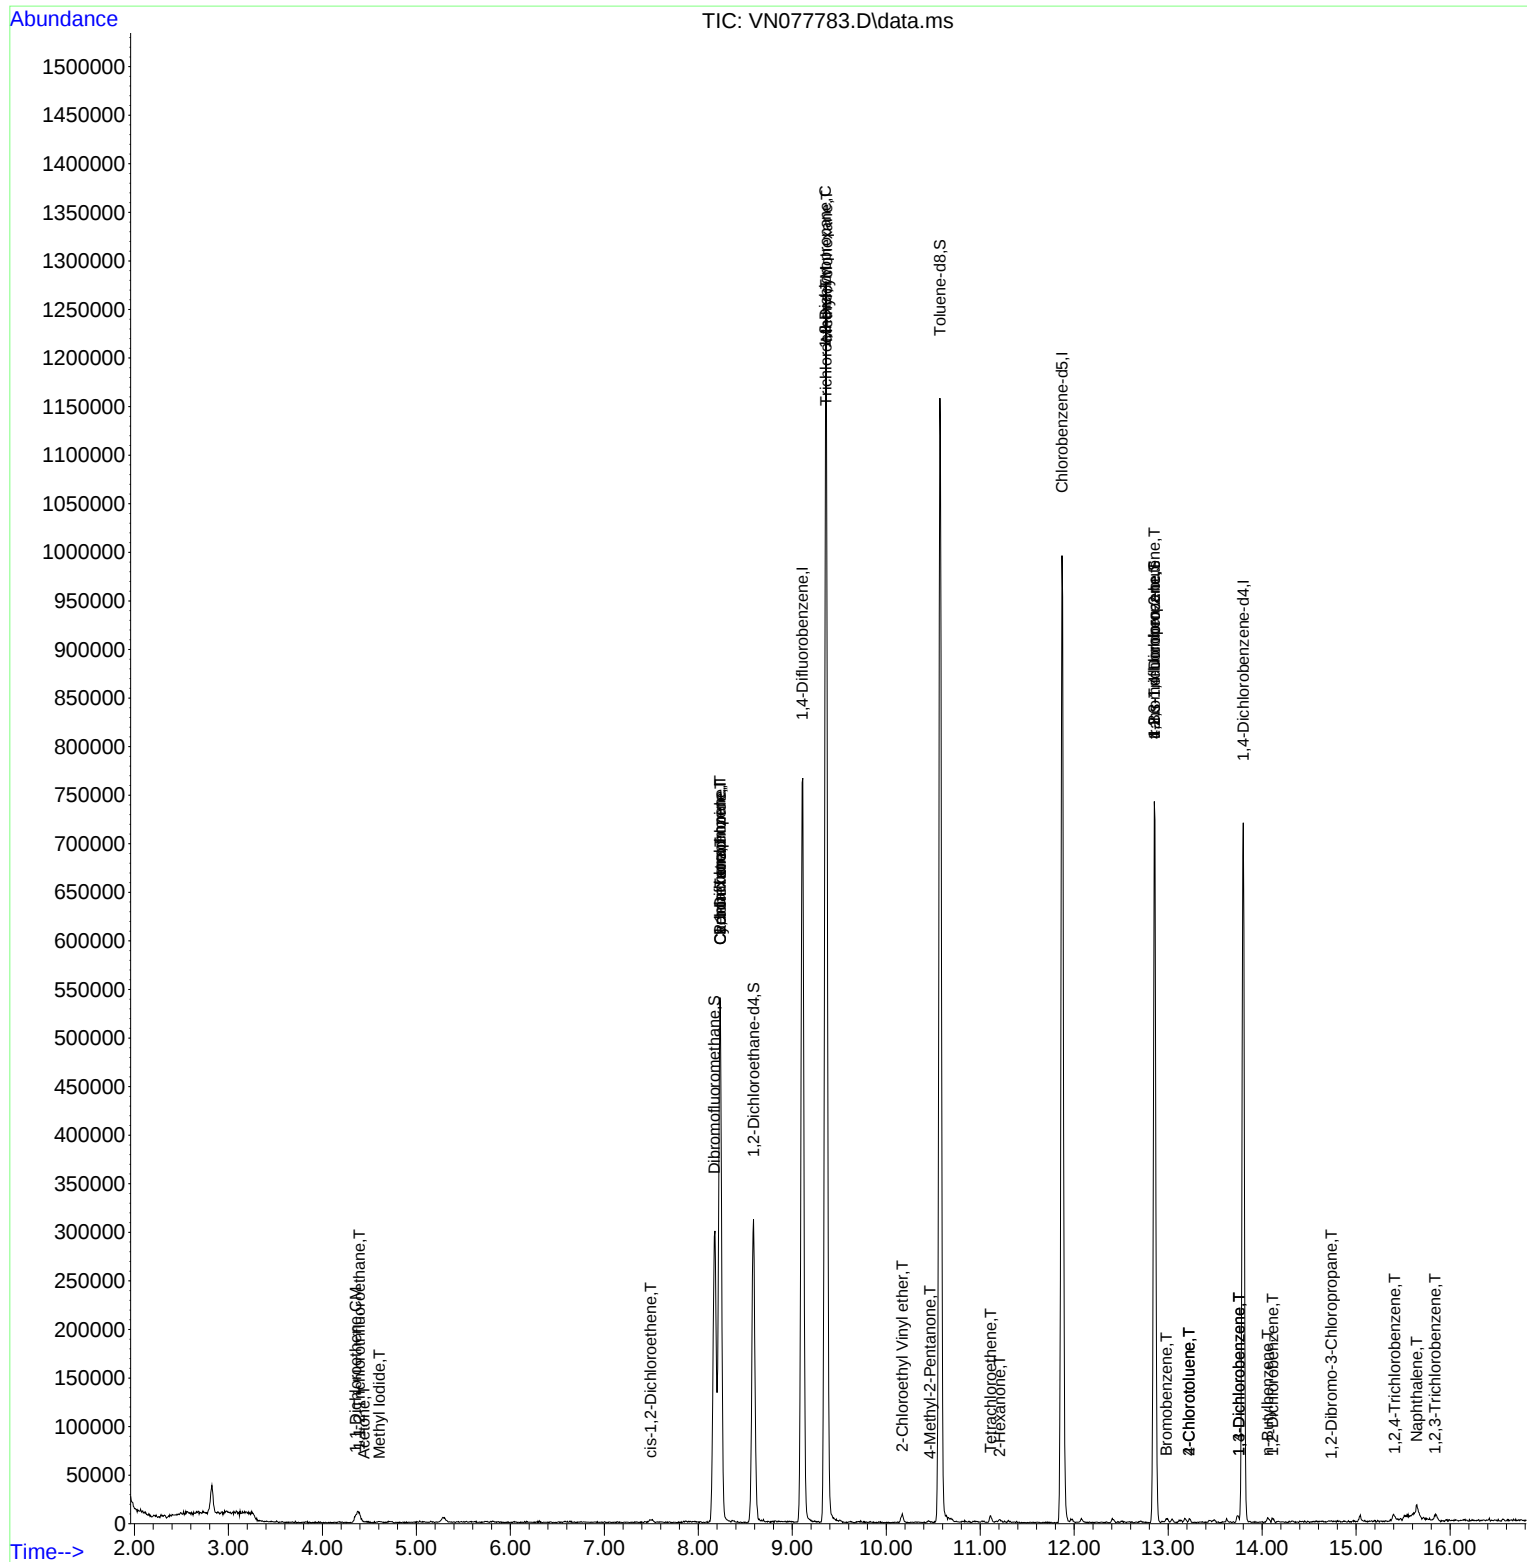




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:168 Resp: 393869
Ion Ratio Lower Upper
168 100
99 60.5 53.0 79.6

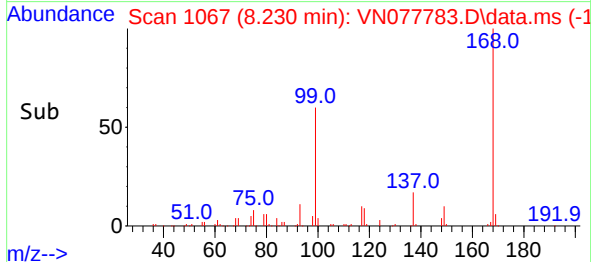

#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 50 Resp: 1296
Ion Ratio Lower Upper
50 100
52 27.4 26.5 39.7


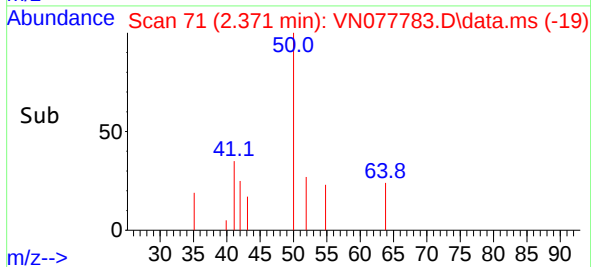

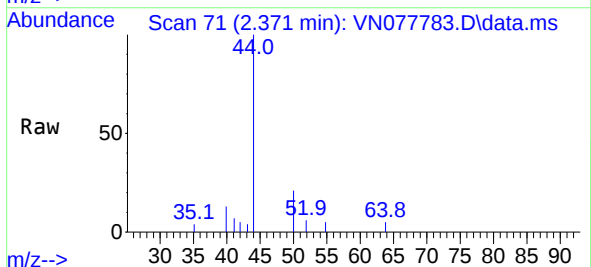




#9
1,1,2-Trichlorotrifluoroethane
Concen: 1.464 ug/l
RT: 4.395 min Scan# 412
Delta R.T. 0.018 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:101 Resp: 6382
Ion Ratio Lower Upper
101 100
85 0.0 36.6 55.0#
151 88.5 57.6 86.4#

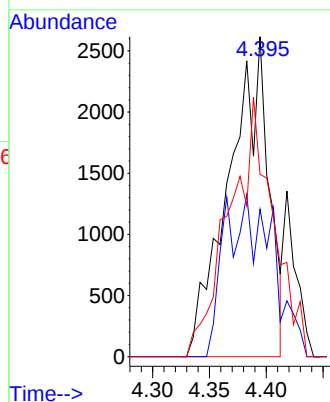

#10
Methyl Iodide
Concen: 0.424 ug/l
RT: 4.606 min Scan# 451
Delta R.T. 0.012 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion:142 Resp: 2203
Ion Ratio Lower Upper
142 100
127 41.3 37.6 56.4
141 23.0 11.4 17.0#


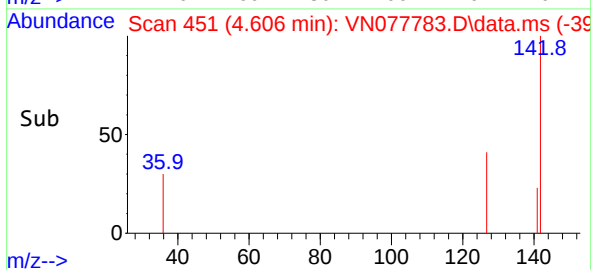






#12
1,1-Dichloroethene
Concen: 0.553 ug/l
RT: 4.353 min Scan# 408
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 96 Resp: 2291
Ion Ratio Lower Upper
96 100
61 94.8 112.7 169.1#
98 33.8 51.2 76.8#



#13
Acrolein
Concen: Below Cal
RT: 4.183 min Scan# 379
Delta R.T. -0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 56 Resp: 309
Ion Ratio Lower Upper
56 100
55 98.1 54.5 81.7#



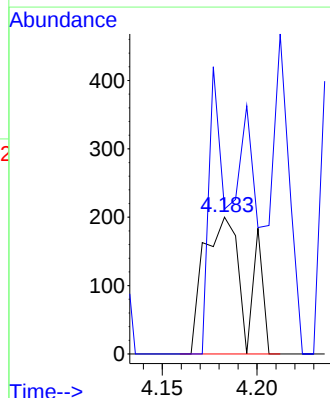





#16
Acetone
Concen: 0.627 ug/l
RT: 4.442 min Scan# 41
Delta R.T. 0.012 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 43 Resp: 1163
Ion Ratio Lower Upper
43 100
58 0.0 28.0 42.0#

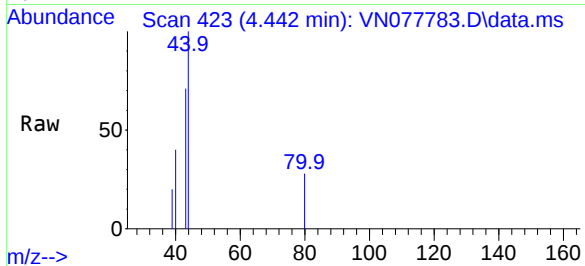

#20
Methylene Chloride
Concen: Below Cal
RT: 5.271 min Scan# 564
Delta R.T. -0.012 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 84 Resp: 2050
Ion Ratio Lower Upper
84 100
49 59.9 79.7 119.5#
51 34.8 25.2 37.8
86 44.0 53.3 79.9#



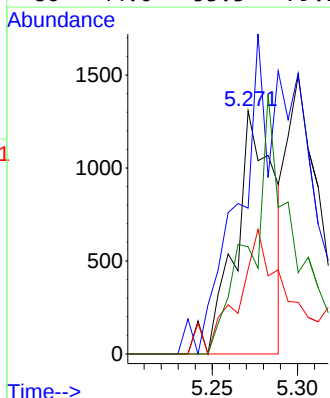
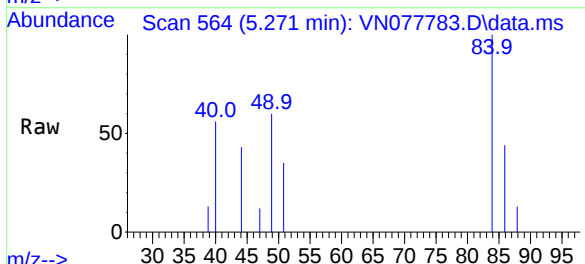




#27
cis-1,2-Dichloroethene
Concen: 0.297 ug/l
RT: 7.494 min Scan# 94
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 96 Resp: 1655
Ion Ratio Lower Upper
96 100
61 112.2 0.0 255.2
98 64.8 0.0 128.8



#31
Cyclohexane
Concen: 1.124 ug/l
RT: 8.236 min Scan# 1068
Delta R.T. -0.030 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 56 Resp: 9002
Ion Ratio Lower Upper
56 100
69 175.0 26.8 40.2#
84 152.2 81.8 122.6#


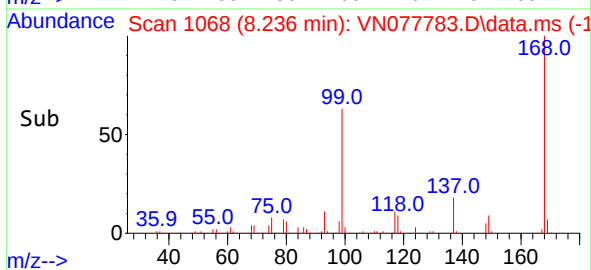

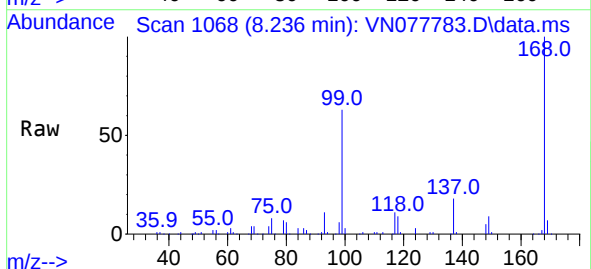




#33
1,2-Dichloroethane-d4
Concen: 43.700 ug/l
RT: 8.588 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 65 Resp: 257535
Ion Ratio Lower Upper
65 100
67 51.9 0.0 106.6

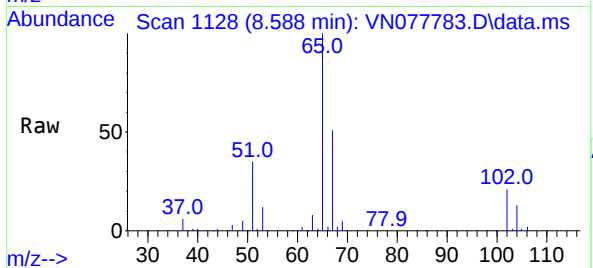

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.106 min Scan# 1216
Delta R.T. 0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42


Tgt Ion: 114 Resp: 696869
Ion Ratio Lower Upper
114 100
63 20.4 0.0 36.4
88 15.3 0.0 30.6

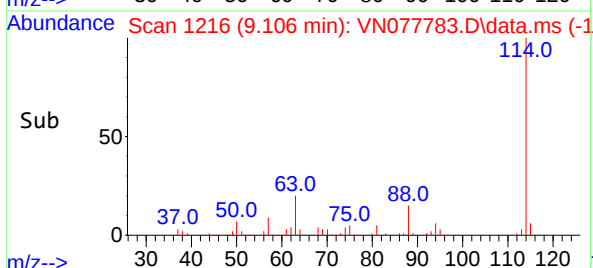



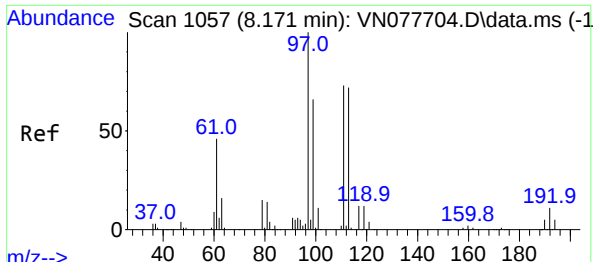


#35
Dibromofluoromethane
Concen: 49.386 ug/l
RT: 8.171 min Scan# 1057
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517



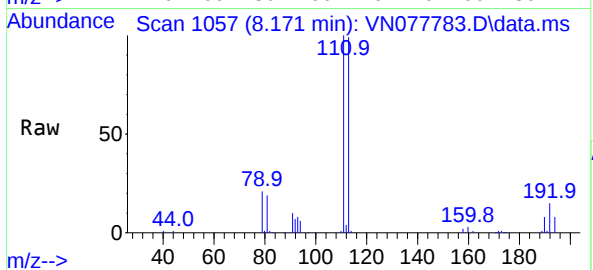



Tgt Ion:113 Resp: 224421
Ion Ratio Lower Upper
113 100
111 101.9 82.6 123.8
192 16.9 12.7 19.1

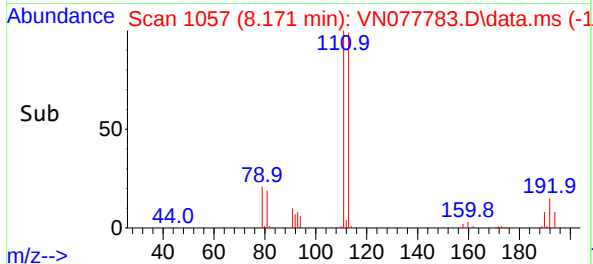

#36
1,1-Dichloropropene
Concen: 4.972 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 75 Resp: 33050
Ion Ratio Lower Upper
75 100
110 11.7 19.1 57.3#
77 0.0 25.0 37.4#


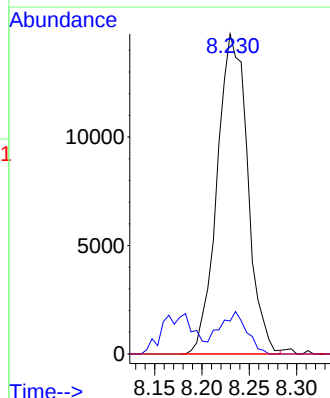
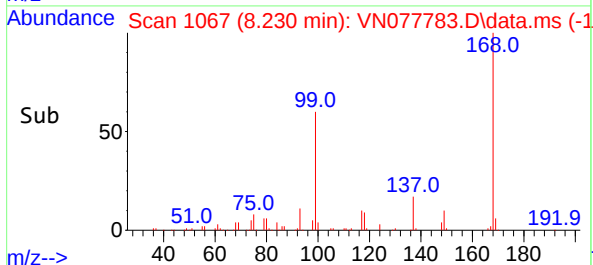
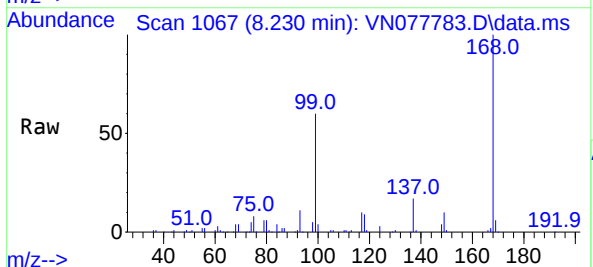




#38
Carbon Tetrachloride
Concen: 6.498 ug/l
RT: 8.236 min Scan# 1091
Delta R.T. -0.136 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:117 Resp: 43611
Ion Ratio Lower Upper
117 100
119 6.5 77.3 115.9#
121 0.0 23.3 34.9#

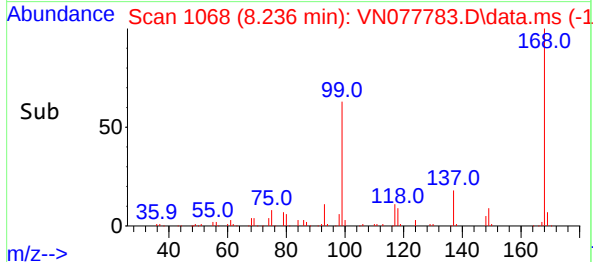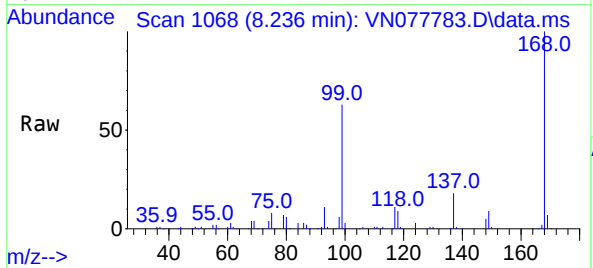

#39
Methylcyclohexane
Concen: 0.718 ug/l
RT: 9.365 min Scan# 1260
Delta R.T. -0.241 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 83 Resp: 5844
Ion Ratio Lower Upper
83 100
55 0.0 49.1 73.7#
98 186.6 40.6 61.0#


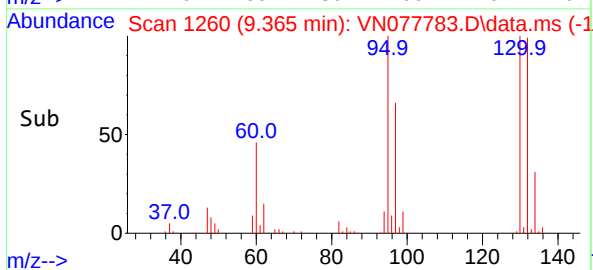

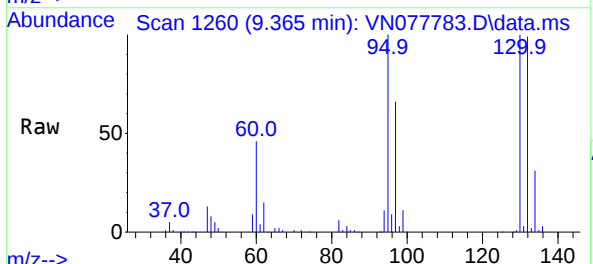




#44
Trichloroethene
Concen: 92.887 ug/l
RT: 9.359 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:130 Resp: 461317
Ion Ratio Lower Upper
130 100
95 99.1 0.0 204.6

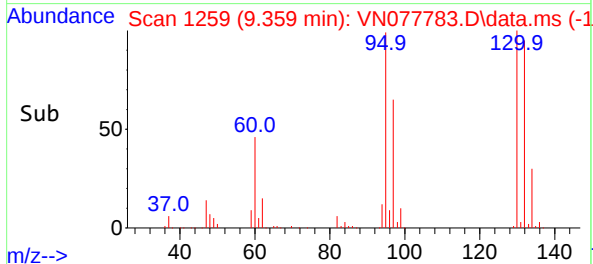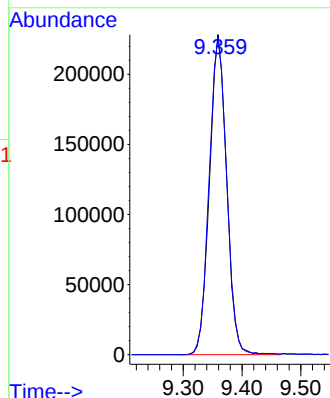

#45
1,2-Dichloropropane
Concen: 0.299 ug/l
RT: 9.353 min Scan# 1258
Delta R.T. -0.271 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 63 Resp: 1496
Ion Ratio Lower Upper
63 100
65 282.5 23.9 35.9#


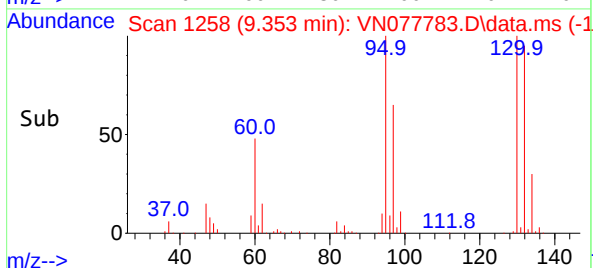

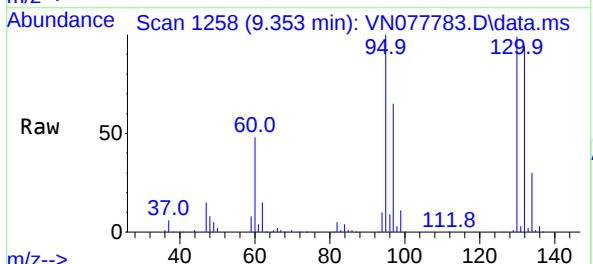




#50
Toluene-d8
Concen: 48.569 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 98 Resp: 849528
Ion Ratio Lower Upper
98 100
100 63.9 52.0 78.0

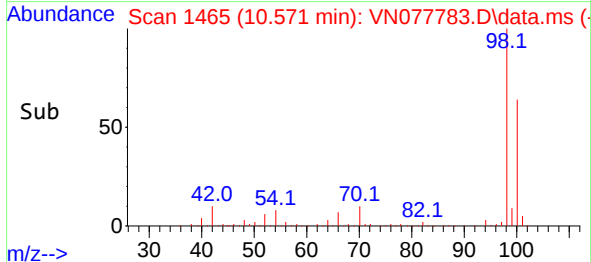

#51
4-Methyl-2-Pentanone
Concen: 0.271 ug/l
RT: 10.465 min Scan# 1447
Delta R.T. 0.018 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 43 Resp: 1561
Ion Ratio Lower Upper
43 100
58 15.8 36.6 54.8#


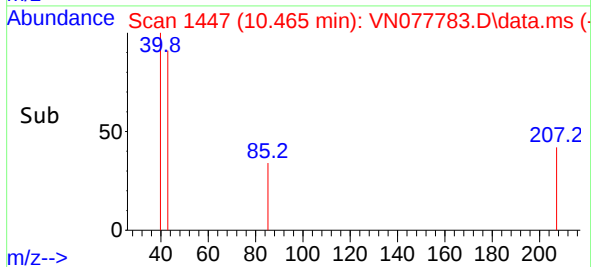

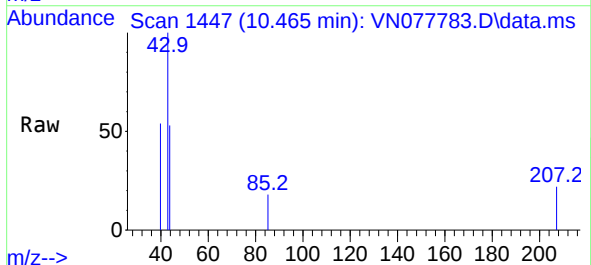




#58
2-Chloroethyl Vinyl ether
Concen: 1.032 ug/l
RT: 10.171 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 63 Resp: 3722
Ion Ratio Lower Upper
63 100
106 30.0 26.2 39.4

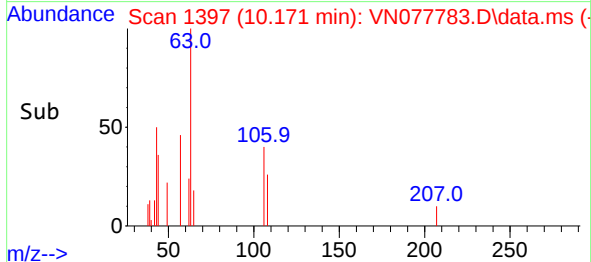

#59
2-Hexanone
Concen: 0.390 ug/l
RT: 11.206 min Scan# 1573
Delta R.T. 0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 43 Resp: 1661
Ion Ratio Lower Upper
43 100
58 64.8 31.7 95.1


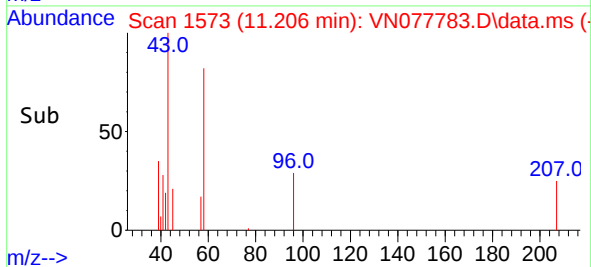

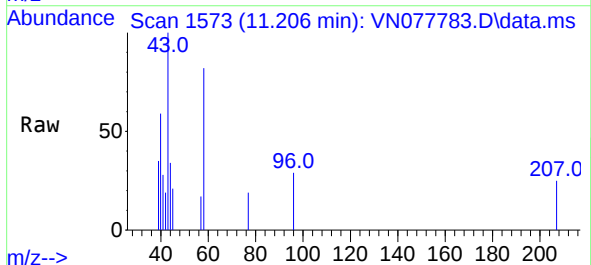


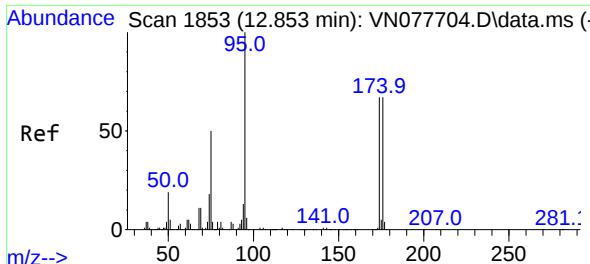

#62
4-Bromofluorobenzene
Concen: 43.680 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 95 Resp: 269830
Ion Ratio Lower Upper
95 100
174 74.3 0.0 143.8
176 71.2 0.0 135.8

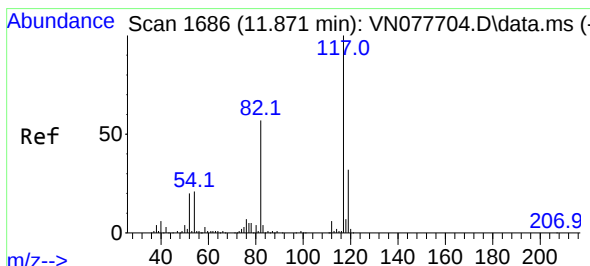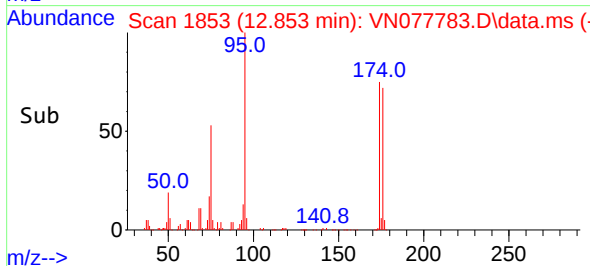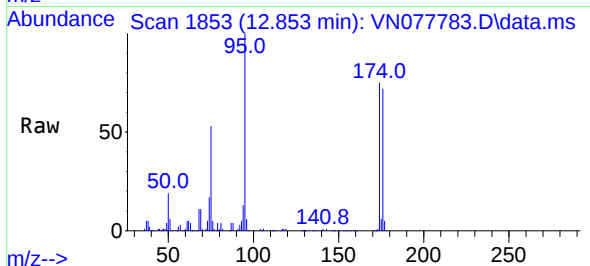

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.001 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42


Tgt Ion: 117 Resp: 603892
Ion Ratio Lower Upper
117 100
82 53.8 44.0 66.0
119 31.8 25.6 38.4

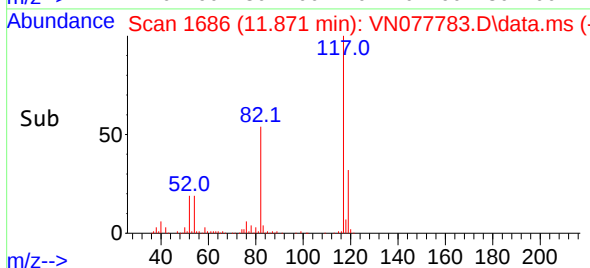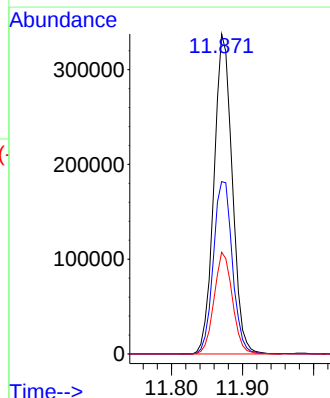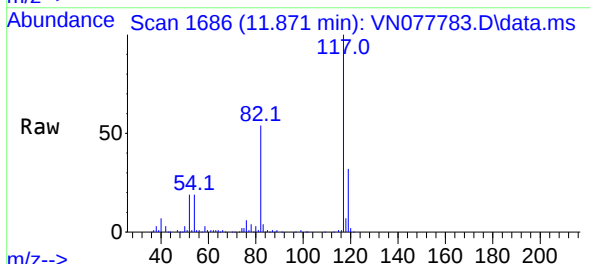





#64
Tetrachloroethene
Concen: 0.345 ug/l
RT: 11.112 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517



Tgt Ion:164 Resp: 1458




Ion	Ratio	Lower	Upper
164	100		
166	117.8	101.4	152.0
129	85.3	82.4	123.6
131	93.1	78.2	117.4




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion:152 Resp: 199907

Ion	Ratio	Lower	Upper
152	100		
115	62.0	32.3	96.8
150	157.9	0.0	355.8


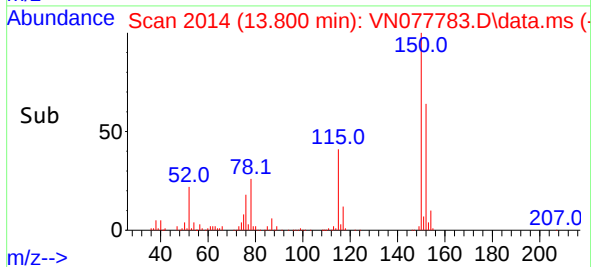

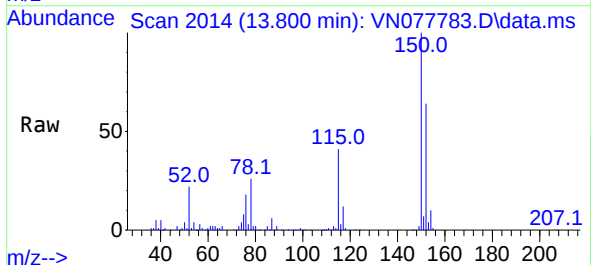


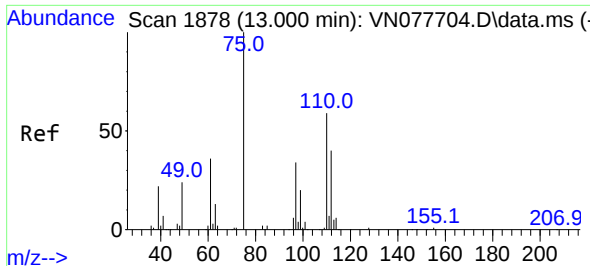

#76
1,2,3-Trichloropropane
Concen: 28.146 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 75 Resp: 140909
Ion Ratio Lower Upper
75 100
77 1.3 84.5 253.5#

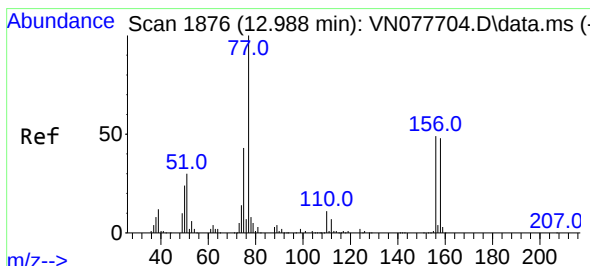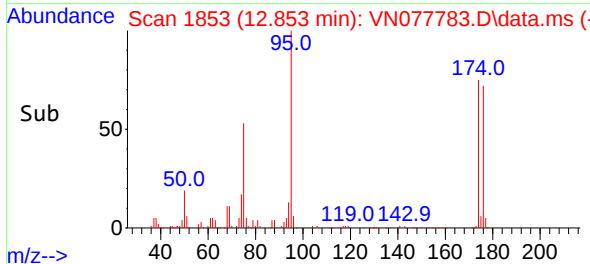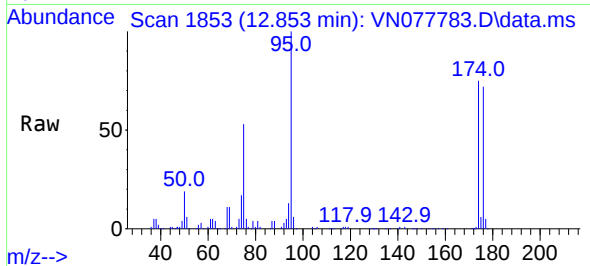

#77
Bromobenzene
Concen: 0.205 ug/l
RT: 12.982 min Scan# 1875
Delta R.T. -0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion:156 Resp: 808
Ion Ratio Lower Upper
156 100
77 217.0 107.7 323.3
158 135.6 48.4 145.3


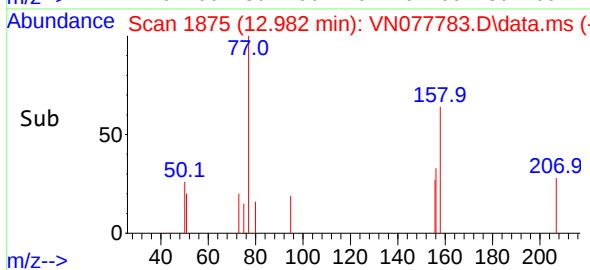

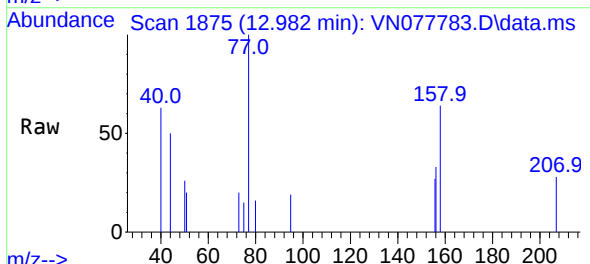




#79
2-Chlorotoluene
Concen: 0.233 ug/l
RT: 13.223 min Scan# 1900
Delta R.T. 0.094 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 91 Resp: 2823
Ion Ratio Lower Upper
91 100
126 31.3 16.3 48.8



#81
trans-1,4-Dichloro-2-butene
Concen: 89.969 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.112 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 75 Resp: 140909
Ion Ratio Lower Upper
75 100
53 0.0 67.4 101.2#
89 0.0 38.8 58.2#


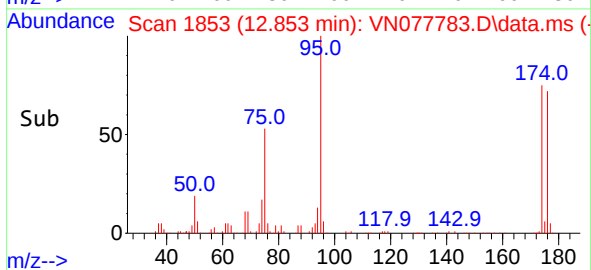






#82
4-Chlorotoluene
Concen: 0.234 ug/l
RT: 13.223 min Scan# 1917
Delta R.T. -0.006 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion: 91 Resp: 2823
Ion Ratio Lower Upper
91 100
126 31.3 16.7 50.0

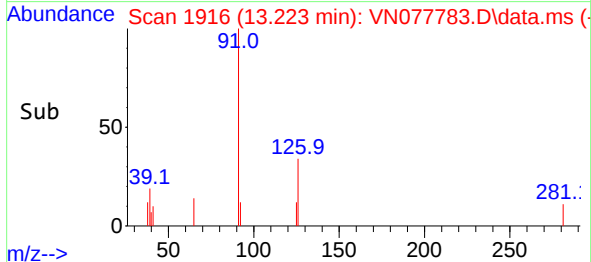

#87
1,3-Dichlorobenzene
Concen: 0.385 ug/l
RT: 13.753 min Scan# 2006
Delta R.T. 0.012 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 146 Resp: 2802
Ion Ratio Lower Upper
146 100
111 29.9 22.1 66.3
148 35.5 32.0 96.0


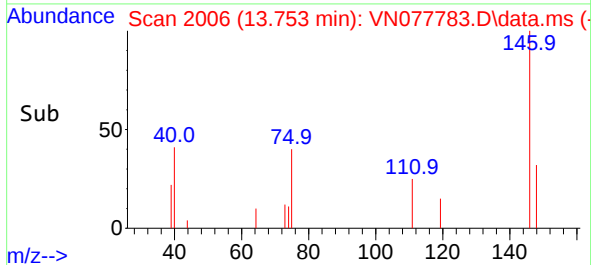

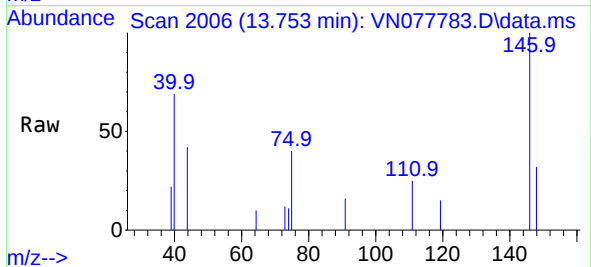




#88
1,4-Dichlorobenzene
Concen: 0.388 ug/l
RT: 13.753 min Scan# 2006
Delta R.T. -0.064 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:146 Resp: 2802
Ion Ratio Lower Upper
146 100
111 29.9 20.6 61.8
148 35.5 31.6 94.8

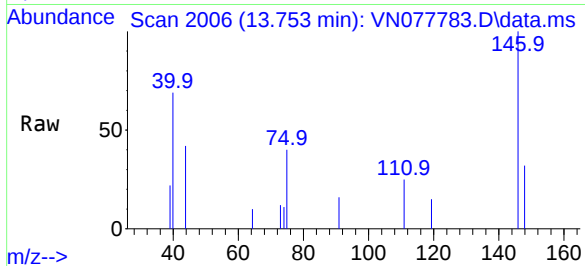

#89
n-Butylbenzene
Concen: 0.261 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.005 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42

Tgt Ion: 91 Resp: 3440
Ion Ratio Lower Upper
91 100
92 45.3 26.4 79.0
134 15.7 12.6 37.6

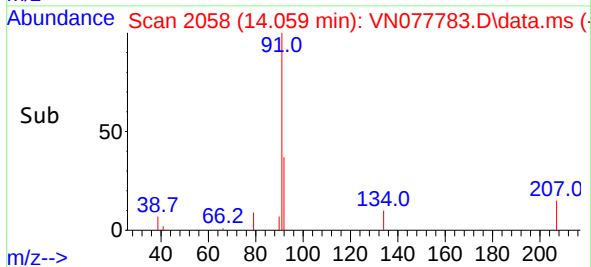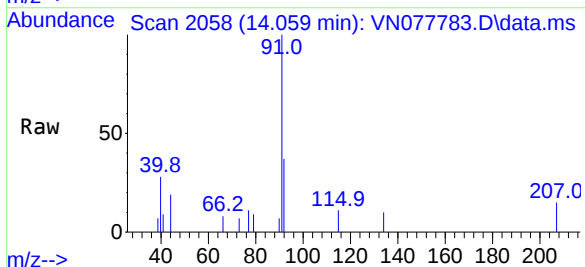



#91

1,2-Dichlorobenzene

Concen: 0.339 ug/l

RT: 14.112 min Scan# 2067

Delta R.T. 0.001 min

Lab File: VN077783.D

Acq: 22 May 2023 12:42

Instrument :

MSVOA_N

ClientSampleId :

RE132D6-20230517





Tgt Ion:146 Resp: 2302

Ion Ratio Lower Upper

146 100

111 36.9 22.0 66.0

148 50.3 31.8 95.3

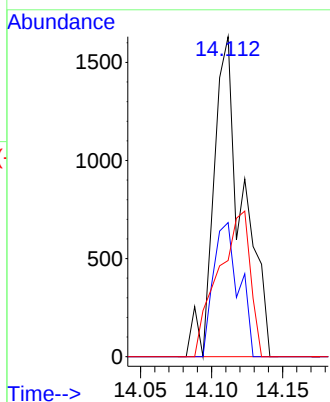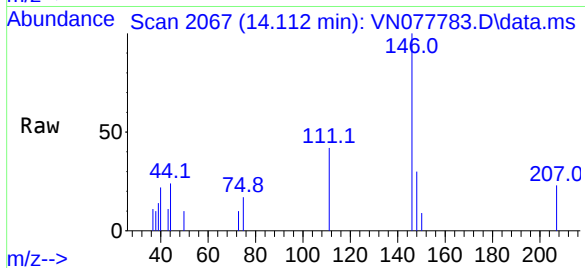

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.332 ug/l

RT: 14.735 min Scan# 2173

Delta R.T. 0.012 min

Lab File: VN077783.D

Acq: 22 May 2023 12:42




Tgt Ion: 75 Resp: 341


Ion Ratio Lower Upper

75 100

155 0.0 39.1 117.2#

157 40.8 50.3 150.9#


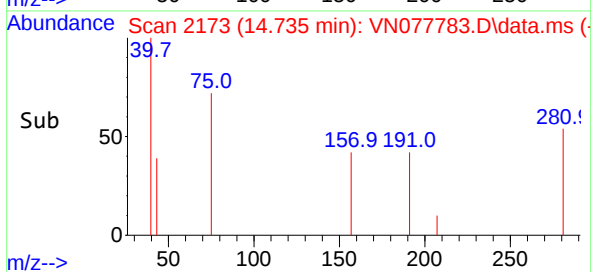

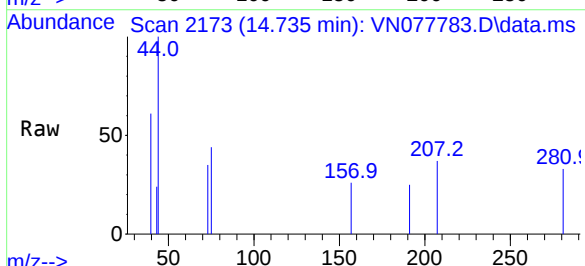




#93
1,2,4-Trichlorobenzene
Concen: 0.537 ug/l
RT: 15.412 min Scan# 2134
Delta R.T. 0.011 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42




Instrument :
MSVOA_N
ClientSampleId :
RE132D6-20230517


Tgt Ion:180 Resp: 2134
Ion Ratio Lower Upper
180 100
182 124.8 46.1 138.2
145 0.0 16.6 49.8#

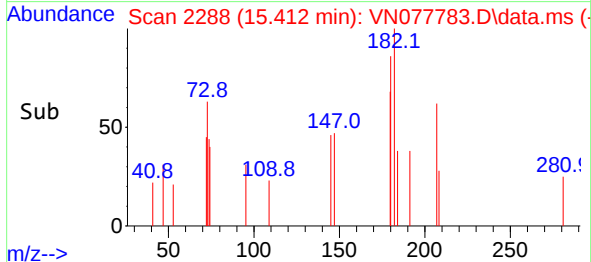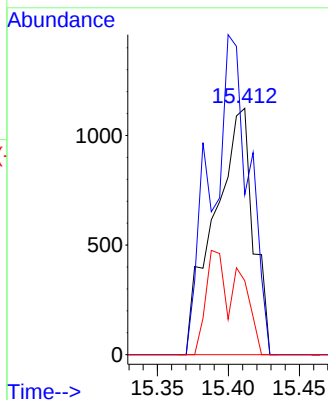

#95
Naphthalene
Concen: 0.623 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN077783.D
Acq: 22 May 2023 12:42


Tgt Ion:128 Resp: 8513
Ion Ratio Lower Upper
128 100
127 13.0 10.0 15.0
129 15.9 8.7 13.1#

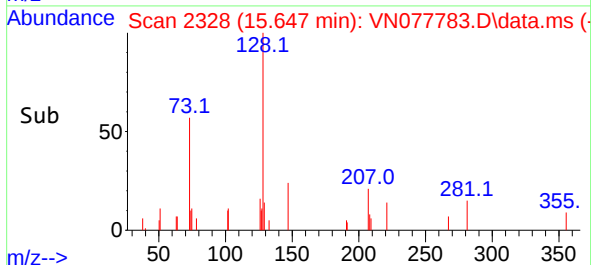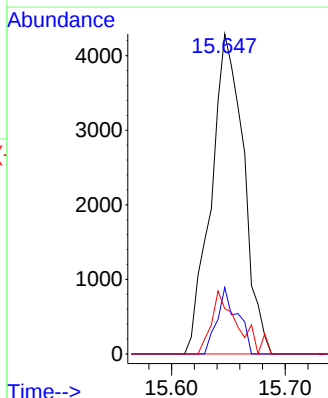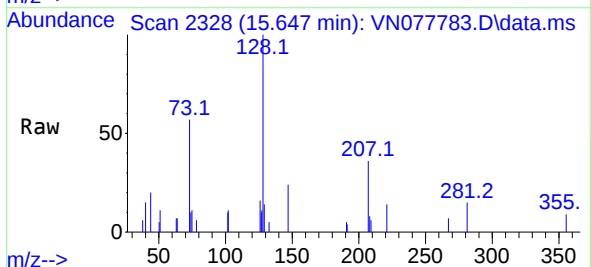



#96
 1,2,3-Trichlorobenzene
 Concen: 0.723 ug/l
 RT: 15.841 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: VN077783.D
 Acq: 22 May 2023 12:42

Instrument :
 MSVOA_N
 ClientSampleId :
 RE132D6-20230517



Tgt Ion:	180	Resp:	2812
Ion	Ratio	Lower	Upper
180	100		
182	96.4	46.2	138.6
145	37.9	17.5	52.6

