
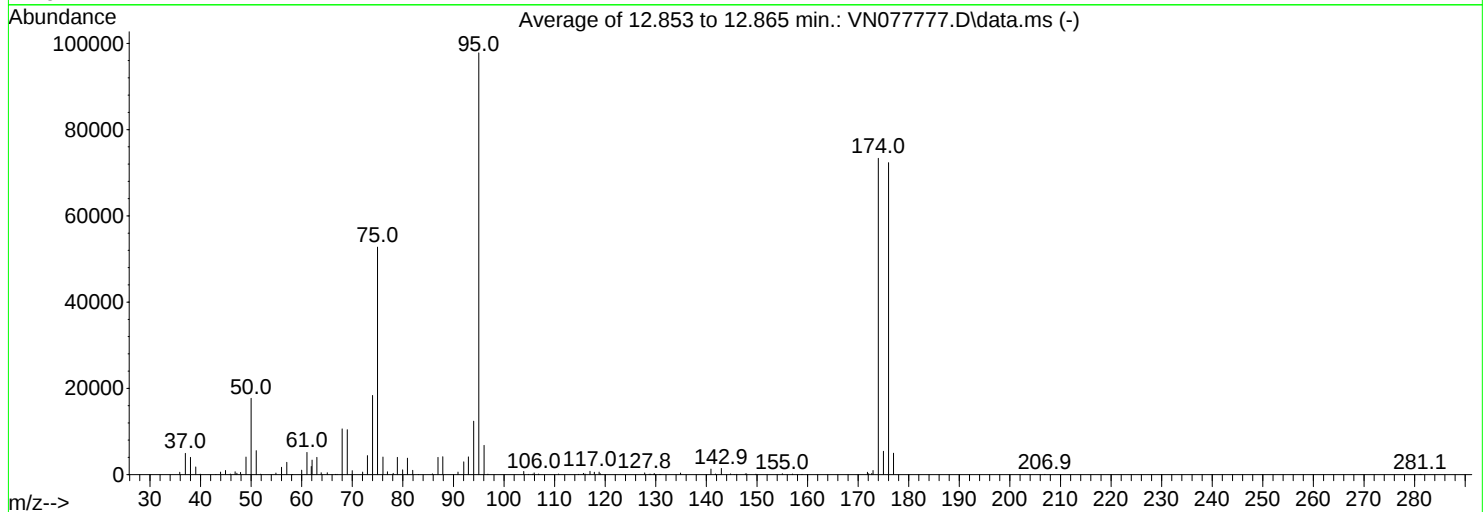


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052223\
Data File : VN077777.D
Acq On : 22 May 2023 09:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

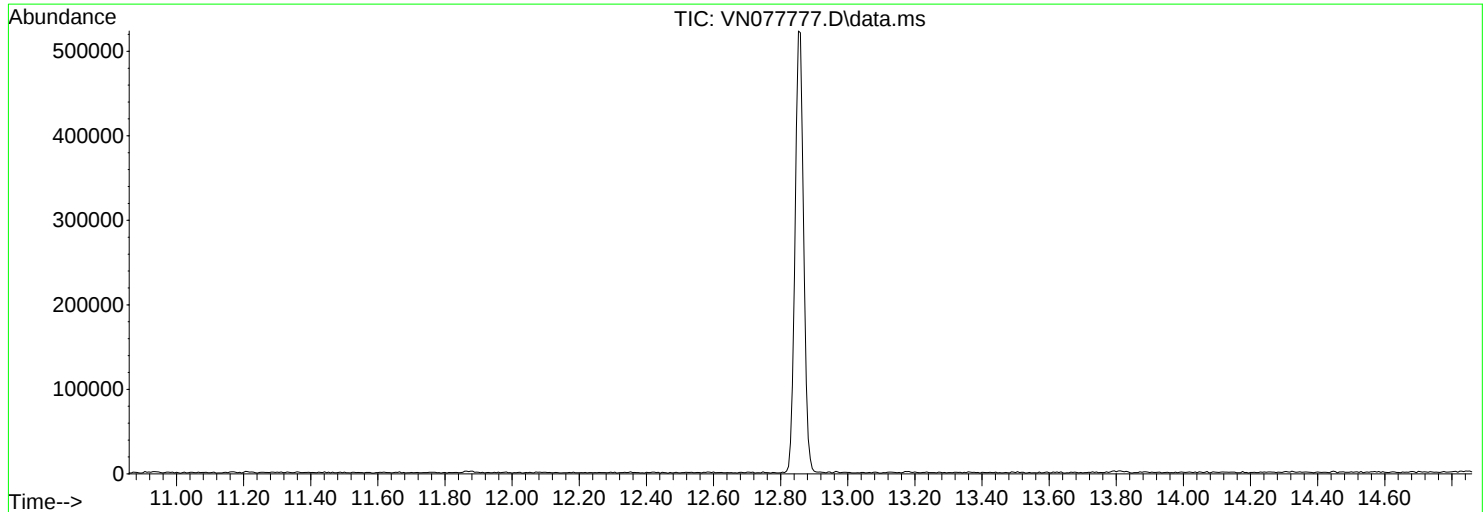

AutoFind: Scans 1853, 1854, 1855; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.1	17680	PASS
75	95	30	60	53.9	52744	PASS
95	95	100	100	100.0	97805	PASS
96	95	5	9	6.9	6794	PASS
173	174	0.00	2	1.3	977	PASS
174	95	50	100	75.0	73365	PASS
175	174	5	9	7.4	5410	PASS
176	174	95	101	98.6	72331	PASS
177	176	5	9	6.9	4982	PASS

Average of 12.853 to 12.865 min.: VN077777.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	570	47.90	511	61.90	1888	73.00	440
37.00	4947	49.00	4099	62.05	3364	74.00	1837
38.00	3995	50.00	17680	63.00	4013	75.00	5274
39.05	1778	51.00	5567	63.85	449	76.05	407
39.95	118	51.90	124	65.05	438	76.95	666
43.05	20	54.90	387	66.70	84	78.10	296
43.95	607	56.00	1693	67.00	95	78.90	3997
44.95	949	57.05	2870	68.00	10606	79.95	1109
45.90	156	58.20	53	69.00	10438	80.90	3843
46.85	667	60.00	1025	70.00	926	81.95	1004
47.20	342	61.05	5171	72.05	610	83.10	54

Average of 12.853 to 12.865 min.: VN077777.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.85	194	104.80	95	119.00	210	142.95	1437
86.95	4018	105.70	98	127.80	398	144.80	185
87.90	4153	105.95	395	128.70	131	145.50	55
90.90	584	106.85	169	129.00	97	146.00	80
92.05	2972	110.80	141	129.60	157	147.70	187
92.95	4123	114.70	83	129.75	212	147.95	192
94.00	12391	115.70	302	130.80	78	149.80	130
95.00	97805	116.00	134	131.00	58	155.00	217
96.05	6794	117.00	764	134.90	358	157.00	136
96.80	119	117.85	570	140.90	1287	158.90	85
103.90	756	118.80	589	141.80	144	171.85	542

Average of 12.853 to 12.865 min.: VN077777.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.10	235						
172.70	261						
172.95	977						
174.00	73365						
175.00	5410						
176.00	72331						
177.00	4982						
206.90	91						
281.10	88						
281.30	59						

Instrument :

MSVOA_N

ClientSampleId :

BFB