

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052224\
 Data File : VN082297.D
 Acq On : 22 May 2024 17:02
 Operator : JC\MD
 Sample : PB161037ZHE#10
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB161037ZHE#10

Quant Time: May 23 01:54:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.230	168	171331	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	306901	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	289903	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	116408	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	143806	53.156	ug/l	0.00
Spiked Amount	50.000	Range 74 - 125	Recovery	= 106.320%		
35) Dibromofluoromethane	8.171	113	100691	53.335	ug/l	0.00
Spiked Amount	50.000	Range 75 - 124	Recovery	= 106.660%		
50) Toluene-d8	10.571	98	391625	54.106	ug/l	0.00
Spiked Amount	50.000	Range 86 - 113	Recovery	= 108.220%		
62) 4-Bromofluorobenzene	12.853	95	134380	52.016	ug/l	0.00
Spiked Amount	50.000	Range 64 - 133	Recovery	= 104.040%		
Target Compounds						
						Qvalue
16) Acetone	4.436	43	36623	33.000	ug/l	90
20) Methylene Chloride	5.277	84	11798	5.269	ug/l #	76
43) Isopropyl Acetate	8.688	43	337248	53.712	ug/l #	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052224\
Data File : VN082297.D
Acq On : 22 May 2024 17:02
Operator : JC\MD
Sample : PB161037ZHE#10
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB161037ZHE#10


Quant Time: May 23 01:54:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration

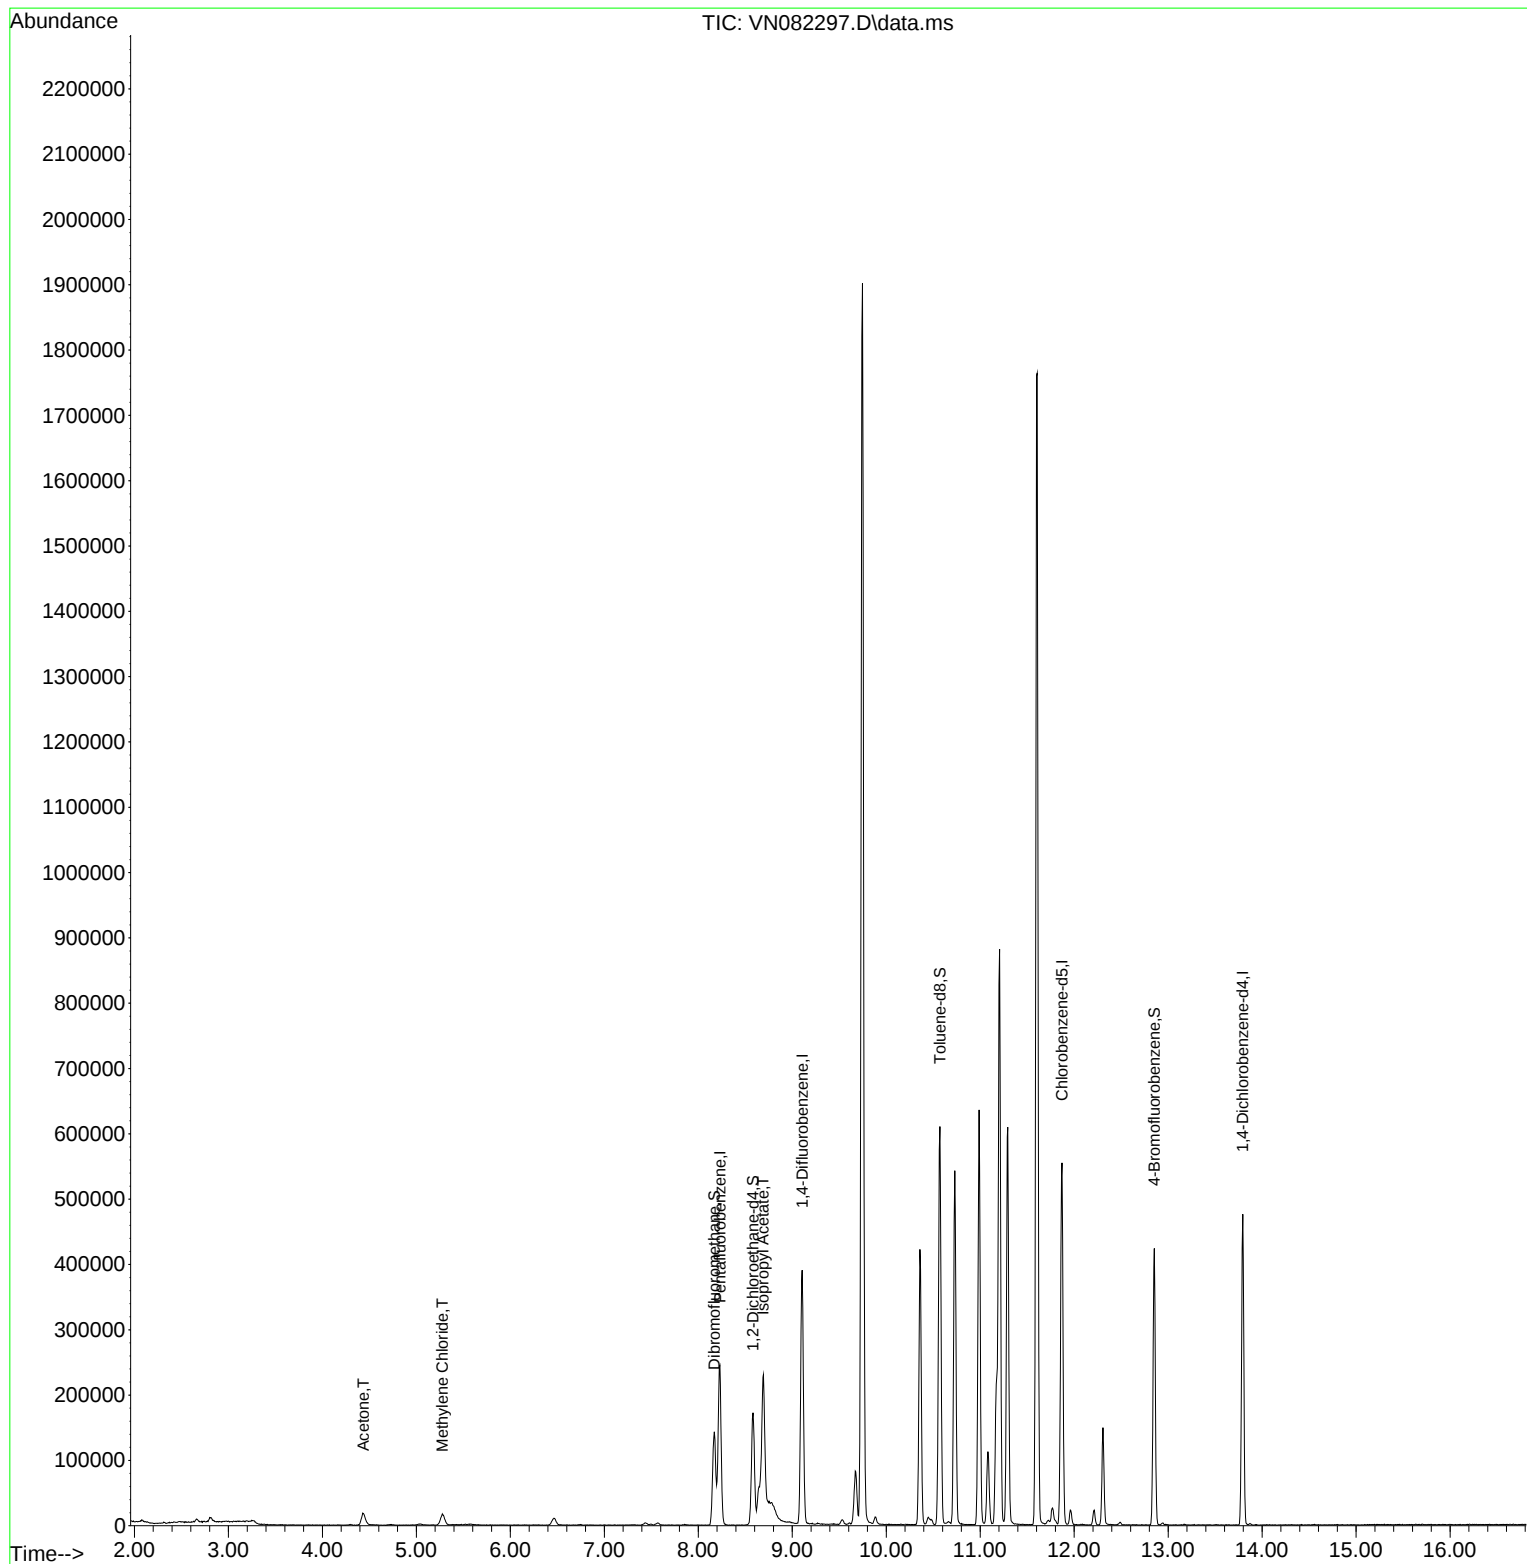


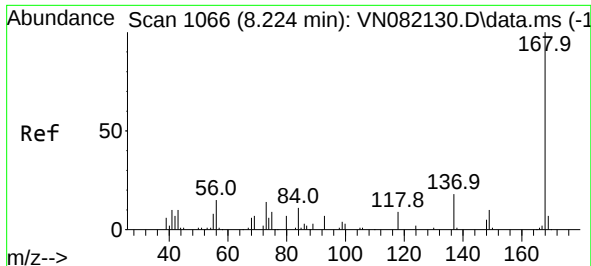


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02

Instrument :
MSVOA_N
ClientSampleId :
PB161037ZHE#10



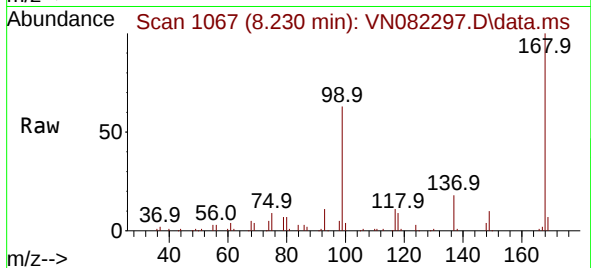


Tgt Ion:168 Resp: 171331
Ion Ratio Lower Upper
168 100
99 62.5 48.2 72.4

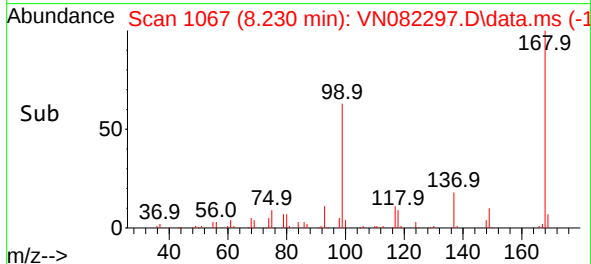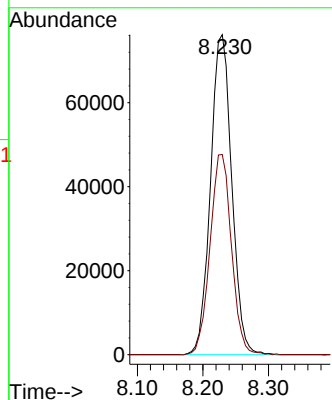

#16
Acetone
Concen: 33.000 ug/l
RT: 4.436 min Scan# 422
Delta R.T. 0.012 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02


Tgt Ion: 43 Resp: 36623
Ion Ratio Lower Upper
43 100
58 26.2 25.2 37.8

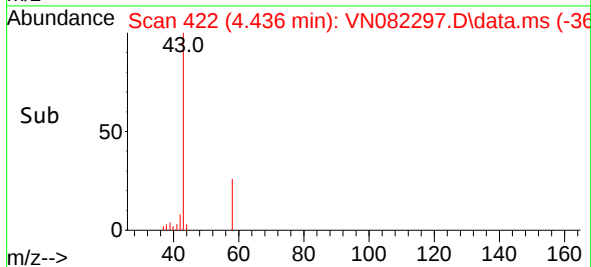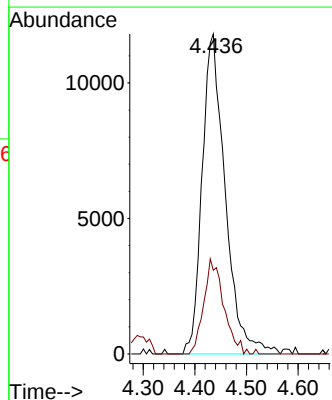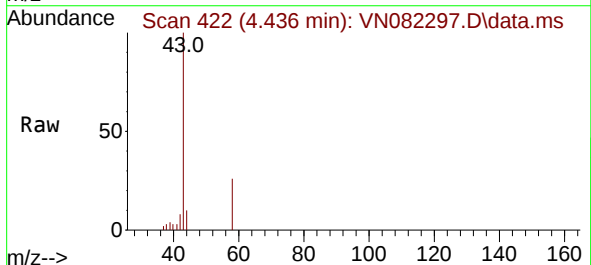






#20
Methylene Chloride
Concen: 5.269 ug/l
RT: 5.277 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02

Instrument :
MSVOA_N
ClientSampleId :
PB161037ZHE#10



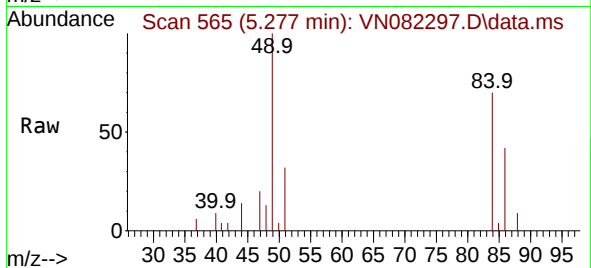



Tgt Ion:	84	Resp:	11798
Ion	Ratio	Lower	Upper
84	100		
49	142.5	84.9	127.3#
51	45.5	27.0	40.6#
86	60.2	52.3	78.5

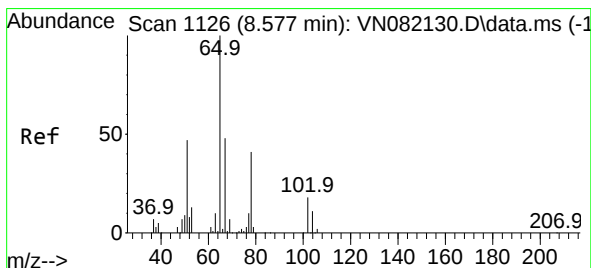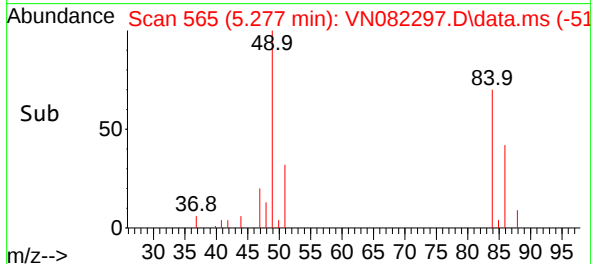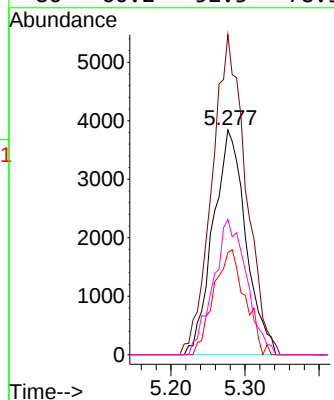

#33
1,2-Dichloroethane-d4
Concen: 53.156 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02

Tgt Ion:	65	Resp:	143806
Ion	Ratio	Lower	Upper
65	100		
67	50.0	0.0	103.0

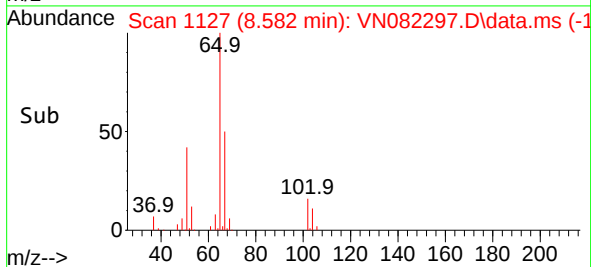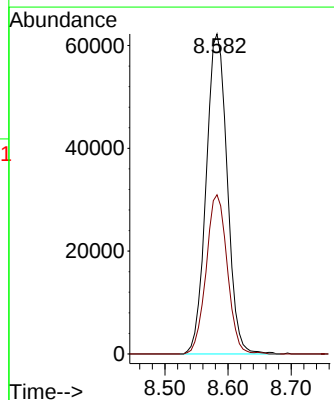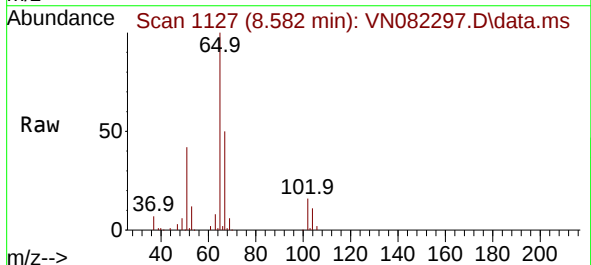

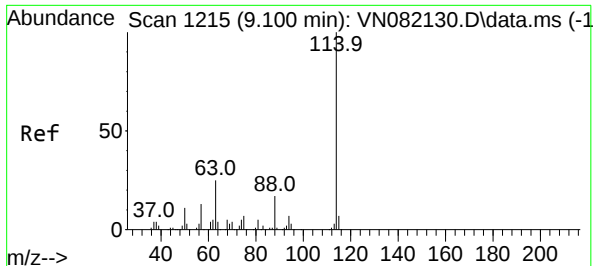

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN082297.D

Acq: 22 May 2024 17:02

Instrument :

MSVOA_N

ClientSampleId :

PB161037ZHE#10





Tgt Ion:114 Resp: 306901

Ion Ratio Lower Upper

114 100

63 23.3 0.0 41.0

88 17.0 0.0 31.4

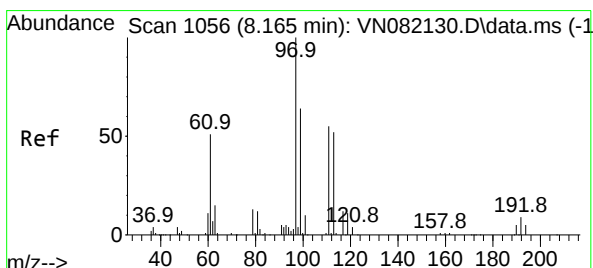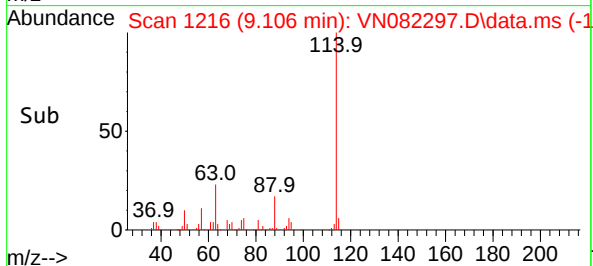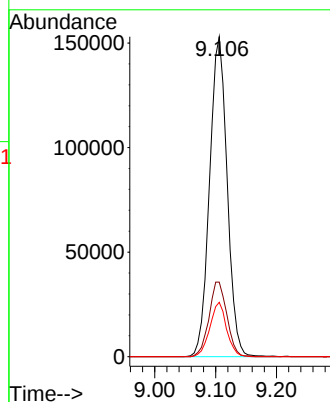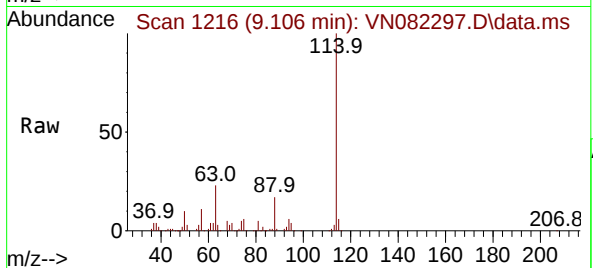

#35

Dibromofluoromethane

Concen: 53.335 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082297.D

Acq: 22 May 2024 17:02




Tgt Ion:113 Resp: 100691


Ion Ratio Lower Upper

113 100

111 102.6 83.4 125.2

192 18.3 14.0 21.0


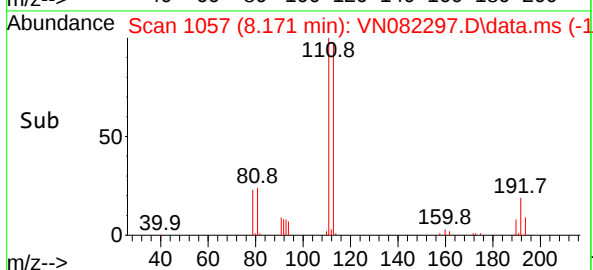
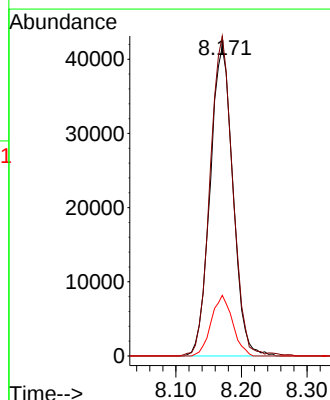
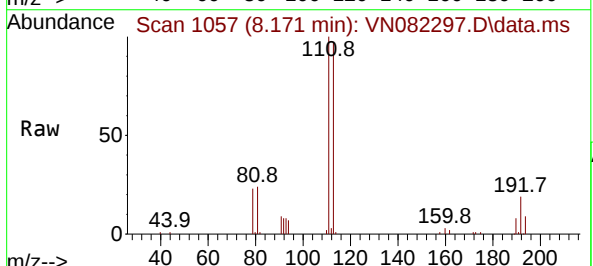


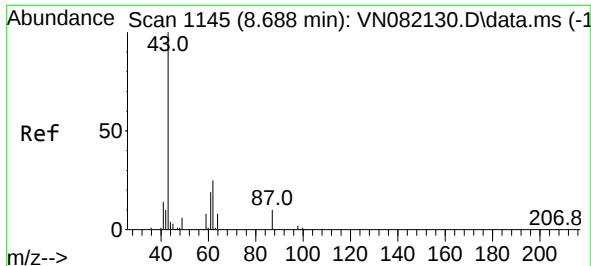

#43
Isopropyl Acetate
Concen: 53.712 ug/l
RT: 8.688 min Scan# 1145
Delta R.T. -0.000 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02




Instrument :
MSVOA_N
ClientSampleId :
PB161037ZHE#10


Tgt Ion: 43 Resp: 337248
Ion Ratio Lower Upper
43 100
61 11.7 22.8 34.2#
87 7.0 12.0 18.0#

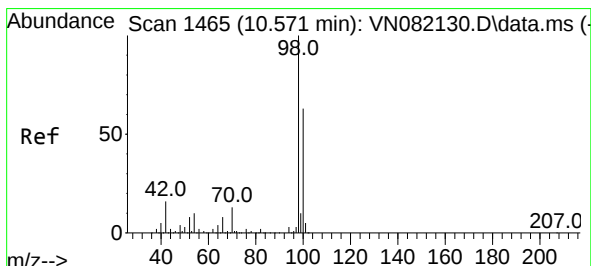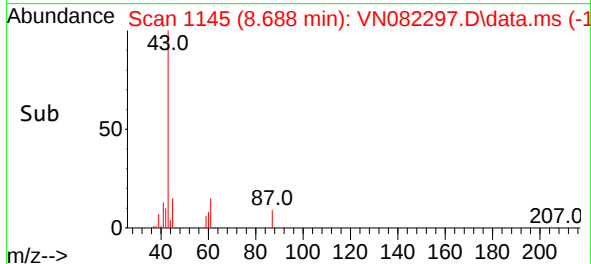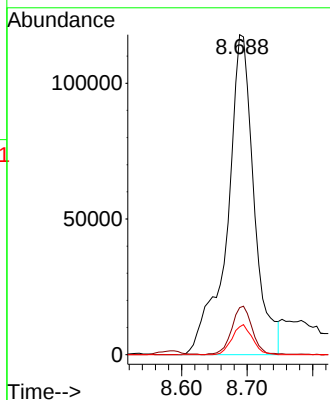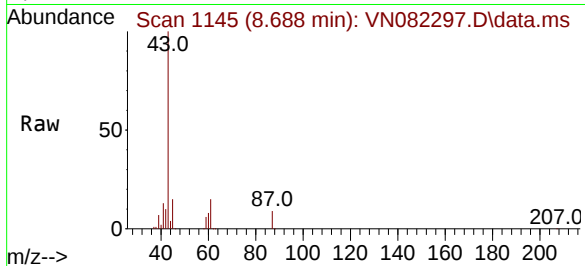

#50
Toluene-d8
Concen: 54.106 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02

Tgt Ion: 98 Resp: 391625
Ion Ratio Lower Upper
98 100
100 65.1 51.8 77.6


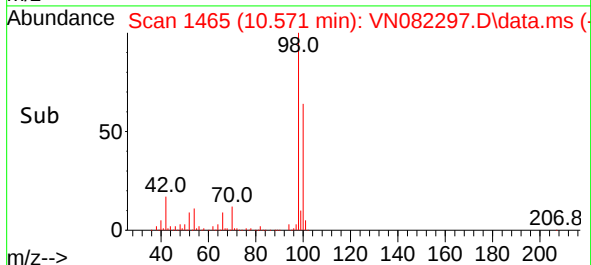
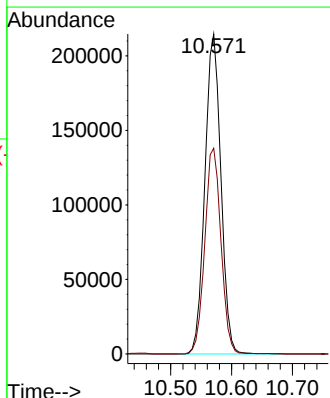
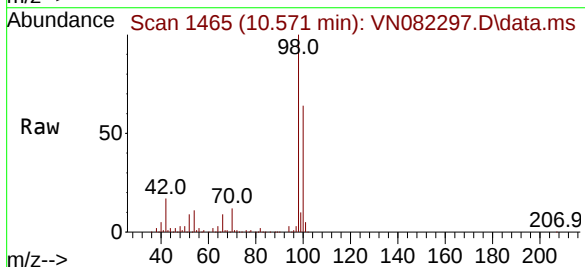


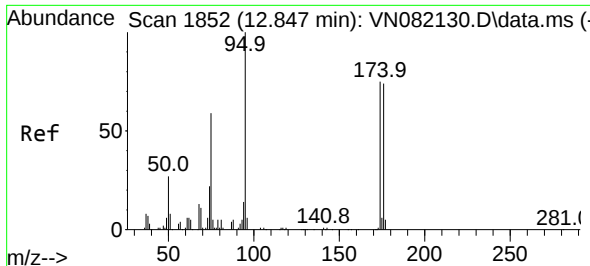

#62
4-Bromofluorobenzene
Concen: 52.016 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02




Instrument :
MSVOA_N
ClientSampleId :
PB161037ZHE#10

Tgt Ion: 95 Resp: 134380
Ion Ratio Lower Upper
95 100
174 74.5 0.0 160.6
176 73.0 0.0 152.8

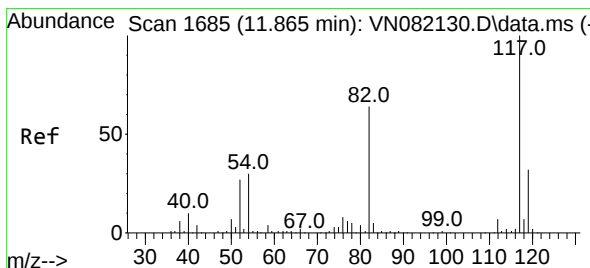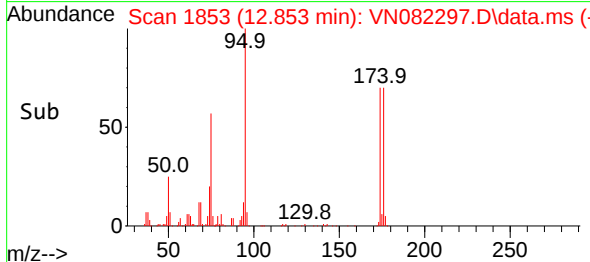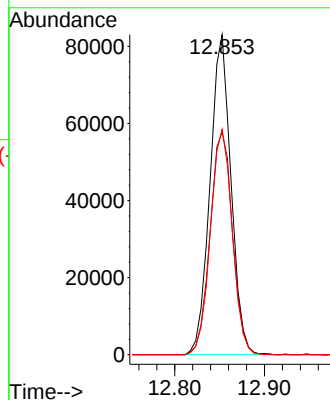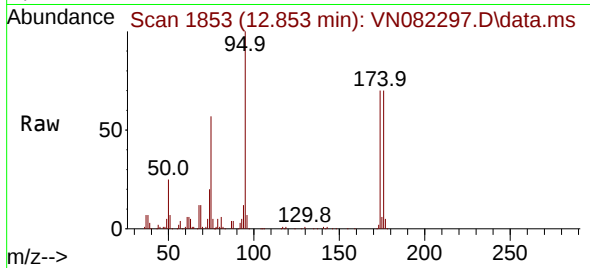

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.006 min
Lab File: VN082297.D
Acq: 22 May 2024 17:02


Tgt Ion: 117 Resp: 289903
Ion Ratio Lower Upper
117 100
82 60.6 44.6 66.8
119 32.6 25.9 38.9

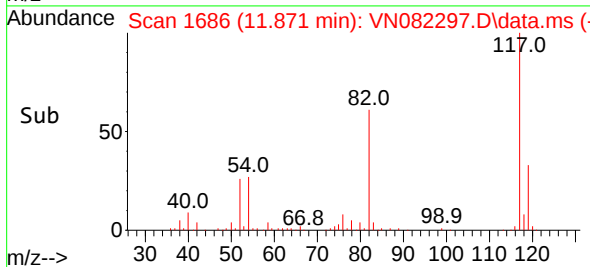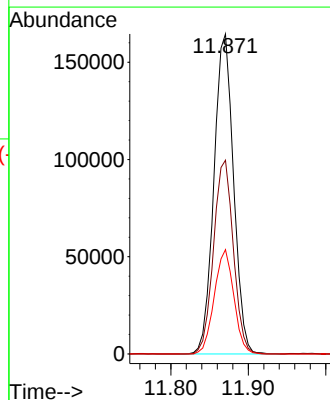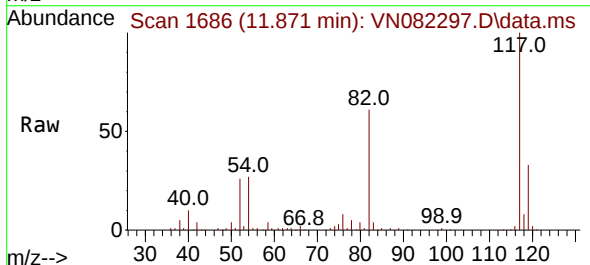



#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.794 min Scan# 20
 Delta R.T. -0.000 min
 Lab File: VN082297.D
 Acq: 22 May 2024 17:02

Instrument :
 MSVOA_N
 ClientSampleId :
 PB161037ZHE#10

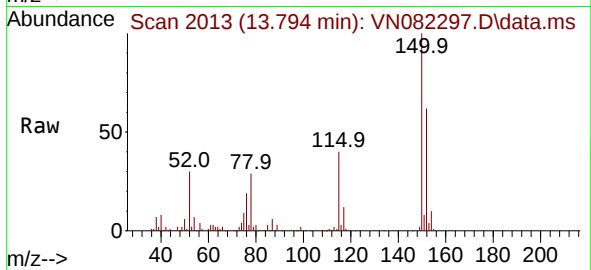

Tgt Ion:152 Resp: 116408
 Ion Ratio Lower Upper
 152 100
 115 61.8 30.4 91.3
 150 160.0 0.0 353.2

