
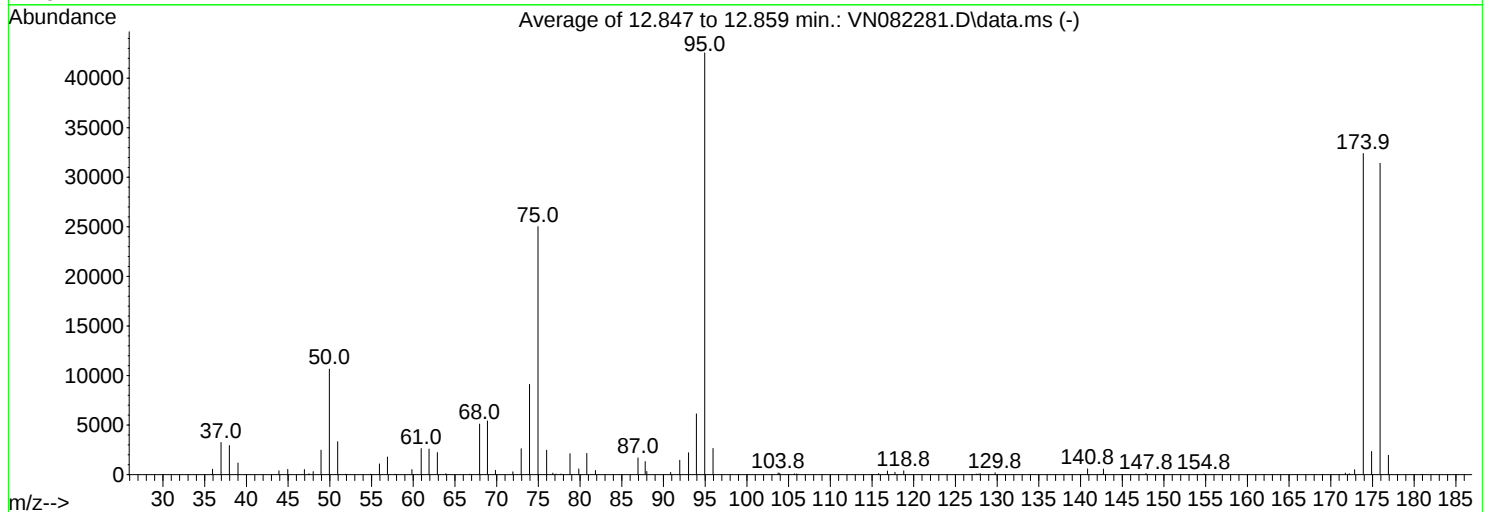


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052224\
Data File : VN082281.D
Acq On : 22 May 2024 09:52
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

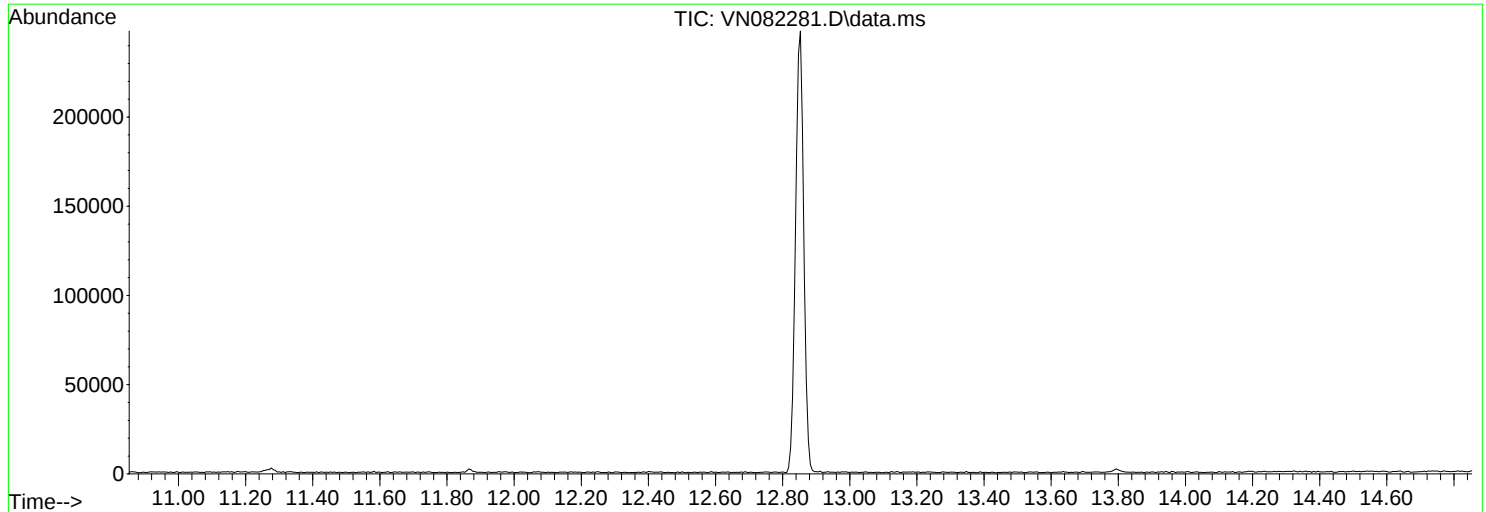

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	10653	PASS
75	95	30	60	58.8	25027	PASS
95	95	100	100	100.0	42552	PASS
96	95	5	9	6.2	2651	PASS
173	174	0.00	2	1.6	507	PASS
174	95	50	100	76.1	32392	PASS
175	174	5	9	7.2	2336	PASS
176	174	95	101	97.0	31421	PASS
177	176	5	9	6.2	1946	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	555	50.95	3325	66.80	52	77.70	64
36.95	3251	51.90	52	67.95	5109	78.80	211
37.95	2936	54.90	55	68.90	5424	79.85	58
39.00	1187	55.95	1076	69.85	433	80.80	214
43.90	381	56.90	1772	71.95	297	81.85	417
44.95	538	57.80	57	72.95	2611	86.95	1692
46.95	523	59.85	514	73.95	9103	87.80	1323
47.50	97	60.95	2631	74.95	25027	88.00	326
48.00	313	61.90	2579	76.00	2477	90.85	231
48.95	2479	62.90	2221	76.75	156	91.95	1461
49.95	10653	63.90	101	77.10	69	93.00	2207

Average of 12.847 to 12.859 min.: VN082281.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.95	6131	127.50	60	173.90	32392		
94.95	42552	127.70	58	174.90	2336		
95.95	2651	127.95	111	175.90	31421		
103.75	182	129.75	198	176.90	1946		
103.95	149	140.85	581				
105.70	83	142.75	570				
106.00	89	147.85	116				
115.80	116	154.80	65				
116.85	368	171.75	169				
117.75	236	172.20	91				
118.80	392	172.85	507				

Instrument :

MSVOA_N

ClientSampleId :

BFB