

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052225\
 Data File : VN086751.D
 Acq On : 22 May 2025 08:55
 Operator : JC\MD
 Sample : VN0522MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0522MBL01

Quant Time: May 23 01:30:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
 Quant Title : SW846 8260
 QLast Update : Sat May 17 00:46:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	229256	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	424494	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	408586	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	174679	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	139341	43.985	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	87.980%
35) Dibromofluoromethane	8.165	113	127130	50.288	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	100.580%
50) Toluene-d8	10.565	98	536584	51.219	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.440%
62) 4-Bromofluorobenzene	12.847	95	192975	52.168	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	104.340%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052225\
Data File : VN086751.D
Acq On : 22 May 2025 08:55
Operator : JC\MD
Sample : VN0522MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0522MBL01

Quant Time: May 23 01:30:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Quant Title : SW846 8260
QLast Update : Sat May 17 00:46:13 2025
Response via : Initial Calibration




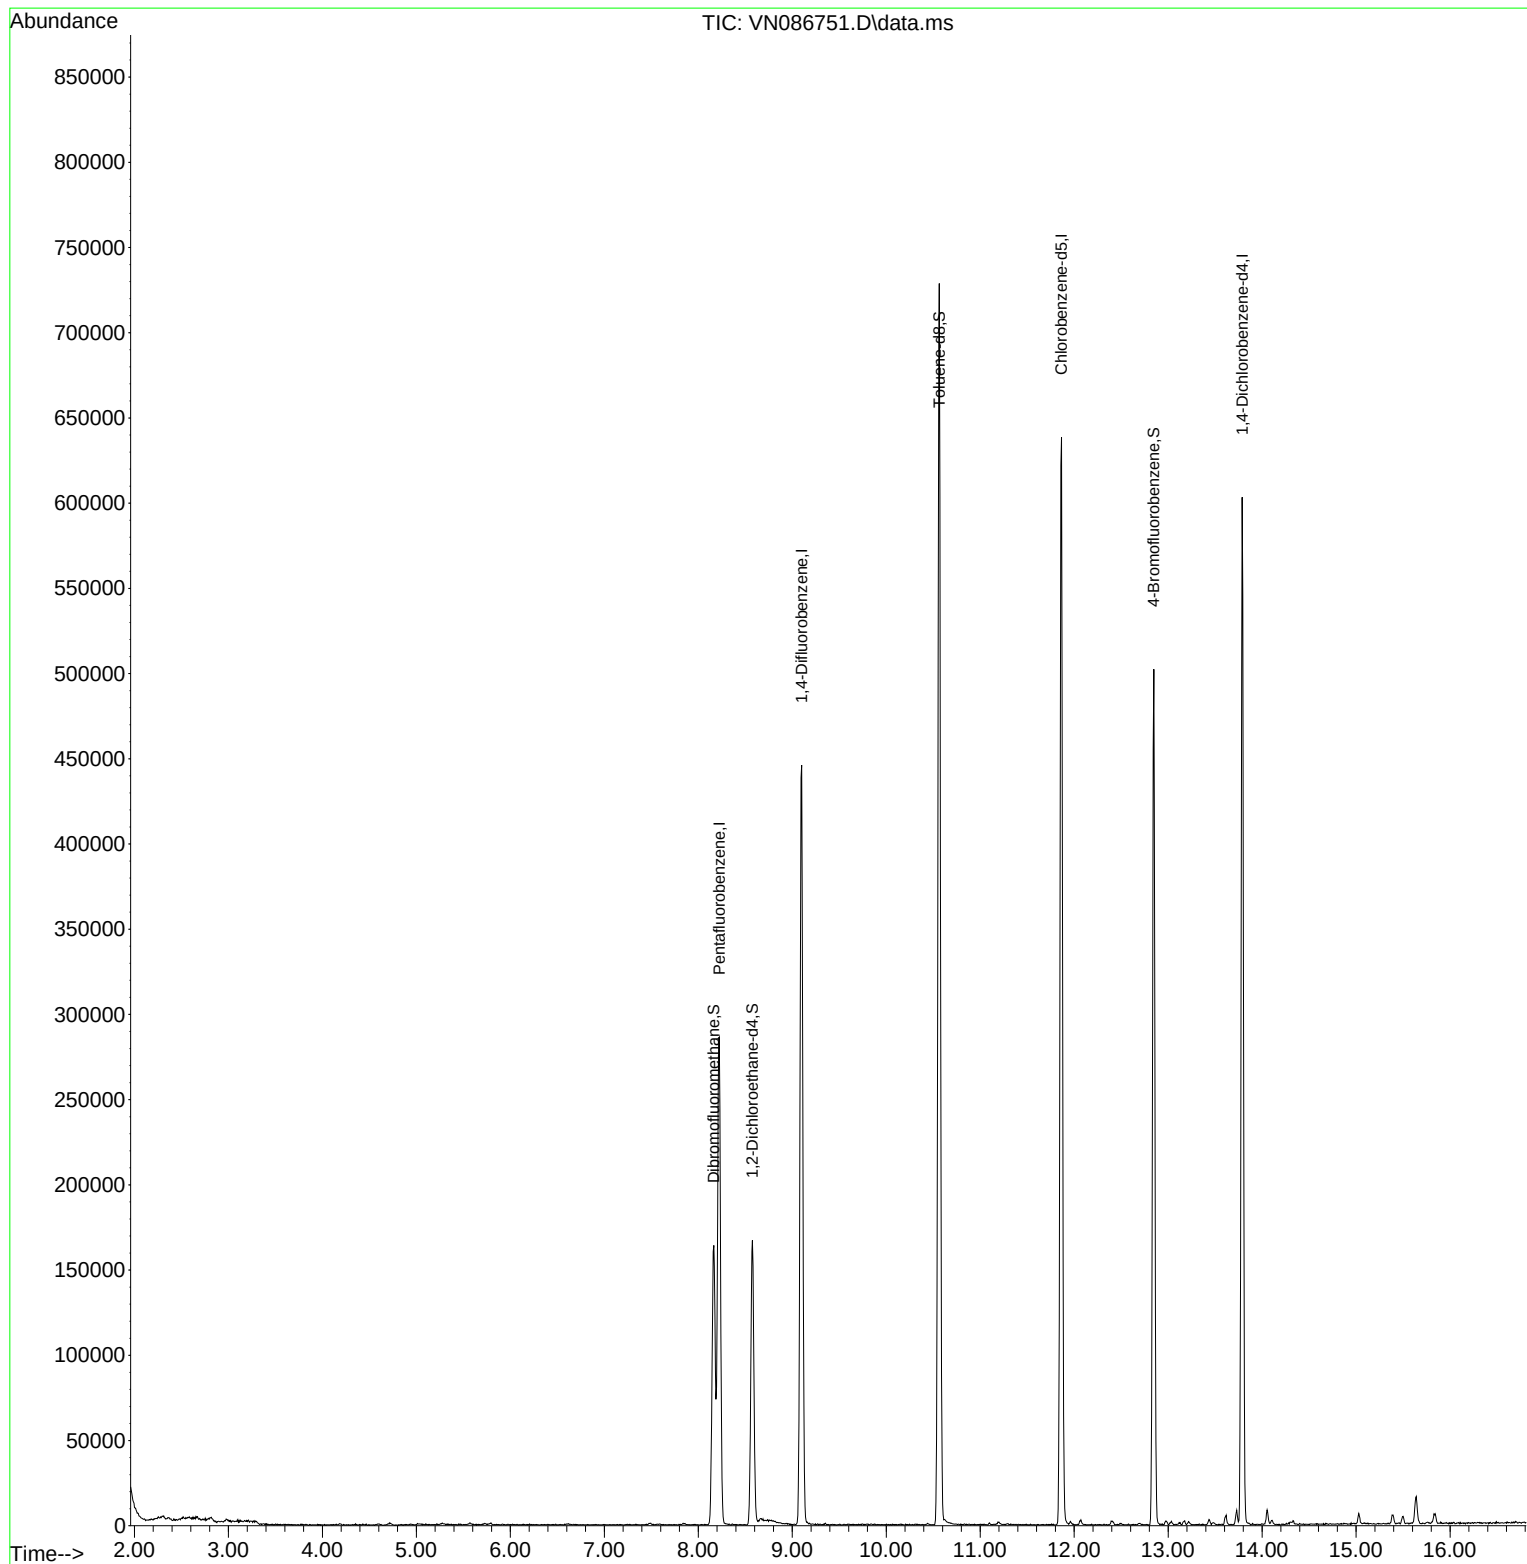


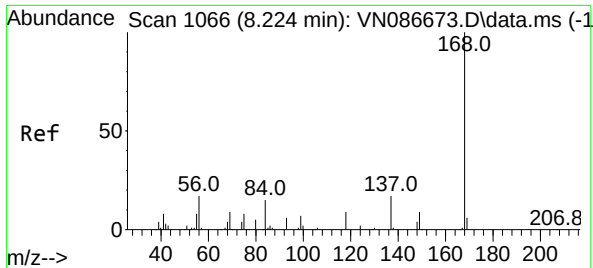

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55




Instrument :
MSVOA_N
ClientSampleId :
VN0522MBL01


Tgt Ion:168 Resp: 229256
Ion Ratio Lower Upper
168 100
99 54.9 47.0 70.4

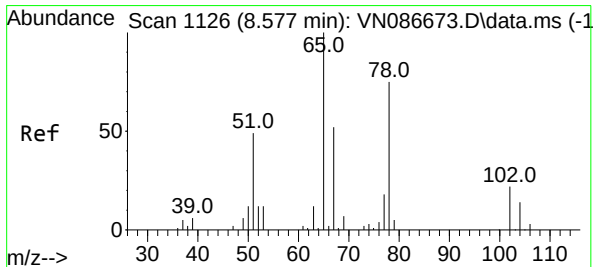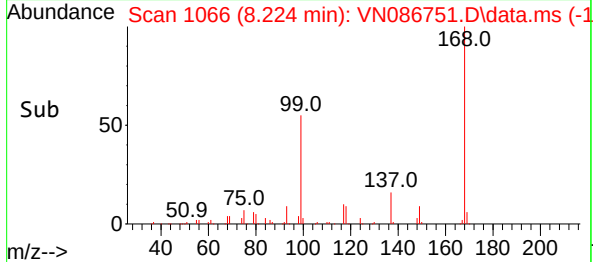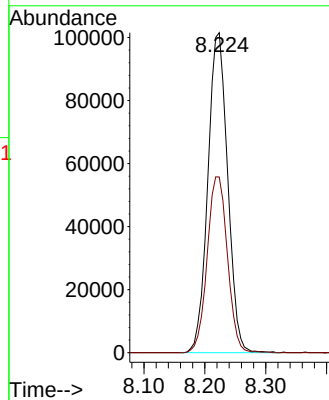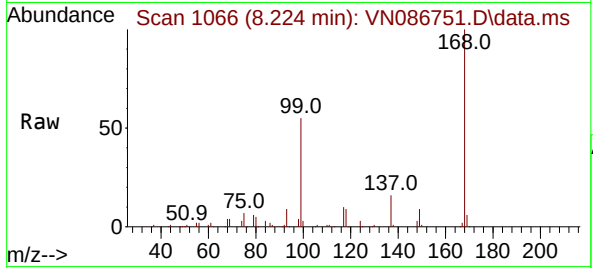

#33
1,2-Dichloroethane-d4
Concen: 43.985 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55

Tgt Ion: 65 Resp: 139341
Ion Ratio Lower Upper
65 100
67 53.2 0.0 106.4


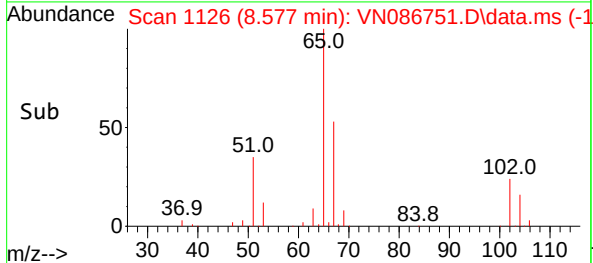
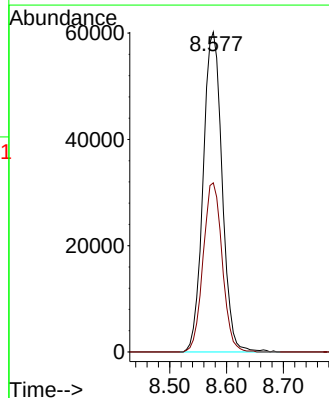
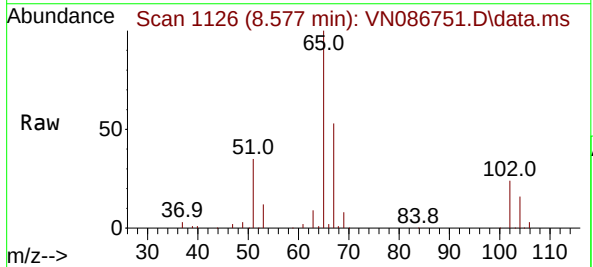


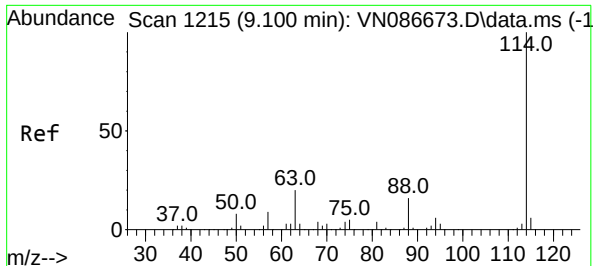

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 9.100 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55




Instrument :
MSVOA_N
ClientSampleId :
VN0522MBL01


Tgt Ion:114 Resp: 424494
Ion Ratio Lower Upper
114 100
63 19.3 0.0 40.2
88 15.2 0.0 31.2

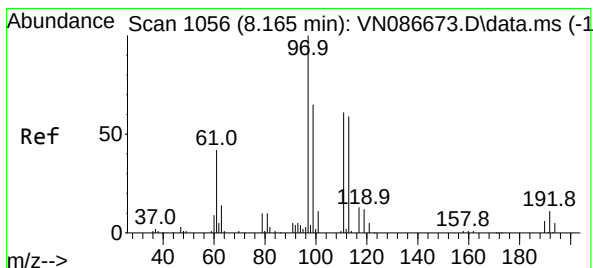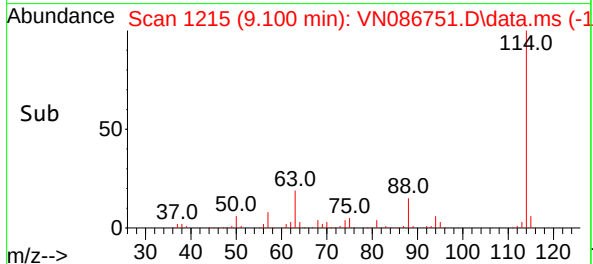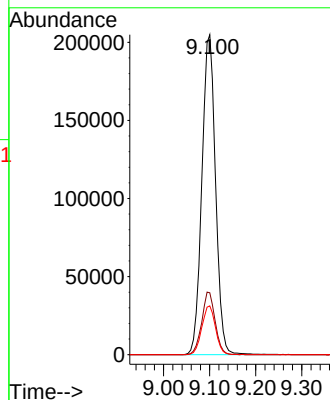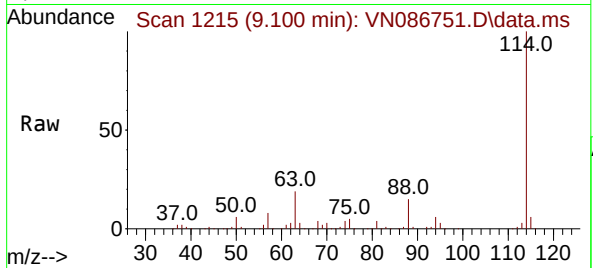

#35
Dibromofluoromethane
Concen: 50.288 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55

Tgt Ion:113 Resp: 127130
Ion Ratio Lower Upper
113 100
111 101.8 82.2 123.2
192 18.0 13.8 20.8


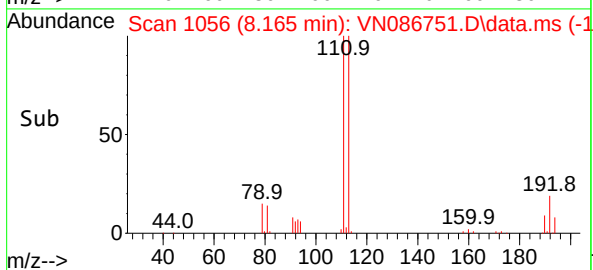
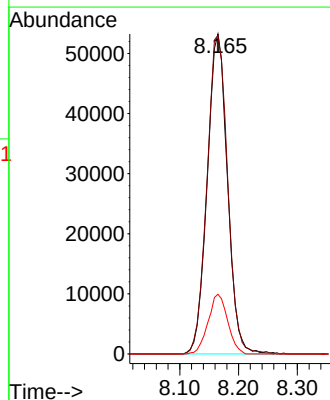
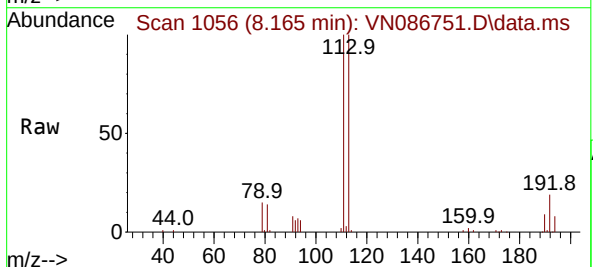


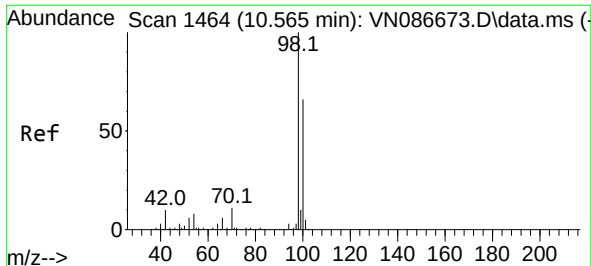

#50
Toluene-d8
Concen: 51.219 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55




Instrument :
MSVOA_N
ClientSampleId :
VN0522MBL01


Tgt Ion: 98 Resp: 536584
Ion Ratio Lower Upper
98 100
100 65.7 52.9 79.3

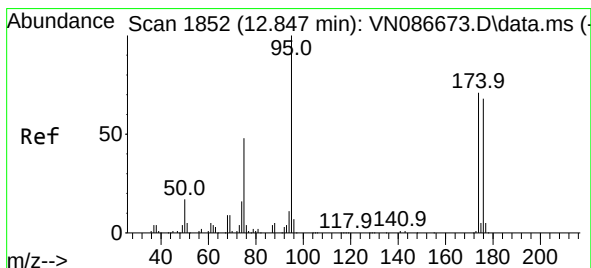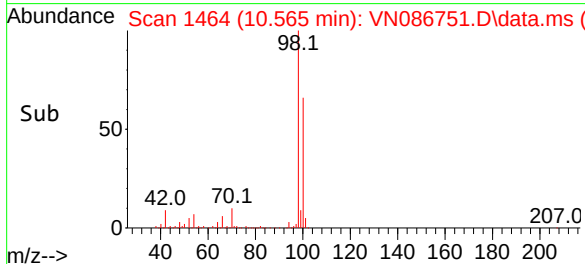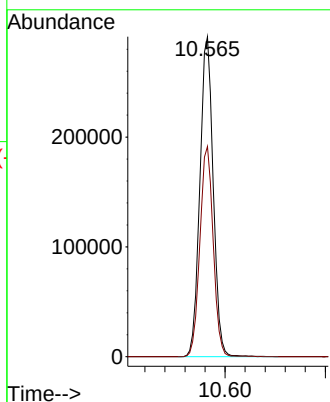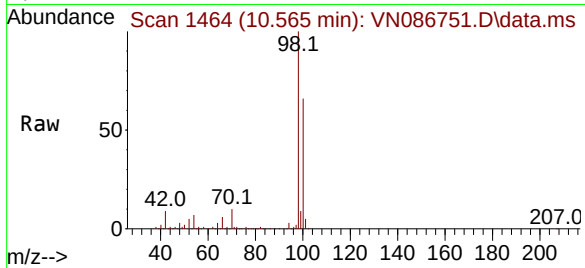

#62
4-Bromofluorobenzene
Concen: 52.168 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55

Tgt Ion: 95 Resp: 192975
Ion Ratio Lower Upper
95 100
174 74.1 0.0 145.4
176 72.0 0.0 137.8


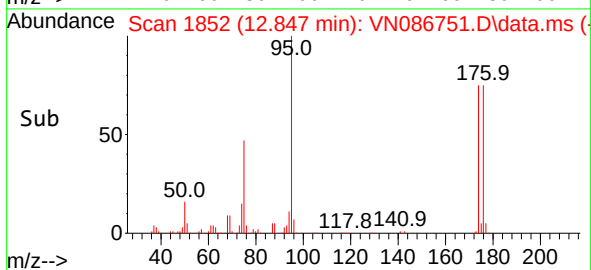
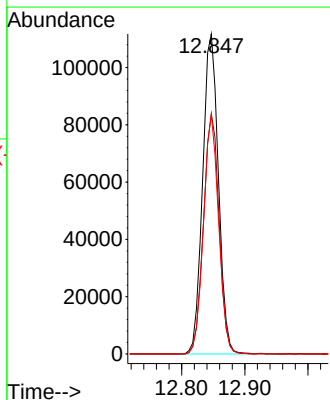
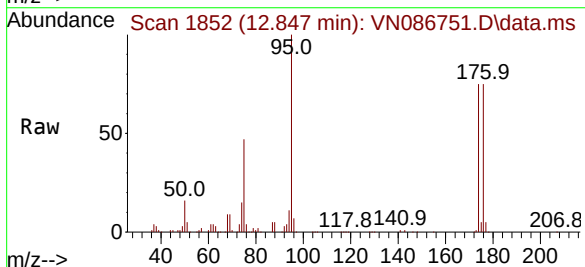


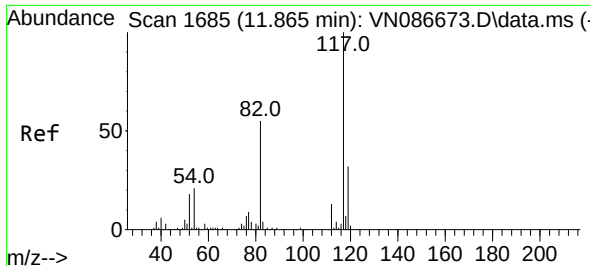

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55

Instrument :
MSVOA_N
ClientSampleId :
VN0522MBL01

Tgt Ion:117 Resp: 408586
Ion Ratio Lower Upper
117 100
82 53.2 44.2 66.2
119 32.2 25.4 38.2

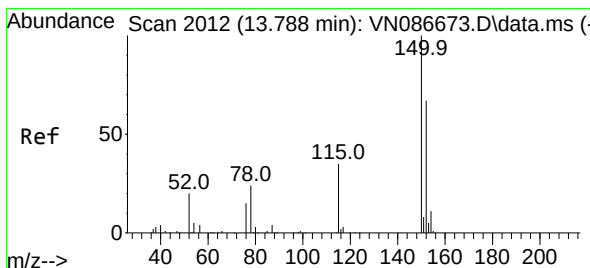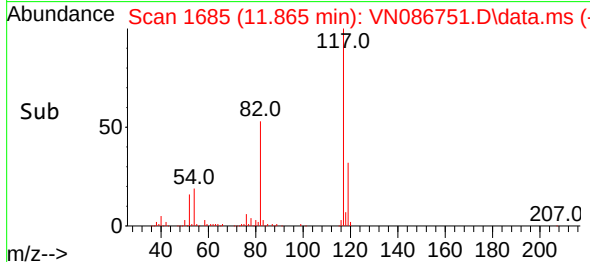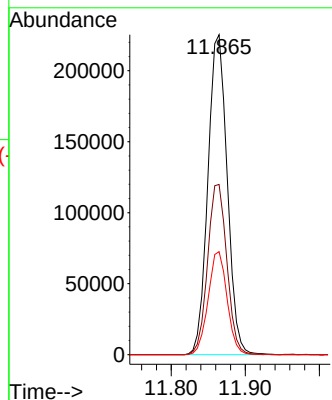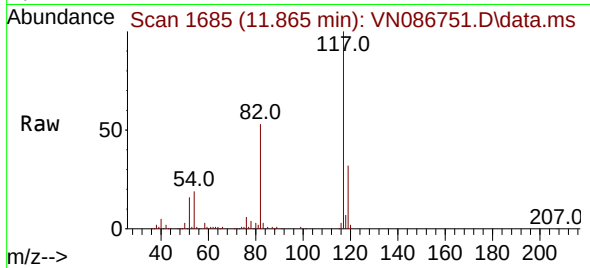

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN086751.D
Acq: 22 May 2025 08:55

Tgt Ion:152 Resp: 174679
Ion Ratio Lower Upper
152 100
115 59.8 30.0 90.1
150 158.1 0.0 347.8

