
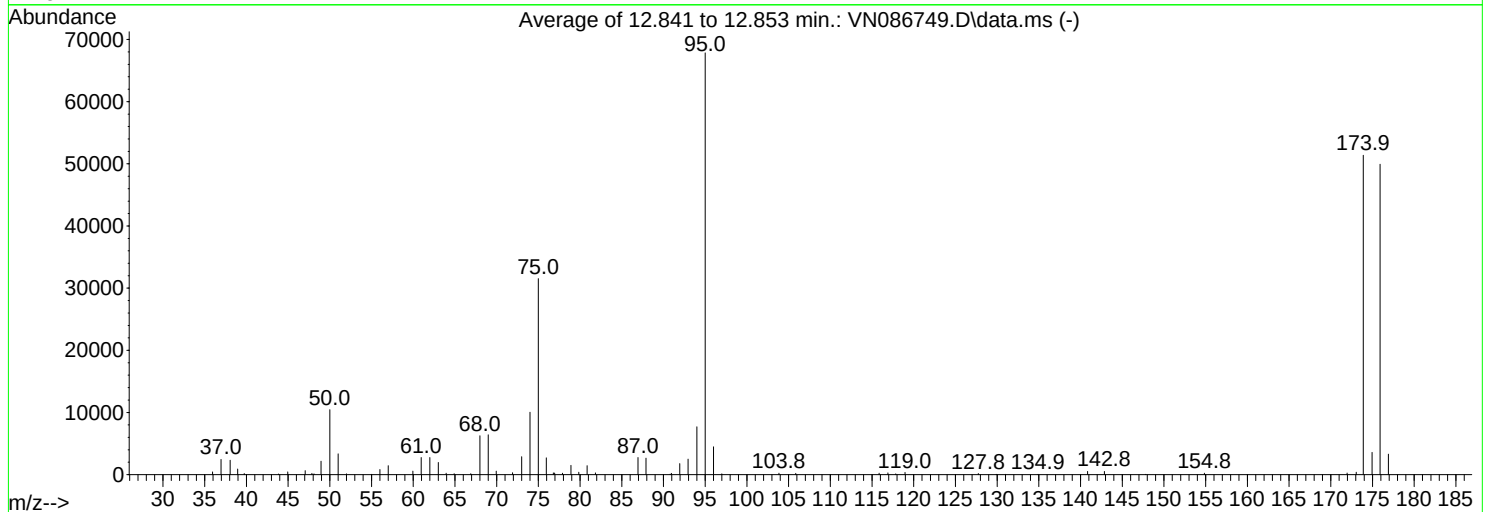


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052225\
Data File : VN086749.D
Acq On : 22 May 2025 07:48
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

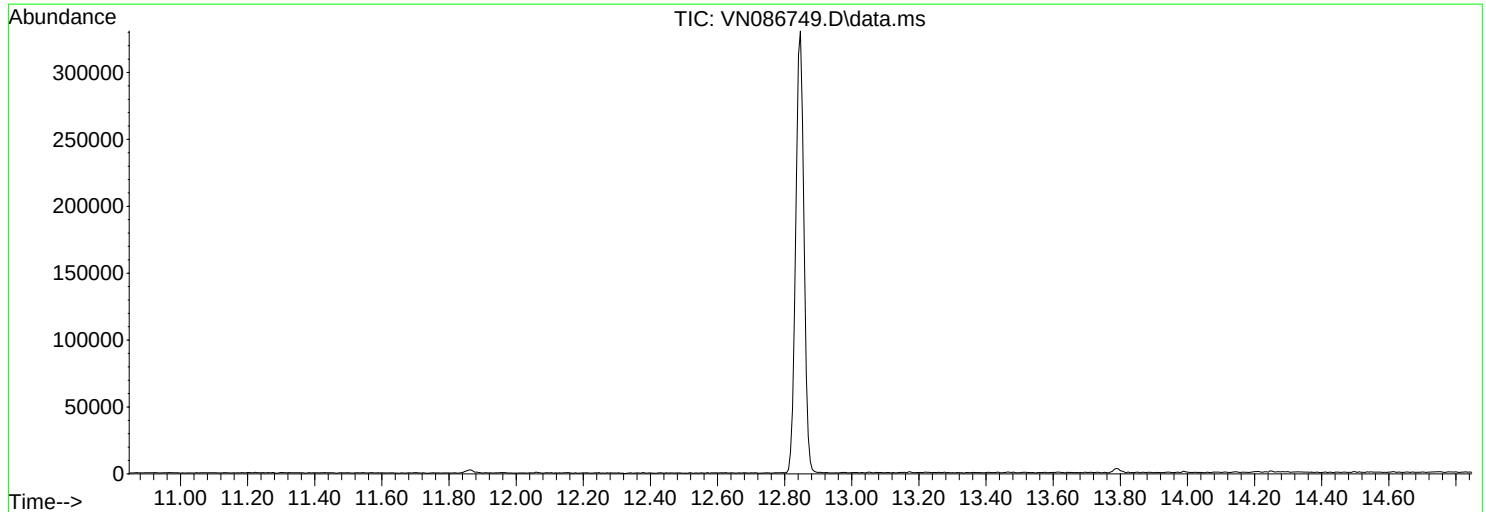

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	10453	PASS
75	95	30	60	46.5	31528	PASS
95	95	100	100	100.0	67853	PASS
96	95	5	9	6.6	4490	PASS
173	174	0.00	2	0.8	391	PASS
174	95	50	100	75.7	51379	PASS
175	174	5	9	6.9	3569	PASS
176	174	95	101	97.2	49947	PASS
177	176	5	9	6.6	3307	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	443	50.00	10453	64.90	145	76.95	25
36.95	2455	51.00	3340	66.90	164	77.90	24
38.05	2322	52.00	141	68.00	6266	78.90	150
38.95	903	55.00	56	69.00	6402	79.85	39
39.75	192	56.00	839	69.95	561	80.85	1447
43.85	108	57.00	1439	71.90	309	81.85	277
44.95	445	59.95	571	73.00	2876	86.95	2762
47.05	652	60.95	2758	74.00	10028	87.90	2650
47.85	217	62.00	2753	75.00	31528	90.80	82
48.10	122	63.00	1958	75.95	2709	90.95	206
48.95	2168	63.95	237	76.80	279	91.95	1772

Average of 12.841 to 12.853 min.: VN086749.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
92.95	2488	127.75	183	174.95	3569		
94.00	7692	129.90	53	175.90	49947		
95.00	67853	131.00	55	176.90	3307		
96.00	4490	134.90	59				
97.00	130	140.85	508				
103.85	237	142.85	524				
105.85	213	147.80	55				
115.85	232	154.85	224				
116.90	285	171.95	260				
117.85	131	173.05	391				
118.95	359	173.90	51379				

Instrument :

MSVOA_N

ClientSampleId :

BFB