



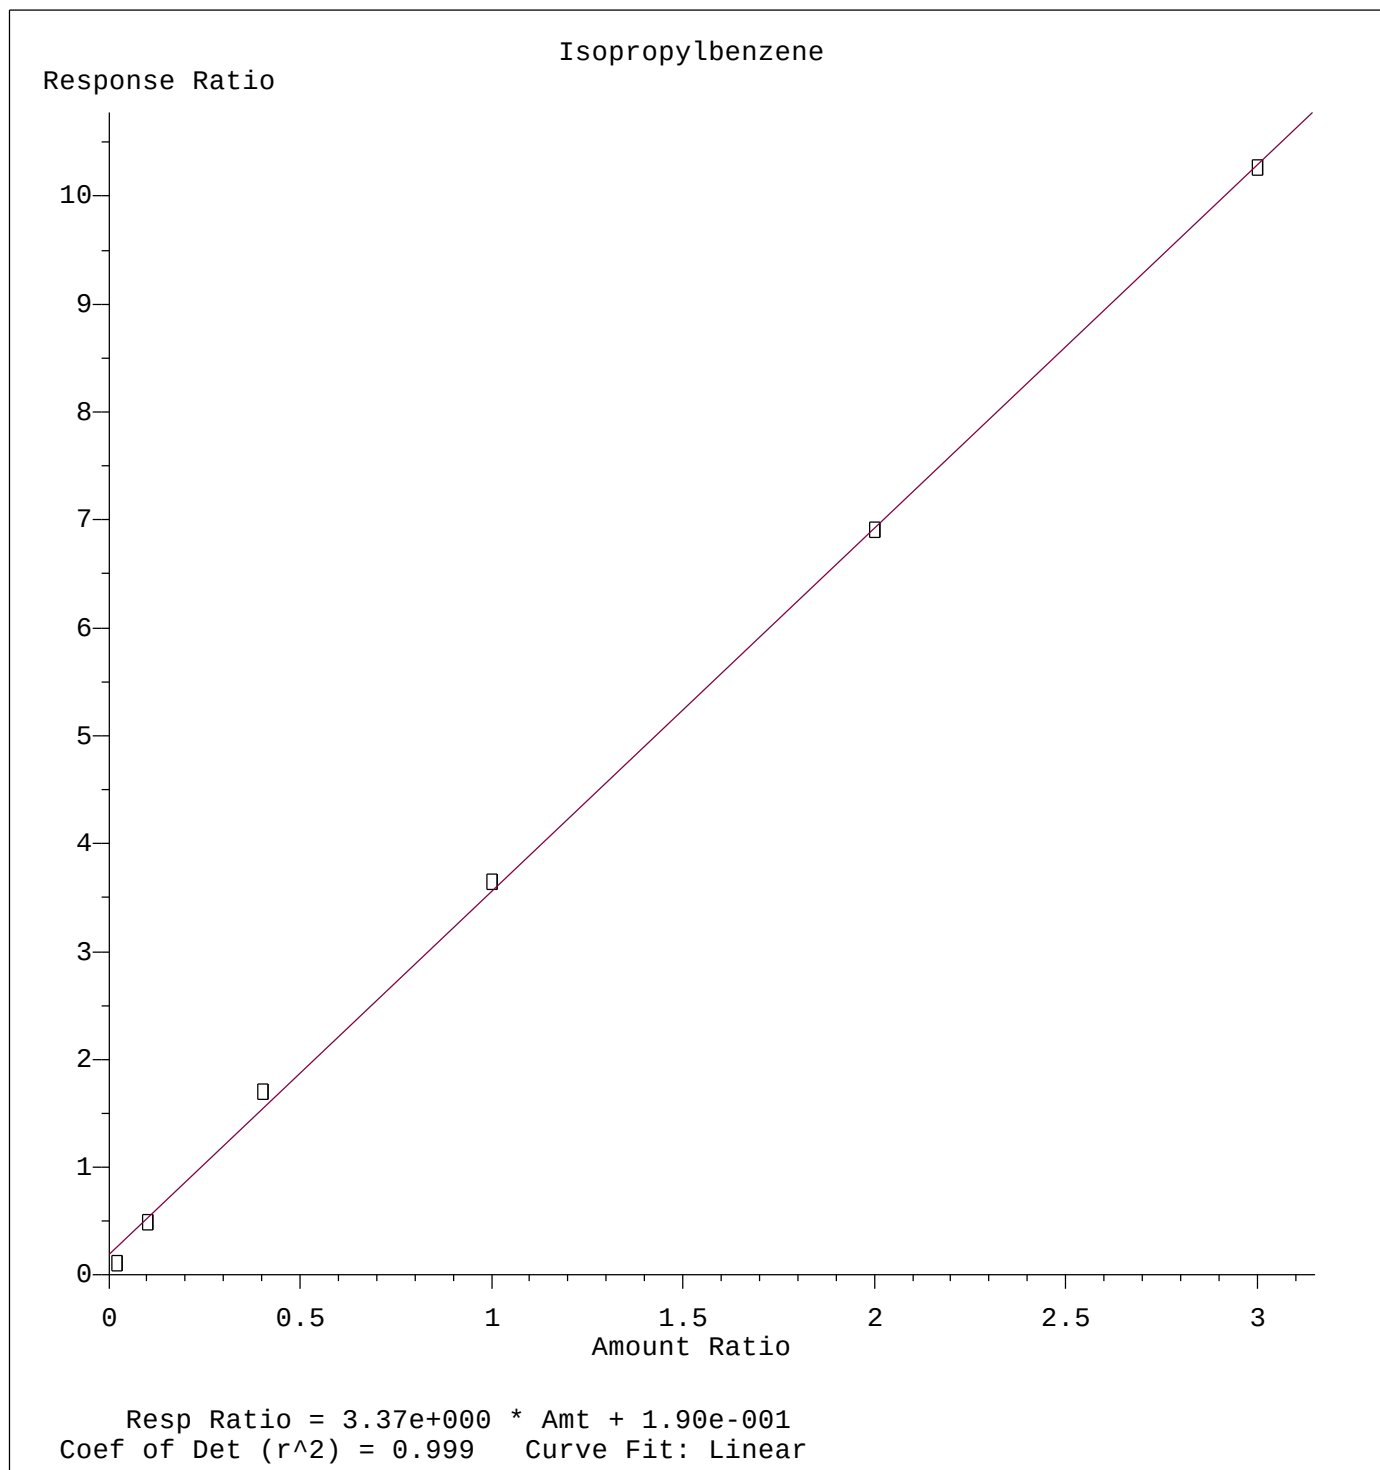


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

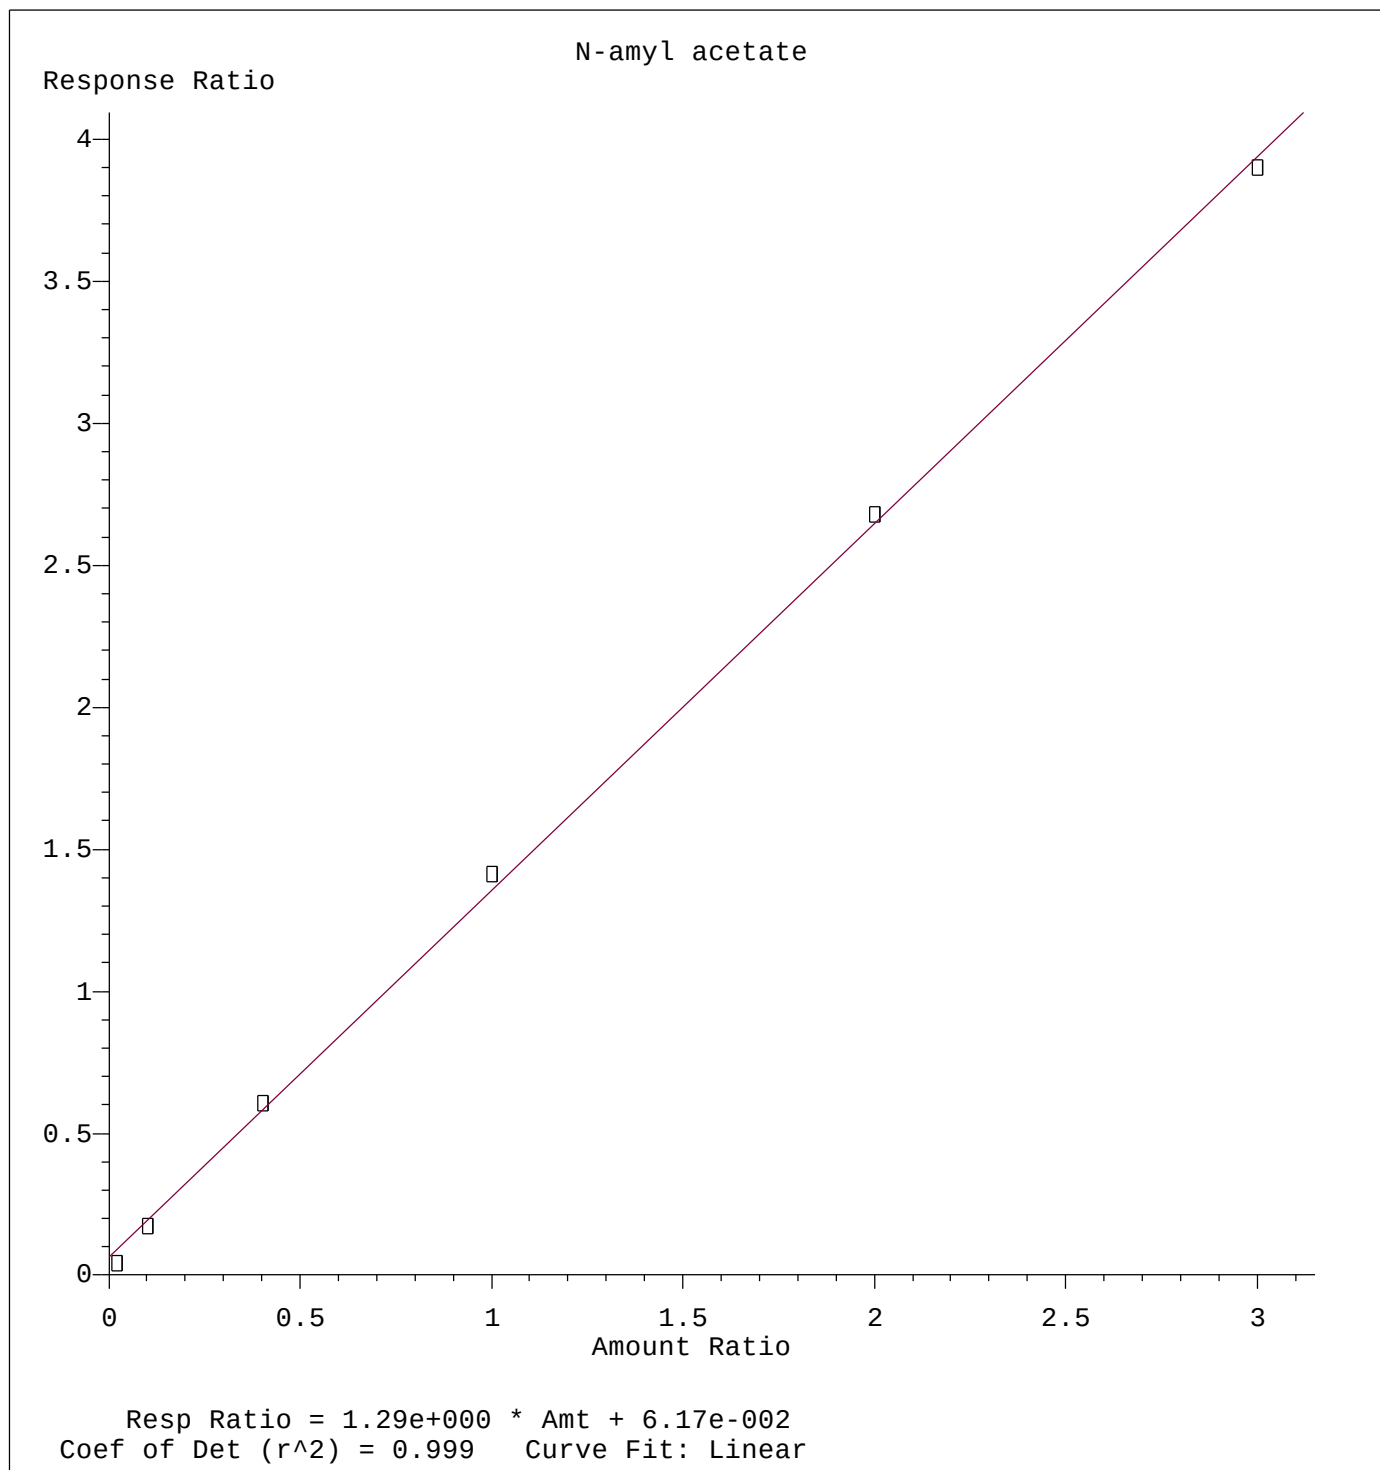

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

1,1,2,2-Tetrachloroethane

Response Ratio

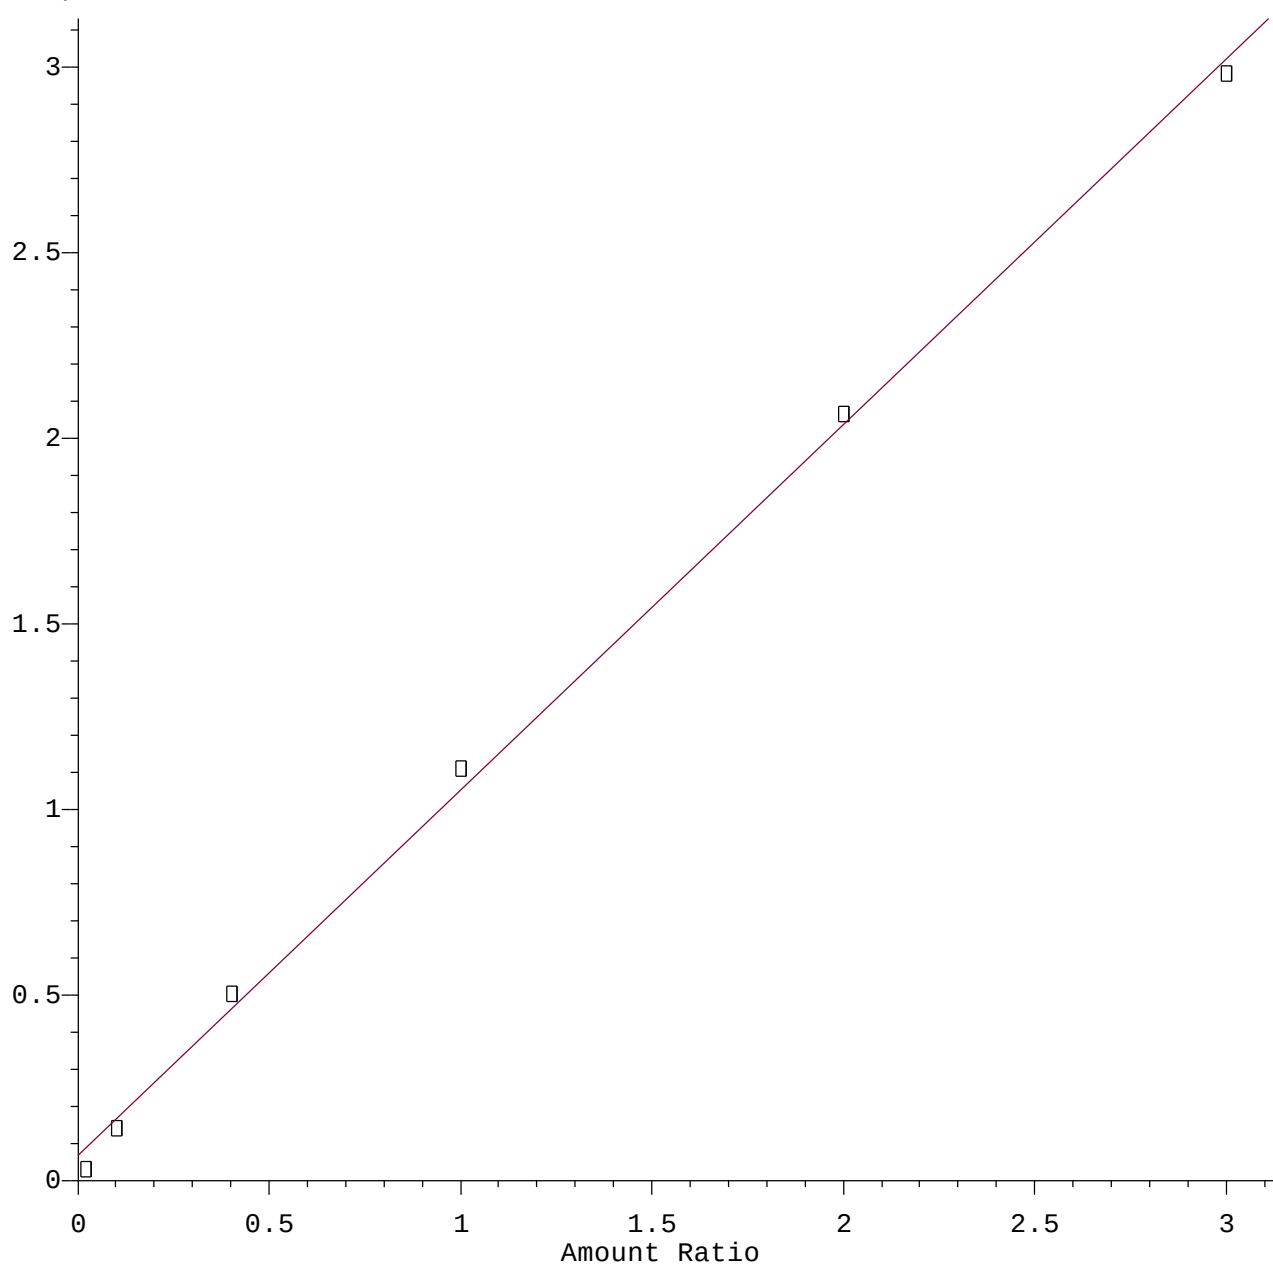


Resp Ratio = $9.84 \times 10^{-1} \times \text{Amt} + 6.98 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

1,2,3-Trichloropropane

Response Ratio

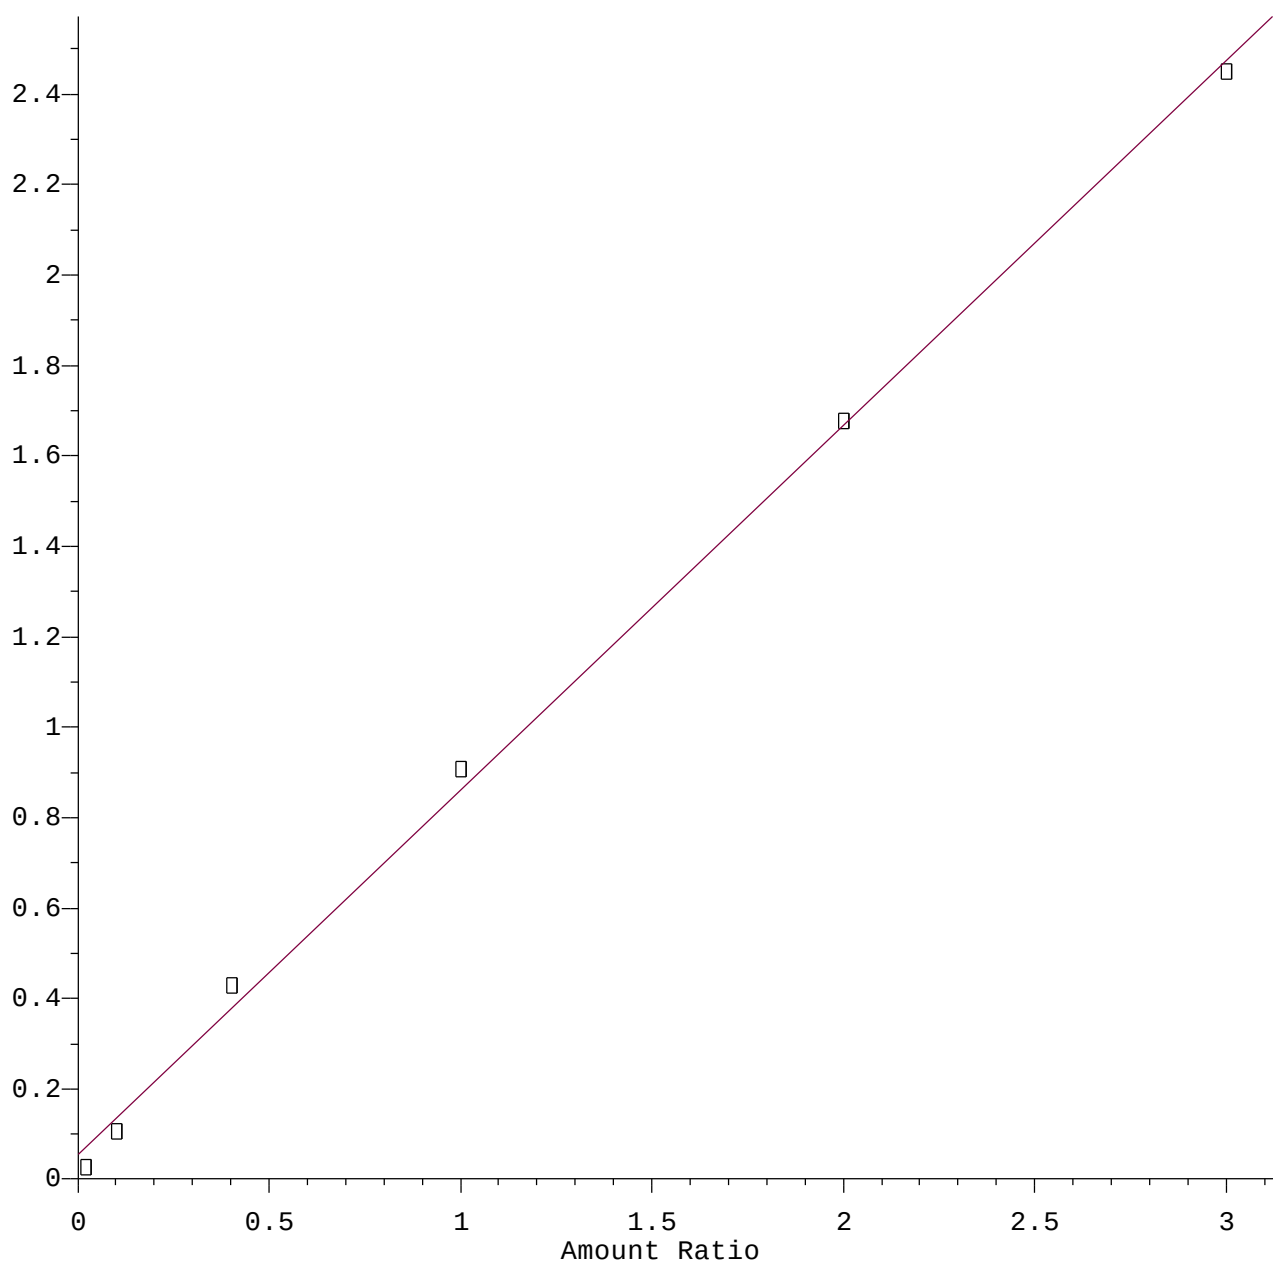


Resp Ratio = $8.07 \times 10^{-1} \times \text{Amt} + 5.42 \times 10^{-2}$
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

2-Chlorotoluene

Response Ratio

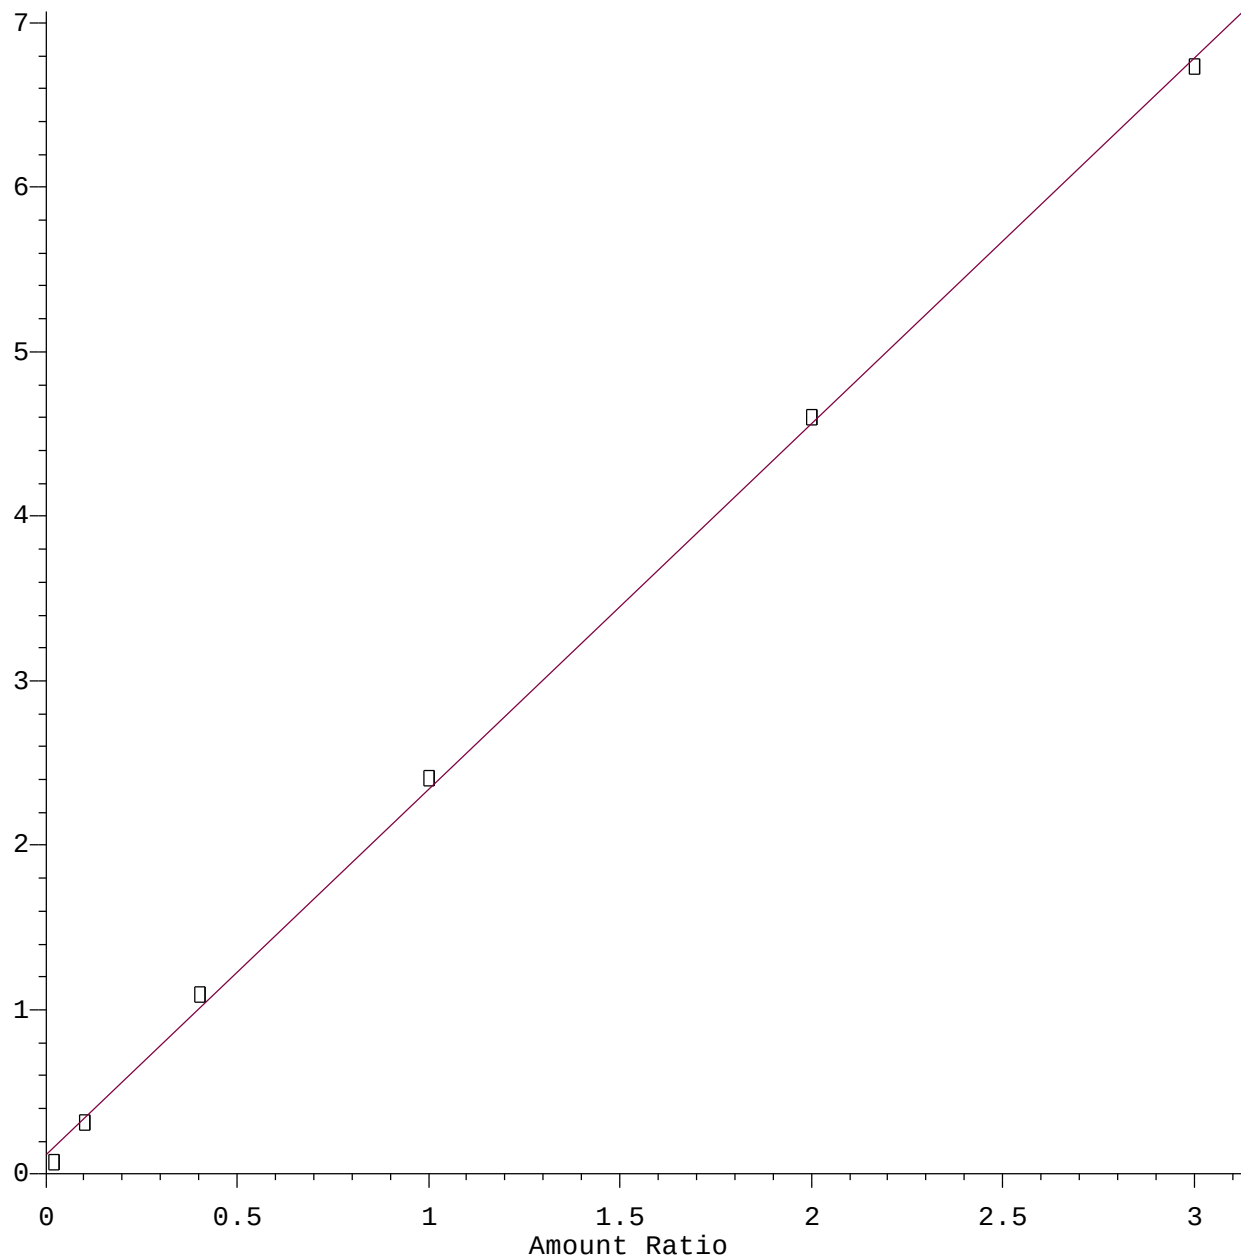


Resp Ratio = 2.22e+000 * Amt + 1.19e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

1,3,5-Trimethylbenzene

Response Ratio

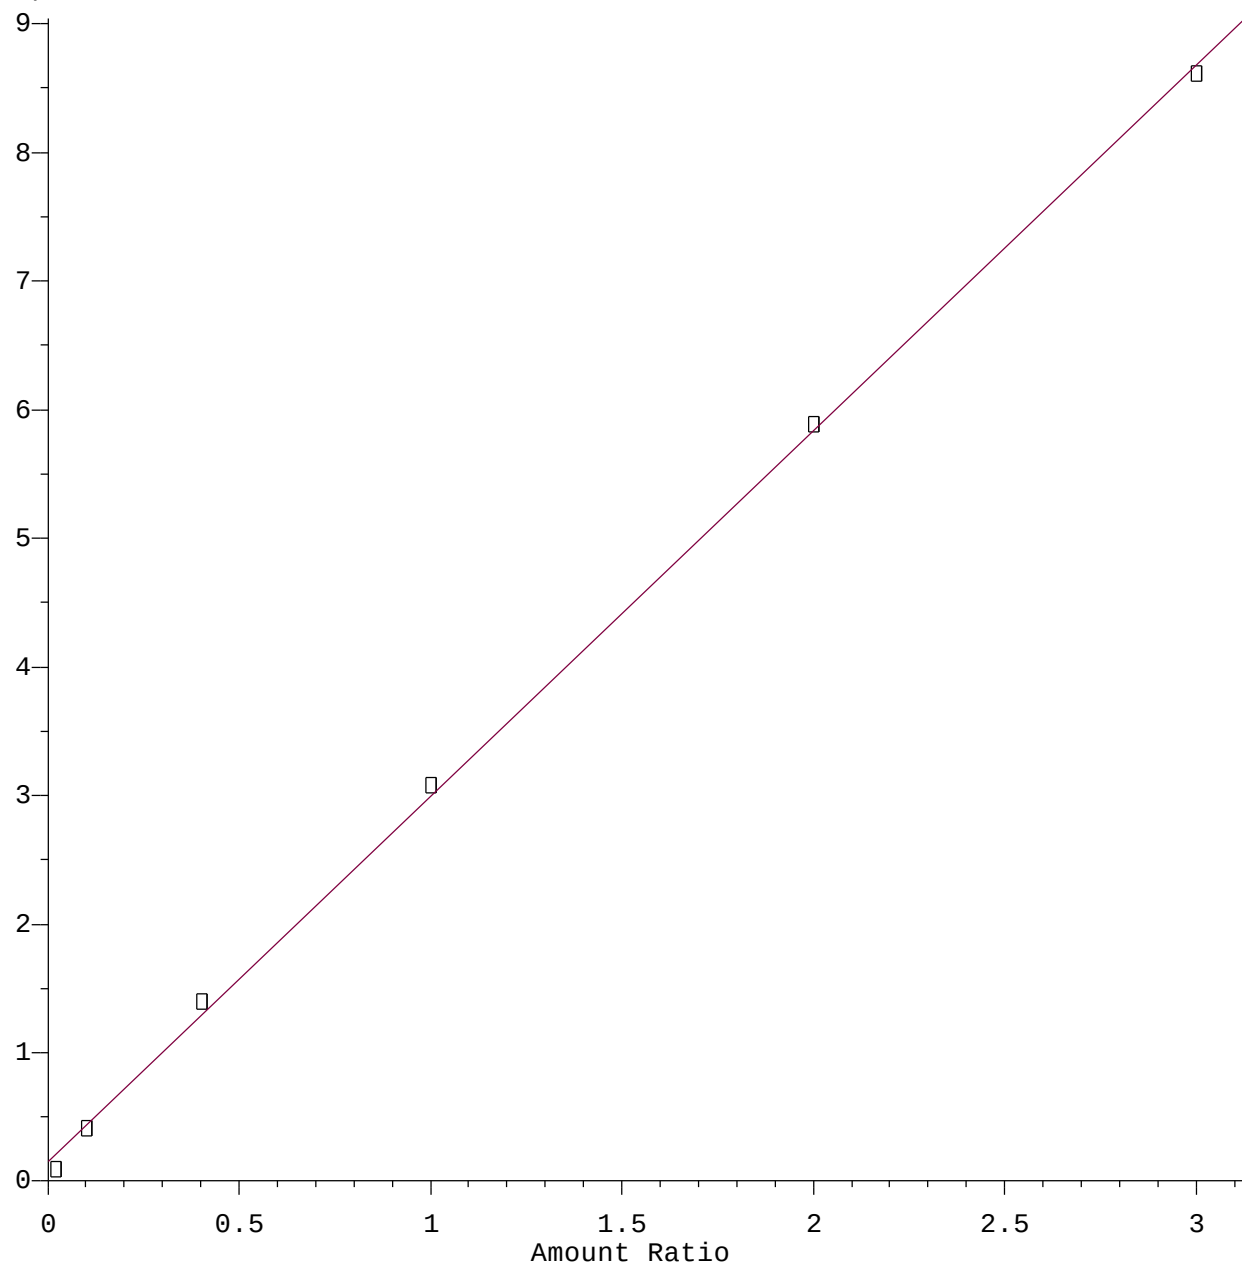


Resp Ratio = 2.84×10^0 * Amt + 1.53×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

tert-Butylbenzene

Response Ratio

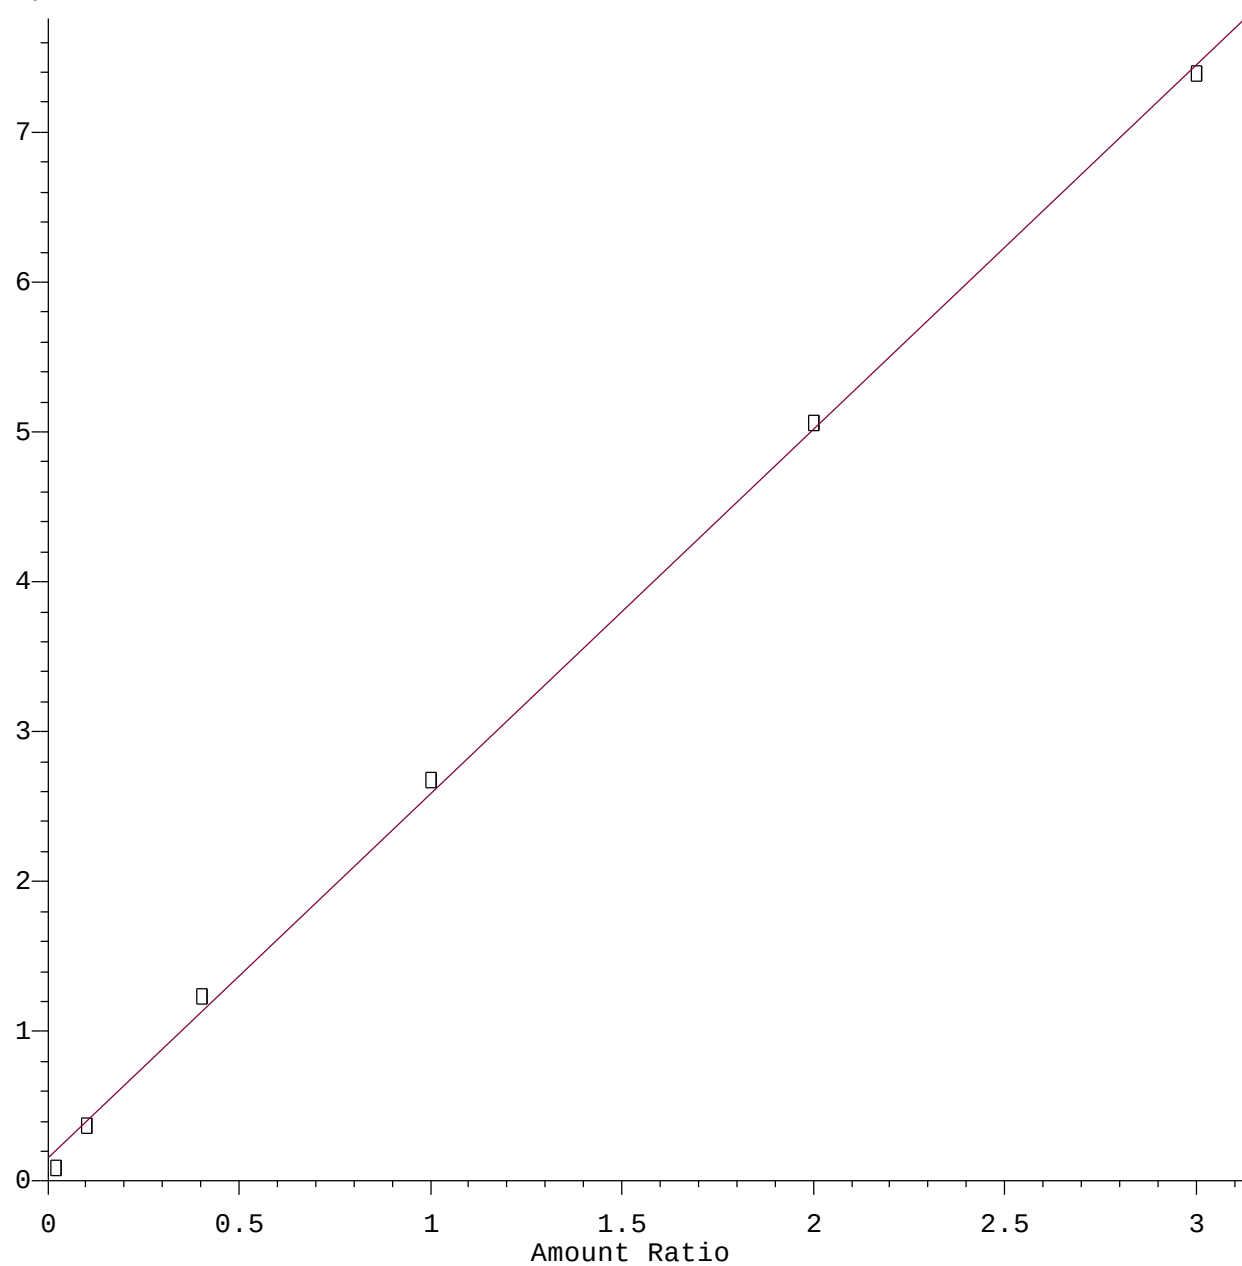


Resp Ratio = 2.43e+000 * Amt + 1.57e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

1,2,4-Trimethylbenzene

Response Ratio

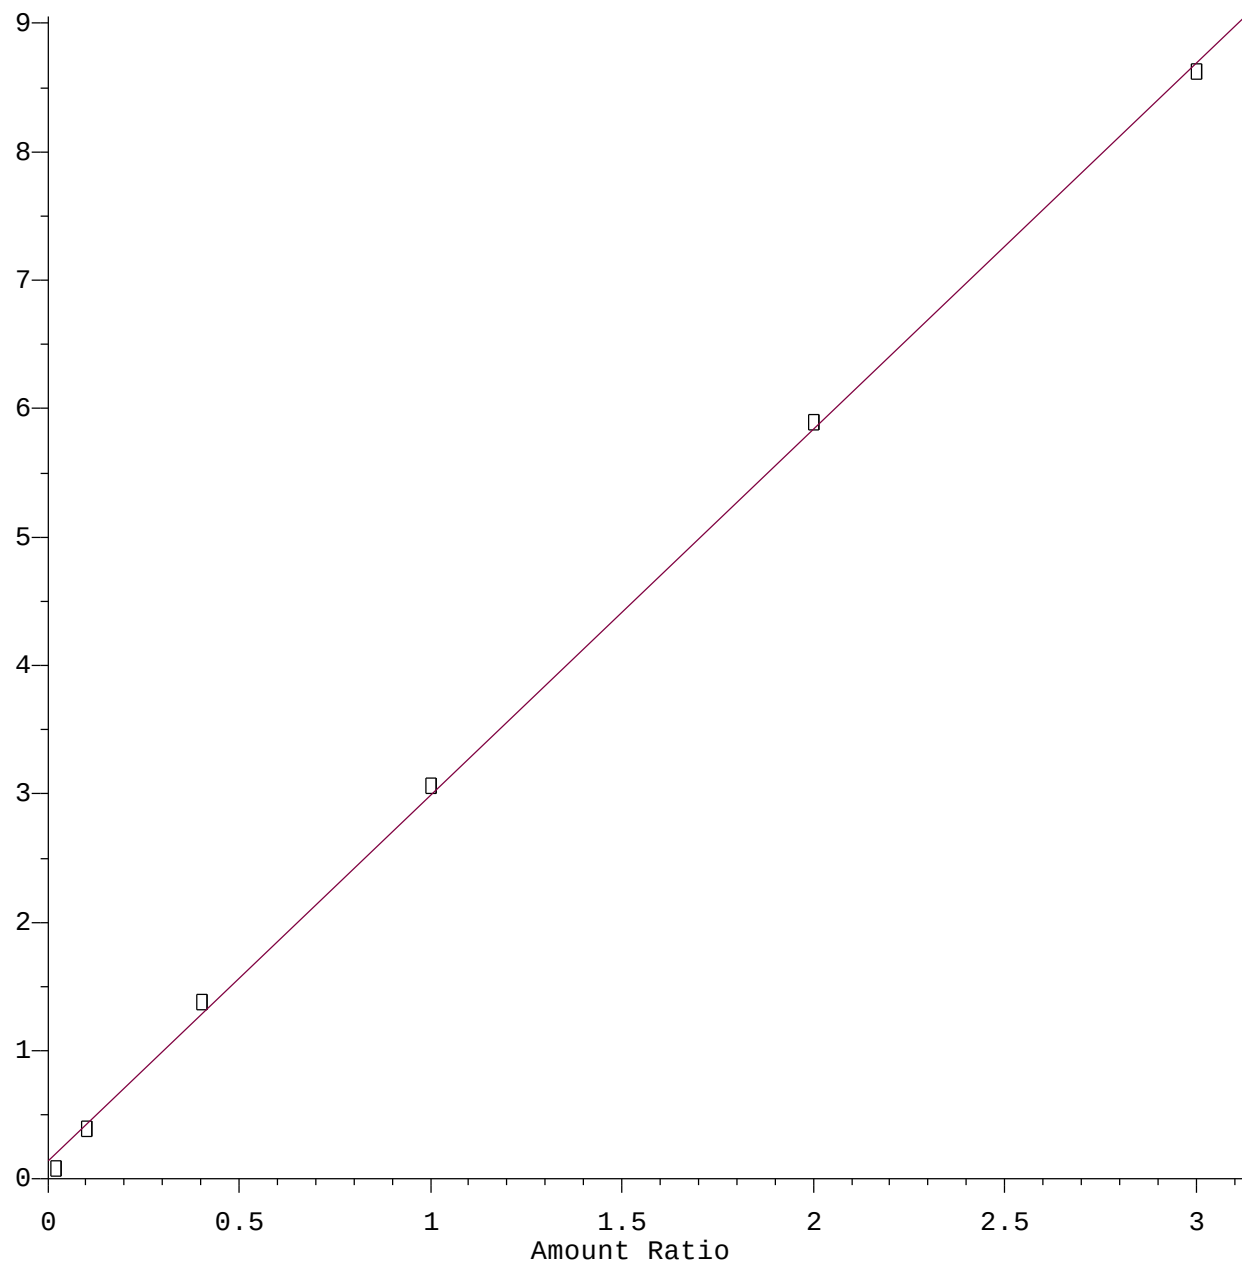


Resp Ratio = 2.85e+000 * Amt + 1.40e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

sec-Butylbenzene

Response Ratio

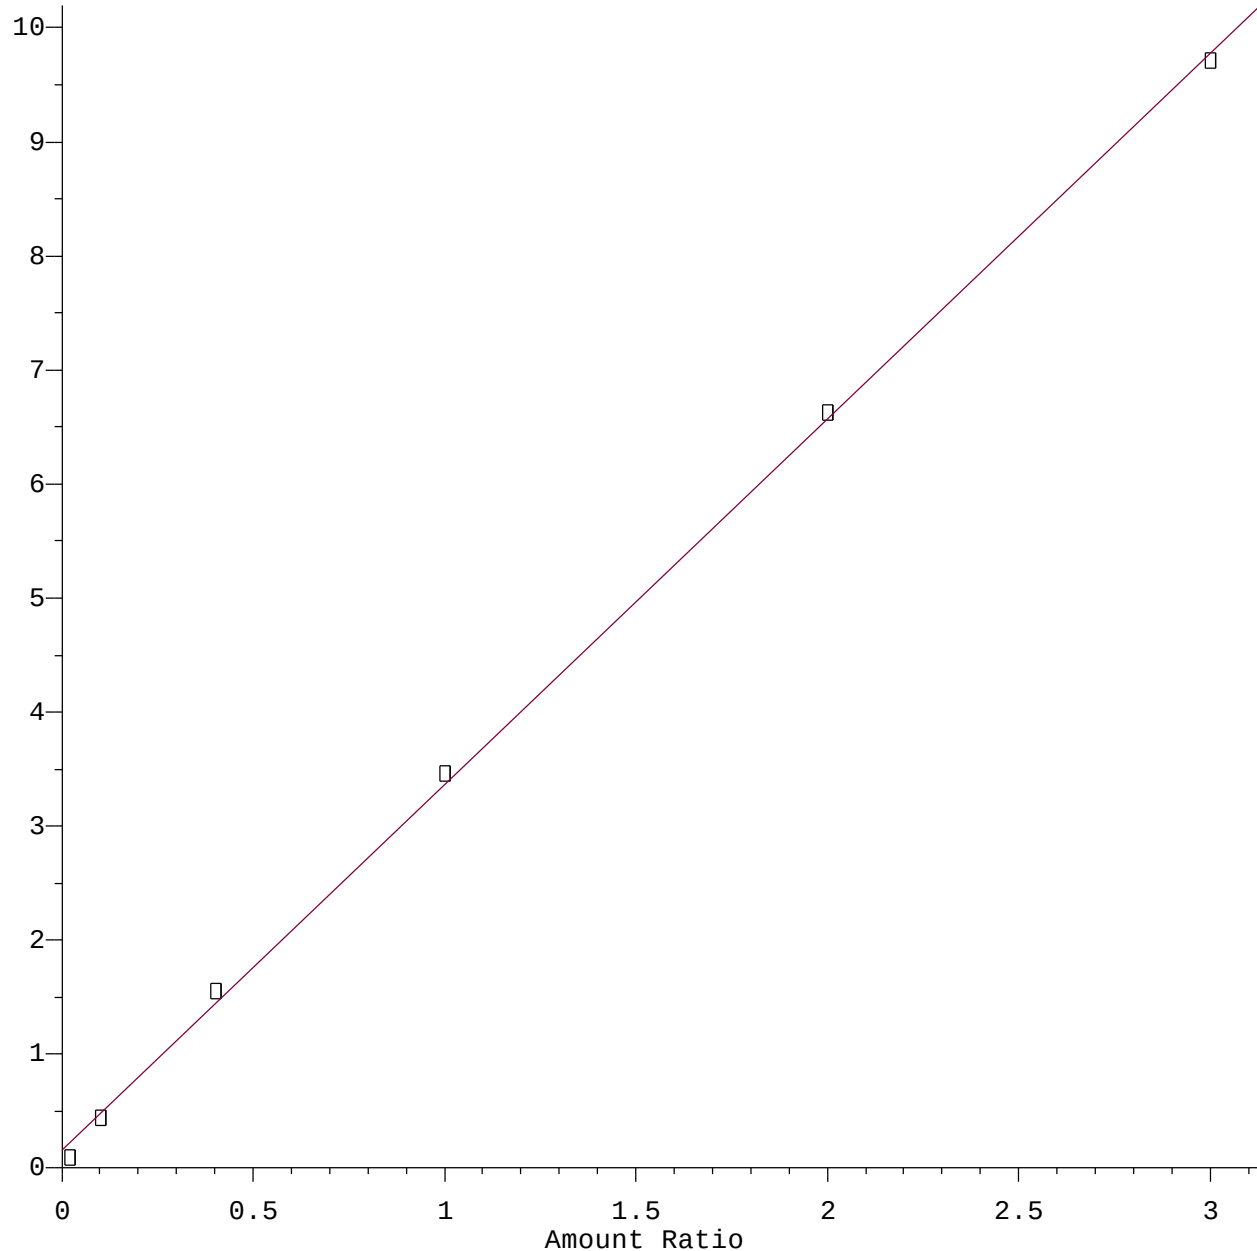


Resp Ratio = 3.21e+000 * Amt + 1.59e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019


1,2,4-Trichlorobenzene

Response Ratio

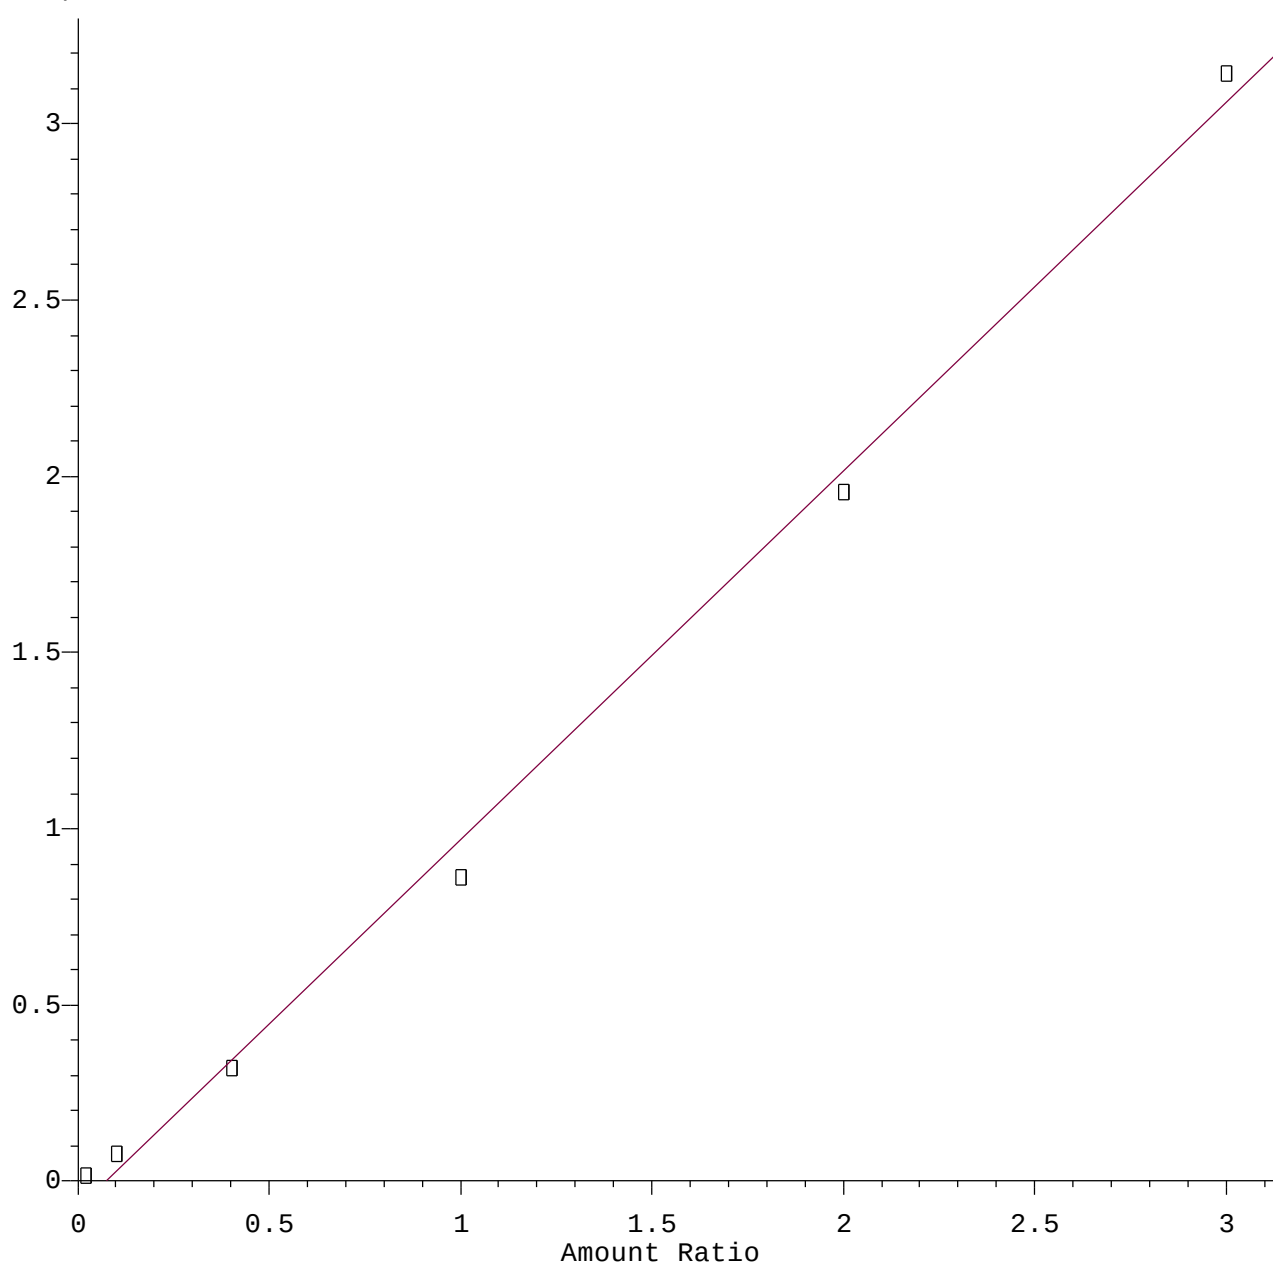


Resp Ratio = 1.05e+000 * Amt - 7.61e-002
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

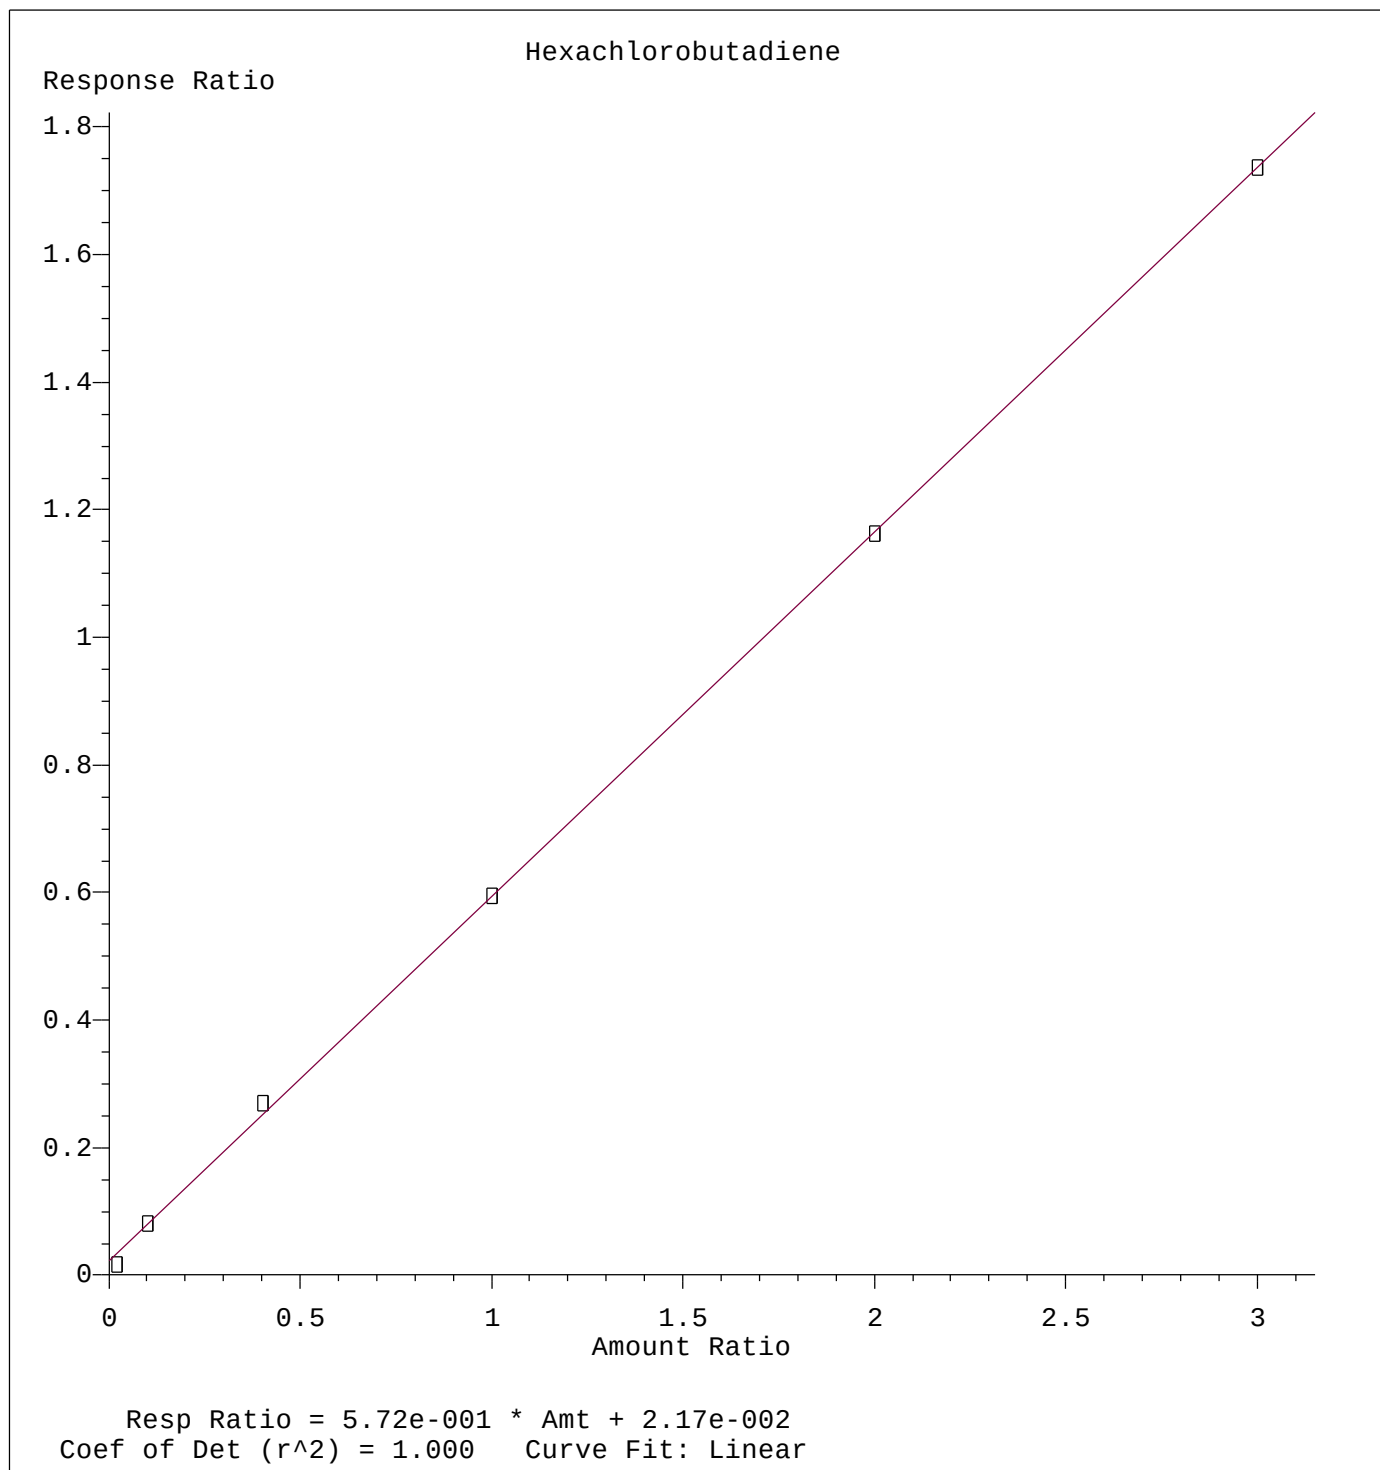

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019

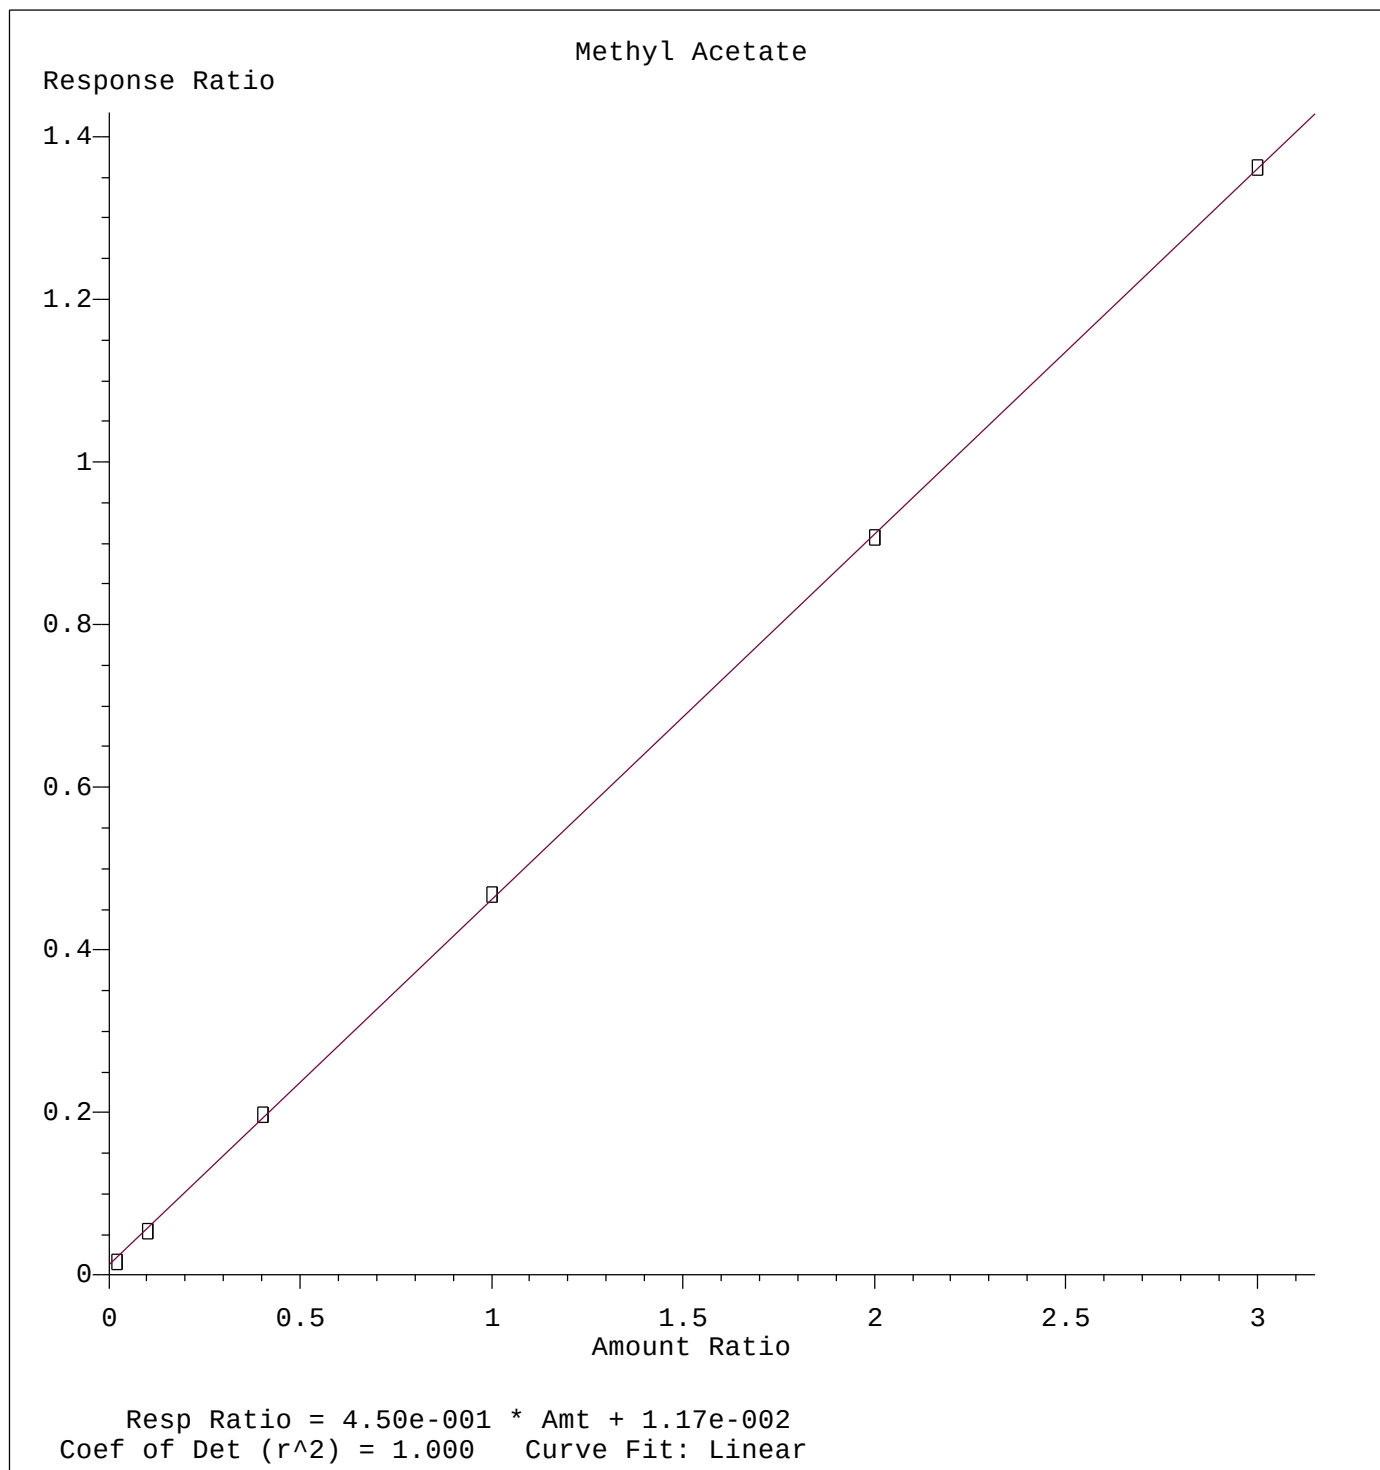

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Calibration Table Last Updated: Fri May 24 06:41:54 2019