
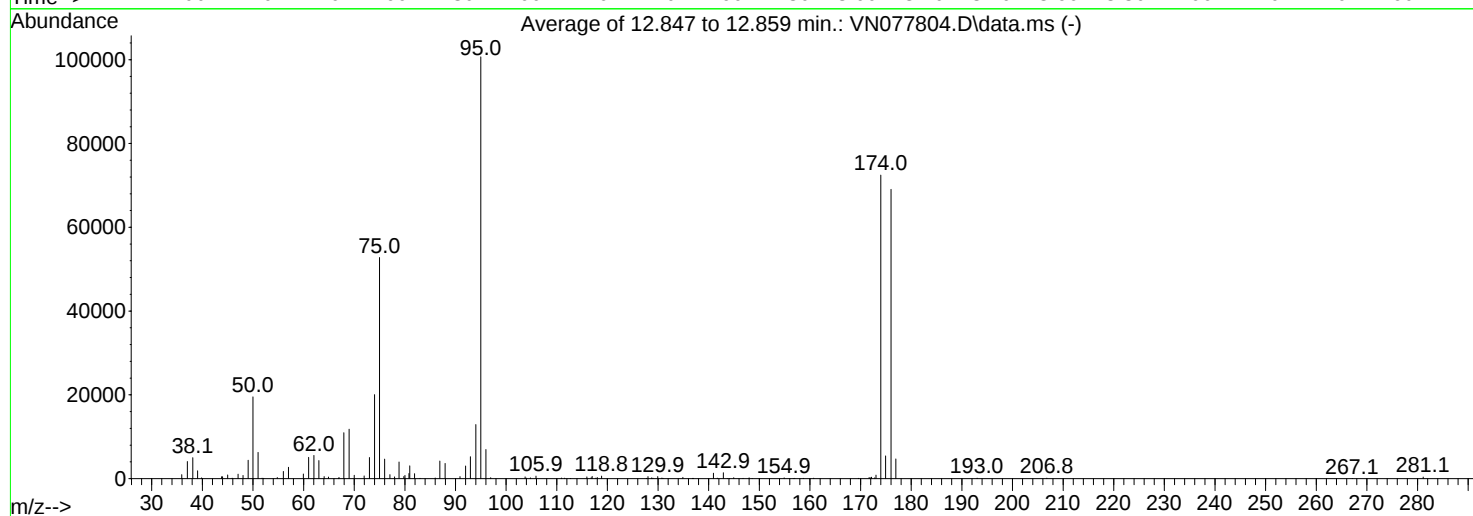


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052323\
Data File : VN077804.D
Acq On : 23 May 2023 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

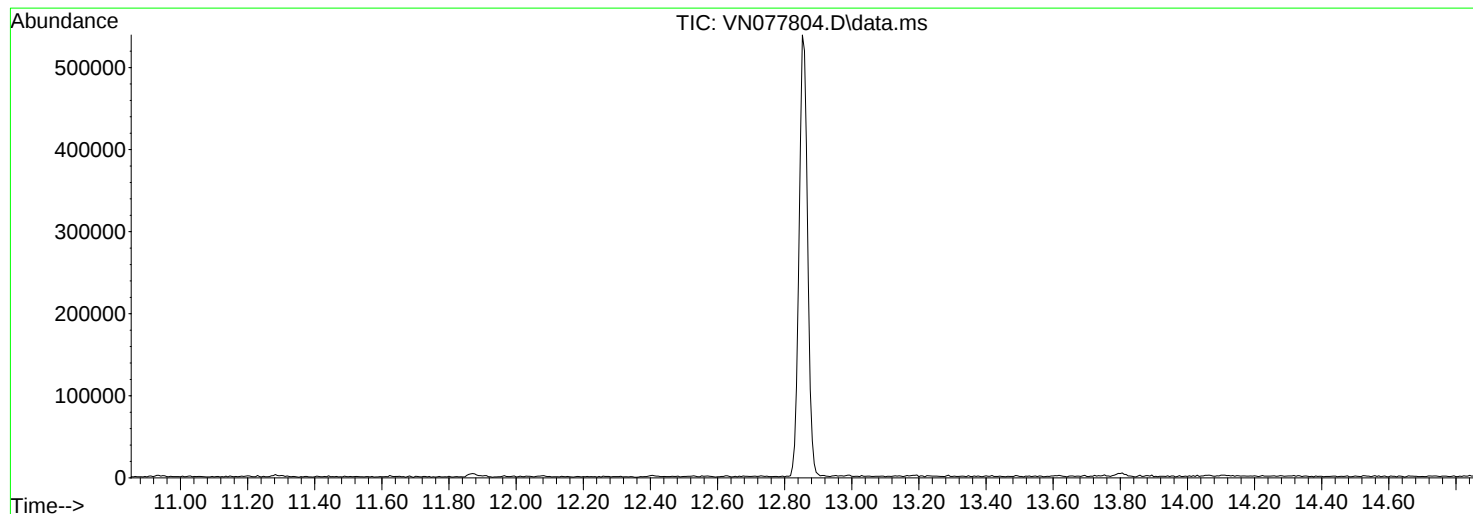

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	19523	PASS
75	95	30	60	52.4	52795	PASS
95	95	100	100	100.0	100685	PASS
96	95	5	9	6.9	6970	PASS
173	174	0.00	2	1.2	834	PASS
174	95	50	100	71.9	72440	PASS
175	174	5	9	7.5	5443	PASS
176	174	95	101	95.3	69037	PASS
177	176	5	9	6.8	4685	PASS

Average of 12.847 to 12.859 min.: VN077804.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	941	49.05	4410	63.00	4317	75.00	5279
37.05	4094	50.00	19523	64.05	488	76.00	464
38.10	5011	51.00	6254	64.90	381	77.05	96
39.05	1889	51.80	116	66.90	108	77.95	42
39.85	183	52.10	60	67.00	252	78.85	3979
43.80	466	54.80	286	67.95	10945	79.80	481
44.00	454	56.00	1723	69.00	11822	80.00	773
45.00	866	57.00	2729	70.00	808	80.80	1223
45.90	126	59.95	1121	71.95	633	80.95	3048
47.05	1059	61.00	5084	73.00	5028	81.90	1204
48.05	766	62.05	5523	74.00	20037	83.00	68

Average of 12.847 to 12.859 min.: VN077804.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	155	104.00	127	118.85	625	140.95	1309
86.90	4198	104.80	208	127.70	68	141.70	129
87.95	3648	105.90	598	128.00	492	142.90	1426
90.90	499	110.95	150	128.75	178	143.70	50
92.00	3019	111.55	111	129.00	114	144.10	52
92.95	5232	112.70	58	129.95	494	144.95	222
94.00	12918	115.95	409	130.75	171	146.80	66
95.00	100685	116.80	245	131.00	61	148.00	193
96.00	6970	117.00	549	134.90	288	148.60	51
96.95	237	117.70	110	136.80	97	154.90	197
103.75	435	118.00	258	137.00	72	156.70	51

Average of 12.847 to 12.859 min.: VN077804.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	66	176.00	69037				
158.70	74	176.95	4685				
160.75	129	193.00	116				
169.60	63	206.80	104				
171.70	281	267.10	51				
171.90	244	281.10	381				
172.15	348						
172.80	208						
173.05	834						
174.00	72440						
174.95	5443						

Instrument :

MSVOA_N

ClientSampleId :

BFB