
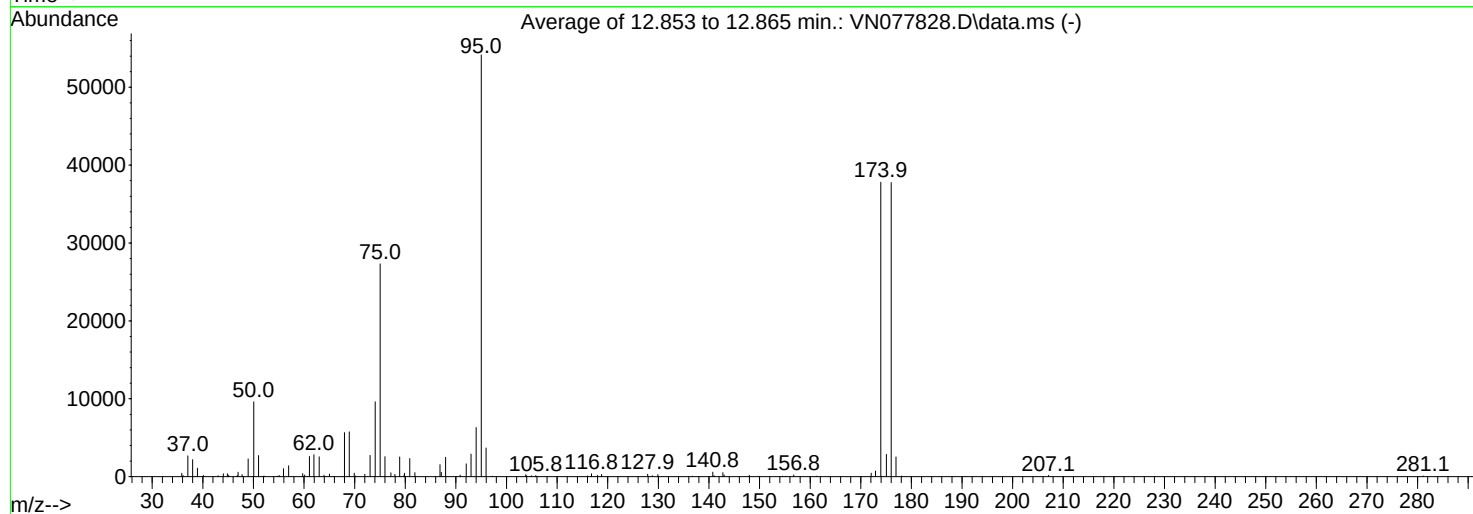


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052323\
Data File : VN077828.D
Acq On : 23 May 2023 22:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

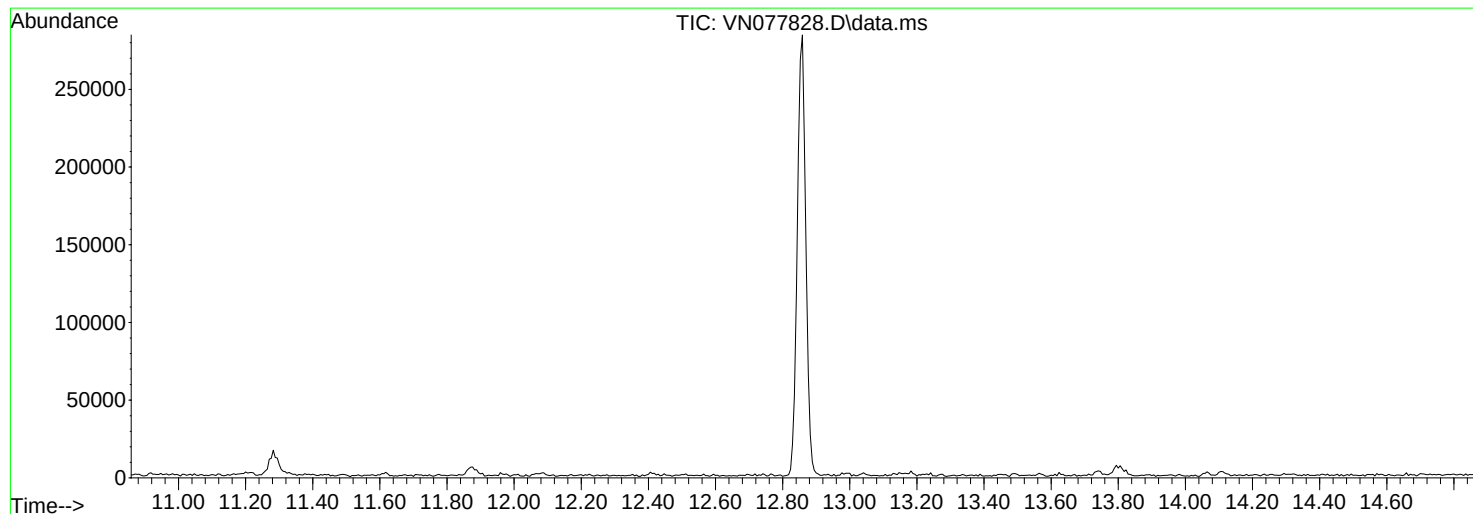

AutoFind: Scans 1853, 1854, 1855; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	9618	PASS
75	95	30	60	50.5	27331	PASS
95	95	100	100	100.0	54163	PASS
96	95	5	9	6.8	3675	PASS
173	174	0.00	2	1.9	721	PASS
174	95	50	100	69.8	37797	PASS
175	174	5	9	7.5	2850	PASS
176	174	95	101	99.9	37768	PASS
177	176	5	9	6.7	2518	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	438	46.95	566	60.10	203	73.05	272
36.10	144	47.75	267	61.05	2582	74.05	962
37.05	2676	48.95	2282	61.95	2821	75.05	2733
38.00	2172	50.05	9618	63.00	2542	76.00	256
38.95	1086	51.00	2721	63.95	188	77.15	494
40.10	175	52.10	81	65.00	336	77.95	282
43.00	125	54.80	56	68.00	5648	78.90	2535
44.05	364	55.10	145	68.95	5754	79.70	114
44.85	369	55.95	1018	69.90	461	79.85	441
45.10	192	56.95	1392	70.20	89	80.90	2320
46.80	153	59.75	388	72.00	319	81.90	510

Average of 12.853 to 12.865 min.: VN077828.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.85	1549	104.00	130	140.75	567	172.90	721
87.10	563	104.90	112	141.00	129	173.95	37797
87.95	2485	105.80	137	142.75	517	175.05	2850
90.85	213	116.00	87	143.00	204	176.00	37768
92.05	1643	116.80	371	147.95	163	176.95	2518
93.00	2905	117.95	175	149.90	61	178.10	75
94.00	6299	118.80	281	154.50	54	207.10	165
95.00	54163	127.90	306	155.10	51	281.10	89
95.95	3675	128.80	118	156.75	215		
97.20	59	129.90	263	161.20	56		
103.80	238	136.70	61	172.05	459		

Instrument :

MSVOA_N

ClientSampleId :

BFB