

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
 Data File : VN082331.D
 Acq On : 23 May 2024 19:09
 Operator : JC\MD
 Sample : P2562-05
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SY-3DD

Quant Time: May 24 04:23:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
 Quant Title : SW846 8260
 QLast Update : Thu May 16 05:21:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	206583	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	362353	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	340549	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	152509	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	161682	49.565	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	99.140%
35) Dibromofluoromethane	8.171	113	115583	51.854	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	103.700%
50) Toluene-d8	10.571	98	454563	53.191	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	106.380%
62) 4-Bromofluorobenzene	12.853	95	167637	54.959	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	109.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082331.D
Acq On : 23 May 2024 19:09
Operator : JC\MD
Sample : P2562-05
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SY-3DD

Quant Time: May 24 04:23:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260
QLast Update : Thu May 16 05:21:06 2024
Response via : Initial Calibration



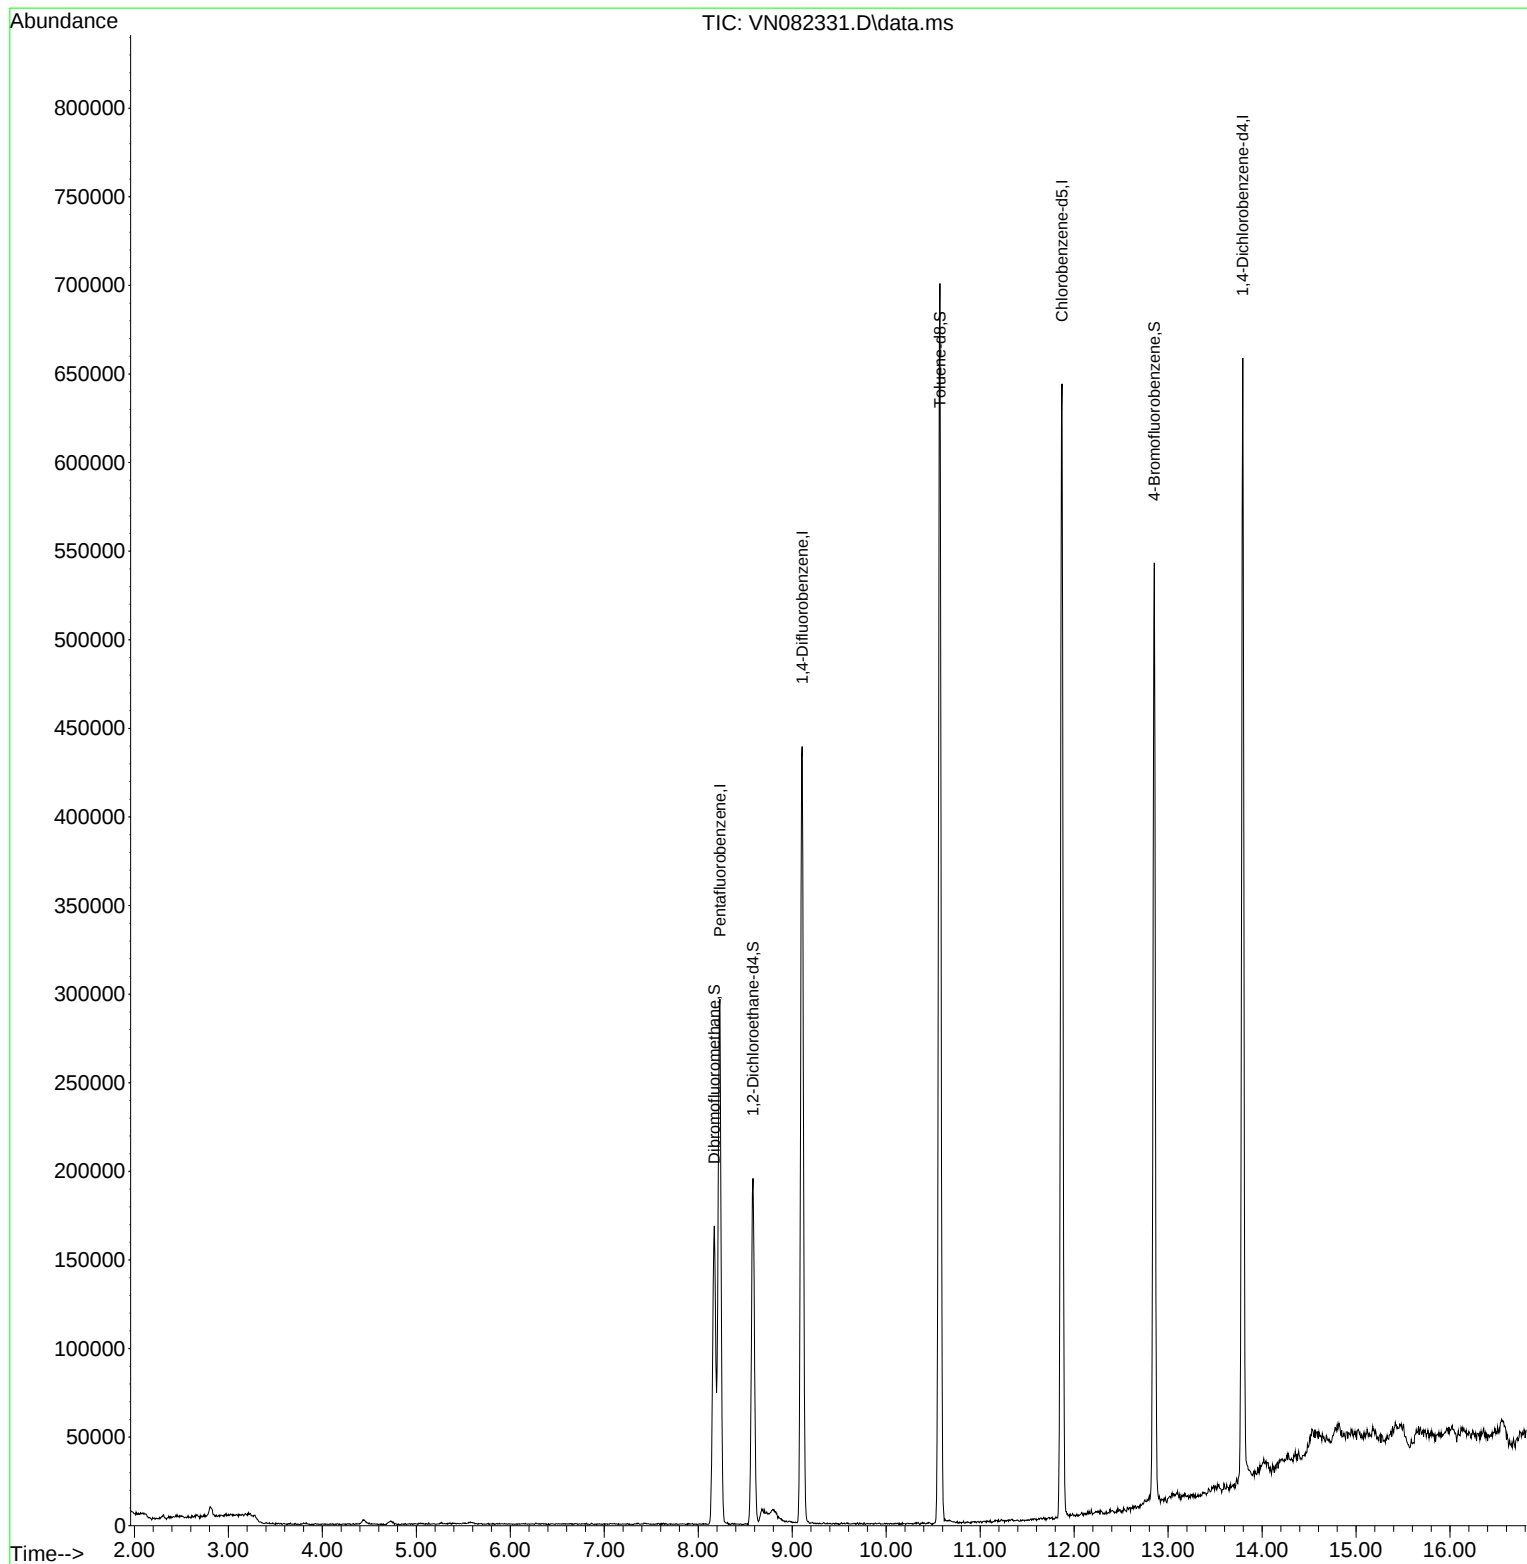


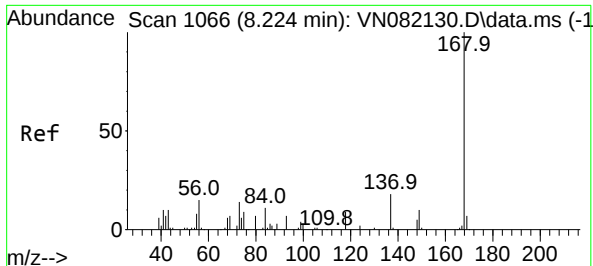

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1107
Delta R.T. 0.006 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09




Instrument :
MSVOA_N
ClientSampleId :
SY-3DD


Tgt Ion:168 Resp: 206583
Ion Ratio Lower Upper
168 100
99 62.8 48.2 72.4

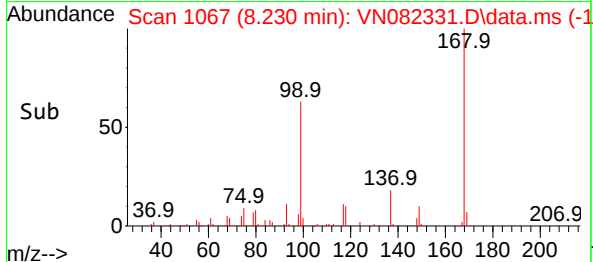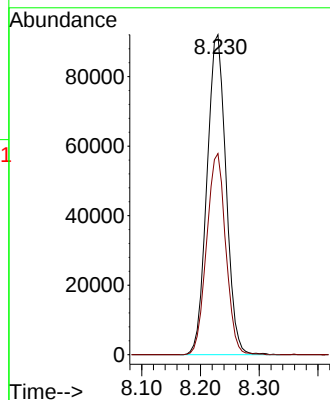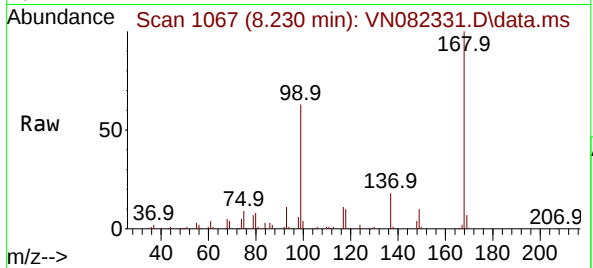

#33
1,2-Dichloroethane-d4
Concen: 49.565 ug/l
RT: 8.583 min Scan# 1127
Delta R.T. 0.006 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09

Tgt Ion: 65 Resp: 161682
Ion Ratio Lower Upper
65 100
67 50.5 0.0 103.0

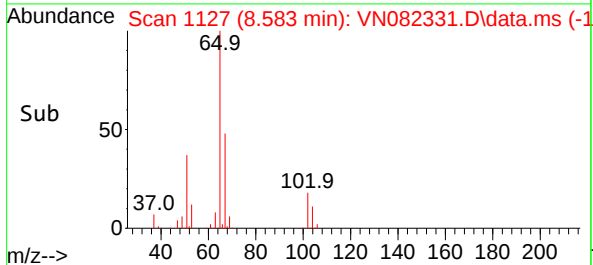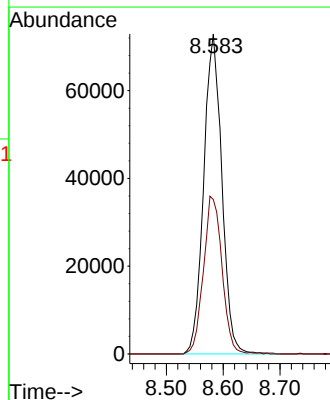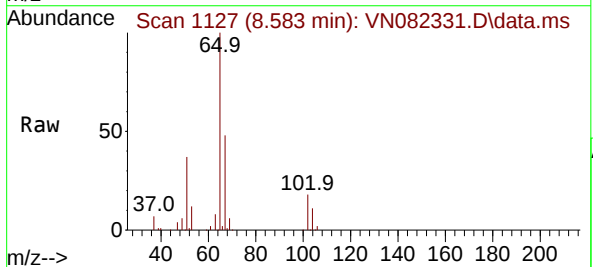

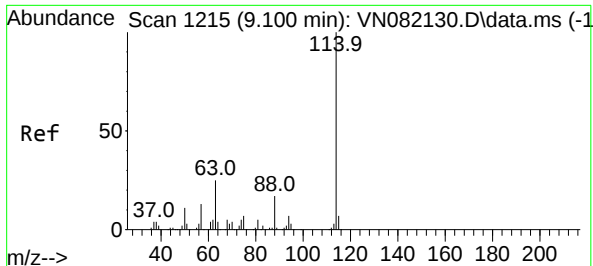

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN082331.D

Acq: 23 May 2024 19:09

Instrument :

MSVOA_N

ClientSampleId :

SY-3DD





Tgt Ion:114 Resp: 362353

Ion Ratio Lower Upper

114 100

63 23.4 0.0 41.0

88 16.1 0.0 31.4

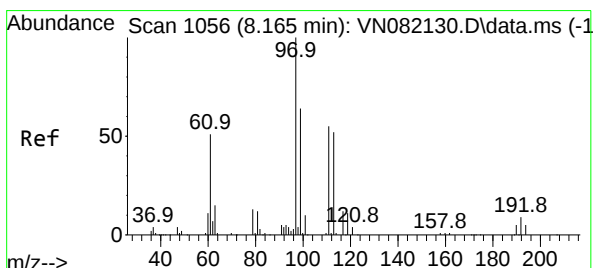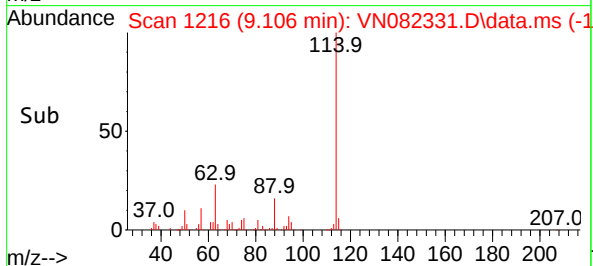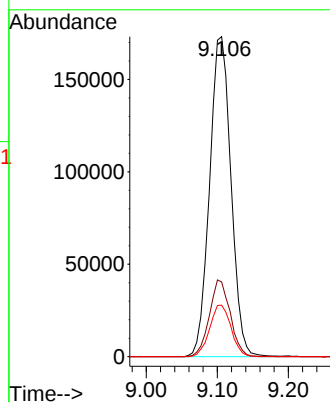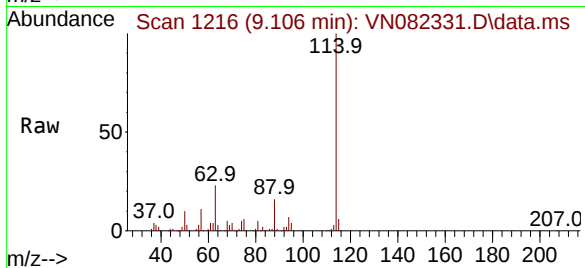

#35

Dibromofluoromethane

Concen: 51.854 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082331.D

Acq: 23 May 2024 19:09




Tgt Ion:113 Resp: 115583


Ion Ratio Lower Upper

113 100

111 103.8 83.4 125.2

192 18.8 14.0 21.0


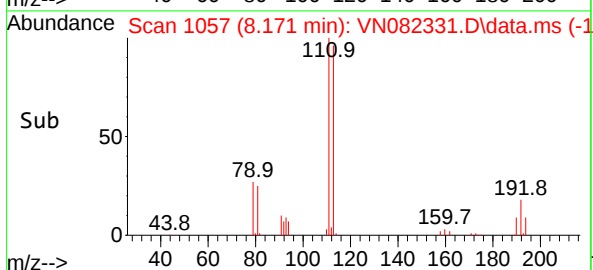
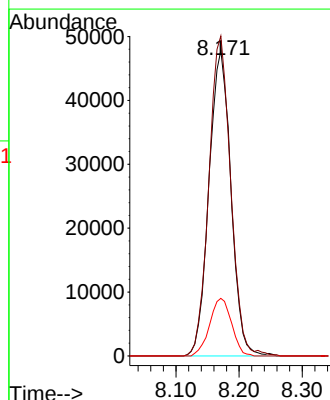
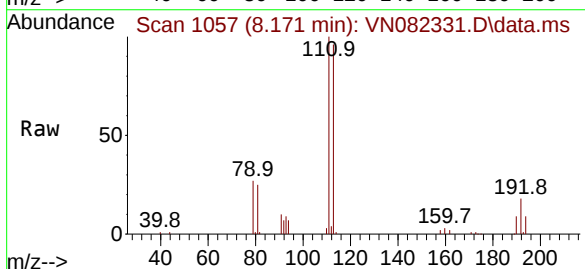


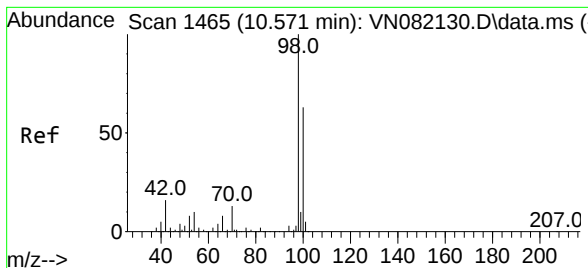

#50
Toluene-d8
Concen: 53.191 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.000 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09




Instrument :
MSVOA_N
ClientSampleId :
SY-3DD


Tgt Ion: 98 Resp: 454563
Ion Ratio Lower Upper
98 100
100 64.3 51.8 77.6

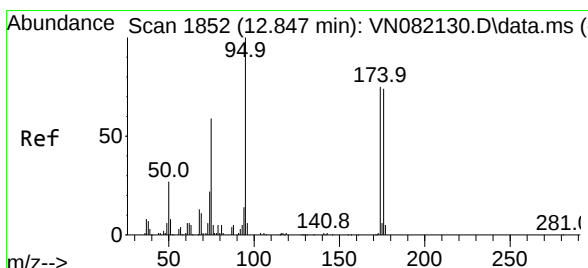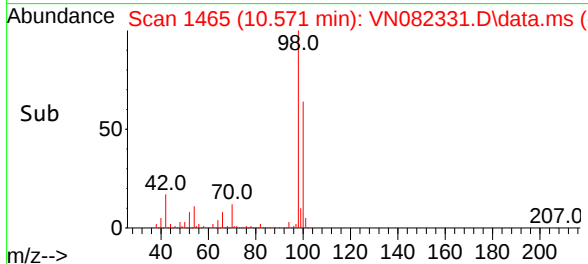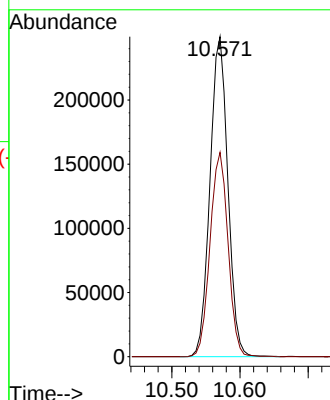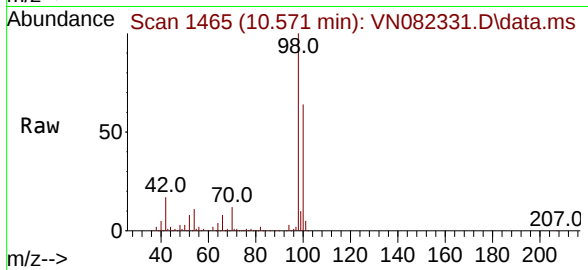

#62
4-Bromofluorobenzene
Concen: 54.959 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09

Tgt Ion: 95 Resp: 167637
Ion Ratio Lower Upper
95 100
174 76.3 0.0 160.6
176 74.4 0.0 152.8


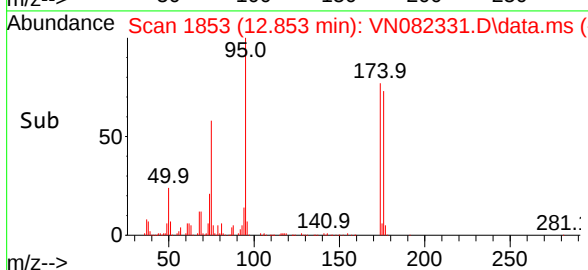
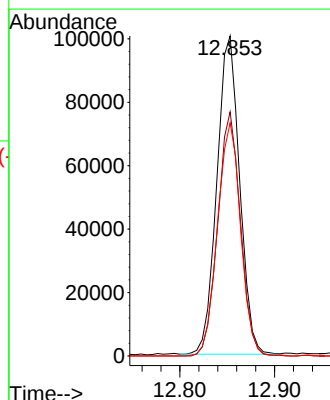
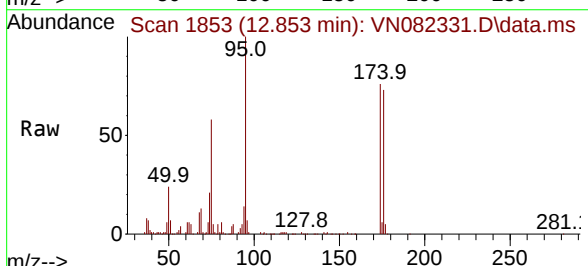


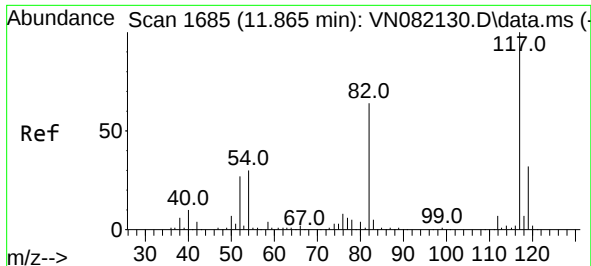

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09

Instrument :
MSVOA_N
ClientSampleId :
SY-3DD

Tgt Ion:117 Resp: 340549
Ion Ratio Lower Upper
117 100
82 59.9 44.6 66.8
119 32.0 25.9 38.9

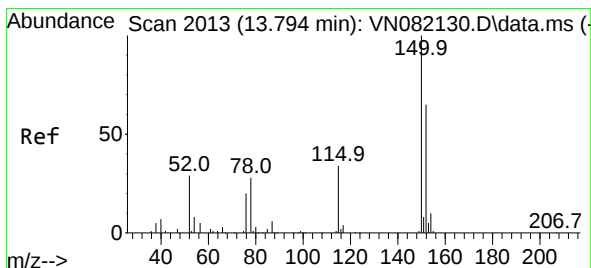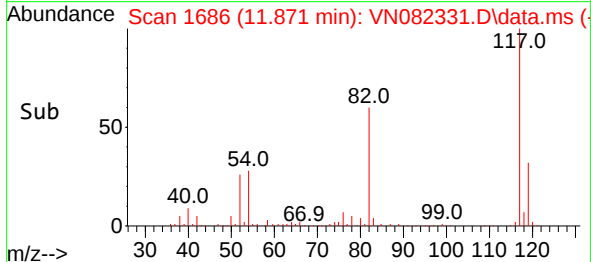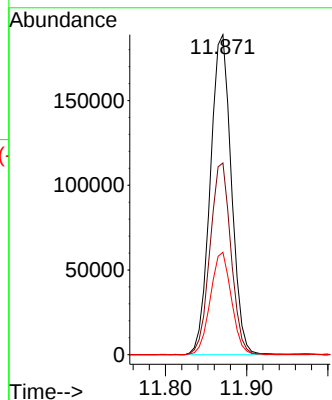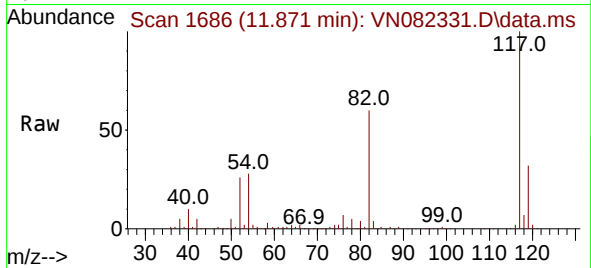

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN082331.D
Acq: 23 May 2024 19:09

Tgt Ion:152 Resp: 152509
Ion Ratio Lower Upper
152 100
115 62.0 30.4 91.3
150 158.7 0.0 353.2

