

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082314.D
Acq On : 23 May 2024 12:16
Operator : JC\MD
Sample : P2554-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1041

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M

Title : SW846 8260

Signal : TIC: VN082314.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.806	142	145	153	rVB3	6651	11901	1.21%	0.235%
2	7.436	923	932	942	rBV2	11010	29627	3.01%	0.585%
3	8.165	1047	1056	1061	rBV	127838	302952	30.78%	5.978%
4	8.224	1061	1066	1076	rVB	215366	487059	49.48%	9.611%
5	8.582	1117	1127	1137	rBV	161742	349174	35.47%	6.890%
6	8.671	1137	1142	1149	rBV6	8092	26832	2.73%	0.529%
7	9.106	1206	1216	1227	rBV	341218	702468	71.37%	13.862%
8	10.571	1456	1465	1472	rBV	530010	984327	100.00%	19.424%
9	11.865	1677	1685	1697	rBV	473756	856782	87.04%	16.907%
10	12.853	1845	1853	1864	rBV	353125	611477	62.12%	12.067%
11	13.794	2006	2013	2024	rBV	420416	704879	71.61%	13.910%




Sum of corrected areas: 5067478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082314.D
Acq On : 23 May 2024 12:16
Operator : JC\MD
Sample : P2554-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

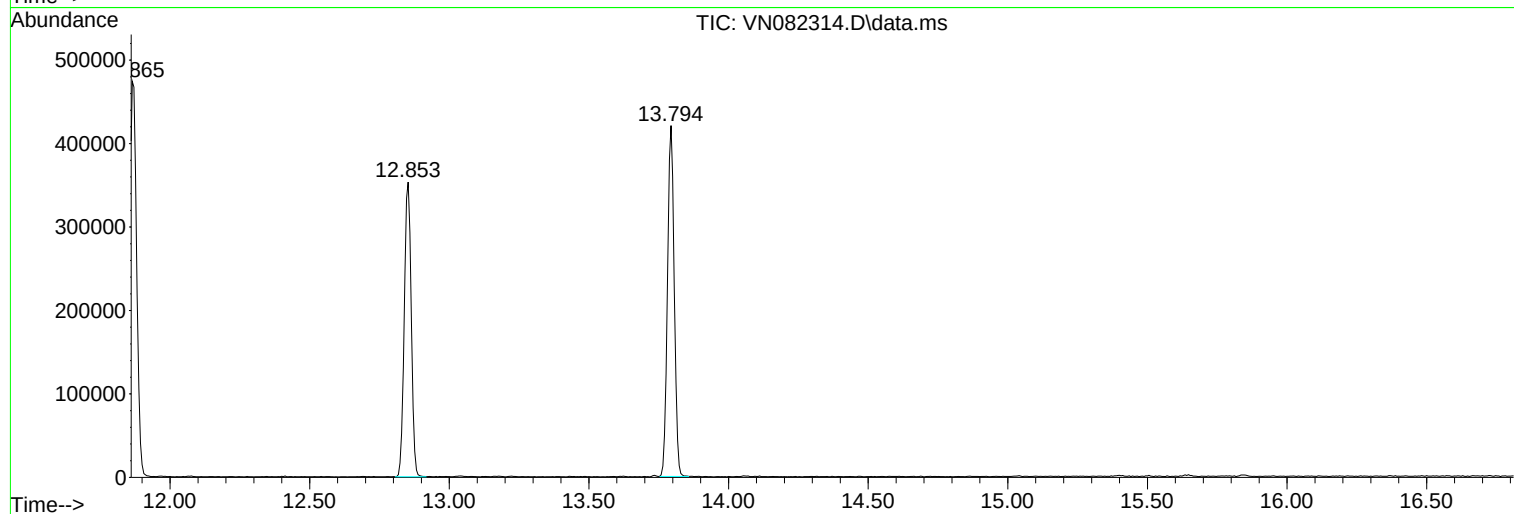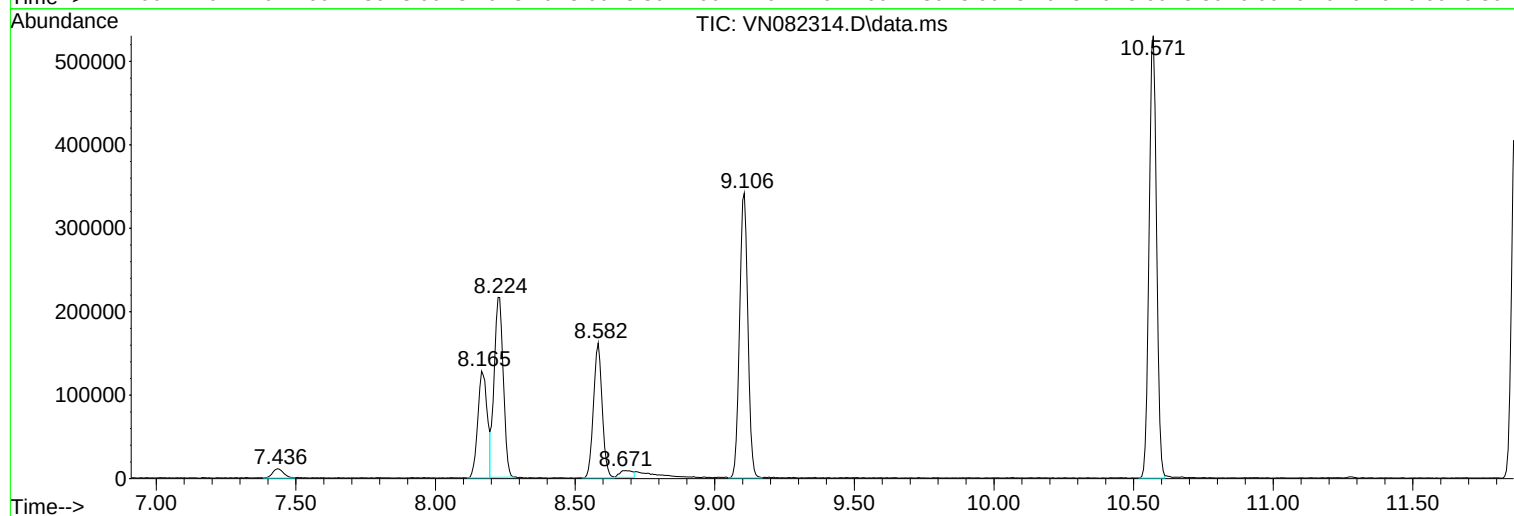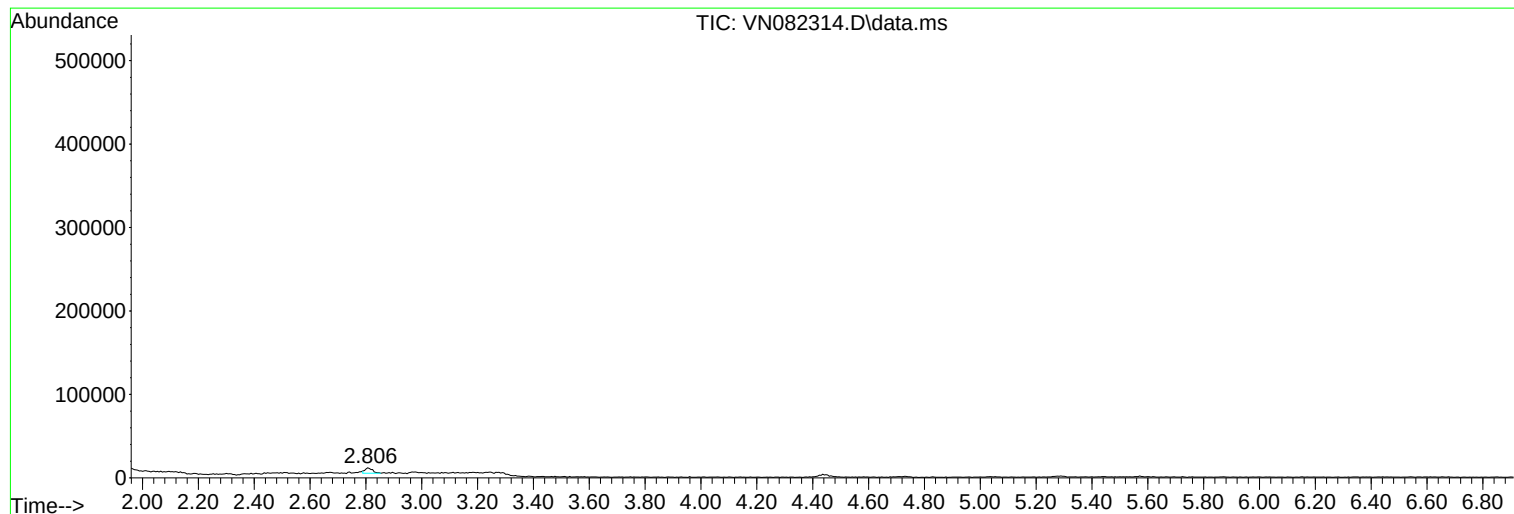

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082314.D
Acq On : 23 May 2024 12:16
Operator : JC\MD
Sample : P2554-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082314.D
Acq On : 23 May 2024 12:16
Operator : JC\MD
Sample : P2554-01 50X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
AUD-1041

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc