
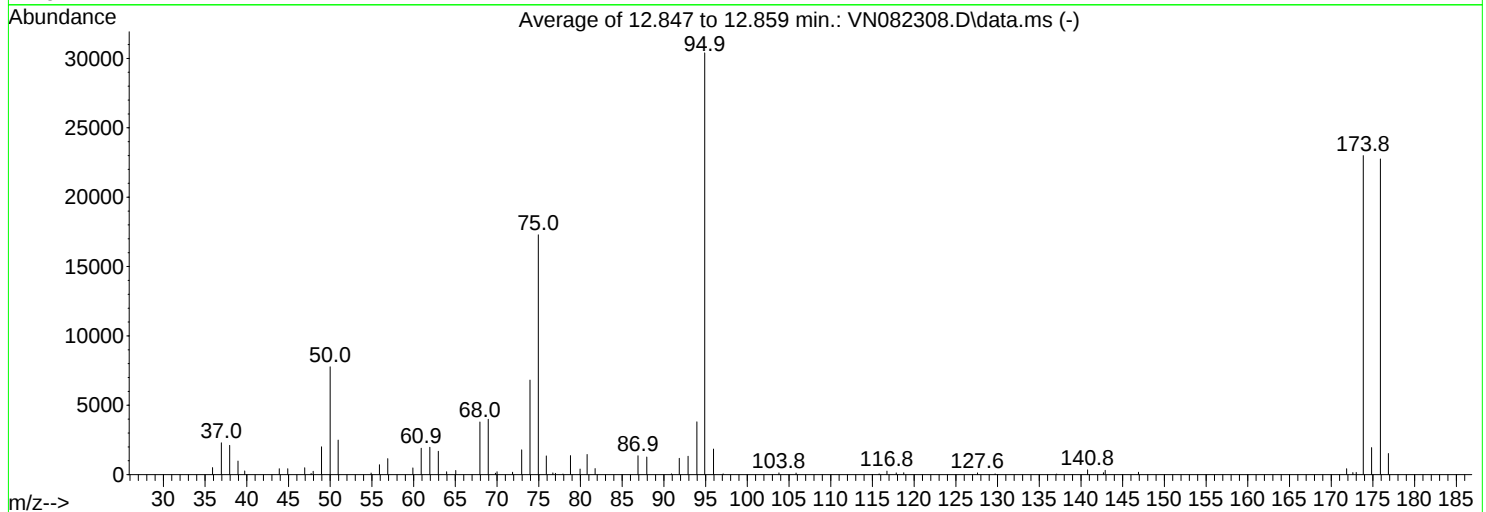


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052324\
Data File : VN082308.D
Acq On : 23 May 2024 09:21
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

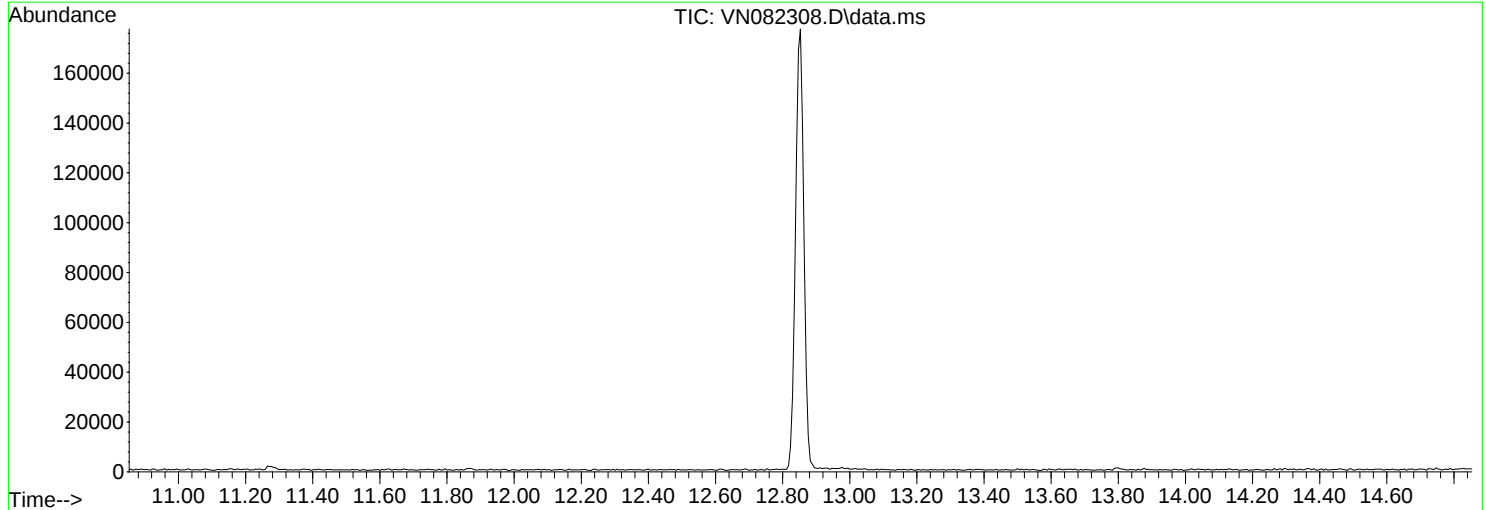

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	25.6	7772	PASS
75	95	30	60	56.8	17284	PASS
95	95	100	100	100.0	30403	PASS
96	95	5	9	6.1	1843	PASS
173	174	0.00	2	0.7	157	PASS
174	95	50	100	75.6	22997	PASS
175	174	5	9	8.5	1949	PASS
176	174	95	101	98.9	22749	PASS
177	176	5	9	6.7	1519	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	505	50.00	7772	67.95	3790	77.90	50
36.95	2291	50.95	2491	68.95	3989	78.80	137
37.95	2108	54.90	118	69.80	101	79.95	40
38.95	977	55.90	715	70.00	205	80.80	145
39.75	260	56.90	1159	71.85	170	81.75	433
43.90	431	59.90	490	72.95	1790	86.90	1357
44.90	427	60.90	1905	73.95	6820	87.95	1273
46.95	492	61.95	1975	74.95	17284	90.90	59
47.70	81	62.95	1686	75.90	1351	91.85	1175
47.95	247	63.95	213	76.70	123	92.90	1327
48.95	2008	65.05	300	77.00	89	93.95	3808

Average of 12.847 to 12.859 min.: VN082308.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
94.90	30403	137.10	51	176.85	1519		
95.95	1843	140.80	346				
97.10	60	142.70	136				
103.80	131	142.90	309				
105.85	119	146.90	177				
115.80	58	171.85	430				
116.75	253	172.60	151				
117.85	122	173.00	157				
118.75	136	173.85	22997				
127.60	125	174.85	1949				
129.70	62	175.90	22749				

Instrument :

MSVOA_N

ClientSampleId :

BFB