


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052419\  
 Data File : VN055780.D  
 Acq On : 24 May 2019 8:26  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.00mL/MSVOA N/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_N\METHODS\82N052319W.M  
 Title : SW846 8260  
 Last Update : Fri May 24 06:41:54 2019

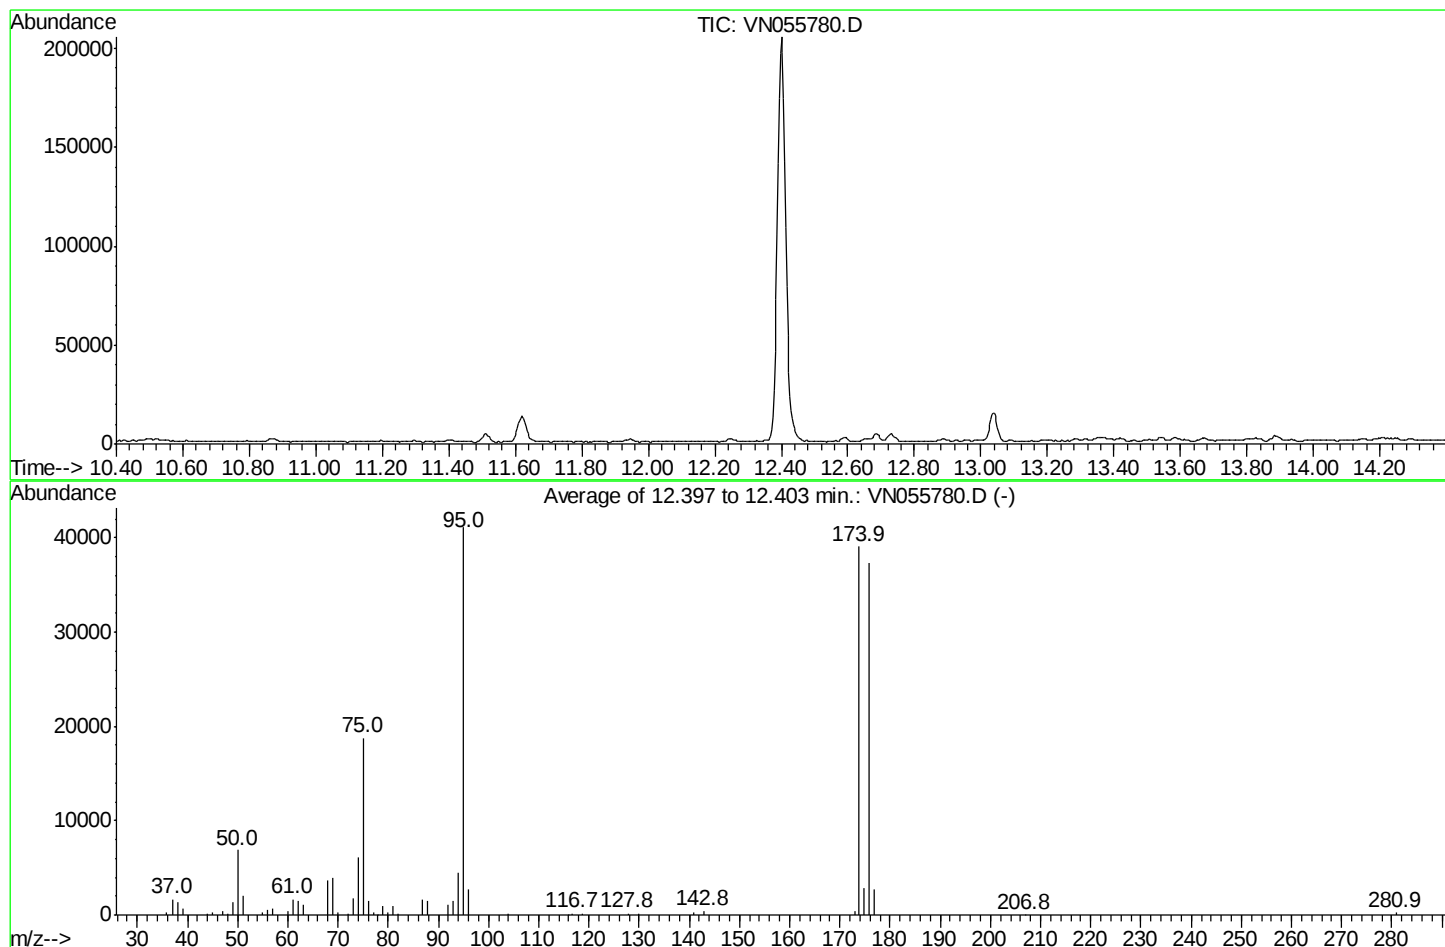

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 16.8      | 6912    | PASS             |
| 75          | 95           | 30           | 60           | 45.6      | 18770   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 41130   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 2781    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.9       | 370     | PASS             |
| 174         | 95           | 50           | 100          | 95.1      | 39104   | PASS             |
| 175         | 174          | 5            | 9            | 7.4       | 2908    | PASS             |
| 176         | 174          | 95           | 101          | 95.6      | 37368   | PASS             |
| 177         | 176          | 5            | 9            | 7.4       | 2777    | PASS             |