


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052419\
Data File : VN055809.D
Acq On : 24 May 2019 21:08
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Title : SW846 8260
Last Update : Fri May 24 06:41:54 2019

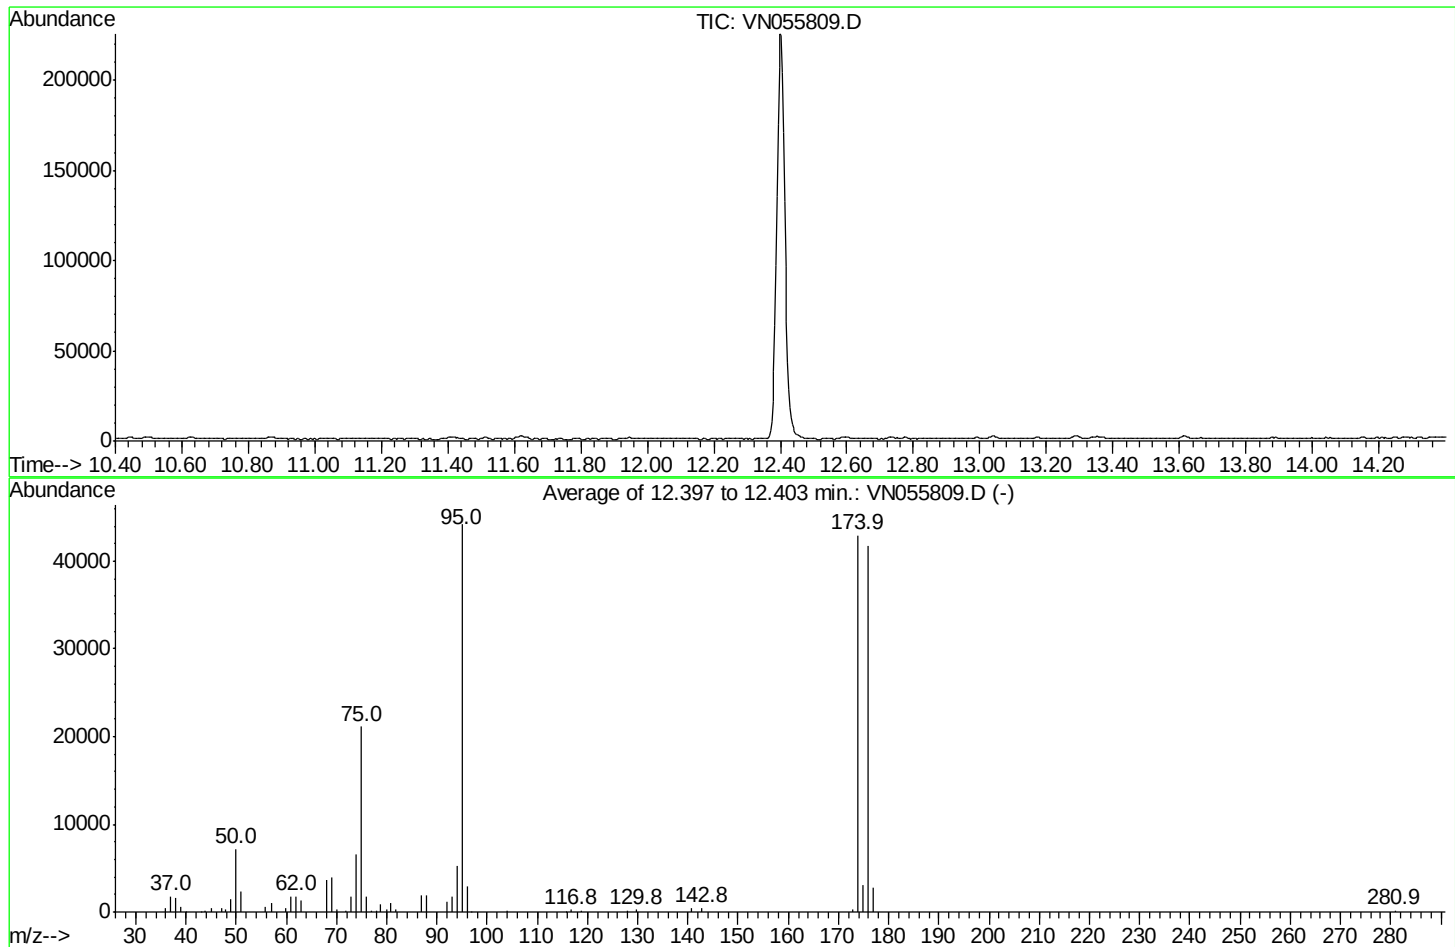

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7171	PASS
75	95	30	60	47.8	21109	PASS
95	95	100	100	100.0	44197	PASS
96	95	5	9	6.7	2971	PASS
173	174	0.00	2	0.8	335	PASS
174	95	50	100	97.1	42930	PASS
175	174	5	9	7.1	3064	PASS
176	174	95	101	97.3	41768	PASS
177	176	5	9	6.7	2801	PASS