

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
 Data File : VN072602.D
 Acq On : 24 May 2022 21:43
 Operator : JC\MD
 Sample : N2968-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-40

Quant Time: May 25 09:22:37 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 25 09:15:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.081	168	157767	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	294065	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	338955	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	129847	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	94919	52.891	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 105.780%			
35) Dibromofluoromethane	8.016	113	85258	44.733	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 89.460%			
50) Toluene-d8	10.439	98	373621	51.340	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 102.680%			
62) 4-Bromofluorobenzene	12.727	95	144105	60.883	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 121.760%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.293	50	389	Below Cal	#	43
6) Chloroethane	2.999	64	78	Below Cal	#	42
11) Tert butyl alcohol	5.363	59	108019	319.642	ug/l	100
16) Acetone	4.299	43	1848	2.095	ug/l #	87
18) Methyl Acetate	4.846	43	179	Below Cal	#	48
19) Methyl tert-butyl Ether	5.610	73	43687	8.883	ug/l	95
20) Methylene Chloride	5.081	84	56	Below Cal	#	10
22) Diisopropyl ether	6.487	45	41069	7.469	ug/l	90
23) Vinyl Acetate	6.493	43	20508	4.392	ug/l #	68
25) 2-Butanone	7.334	43	810	0.544	ug/l #	45
29) Tetrahydrofuran	7.675	42	280	0.302	ug/l #	46
31) Cyclohexane	8.092	56	5021	1.766	ug/l #	62
36) 1,1-Dichloropropene	8.081	75	10670	3.957	ug/l #	45
37) Ethyl Acetate	7.334	43	810	0.230	ug/l #	67
38) Carbon Tetrachloride	8.081	117	15184	5.335	ug/l #	17
39) Methylcyclohexane	9.457	83	1203	0.362	ug/l #	86
40) Benzene	8.457	78	618426	71.075	ug/l	100
42) 1,2-Dichloroethane	8.451	62	4578	1.624	ug/l	77
43) Isopropyl Acetate	8.528	43	2695	0.539	ug/l #	53
48) Methyl methacrylate	9.451	41	573	0.236	ug/l #	22
52) Toluene	10.498	92	2560	0.465	ug/l	86
59) 2-Hexanone	11.122	43	3243	1.337	ug/l	82
67) Ethyl Benzene	11.839	91	5208	0.403	ug/l	90
68) m/p-Xylenes	11.951	106	1603	0.326	ug/l	98
69) o-Xylene	12.275	106	2679	0.563	ug/l	89
73) Isopropylbenzene	12.575	105	5386	0.466	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	69849	19.814	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.051	105	2427	0.270	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.727	75	69849	58.146	ug/l #	10
84) 1,2,4-Trimethylbenzene	13.363	105	4192	0.475	ug/l	92
90) Hexachloroethane	14.269	117	488	0.279	ug/l #	9


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072602.D
Acq On : 24 May 2022 21:43
Operator : JC\MD
Sample : N2968-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Time: May 25 09:22:37 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260
QLast Update : Wed May 25 09:15:20 2022
Response via : Initial Calibration




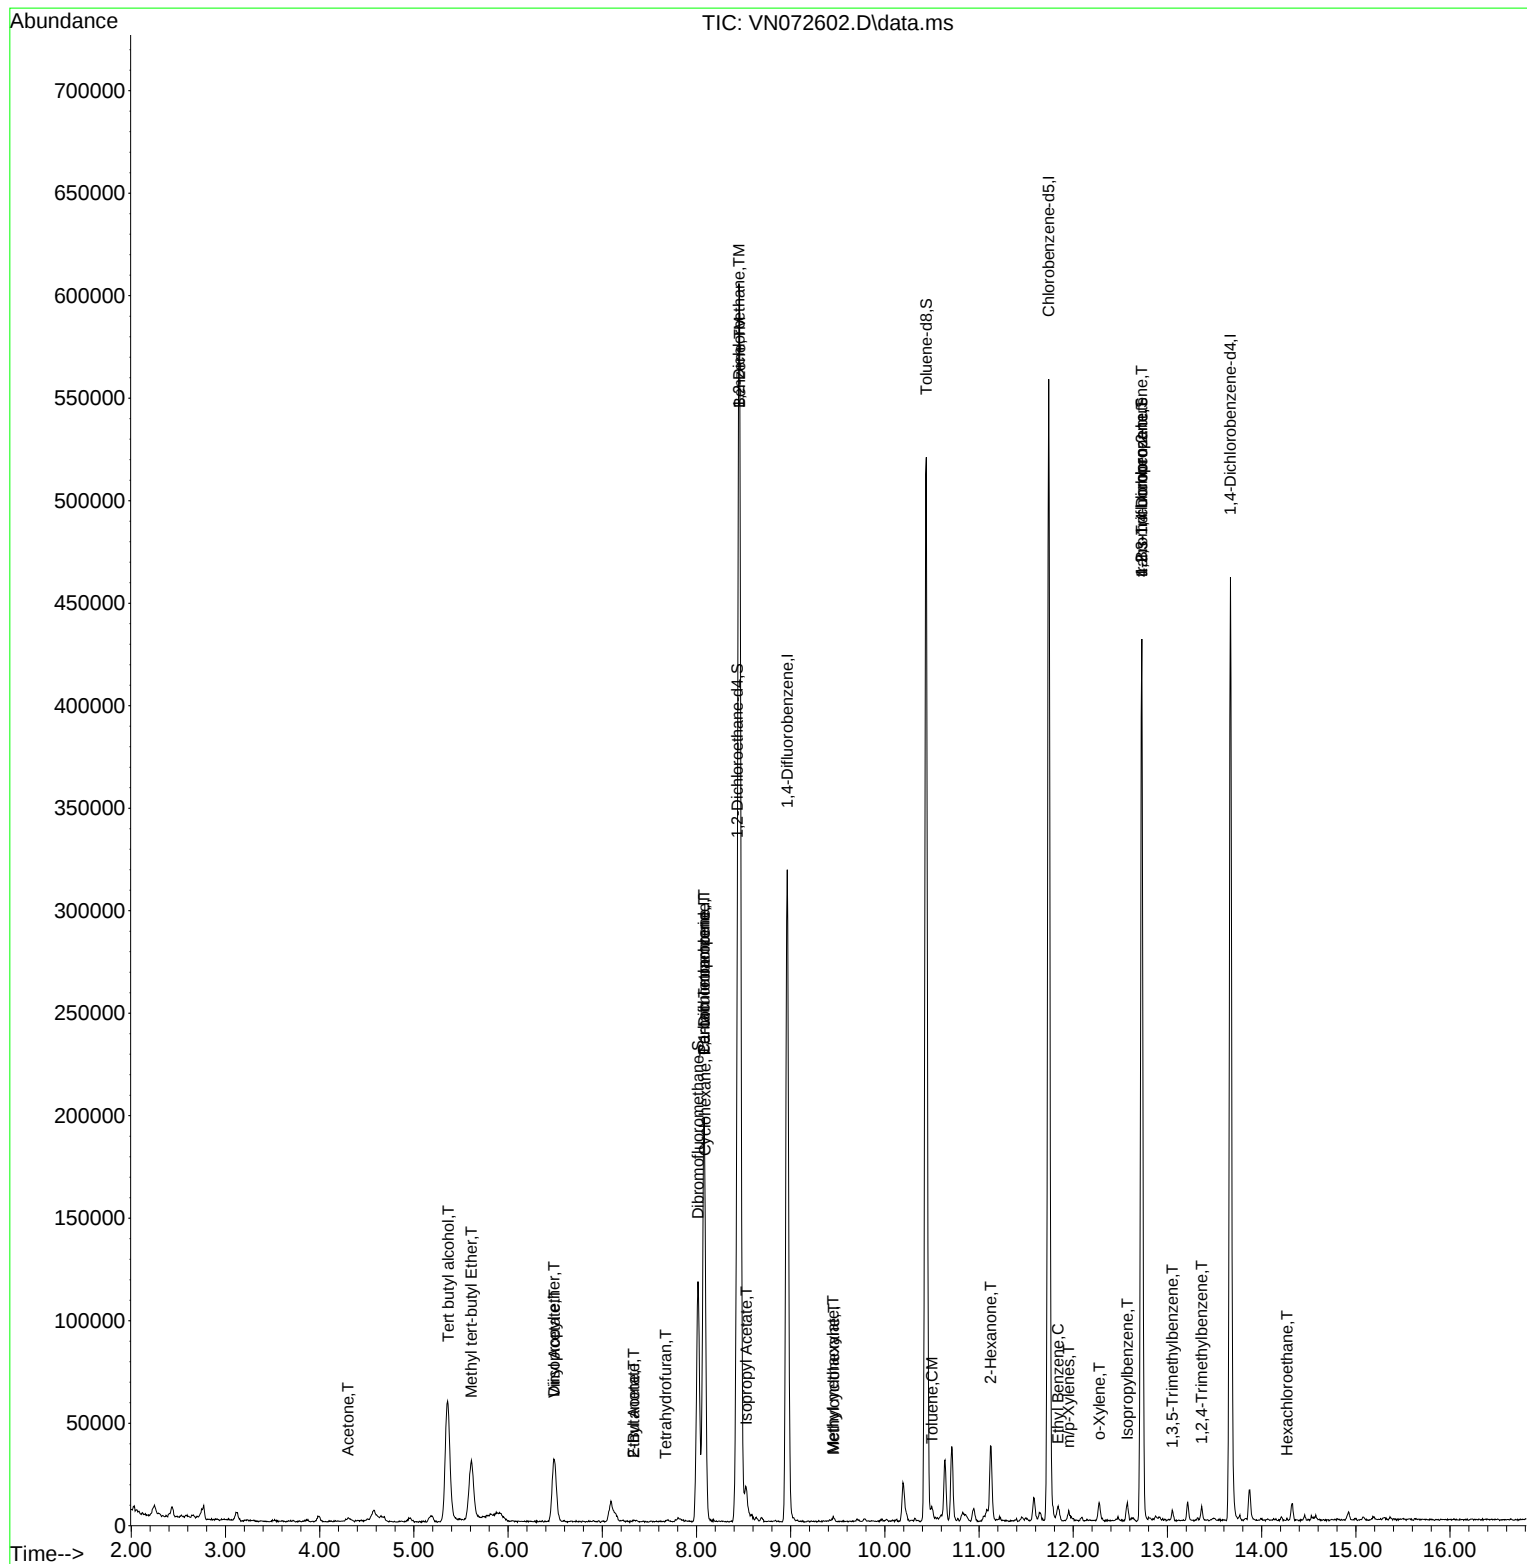




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 157767
Ion Ratio Lower Upper
168 100
99 53.0 42.3 63.5

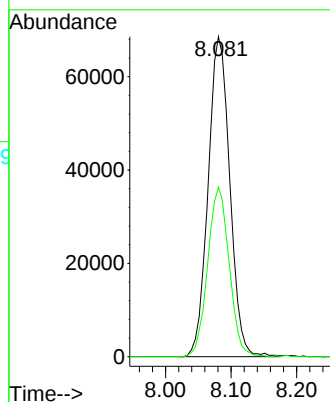

#3
Chloromethane
Concen: Below Cal
RT: 2.293 min Scan# 52
Delta R.T. -0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 50 Resp: 389
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#


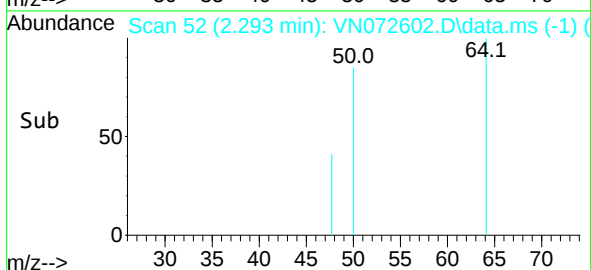
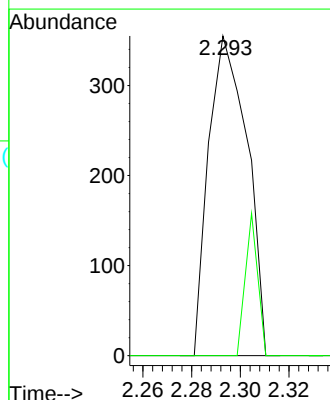
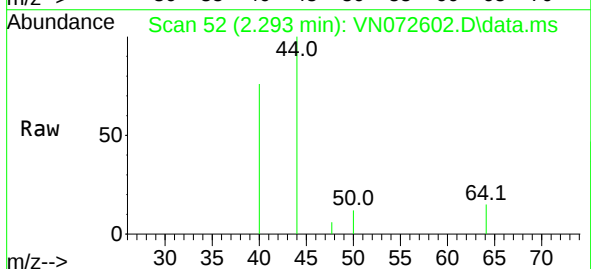




#6
Chloroethane
Concen: Below Cal
RT: 2.999 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 64 Resp: 78
Ion Ratio Lower Upper
64 100
66 0.0 26.2 39.4#

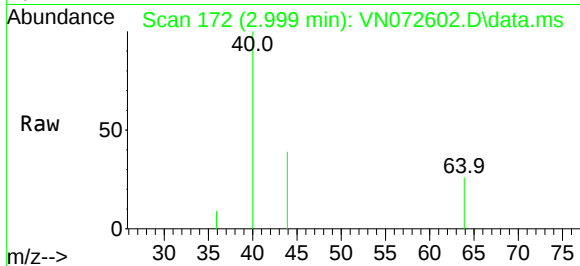

#11
Tert butyl alcohol
Concen: 319.642 ug/l
RT: 5.363 min Scan# 574
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 59 Resp: 108019
Ion Ratio Lower Upper
59 100
57 10.3 8.3 12.5


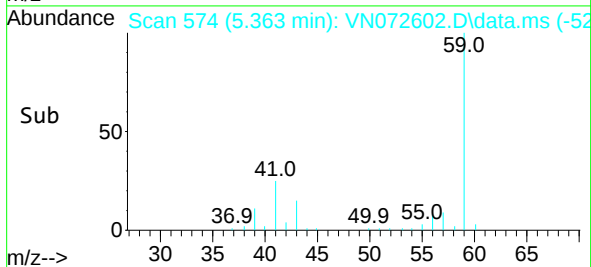

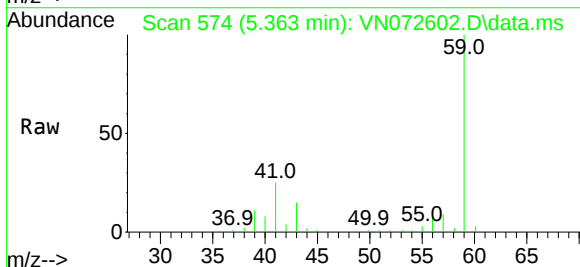




#16
Acetone
Concen: 2.095 ug/l
RT: 4.299 min Scan# 393
Delta R.T. 0.024 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 1848
Ion Ratio Lower Upper
43 100
58 25.3 26.0 39.0#



#18
Methyl Acetate
Concen: Below Cal
RT: 4.846 min Scan# 486
Delta R.T. 0.001 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 43 Resp: 179
Ion Ratio Lower Upper
43 100
74 0.0 21.6 32.4#


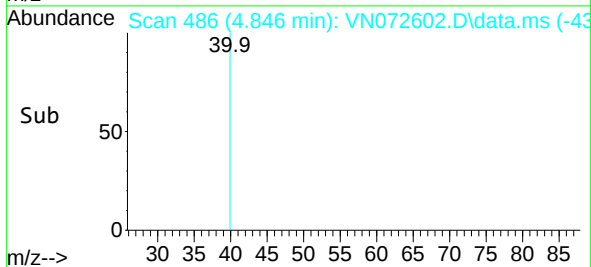

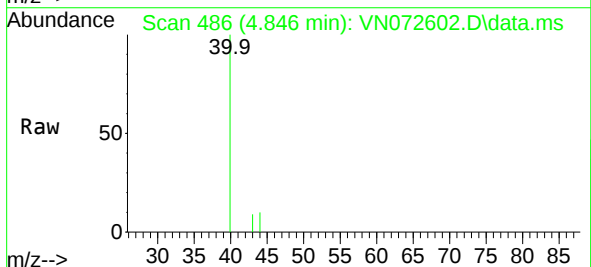


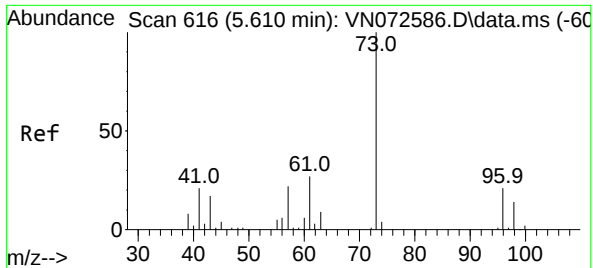

#19
Methyl tert-butyl Ether
Concen: 8.883 ug/l
RT: 5.610 min Scan# 616
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 73 Resp: 43687
Ion Ratio Lower Upper
73 100
57 24.4 17.6 26.4

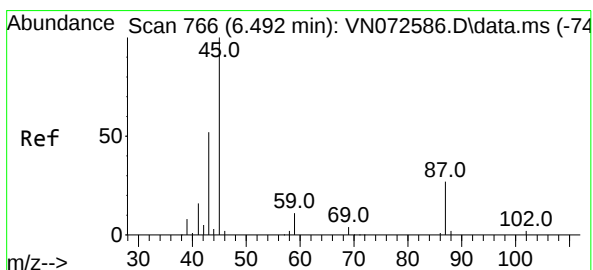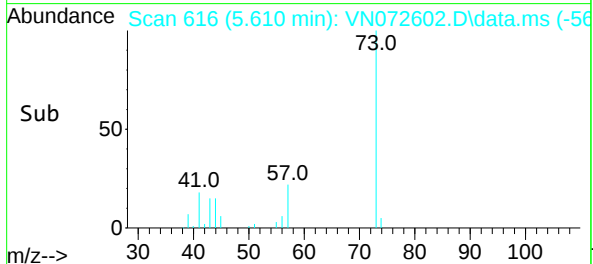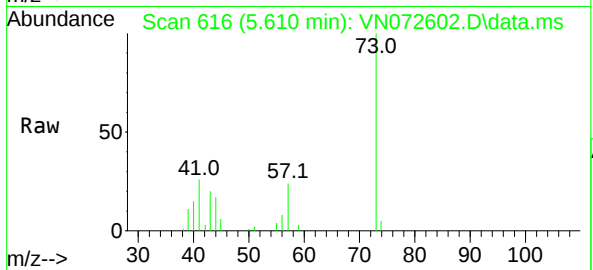

#22
Diisopropyl ether
Concen: 7.469 ug/l
RT: 6.487 min Scan# 765
Delta R.T. -0.005 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 45 Resp: 41069
Ion Ratio Lower Upper
45 100
43 48.1 46.6 70.0
87 26.9 24.3 36.5
59 13.1 9.6 14.4


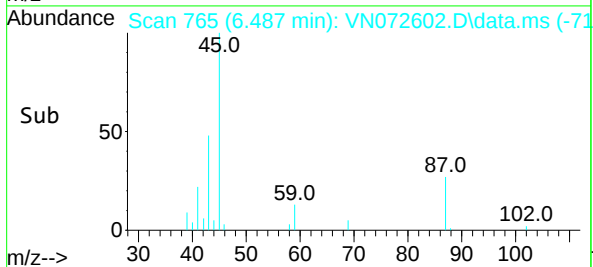

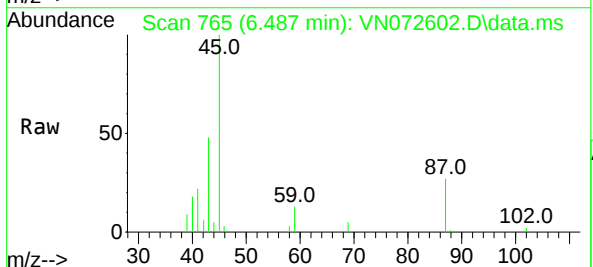




#23
 Vinyl Acetate
 Concen: 4.392 ug/l
 RT: 6.493 min Scan# 71
 Delta R.T. 0.065 min
 Lab File: VN072602.D
 Acq: 24 May 2022 21:43




Instrument :
 MSVOA_N
 ClientSampleId :
 MW-40


Tgt Ion: 43 Resp: 20508
 Ion Ratio Lower Upper
 43 100
 86 0.0 10.0 15.0#

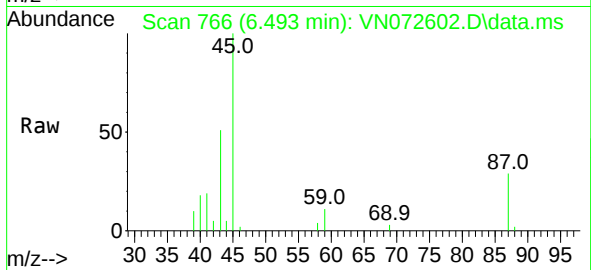

#25
 2-Butanone
 Concen: 0.544 ug/l
 RT: 7.334 min Scan# 909
 Delta R.T. 0.006 min
 Lab File: VN072602.D
 Acq: 24 May 2022 21:43

Tgt Ion: 43 Resp: 810
 Ion Ratio Lower Upper
 43 100
 72 0.0 23.7 35.5#

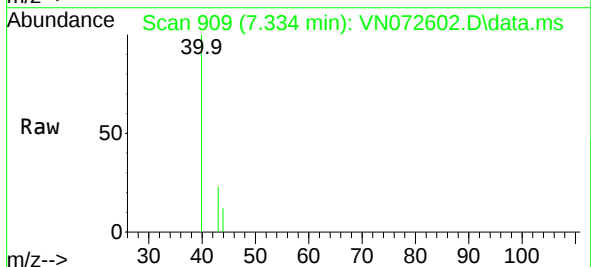



#29

Tetrahydrofuran

Concen: 0.302 ug/l

RT: 7.675 min Scan# 9

Delta R.T. -0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion: 42 Resp: 280

Ion Ratio Lower Upper

42 100

72 0.0 39.7 59.5#

71 23.9 36.6 55.0#

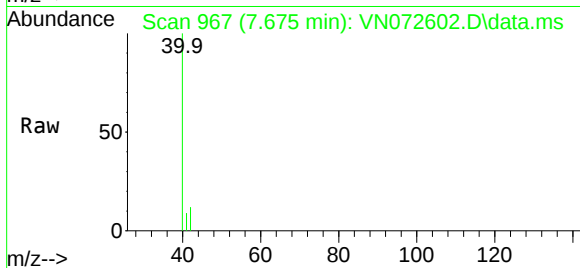

#31

Cyclohexane

Concen: 1.766 ug/l

RT: 8.092 min Scan# 1038

Delta R.T. 0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 56 Resp: 5021


Ion Ratio Lower Upper

56 100

69 82.4 27.8 41.8#

84 74.8 76.9 115.3#

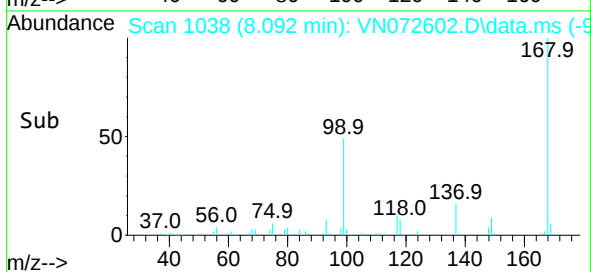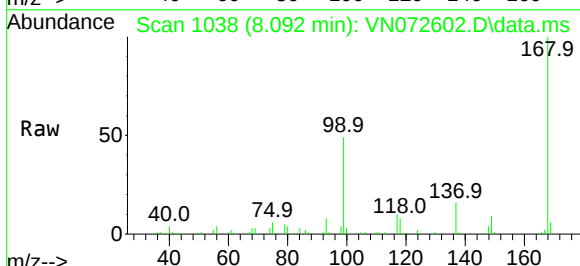

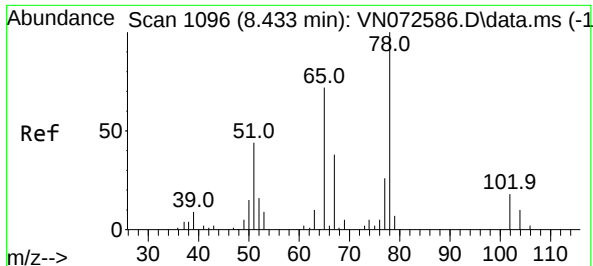

#33

1,2-Dichloroethane-d4

Concen: 52.891 ug/l

RT: 8.434 min Scan# 1109

Delta R.T. 0.001 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion: 65 Resp: 94919

Ion Ratio Lower Upper

65 100

67 52.9 0.0 104.8

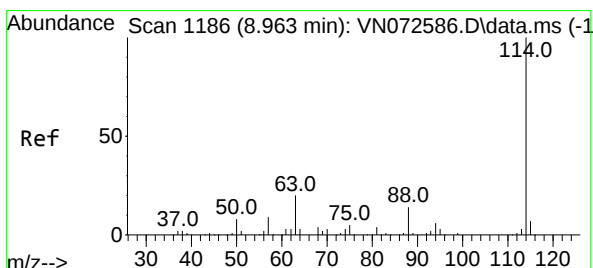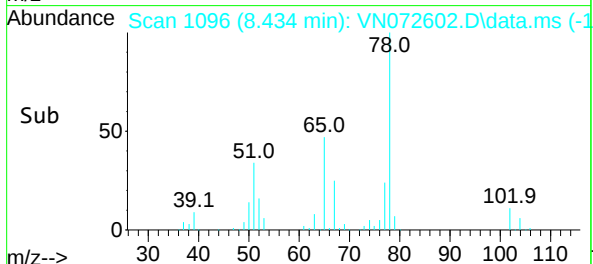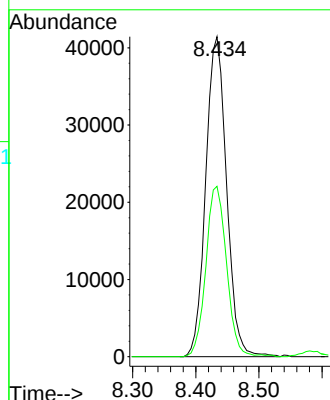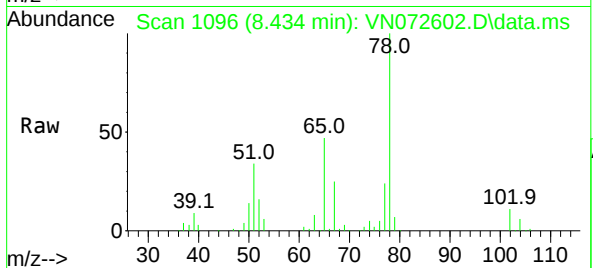

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. -0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 114 Resp: 294065


Ion Ratio Lower Upper

114 100

63 21.4 0.0 40.0

88 15.5 0.0 32.6

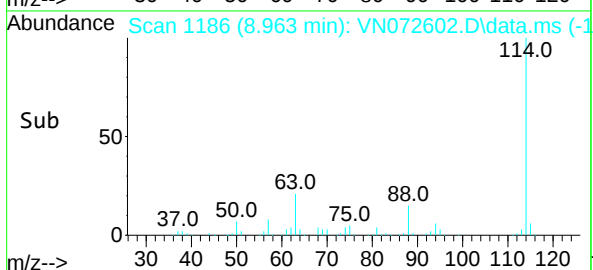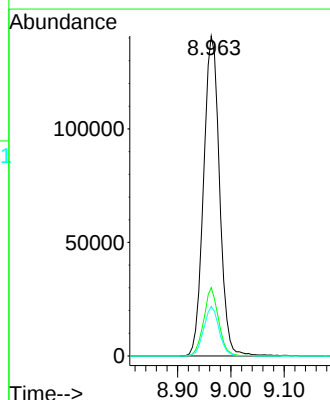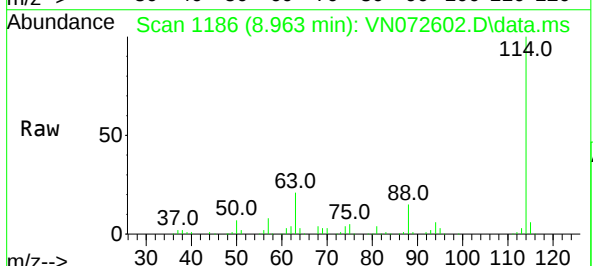

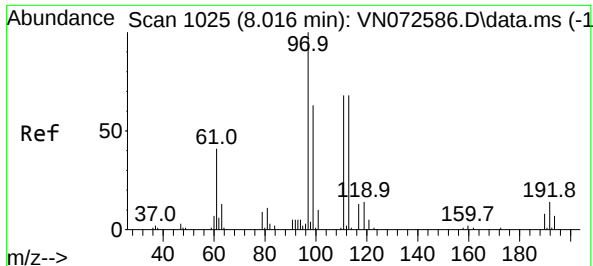

#35

Dibromofluoromethane

Concen: 44.733 ug/l

RT: 8.016 min Scan# 1035

Delta R.T. 0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion:113 Resp: 85258

Ion Ratio Lower Upper

113 100

111 103.0 81.4 122.0

192 21.8 17.0 25.6

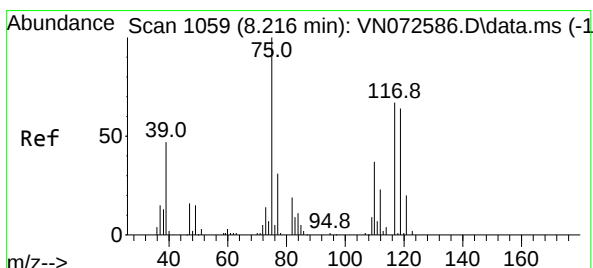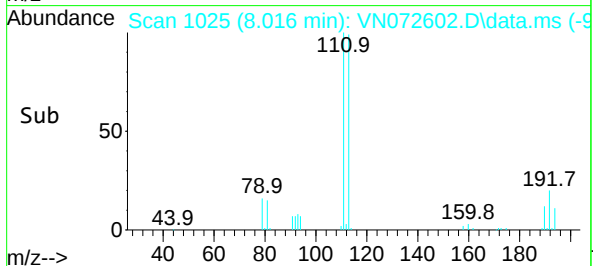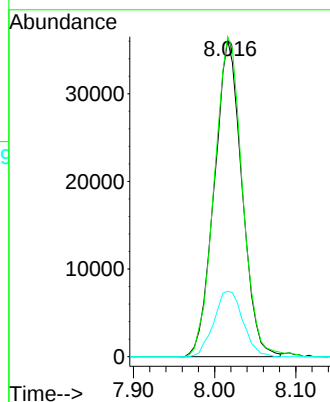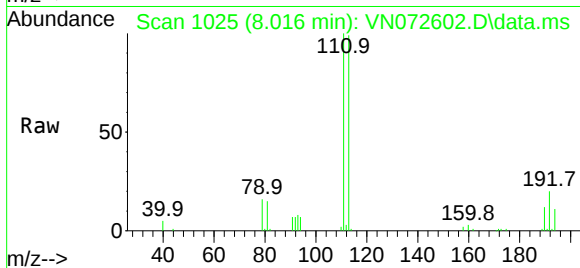

#36

1,1-Dichloropropene

Concen: 3.957 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.135 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 75 Resp: 10670


Ion Ratio Lower Upper

75 100

110 4.7 18.3 54.8#

77 0.0 25.1 37.7#

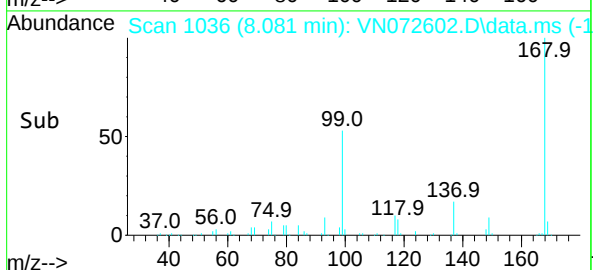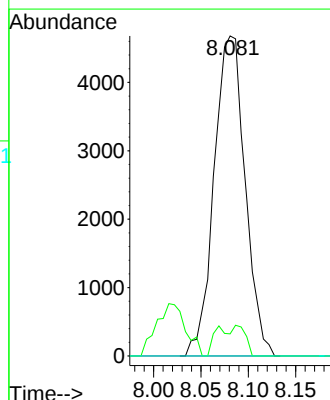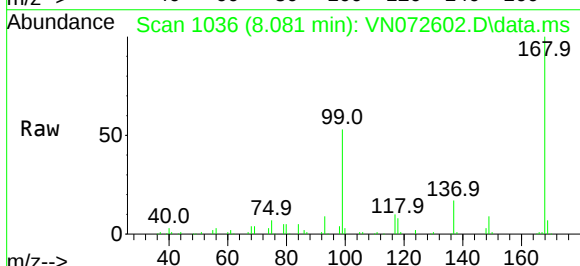



#37

Ethyl Acetate

Concen: 0.230 ug/l

RT: 7.334 min Scan# 90

Delta R.T. -0.070 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion: 43 Resp: 810

Ion Ratio Lower Upper

43 100

61 0.0 11.8 17.6#

70 0.0 9.3 13.9#

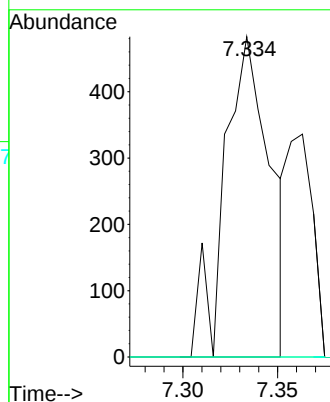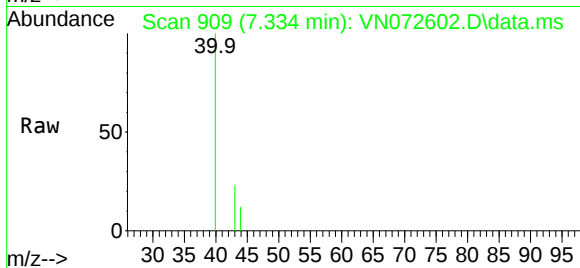

#38

Carbon Tetrachloride

Concen: 5.335 ug/l

RT: 8.081 min Scan# 1036

Delta R.T. -0.117 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 117 Resp: 15184


Ion Ratio Lower Upper

117 100

119 6.0 75.8 113.8#

121 0.0 24.6 37.0#

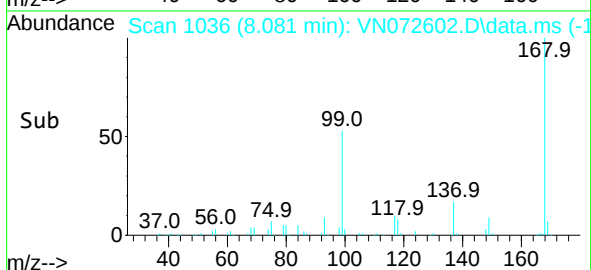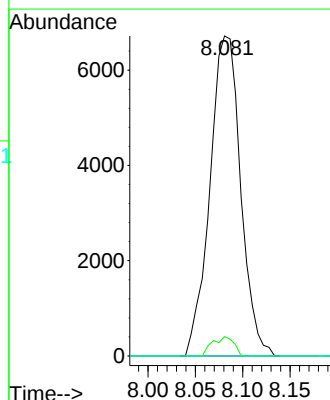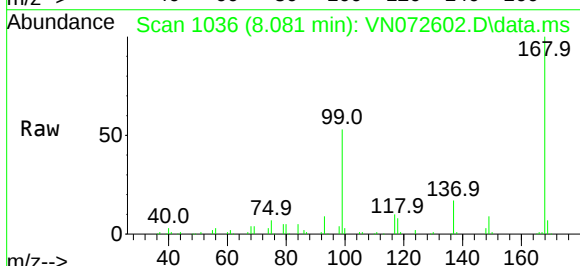

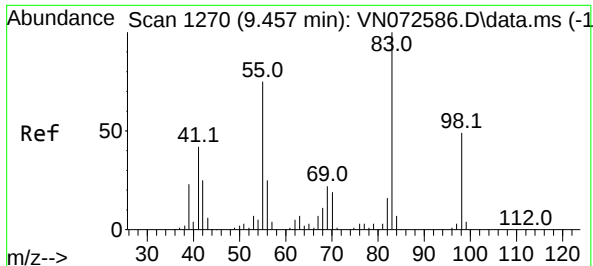

#39

Methylcyclohexane

Concen: 0.362 ug/l

RT: 9.457 min Scan# 1100

Delta R.T. 0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion: 83 Resp: 1203

Ion Ratio Lower Upper

83 100

55 66.9 57.8 86.8

98 66.3 39.4 59.2#

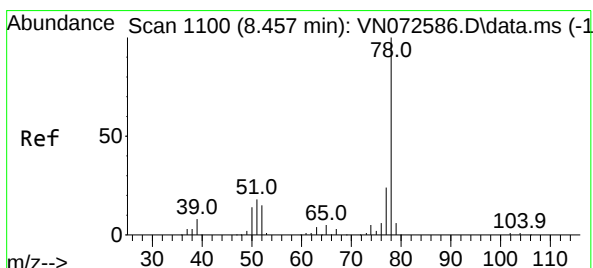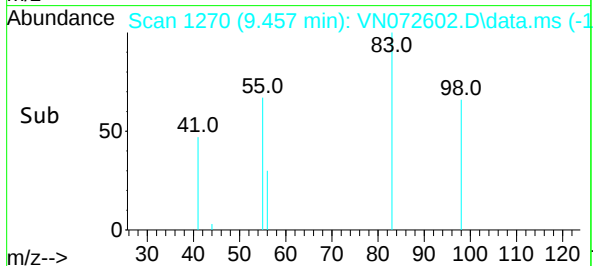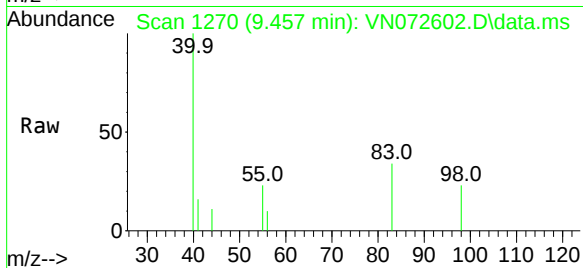

#40

Benzene

Concen: 71.075 ug/l

RT: 8.457 min Scan# 1100

Delta R.T. 0.000 min

Lab File: VN072602.D




Acq: 24 May 2022 21:43


Tgt Ion: 78 Resp: 618426

Ion Ratio Lower Upper

78 100

77 24.3 19.4 29.0

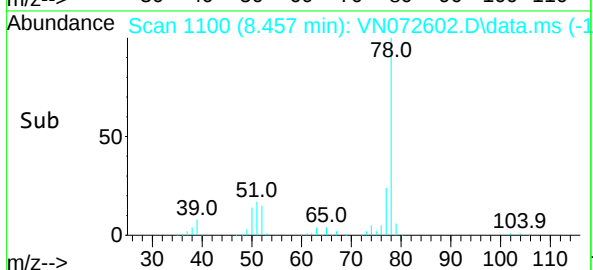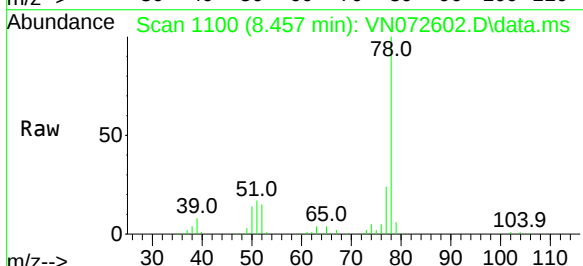

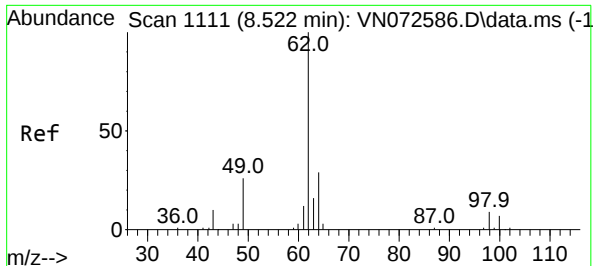

#42

1,2-Dichloroethane

Concen: 1.624 ug/l

RT: 8.451 min Scan# 1109

Delta R.T. -0.071 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion: 62 Resp: 4578

Ion Ratio Lower Upper

62 100

98 1.4 0.0 19.4

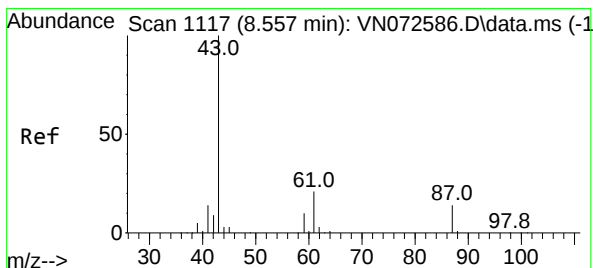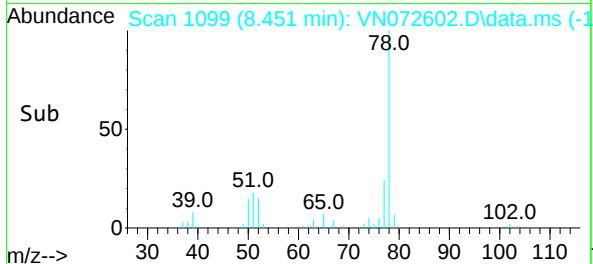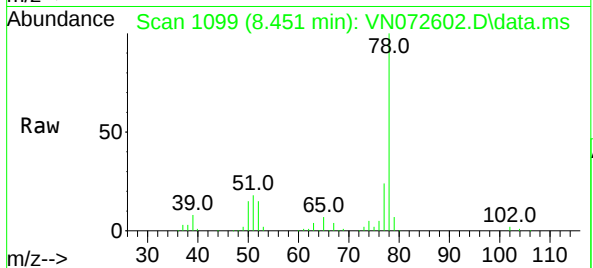

#43

Isopropyl Acetate

Concen: 0.539 ug/l

RT: 8.528 min Scan# 1112

Delta R.T. -0.029 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 43 Resp: 2695


Ion Ratio Lower Upper

43 100

61 0.0 21.9 32.9#

87 0.0 12.0 18.0#


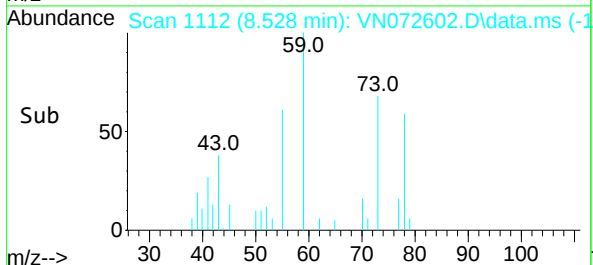
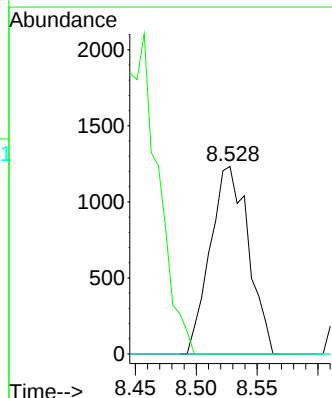
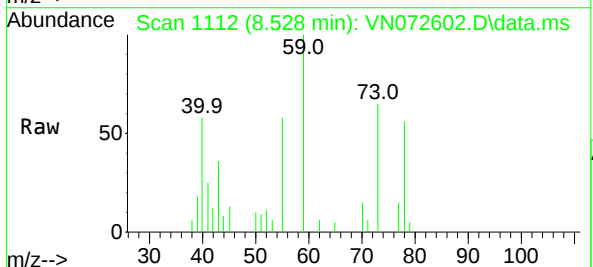


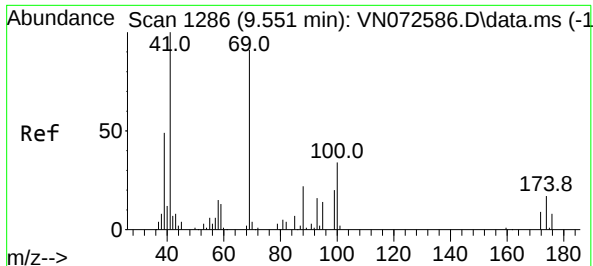

#48
Methyl methacrylate
Concen: 0.236 ug/l
RT: 9.451 min Scan# 1286
Delta R.T. -0.100 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 41 Resp: 573
Ion Ratio Lower Upper
41 100
69 9.4 74.7 112.1#
39 9.9 45.6 68.4#

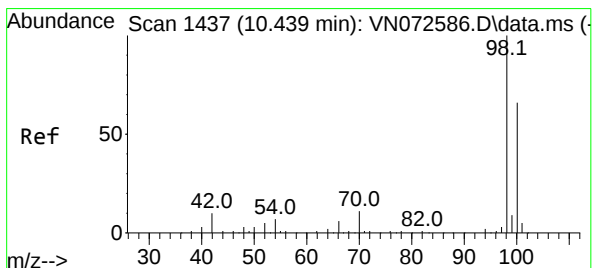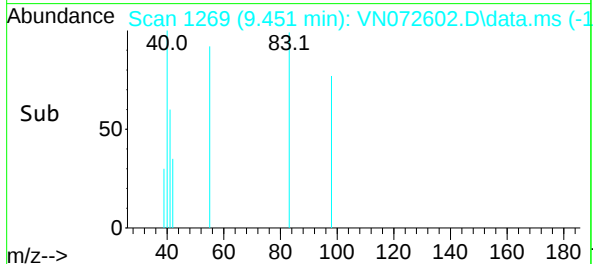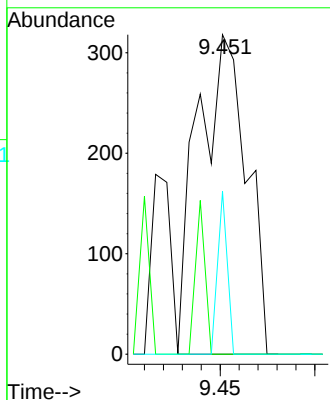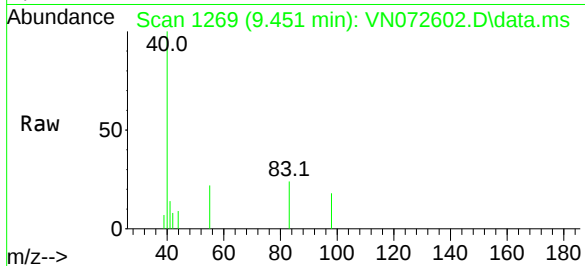

#50
Toluene-d8
Concen: 51.340 ug/l
RT: 10.439 min Scan# 1437
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 98 Resp: 373621
Ion Ratio Lower Upper
98 100
100 65.4 52.6 78.8


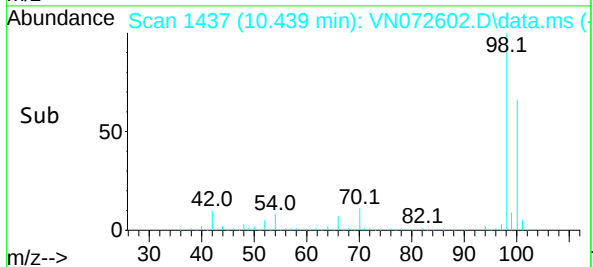
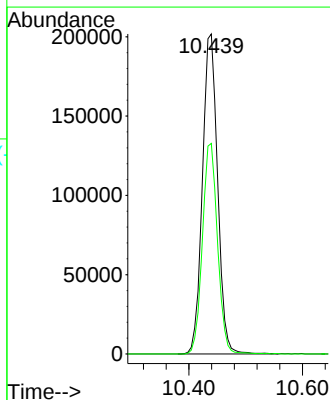
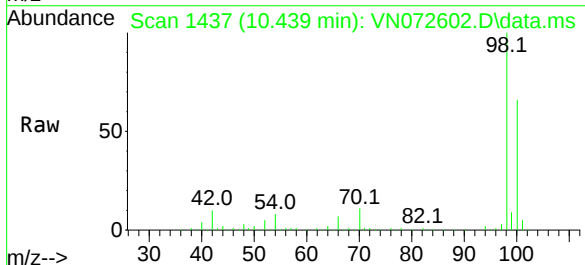




#52
Toluene
Concen: 0.465 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 92 Resp: 2560
Ion Ratio Lower Upper
92 100
91 154.4 138.6 207.8

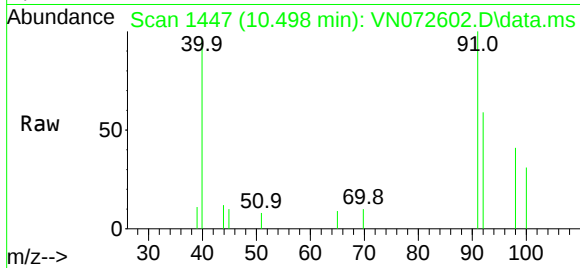

#59
2-Hexanone
Concen: 1.337 ug/l
RT: 11.122 min Scan# 1553
Delta R.T. 0.042 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 43 Resp: 3243
Ion Ratio Lower Upper
43 100
58 46.1 29.7 89.1


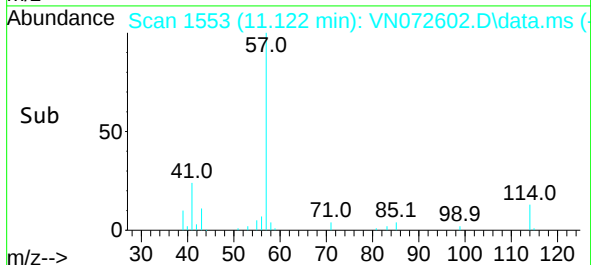

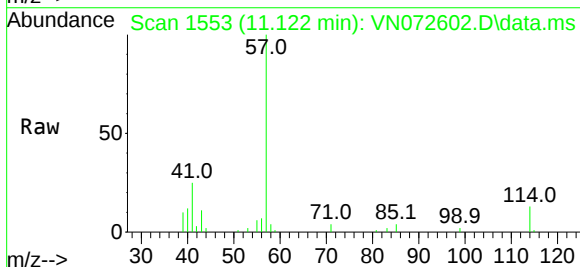


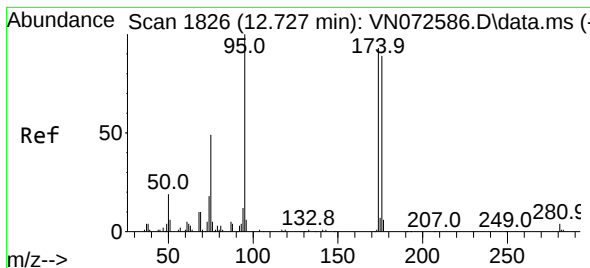

#62
4-Bromofluorobenzene
Concen: 60.883 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 95 Resp: 144105
Ion Ratio Lower Upper
95 100
174 88.7 0.0 167.6
176 85.3 0.0 163.4

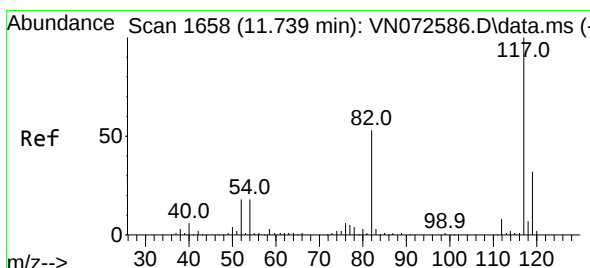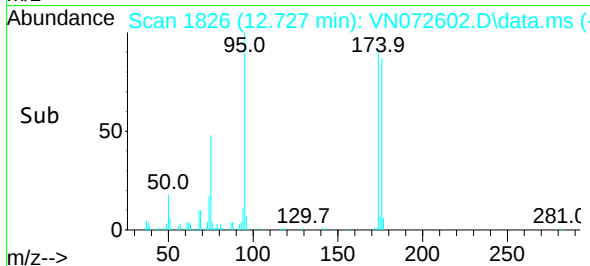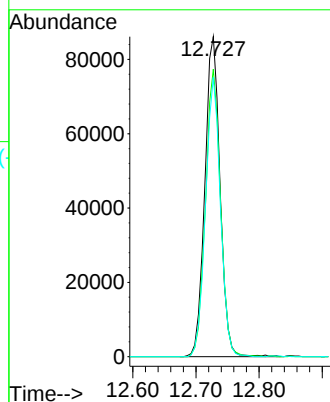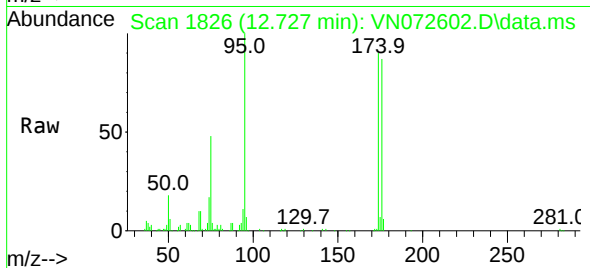

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 117 Resp: 338955
Ion Ratio Lower Upper
117 100
82 51.4 44.2 66.2
119 31.5 25.4 38.0


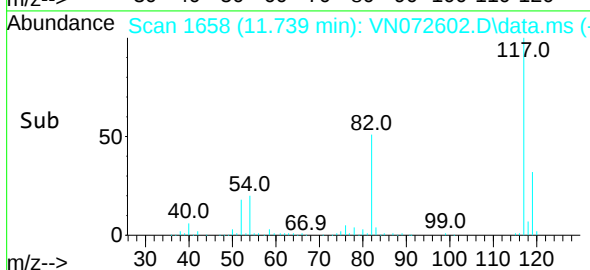
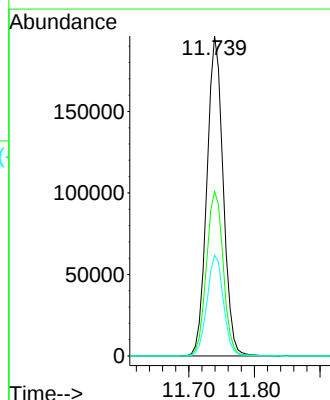
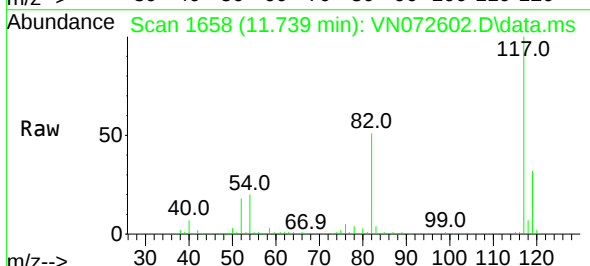


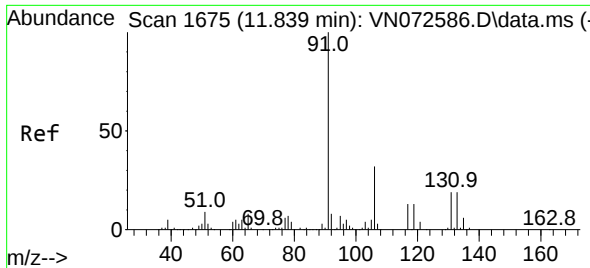

#67
Ethyl Benzene
Concen: 0.403 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 91 Resp: 5208
Ion Ratio Lower Upper
91 100
106 36.7 24.9 37.3

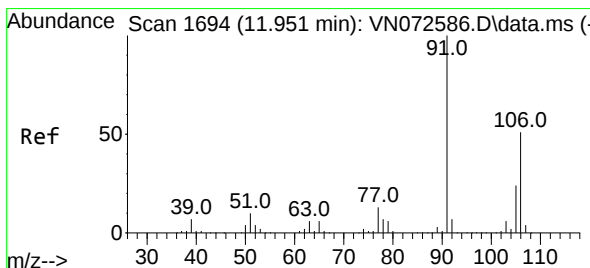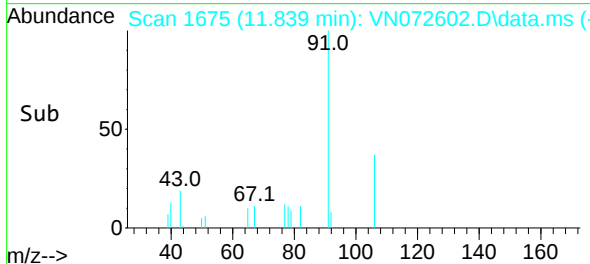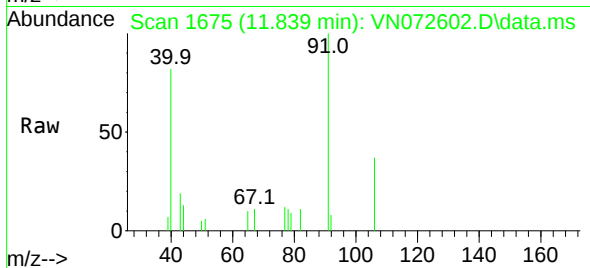

#68
m/p-Xylenes
Concen: 0.326 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. 0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion: 106 Resp: 1603
Ion Ratio Lower Upper
106 100
91 201.8 158.9 238.3

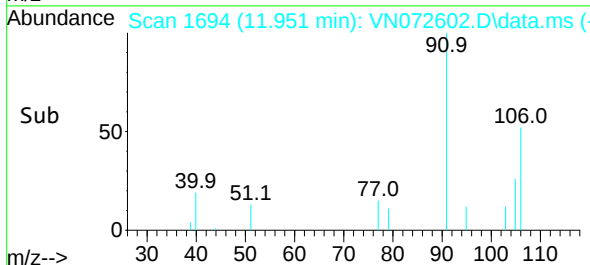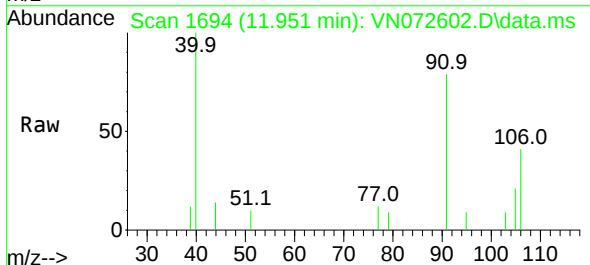



#69

o-Xylene

Concen: 0.563 ug/l

RT: 12.275 min Scan# 11

Delta R.T. 0.001 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion:106 Resp: 2679

Ion Ratio Lower Upper

106 100

91 229.3 106.0 318.0

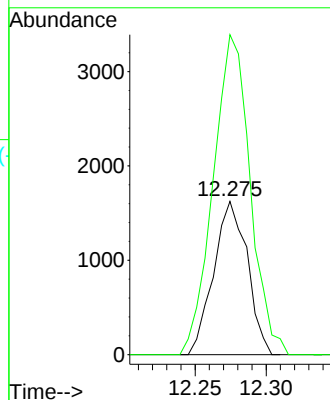

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.669 min Scan# 1986

Delta R.T. 0.001 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion:152 Resp: 129847


Ion Ratio Lower Upper

152 100

115 55.9 28.9 86.7

150 158.0 0.0 356.2

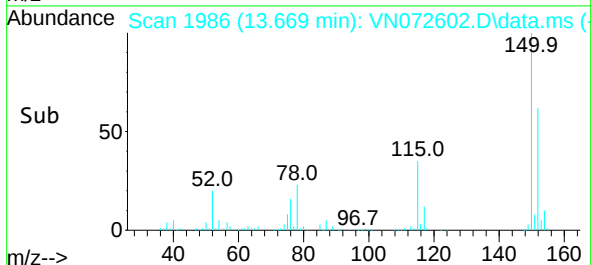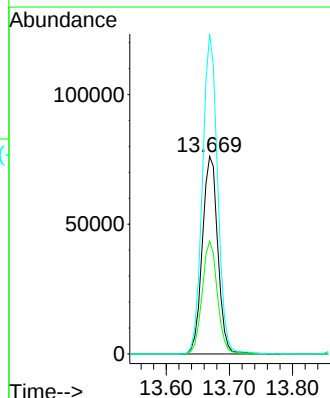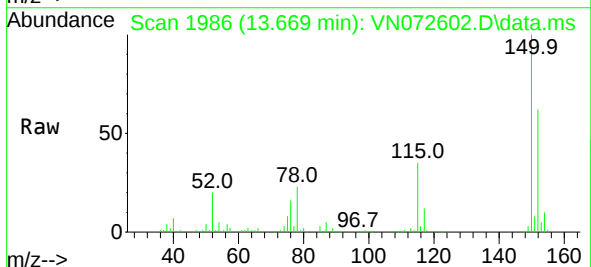



#73

Isopropylbenzene

Concen: 0.466 ug/l

RT: 12.575 min Scan# 1800

Delta R.T. 0.001 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion:105 Resp: 5386

Ion Ratio Lower Upper

105 100

120 27.7 13.5 40.4

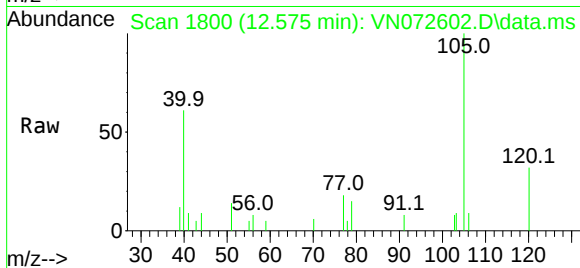

#76

1,2,3-Trichloropropane

Concen: 19.814 ug/l

RT: 12.727 min Scan# 1826

Delta R.T. -0.147 min

Lab File: VN072602.D




Acq: 24 May 2022 21:43


Tgt Ion: 75 Resp: 69849

Ion Ratio Lower Upper

75 100

77 0.9 98.5 295.5#

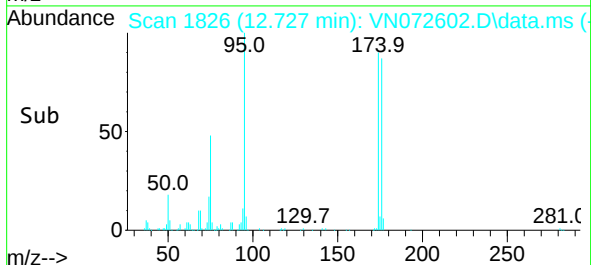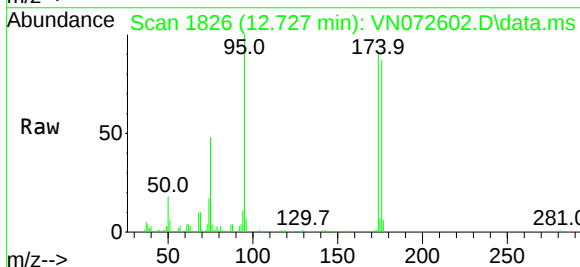

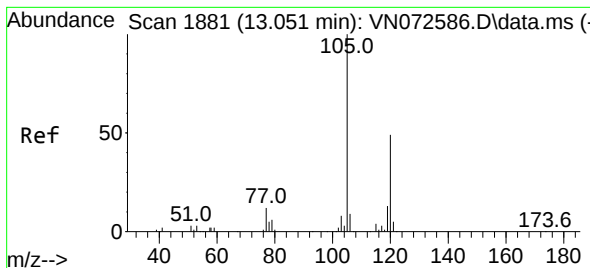

#80

1,3,5-Trimethylbenzene

Concen: 0.270 ug/l

RT: 13.051 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion:105 Resp: 2427

Ion Ratio Lower Upper

105 100

120 43.9 24.9 74.7

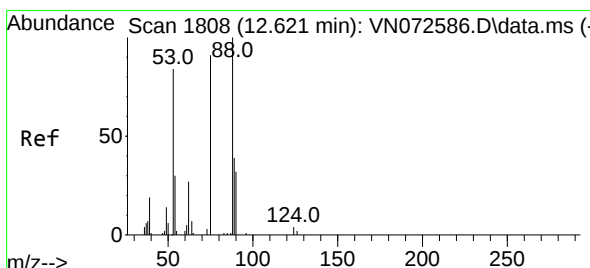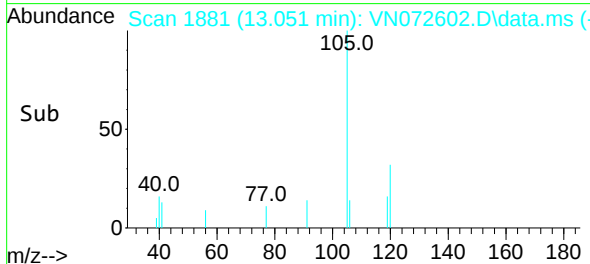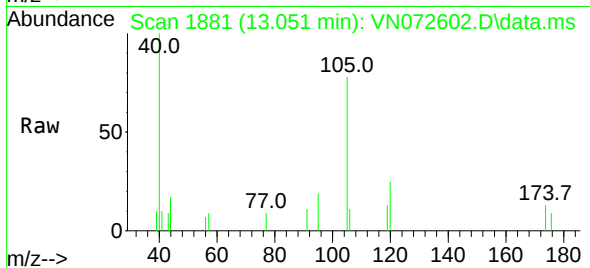

#81

trans-1,4-Dichloro-2-butene

Concen: 58.146 ug/l

RT: 12.727 min Scan# 1826

Delta R.T. 0.106 min

Lab File: VN072602.D

Acq: 24 May 2022 21:43




Tgt Ion: 75 Resp: 69849


Ion Ratio Lower Upper

75 100

53 0.0 78.0 117.0#

89 0.0 37.2 55.8#


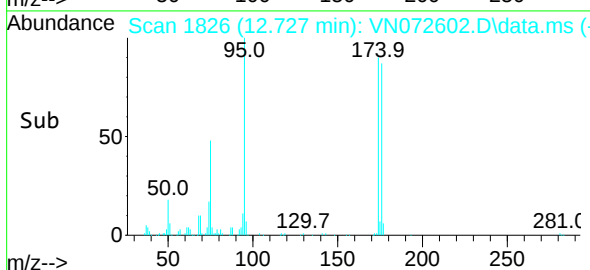

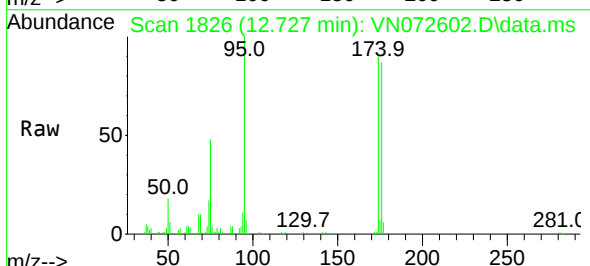




#84
1,2,4-Trimethylbenzene
Concen: 0.475 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Tgt Ion:105 Resp: 4192
Ion Ratio Lower Upper
105 100
120 41.5 23.3 69.8

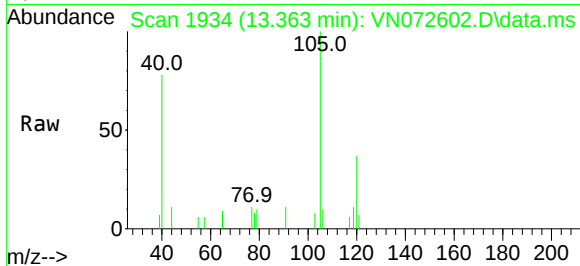

#90
Hexachloroethane
Concen: 0.279 ug/l
RT: 14.269 min Scan# 2088
Delta R.T. 0.065 min
Lab File: VN072602.D
Acq: 24 May 2022 21:43

Tgt Ion:117 Resp: 488
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#

