

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
 Data File : VN072614.D
 Acq On : 25 May 2022 02:34
 Operator : JC\MD
 Sample : VN0524WBSD02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0524WBSD02

Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/25/2022
 Supervised By : Mahesh Dadoda 05/25/2022

Quant Time: May 25 09:26:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 25 09:15:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.710	168	166007m	50.000	ug/l	-0.37
34) 1,4-Difluorobenzene	8.710	114	267756	50.000	ug/l	-0.25
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.74
72) 1,4-Dichlorobenzene-d4	13.663	152	58170	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.098	65	101895	53.960	ug/l	-0.33
Spiked Amount 50.000	Range 61 - 141		Recovery = 107.920%			
35) Dibromofluoromethane	7.622	113	80890	46.612	ug/l	-0.39
Spiked Amount 50.000	Range 69 - 133		Recovery = 93.220%			
50) Toluene-d8	10.316	98	275167	41.526	ug/l	-0.12
Spiked Amount 50.000	Range 65 - 126		Recovery = 83.060%			
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount 50.000	Range 58 - 135		Recovery = 0.000%#			
Target Compounds						
3) Chloromethane	2.358	50	259	Below Cal	#	43
7) Trichlorofluoromethane	3.193	101	26703	10.213	ug/l	95
8) Diethyl Ether	3.840	74	11216	11.120	ug/l #	12
14) Allyl chloride	4.657	41	20490	7.525	ug/l #	24
16) Acetone	4.375	43	4821	5.194	ug/l #	42
18) Methyl Acetate	4.640	43	18940	7.074	ug/l #	67
25) 2-Butanone	7.193	43	21996	14.045	ug/l #	1
28) Bromochloromethane	7.169	49	24389	18.945	ug/l	95
29) Tetrahydrofuran	7.198	42	97036	99.578	ug/l	93
30) Chloroform	7.369	83	58172	17.734	ug/l	99
31) Cyclohexane	7.687	56	54137	18.098	ug/l	97
32) 1,1,1-Trichloroethane	7.593	97	51928	18.901	ug/l	98
36) 1,1-Dichloropropene	7.840	75	47366	19.292	ug/l	99
37) Ethyl Acetate	7.193	43	21996	6.853	ug/l #	70
38) Carbon Tetrachloride	7.822	117	48198	18.598	ug/l	92
39) Methylcyclohexane	9.245	83	55794	18.442	ug/l	96
40) Benzene	8.116	78	155892	19.677	ug/l	97
41) Methacrylonitrile	7.198	41	56615	35.059	ug/l #	33
42) 1,2-Dichloroethane	8.204	62	48862	19.036	ug/l	99
43) Isopropyl Acetate	8.263	43	96404	21.183	ug/l #	90
44) Trichloroethene	8.981	130	38100	18.703	ug/l	98
45) 1,2-Dichloropropane	9.281	63	39679	19.300	ug/l	97
46) Dibromomethane	9.375	93	25735	18.754	ug/l	98
47) Bromodichloromethane	9.586	83	49567	18.536	ug/l	100
48) Methyl methacrylate	9.245	41	22717	10.262	ug/l #	72
49) 1,4-Dioxane	9.381	88	19106	452.210	ug/l	95
51) 4-Methyl-2-Pentanone	10.204	43	264167	84.789	ug/l	94
52) Toluene	10.386	92	71944	14.340	ug/l	99
53) t-1,3-Dichloropropene	10.616	75	33395	12.217	ug/l	94
54) cis-1,3-Dichloropropene	10.051	75	47020	15.276	ug/l	95
55) 1,1,2-Trichloroethane	10.804	97	23984	11.523	ug/l	94
56) Ethyl methacrylate	10.669	69	38051	11.868	ug/l #	81
57) 1,3-Dichloropropane	10.957	76	42137	12.011	ug/l	98
58) 2-Chloroethyl Vinyl ether	9.898	63	122708	89.446	ug/l	95
59) 2-Hexanone	11.010	43	152604	69.092	ug/l	90
60) Dibromochloromethane	11.157	129	25145	11.286	ug/l	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
 Data File : VN072614.D
 Acq On : 25 May 2022 02:34
 Operator : JC\MD
 Sample : VN0524WBSD02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0524WBSD02


Manual Integrations
 APPROVED

Reviewed By : John Carlone 05/25/2022
 Supervised By : Mahesh Dadoda 05/25/2022

Quant Time: May 25 09:26:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 25 09:15:20 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
61) 1,2-Dibromoethane	11.269	107	24834	11.444	ug/l	98
73) Isopropylbenzene	12.545	105	106887	20.628	ug/l	99
74) N-amyl acetate	12.357	43	45493	24.460	ug/l	90
75) 1,1,2,2-Tetrachloroethane	12.798	83	36573	19.987	ug/l	97
76) 1,2,3-Trichloropropane	12.857	75	44335	28.073	ug/l #	1
77) Bromobenzene	12.827	156	24353	18.946	ug/l	94
78) n-propylbenzene	12.892	91	116483	20.274	ug/l	97
79) 2-Chlorotoluene	12.980	91	70058	19.738	ug/l	99
80) 1,3,5-Trimethylbenzene	13.039	105	80801	20.048	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.598	75	10422	19.366	ug/l	95
82) 4-Chlorotoluene	13.080	91	64681	19.927	ug/l	96
83) tert-Butylbenzene	13.304	119	77479	20.644	ug/l	99
84) 1,2,4-Trimethylbenzene	13.345	105	79180	20.034	ug/l	100
85) sec-Butylbenzene	13.480	105	100706	20.065	ug/l	97
86) p-Isopropyltoluene	13.598	119	77465	19.575	ug/l	99
87) 1,3-Dichlorobenzene	13.598	146	39831	18.360	ug/l	96
88) 1,4-Dichlorobenzene	13.674	146	40385	18.974	ug/l	98
89) n-Butylbenzene	13.927	91	57641	18.052	ug/l	97
90) Hexachloroethane	14.198	117	16215	20.726	ug/l	94
91) 1,2-Dichlorobenzene	13.974	146	38849	18.694	ug/l	98
92) 1,2-Dibromo-3-Chloropr...	14.592	75	6534	20.947	ug/l	95
93) 1,2,4-Trichlorobenzene	15.257	180	20244	18.494	ug/l	99
94) Hexachlorobutadiene	15.363	225	10844	16.788	ug/l	98
95) Naphthalene	15.498	128	72985	20.161	ug/l	99
96) 1,2,3-Trichlorobenzene	15.692	180	20997	17.916	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

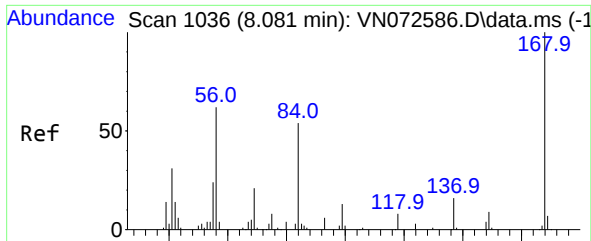

#1
Pentafluorobenzene
Concen: 50.000 ug/l m
RT: 7.710 min Scan# 91
Delta R.T. -0.371 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

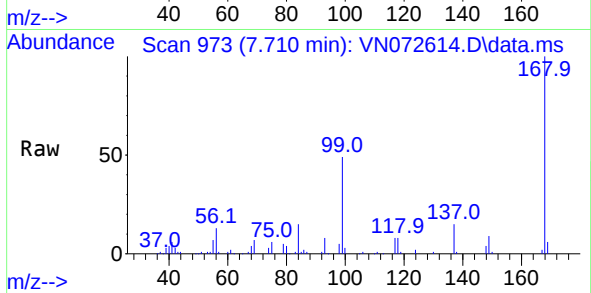

Tgt Ion:168 Resp: 16600
Ion Ratio Lower Upper
168 100
99 49.4 42.3 63.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

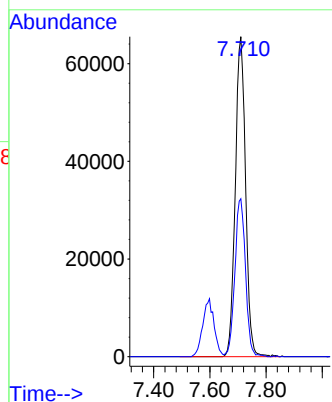

#3
Chloromethane
Concen: Below Cal
RT: 2.358 min Scan# 63
Delta R.T. 0.065 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 50 Resp: 259
Ion Ratio Lower Upper
50 100
52 0.0 25.7 38.5#

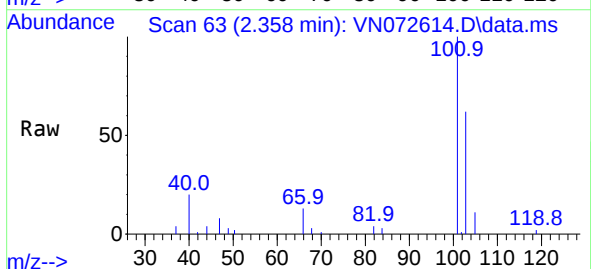







#7
Trichlorofluoromethane
Concen: 10.213 ug/l
RT: 3.193 min Scan# 205
Delta R.T. -0.164 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion:101 Resp: 2670
Ion Ratio Lower Upper
101 100
103 60.5 51.5 77.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

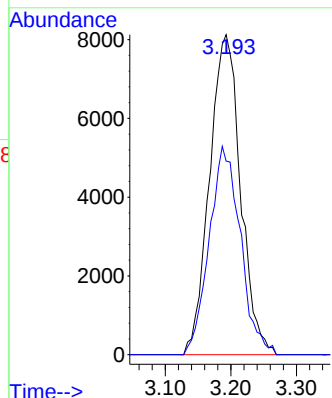

#8
Diethyl Ether
Concen: 11.120 ug/l
RT: 3.840 min Scan# 315
Delta R.T. 0.018 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 74 Resp: 11216
Ion Ratio Lower Upper
74 100
45 4.6 42.9 128.5#

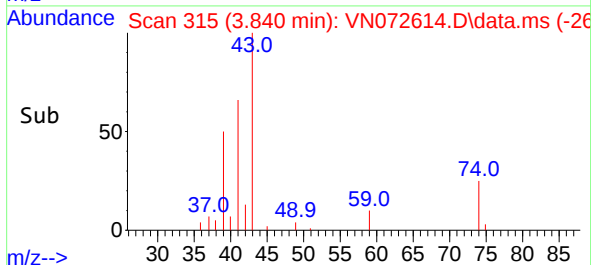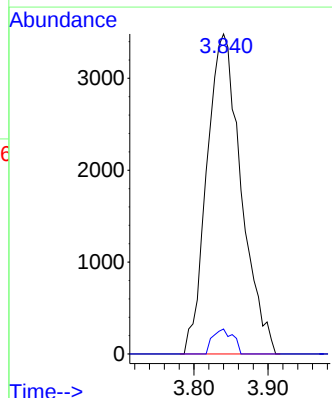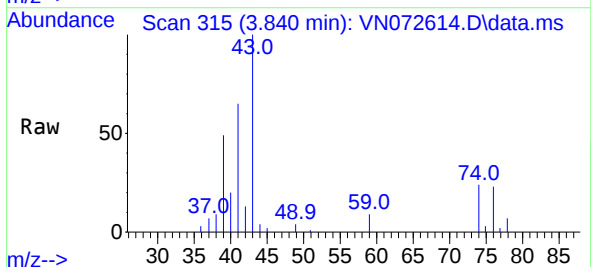



#14

Allyl chloride

Concen: 7.525 ug/l

RT: 4.657 min Scan# 41

Delta R.T. -0.177 min

Lab File: VN072614.D

Acq: 25 May 2022 02:34

Instrument :

MSVOA_N

ClientSampleId :

VN0524WBSD02





Tgt Ion: 41 Resp: 20490
 Ion Ratio Lower Upper
 41 100
 39 0.0 53.2 79.8
 76 0.0 29.9 44.9

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2022

Supervised By :Mahesh Dadoda 05/25/2022



#16

Acetone

Concen: 5.194 ug/l




RT: 4.375 min Scan# 406


Delta R.T. 0.100 min

Lab File: VN072614.D

Acq: 25 May 2022 02:34


Tgt Ion: 43 Resp: 4821
 Ion Ratio Lower Upper
 43 100
 58 0.0 26.0 39.0

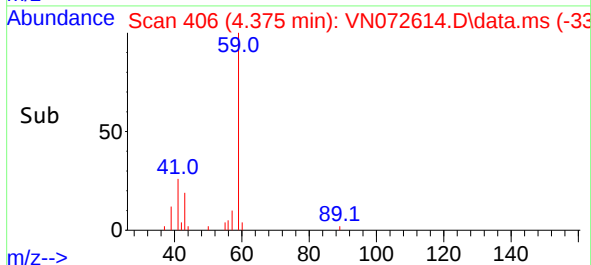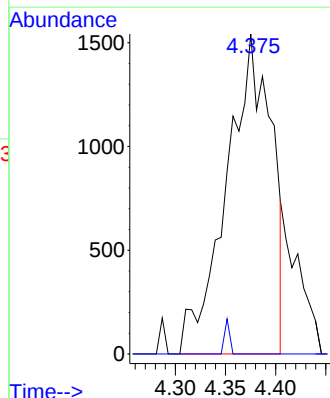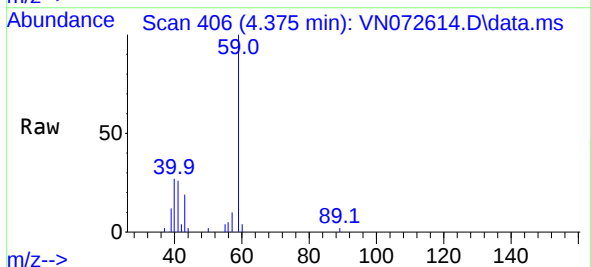



#18
Methyl Acetate
Concen: 7.074 ug/l
RT: 4.640 min Scan# 41
Delta R.T. -0.205 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 43 Resp: 18940
Ion Ratio Lower Upper
43 100
74 10.0 21.6 32.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

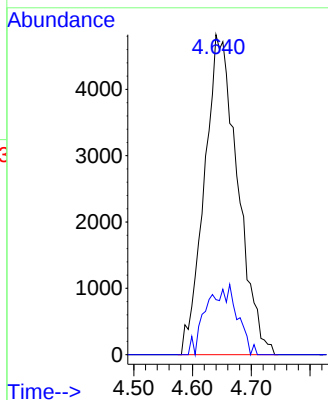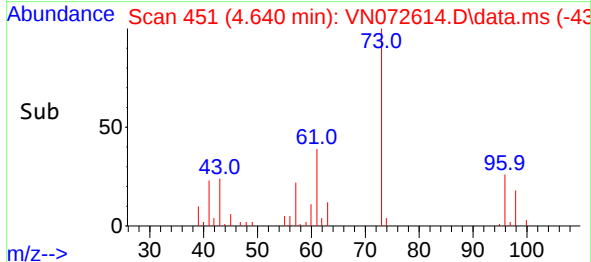


#25
2-Butanone
Concen: 14.045 ug/l
RT: 7.193 min Scan# 885
Delta R.T. -0.135 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 43 Resp: 21996
Ion Ratio Lower Upper
43 100
72 190.5 23.7 35.5

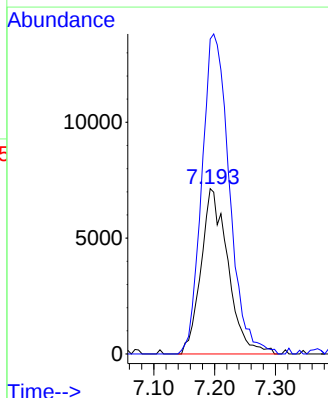



#28
Bromochloromethane
Concen: 18.945 ug/l
RT: 7.169 min Scan# 881
Delta R.T. -0.482 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 49 Resp: 24389
Ion Ratio Lower Upper
49 100
129 0.8 0.0 4.6
130 82.4 69.7 104.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

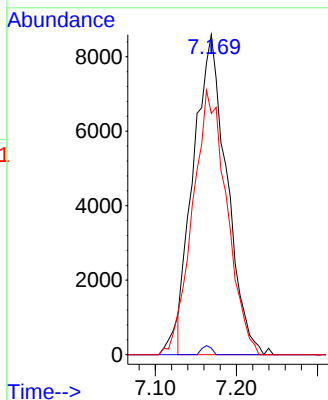


#29
Tetrahydrofuran
Concen: 99.578 ug/l
RT: 7.198 min Scan# 886
Delta R.T. -0.477 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 42 Resp: 97036
Ion Ratio Lower Upper
42 100
72 44.5 39.7 59.5
71 41.4 36.6 55.0

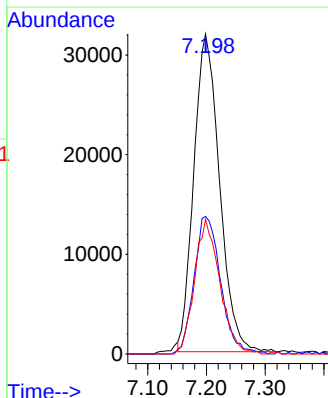



#30
Chloroform
Concen: 17.734 ug/l
RT: 7.369 min Scan# 911
Delta R.T. -0.441 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 83 Resp: 58172
Ion Ratio Lower Upper
83 100
85 65.2 51.8 77.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#31
Cyclohexane
Concen: 18.098 ug/l
RT: 7.687 min Scan# 969
Delta R.T. -0.405 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34



Tgt Ion: 56 Resp: 54137
Ion Ratio Lower Upper
56 100
69 35.7 27.8 41.8
84 93.1 76.9 115.3

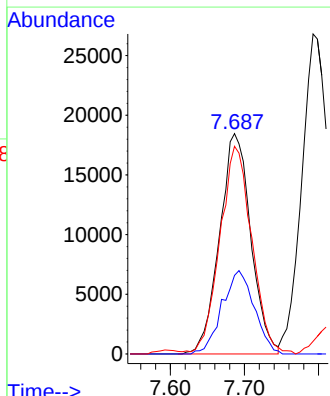



#32
1,1,1-Trichloroethane
Concen: 18.901 ug/l
RT: 7.593 min Scan# 91
Delta R.T. -0.417 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :

MSVOA_N

ClientSampleId :





VN0524WBSD02

Tgt Ion: 97 Resp: 51928
Ion Ratio Lower Upper
97 100
99 64.2 50.6 76.0
61 42.9 36.0 54.0

Manual Integrations




APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#33
1,2-Dichloroethane-d4
Concen: 53.960 ug/l
RT: 8.098 min Scan# 1039
Delta R.T. -0.335 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 65 Resp: 101895
Ion Ratio Lower Upper
65 100
67 53.7 0.0 104.8

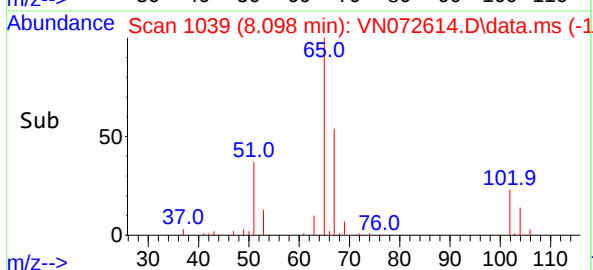







#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.710 min Scan# 1186
Delta R.T. -0.253 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion:114 Resp: 267750
Ion Ratio Lower Upper
114 100
63 19.5 0.0 40.0
88 14.9 0.0 32.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#35
Dibromofluoromethane
Concen: 46.612 ug/l
RT: 7.622 min Scan# 958
Delta R.T. -0.394 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion:113 Resp: 80890
Ion Ratio Lower Upper
113 100
111 102.9 81.4 122.0
192 22.2 17.0 25.6

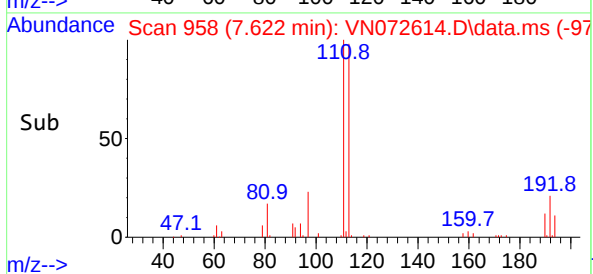




#36
1,1-Dichloropropene
Concen: 19.292 ug/l
RT: 7.840 min Scan# 911
Delta R.T. -0.376 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :

MSVOA_N

ClientSampleId :

VN0524WBSD02






Tgt Ion: 75 Resp: 47360
Ion Ratio Lower Upper
75 100
110 36.1 18.3 54.8
77 31.8 25.1 37.7

Manual Integrations


APPROVED

Reviewed By :John Carlone 05/25/2022



Supervised By :Mahesh Dadoda 05/25/2022

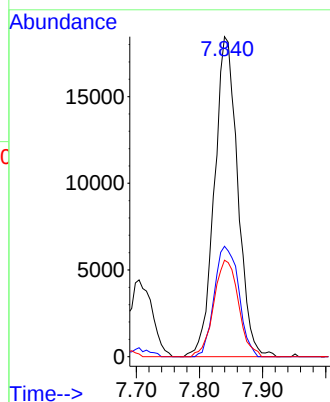


#37
Ethyl Acetate
Concen: 6.853 ug/l
RT: 7.193 min Scan# 885
Delta R.T. -0.211 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 43 Resp: 21996
Ion Ratio Lower Upper
43 100
61 0.0 11.8 17.6#
70 3.2 9.3 13.9#

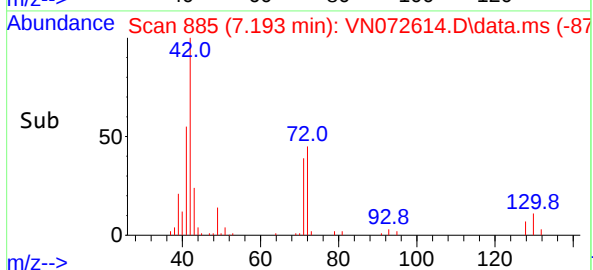



#38
Carbon Tetrachloride
Concen: 18.598 ug/l
RT: 7.822 min Scan# 91
Delta R.T. -0.376 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion:117 Resp: 48198
Ion Ratio Lower Upper
117 100
119 103.6 75.8 113.8
121 29.3 24.6 37.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

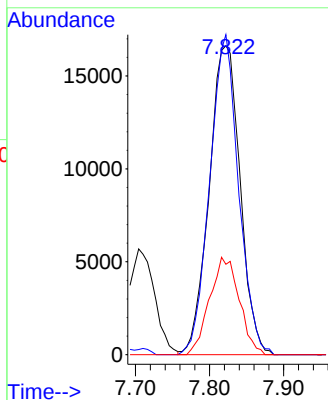


#39
Methylcyclohexane
Concen: 18.442 ug/l
RT: 9.245 min Scan# 1234
Delta R.T. -0.212 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34



Tgt Ion: 83 Resp: 55794
Ion Ratio Lower Upper
83 100
55 78.0 57.8 86.8
98 49.1 39.4 59.2

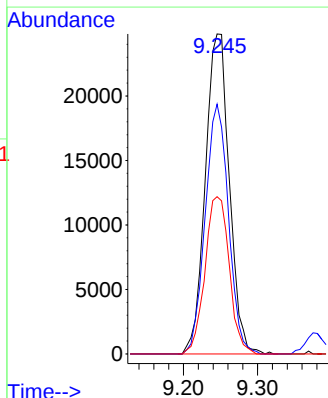







#40
Benzene
Concen: 19.677 ug/l
RT: 8.116 min Scan# 1042
Delta R.T. -0.341 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion: 78 Resp: 155892
Ion Ratio Lower Upper
78 100
77 22.9 19.4 29.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

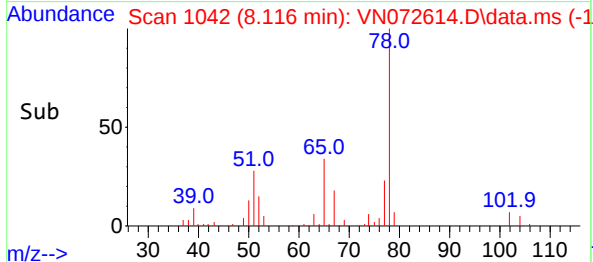

#41
Methacrylonitrile
Concen: 35.059 ug/l
RT: 7.198 min Scan# 886
Delta R.T. -0.436 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 41 Resp: 56615
Ion Ratio Lower Upper
41 100
39 39.7 48.6 73.0#
67 0.0 73.4 110.2#
52 0.0 27.7 41.5#

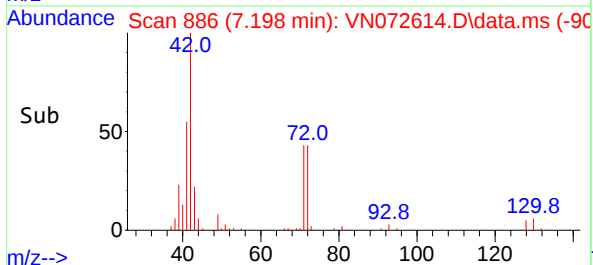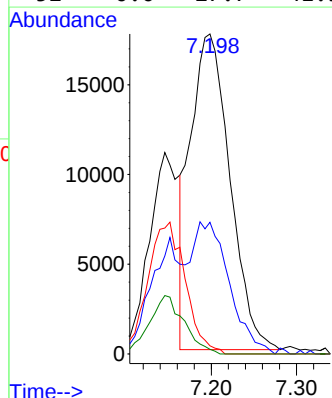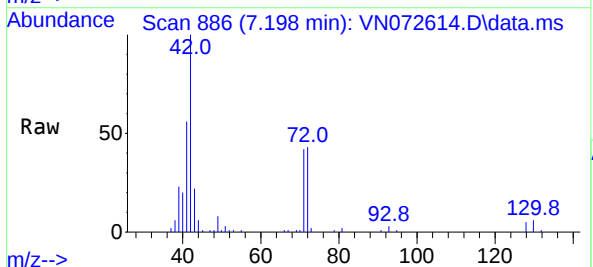



#42

1,2-Dichloroethane

Concen: 19.036 ug/l

RT: 8.204 min Scan# 1057

Delta R.T. -0.318 min

Lab File: VN072614.D

Acq: 25 May 2022 02:34

Instrument :

MSVOA_N

ClientSampleId :

VN0524WBSD02

Tgt Ion: 62 Resp: 48862

Ion Ratio Lower Upper

62 100





98 10.0 0.0 19.4

Manual Integrations

APPROVED

Reviewed By :John Carlone 05/25/2022

Supervised By :Mahesh Dadoda 05/25/2022



#43

Isopropyl Acetate

Concen: 21.183 ug/l

RT: 8.263 min Scan# 1067

Delta R.T. -0.294 min

Lab File: VN072614.D

Acq: 25 May 2022 02:34




Tgt Ion: 43 Resp: 96404


Ion Ratio Lower Upper

43 100

61 20.3 21.9 32.9#


87 13.7 12.0 18.0

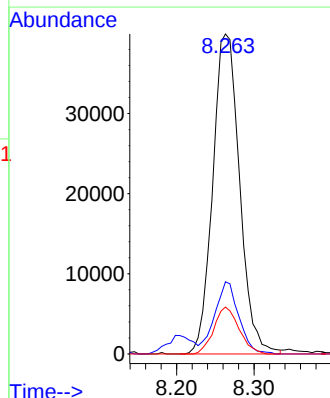



#44
Trichloroethene
Concen: 18.703 ug/l
RT: 8.981 min Scan# 1189
Delta R.T. -0.229 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion:130 Resp: 38100
Ion Ratio Lower Upper
130 100
95 91.3 0.0 186.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#45
1,2-Dichloropropane
Concen: 19.300 ug/l
RT: 9.281 min Scan# 1240
Delta R.T. -0.205 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 63 Resp: 39679
Ion Ratio Lower Upper
63 100
65 29.4 24.9 37.3

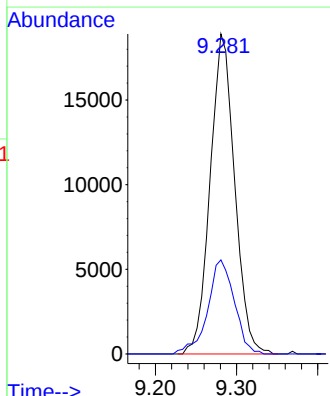



#46
Dibromomethane
Concen: 18.754 ug/l
RT: 9.375 min Scan# 1256
Delta R.T. -0.194 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 93 Resp: 25738
Ion Ratio Lower Upper
93 100
95 84.2 66.9 100.3
174 111.4 86.6 130.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#47
Bromodichloromethane
Concen: 18.536 ug/l
RT: 9.586 min Scan# 1292
Delta R.T. -0.171 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 83 Resp: 49567
Ion Ratio Lower Upper
83 100
85 63.1 50.5 75.7
127 7.6 6.8 10.2

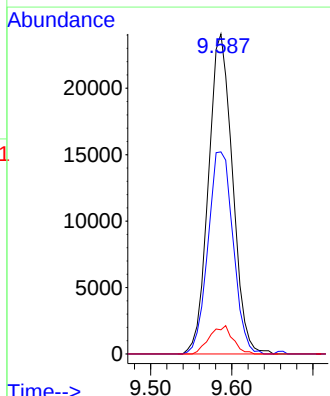



#48
Methyl methacrylate
Concen: 10.262 ug/l
RT: 9.245 min Scan# 1234
Delta R.T. -0.306 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 41 Resp: 2271
Ion Ratio Lower Upper
41 100
69 51.8 74.7 112.1
39 59.3 45.6 68.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

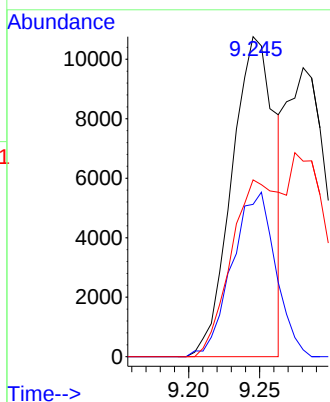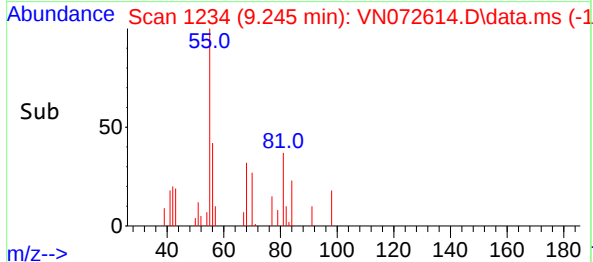


#49
1,4-Dioxane
Concen: 452.210 ug/l
RT: 9.381 min Scan# 1257
Delta R.T. -0.182 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

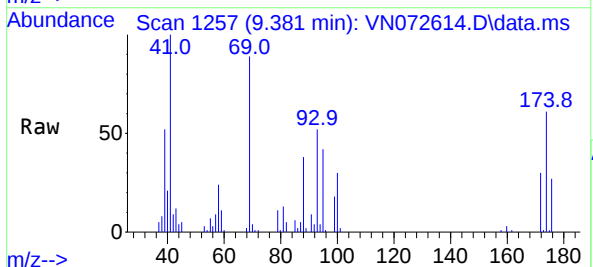

Tgt Ion: 88 Resp: 19106
Ion Ratio Lower Upper
88 100
43 30.3 20.2 30.4
58 65.6 54.2 81.4

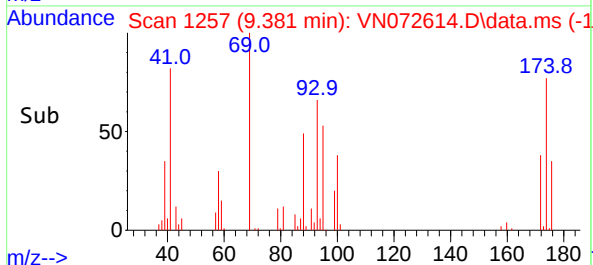







#50
Toluene-d8
Concen: 41.526 ug/l
RT: 10.316 min Scan# 1437
Delta R.T. -0.123 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion: 98 Resp: 275167
Ion Ratio Lower Upper
98 100
100 63.5 52.6 78.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#51
4-Methyl-2-Pentanone
Concen: 84.789 ug/l
RT: 10.204 min Scan# 1397
Delta R.T. -0.123 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion: 43 Resp: 264167
Ion Ratio Lower Upper
43 100
58 38.7 34.1 51.1

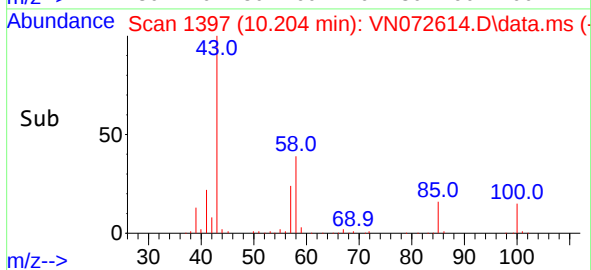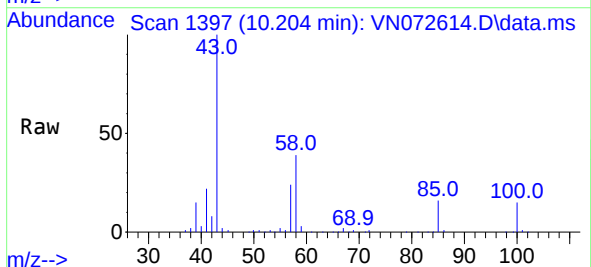



#52
Toluene
Concen: 14.340 ug/l
RT: 10.386 min Scan# 1447
Delta R.T. -0.112 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02



Tgt Ion: 92 Resp: 71944
Ion Ratio Lower Upper
92 100
91 174.0 138.6 207.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

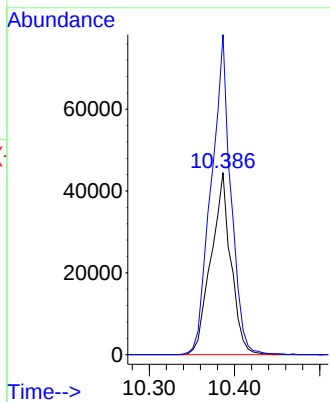

#53
t-1,3-Dichloropropene
Concen: 12.217 ug/l
RT: 10.616 min Scan# 1467
Delta R.T. -0.100 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 75 Resp: 33395
Ion Ratio Lower Upper
75 100
77 28.4 25.6 38.4

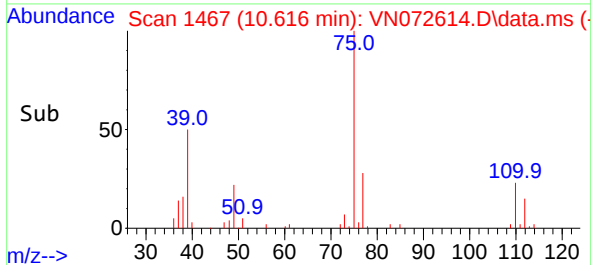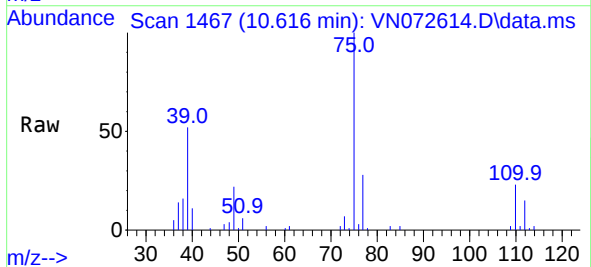

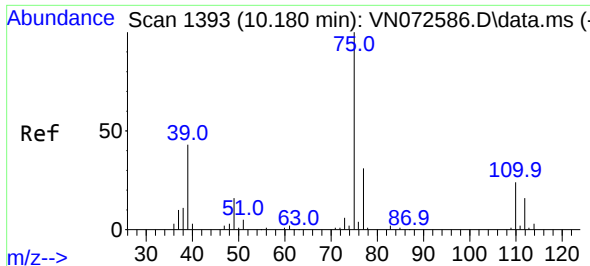





#54
cis-1,3-Dichloropropene
Concen: 15.276 ug/l
RT: 10.051 min Scan# 1499
Delta R.T. -0.129 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion: 75 Resp: 47020
Ion Ratio Lower Upper
75 100
77 32.9 25.2 37.8
39 48.8 35.7 53.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

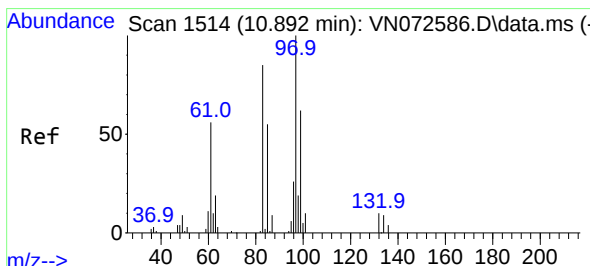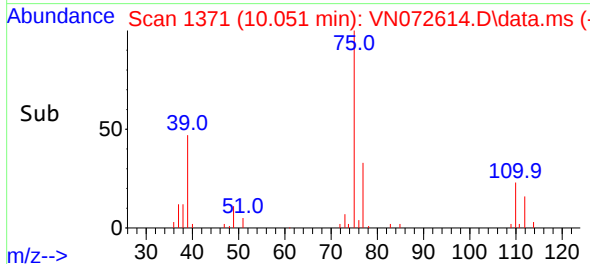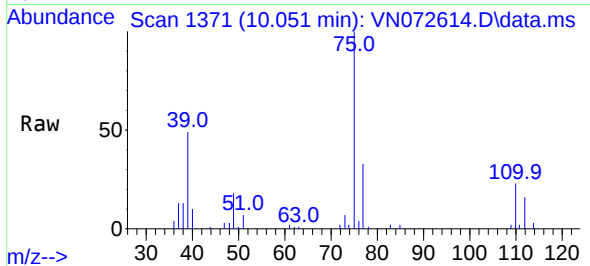

#55
1,1,2-Trichloroethane
Concen: 11.523 ug/l
RT: 10.804 min Scan# 1499
Delta R.T. -0.088 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion: 97 Resp: 23984
Ion Ratio Lower Upper
97 100
83 90.5 66.2 99.4
85 57.3 43.9 65.9
99 66.2 50.6 76.0

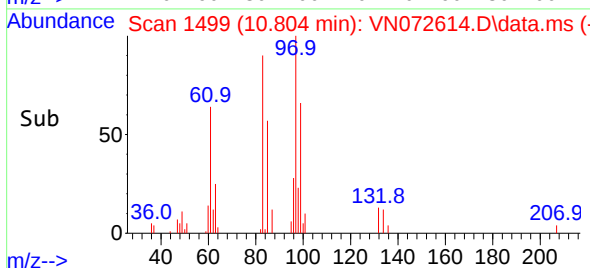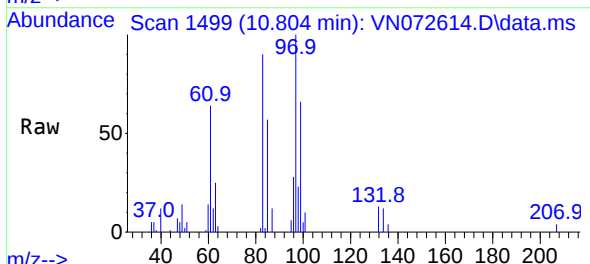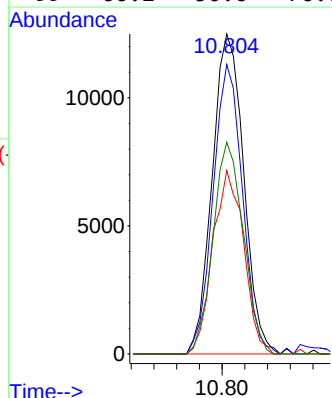



#56
Ethyl methacrylate
Concen: 11.868 ug/l
RT: 10.669 min Scan# 1491
Delta R.T. -0.088 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02



Tgt Ion: 69 Resp: 3805
Ion Ratio Lower Upper
69 100
41 73.8 47.8 71.6
39 44.7 27.3 40.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

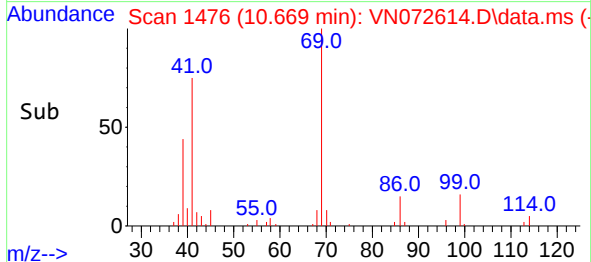

#57
1,3-Dichloropropane
Concen: 12.011 ug/l
RT: 10.957 min Scan# 1525
Delta R.T. -0.082 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 76 Resp: 42137
Ion Ratio Lower Upper
76 100
78 31.7 26.2 39.2

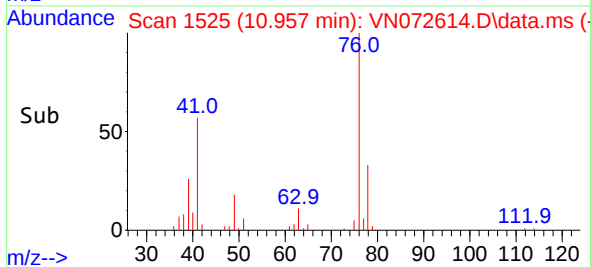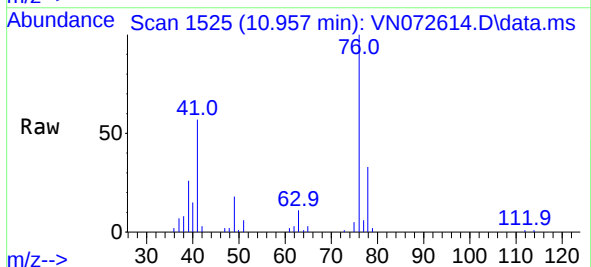



#58
2-Chloroethyl Vinyl ether
Concen: 89.446 ug/l
RT: 9.898 min Scan# 1111
Delta R.T. -0.141 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :

MSVOA_N

ClientSampleId :





VN0524WBSD02

Tgt Ion: 63 Resp: 122708
Ion Ratio Lower Upper
63 100
106 27.9 24.6 36.8

Manual Integrations




APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#59
2-Hexanone
Concen: 69.092 ug/l
RT: 11.010 min Scan# 1534
Delta R.T. -0.070 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 43 Resp: 152604
Ion Ratio Lower Upper
43 100
58 51.6 29.7 89.1

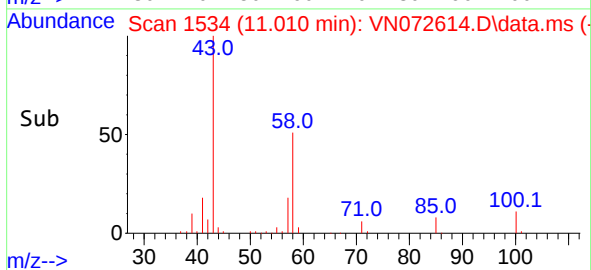

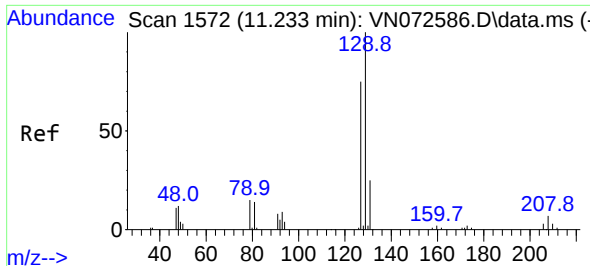





#60
Dibromochloromethane
Concen: 11.286 ug/l
RT: 11.157 min Scan# 1157
Delta R.T. -0.076 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion:129 Resp: 2514
Ion Ratio Lower Upper
129 100
127 80.9 38.8 116.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

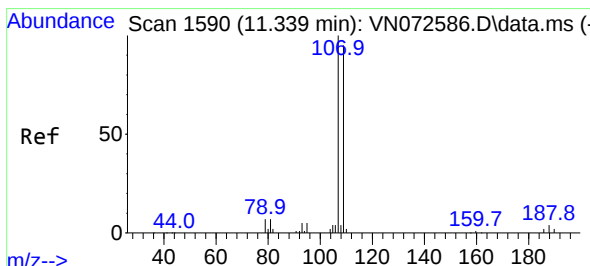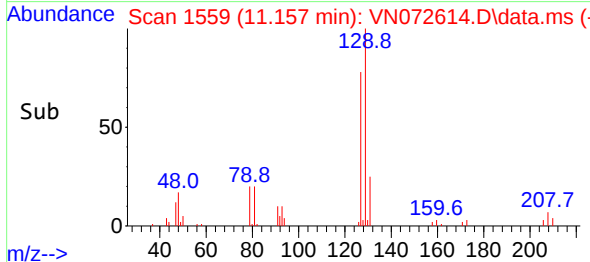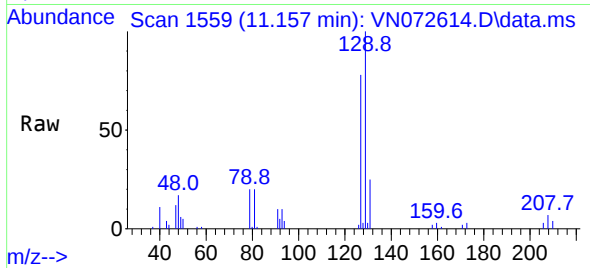

#61
1,2-Dibromoethane
Concen: 11.444 ug/l
RT: 11.269 min Scan# 1578
Delta R.T. -0.070 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion:107 Resp: 24834
Ion Ratio Lower Upper
107 100
109 92.2 75.0 112.6

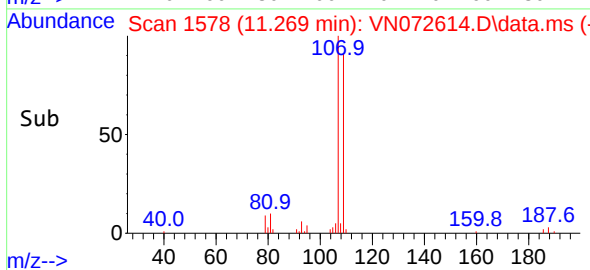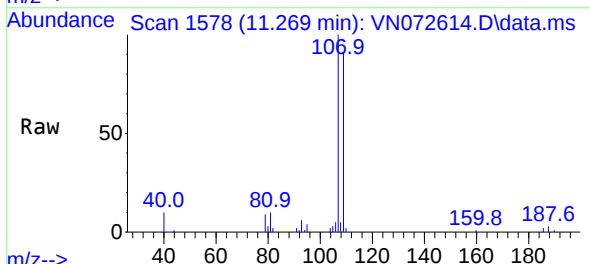

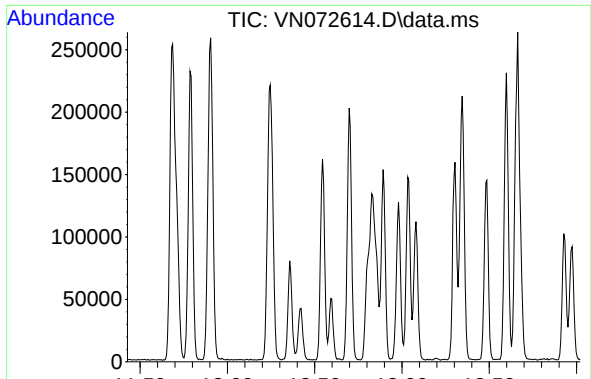

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.73 min



Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 95
Sig Exp Ratio
95 100
174 83.8
176 81.7

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Manual Integrations APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

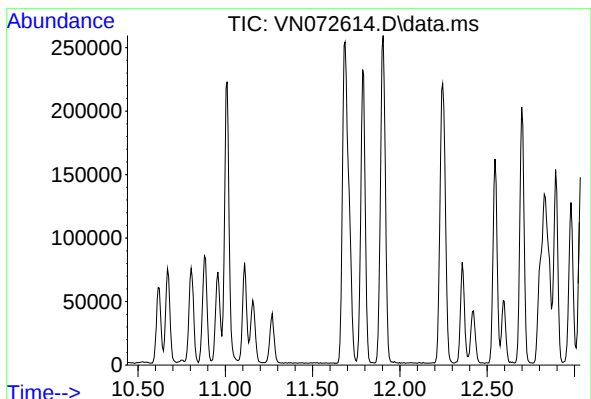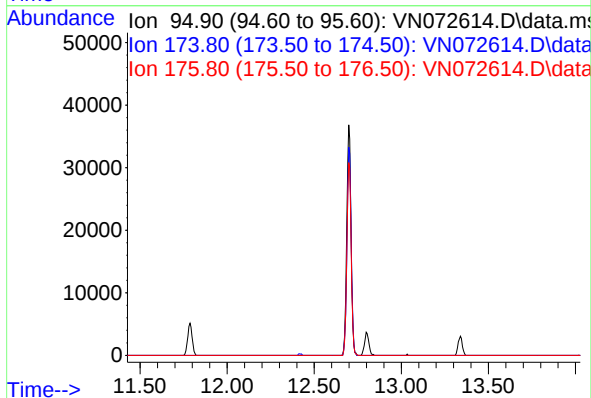


#63
Chlorobenzene-d5
Concen: 0.000 ug/l
Expected RT: 11.74 min

Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion: 117
Sig Exp Ratio
117 100
82 55.2
119 31.7

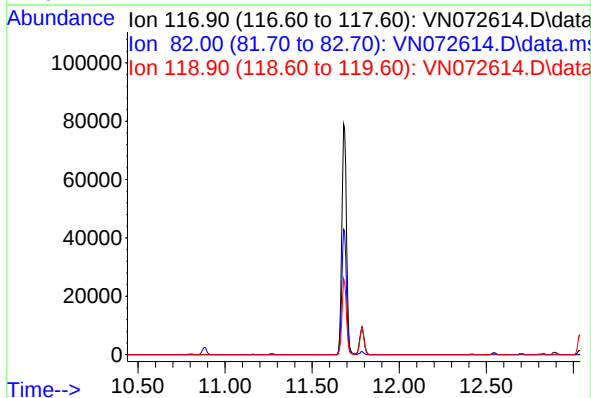



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.663 min Scan# 1985
Delta R.T. -0.005 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion:152 Resp: 58170
Ion Ratio Lower Upper
152 100
115 55.9 28.9 86.7
150 163.9 0.0 356.2

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#73
Isopropylbenzene
Concen: 20.628 ug/l
RT: 12.545 min Scan# 1795
Delta R.T. -0.029 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion:105 Resp: 106887
Ion Ratio Lower Upper
105 100
120 26.4 13.5 40.4

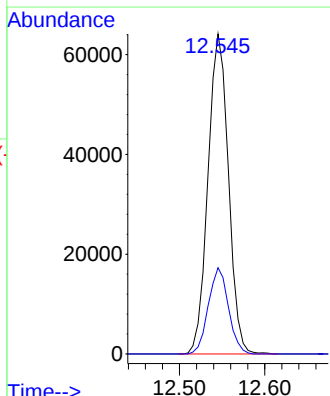



#74
N-amy1 acetate
Concen: 24.460 ug/l
RT: 12.357 min Scan# 11
Delta R.T. -0.023 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion: 43 Resp: 4549
Ion Ratio Lower Upper
43 100
70 40.2 39.0 58.4
55 23.1 21.1 31.7
61 21.7 21.1 31.7

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#75
1,1,2,2-Tetrachloroethane
Concen: 19.987 ug/l
RT: 12.798 min Scan# 1838
Delta R.T. -0.023 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion: 83 Resp: 36573
Ion Ratio Lower Upper
83 100
131 9.2 5.3 15.9
85 62.7 32.3 96.9

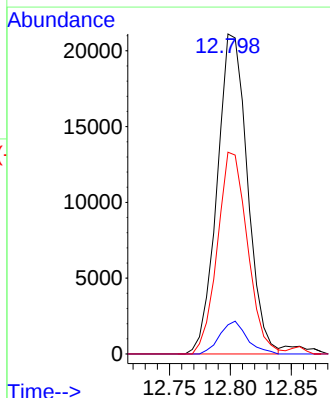

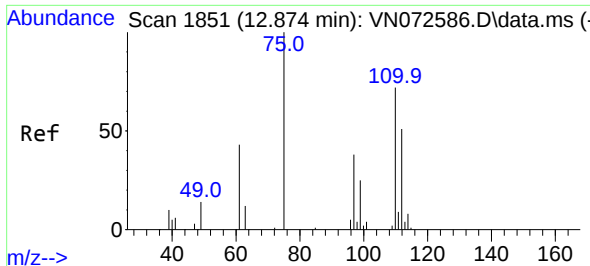

#76
1,2,3-Trichloropropane
Concen: 28.073 ug/l
RT: 12.857 min Scan# 1843
Delta R.T. -0.017 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

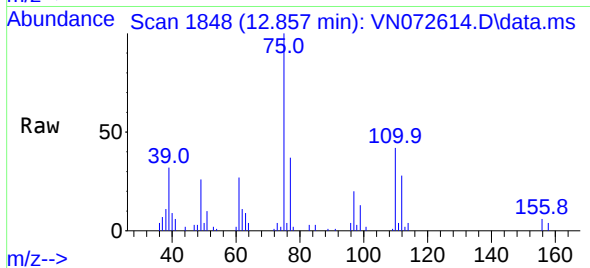


Tgt Ion: 75 Resp: 4433
Ion Ratio Lower Upper
75 100
77 0.0 98.5 295.5

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

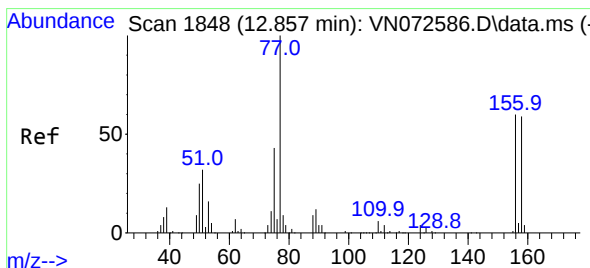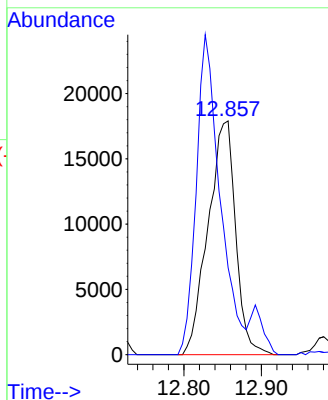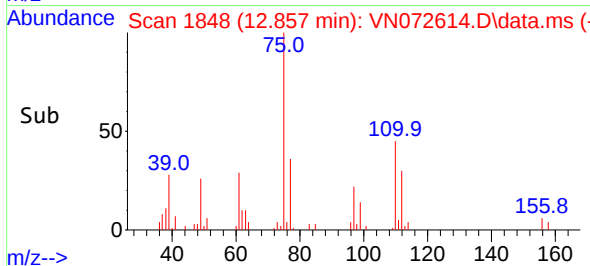


#77
Bromobenzene
Concen: 18.946 ug/l
RT: 12.827 min Scan# 1843
Delta R.T. -0.030 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

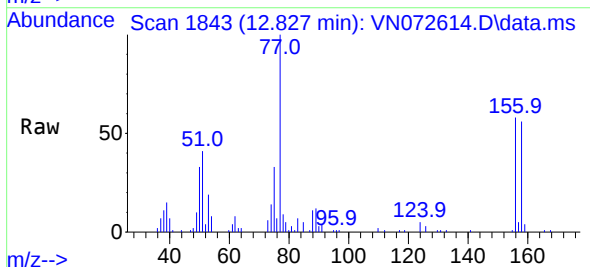

Tgt Ion:156 Resp: 24353
Ion Ratio Lower Upper
156 100
77 214.8 100.5 301.5
158 97.5 48.9 146.6

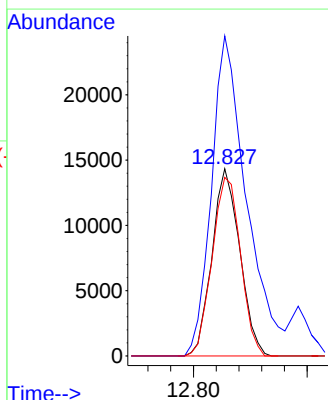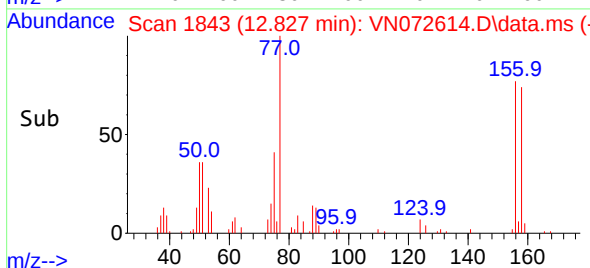







#78
n-propylbenzene
Concen: 20.274 ug/l
RT: 12.892 min Scan# 11648
Delta R.T. -0.024 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion: 91 Resp: 11648
Ion Ratio Lower Upper
91 100
120 22.1 11.9 35.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

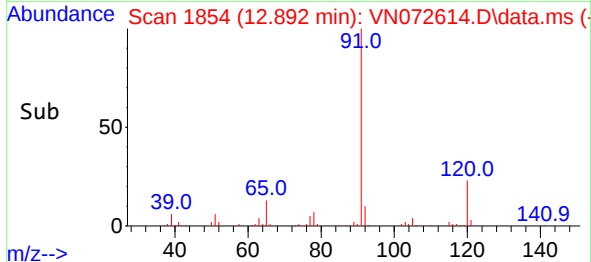

#79
2-Chlorotoluene
Concen: 19.738 ug/l
RT: 12.980 min Scan# 1869
Delta R.T. -0.024 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion: 91 Resp: 70058
Ion Ratio Lower Upper
91 100
126 33.8 17.3 51.9

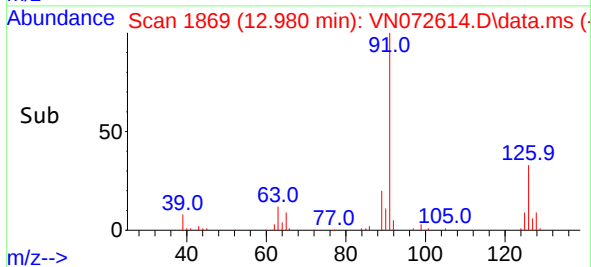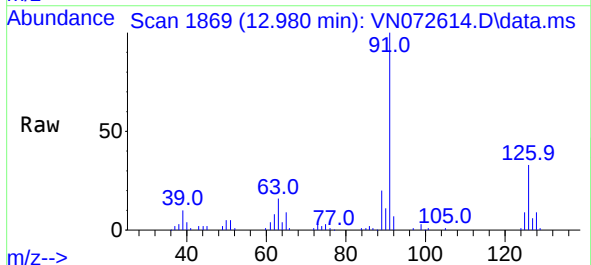



#80
1,3,5-Trimethylbenzene
Concen: 20.048 ug/l
RT: 13.039 min Scan# 11
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02



Tgt Ion:105 Resp: 8080
Ion Ratio Lower Upper
105 100
120 48.2 24.9 74.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#81
trans-1,4-Dichloro-2-butene
Concen: 19.366 ug/l
RT: 12.598 min Scan# 1804
Delta R.T. -0.023 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion: 75 Resp: 10422
Ion Ratio Lower Upper
75 100
53 103.4 78.0 117.0
89 45.3 37.2 55.8

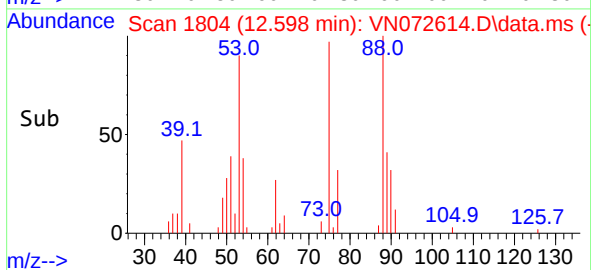

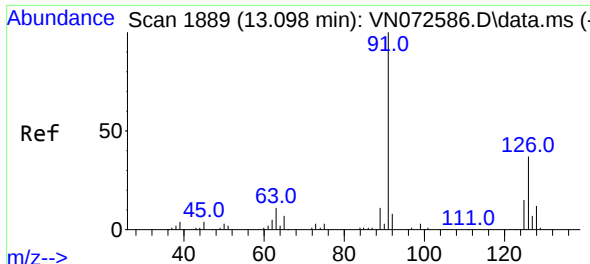





#82
4-Chlorotoluene
Concen: 19.927 ug/l
RT: 13.080 min Scan# 11
Delta R.T. -0.018 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion: 91 Resp: 6468
Ion Ratio Lower Upper
91 100
126 32.3 17.2 51.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

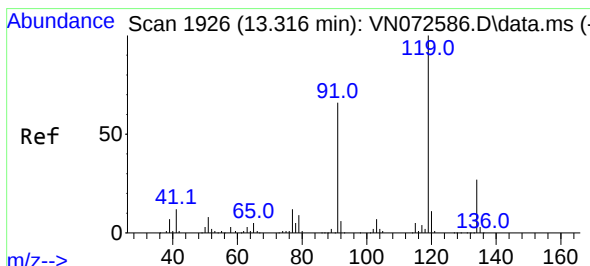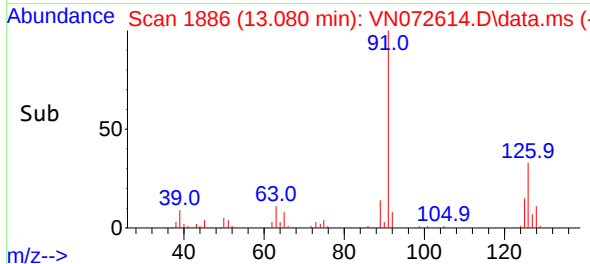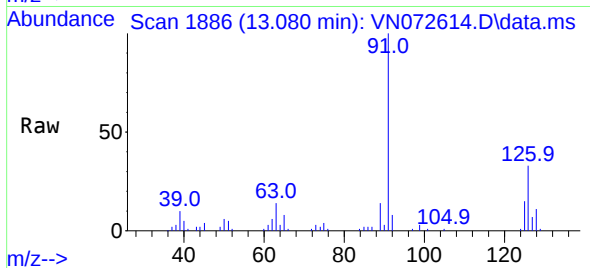

#83
tert-Butylbenzene
Concen: 20.644 ug/l
RT: 13.304 min Scan# 1924
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion:119 Resp: 77479
Ion Ratio Lower Upper
119 100
91 64.3 31.6 94.8
134 26.9 13.7 41.1

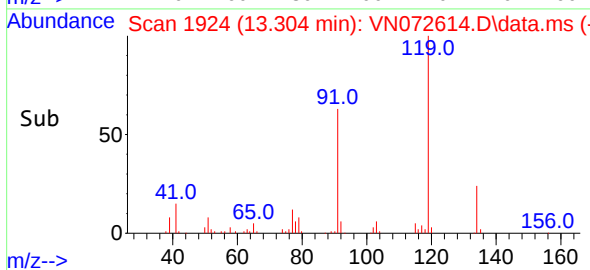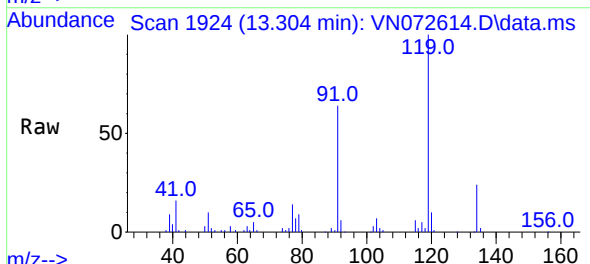



#84
1,2,4-Trimethylbenzene
Concen: 20.034 ug/l
RT: 13.345 min Scan# 1931
Delta R.T. -0.018 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

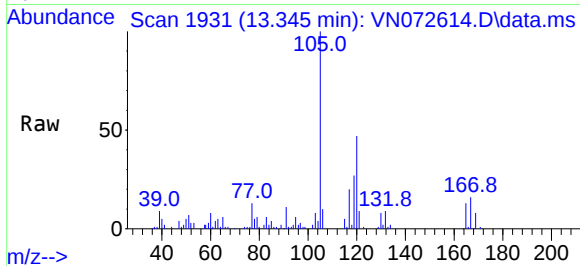


Tgt Ion:105 Resp: 79180
Ion Ratio Lower Upper
105 100
120 46.8 23.3 69.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#85
sec-Butylbenzene
Concen: 20.065 ug/l
RT: 13.480 min Scan# 1954
Delta R.T. -0.018 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

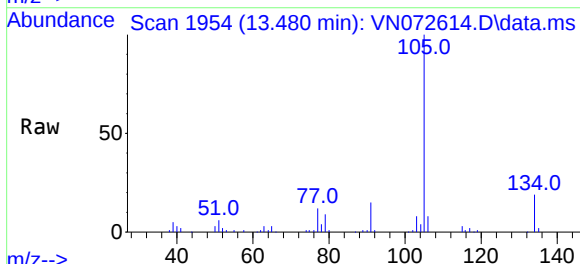

Tgt Ion:105 Resp: 100706
Ion Ratio Lower Upper
105 100
134 19.2 10.4 31.1

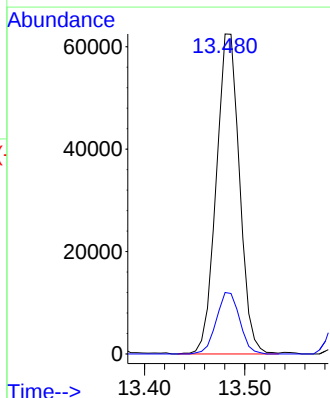







#86
p-Isopropyltoluene
Concen: 19.575 ug/l
RT: 13.598 min Scan# 1974
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion:119 Resp: 7746
Ion Ratio Lower Upper
119 100
134 25.8 13.3 39.8
91 22.6 11.3 33.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022

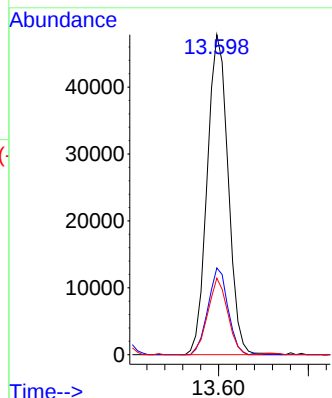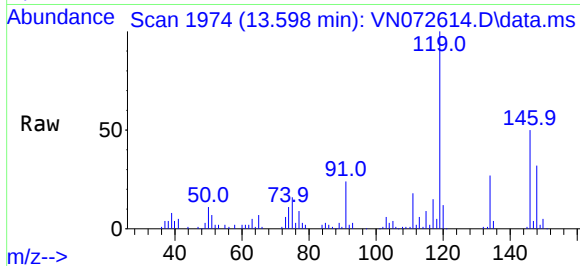

#87
1,3-Dichlorobenzene
Concen: 18.360 ug/l
RT: 13.598 min Scan# 1974
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Tgt Ion:146 Resp: 39831
Ion Ratio Lower Upper
146 100
111 36.7 20.0 60.0
148 61.1 32.0 96.0

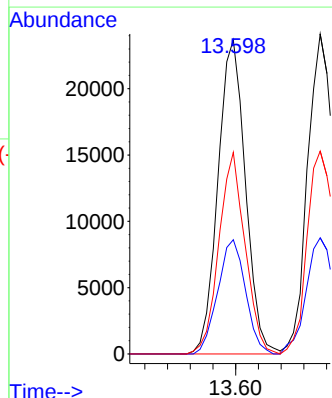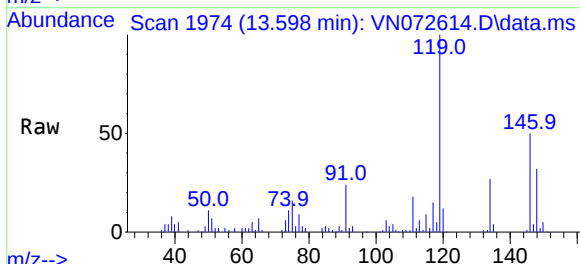







#88
1,4-Dichlorobenzene
Concen: 18.974 ug/l
RT: 13.674 min Scan# 1989
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

Tgt Ion:146 Resp: 40385
Ion Ratio Lower Upper
146 100
111 37.7 19.1 57.1
148 65.3 31.4 94.3




Manual Integrations
APPROVED


Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022



#89
n-Butylbenzene
Concen: 18.052 ug/l
RT: 13.927 min Scan# 2030
Delta R.T. -0.012 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34


Tgt Ion: 91 Resp: 57641
Ion Ratio Lower Upper
91 100
92 52.2 26.9 80.7
134 25.0 13.6 40.8

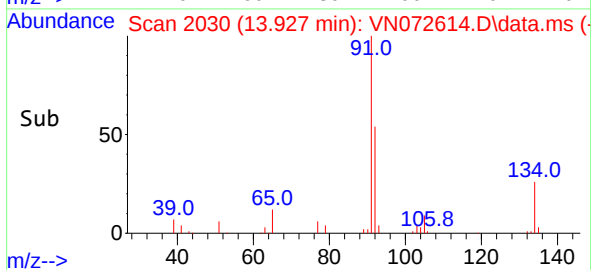



#90
Hexachloroethane
Concen: 20.726 ug/l
RT: 14.198 min Scan# 2077
Delta R.T. -0.006 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion:117 Resp: 16215
Ion Ratio Lower Upper
117 100
201 76.2 40.6 122.0

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#91
1,2-Dichlorobenzene
Concen: 18.694 ug/l
RT: 13.974 min Scan# 2038
Delta R.T. -0.006 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion:146 Resp: 38849
Ion Ratio Lower Upper
146 100
111 38.3 20.9 62.8
148 64.3 32.1 96.3

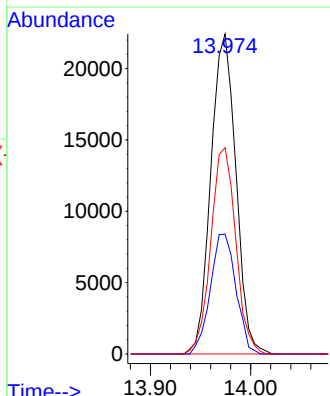



#92
1,2-Dibromo-3-Chloropropane
Concen: 20.947 ug/l
RT: 14.592 min Scan# 2143
Delta R.T. -0.006 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02

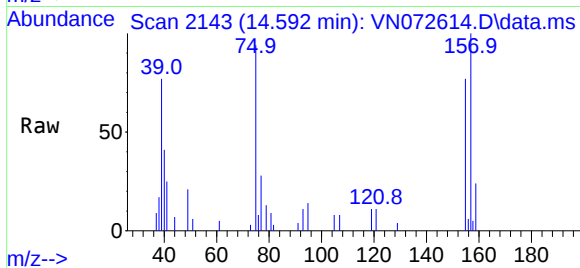


Tgt Ion: 75 Resp: 6534
Ion Ratio Lower Upper
75 100
155 88.8 44.9 134.5
157 109.5 59.0 176.8

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#93
1,2,4-Trichlorobenzene
Concen: 18.494 ug/l
RT: 15.257 min Scan# 2256
Delta R.T. -0.000 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34

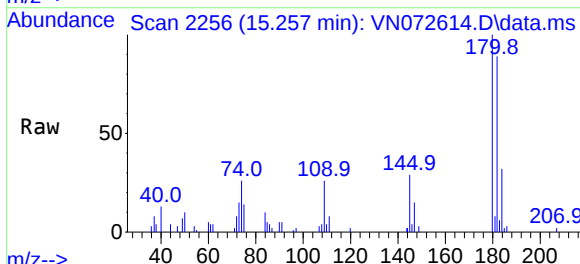


Tgt Ion:180 Resp: 20244
Ion Ratio Lower Upper
180 100
182 93.7 47.5 142.5
145 29.1 14.5 43.5

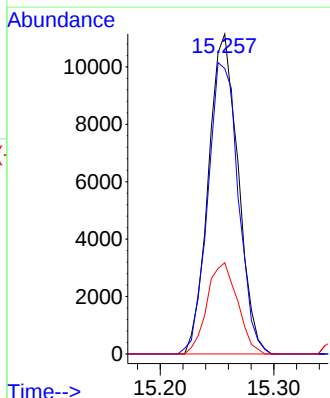



#94
Hexachlorobutadiene
Concen: 16.788 ug/l
RT: 15.363 min Scan# 21
Delta R.T. 0.001 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Instrument :
MSVOA_N
ClientSampleId :
VN0524WBSD02




Tgt Ion:225 Resp: 10844
Ion Ratio Lower Upper
225 100
223 63.8 32.4 97.2
227 66.4 31.8 95.4

Manual Integrations
APPROVED



Reviewed By :John Carlone 05/25/2022
Supervised By :Mahesh Dadoda 05/25/2022




#95
Naphthalene
Concen: 20.161 ug/l
RT: 15.498 min Scan# 2297
Delta R.T. -0.000 min
Lab File: VN072614.D
Acq: 25 May 2022 02:34




Tgt Ion:128 Resp: 72985
Ion Ratio Lower Upper
128 100
127 13.2 10.3 15.5
129 10.9 8.6 13.0

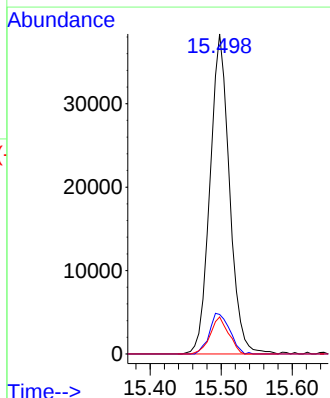



#96
 1,2,3-Trichlorobenzene
 Concen: 17.916 ug/l
 RT: 15.692 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN072614.D
 Acq: 25 May 2022 02:34

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0524WBSD02



Tgt Ion:180 Resp: 2099
 Ion Ratio Lower Upper
 180 100
 182 96.6 47.8 143.3
 145 29.6 15.5 46.5

Manual Integrations
 APPROVED

Reviewed By :John Carlone 05/25/2022
 Supervised By :Mahesh Dadoda 05/25/2022

