

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
 Data File : VN072600.D
 Acq On : 24 May 2022 20:55
 Operator : JC\MD
 Sample : N2968-01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-24

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
 Title : SW846 8260

Signal : TIC: VN072600.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	35	43	47	rBV4	4567	10748	1.12%	0.200%
2	2.781	129	135	140	rVB6	7208	15664	1.63%	0.291%
3	5.616	604	617	631	rBV4	18529	72246	7.51%	1.344%
4	8.016	1015	1025	1030	rBV	117076	277452	28.86%	5.162%
5	8.080	1030	1036	1047	rVB	200418	451369	46.95%	8.398%
6	8.433	1087	1096	1109	rVB	114546	263128	27.37%	4.895%
7	8.963	1176	1186	1196	rBV	327576	658838	68.53%	12.257%
8	10.439	1428	1437	1446	rBV	532508	953700	99.20%	17.743%
9	10.821	1496	1502	1506	rBV2	5272	11013	1.15%	0.205%
10	11.739	1650	1658	1672	rBV	561551	961427	100.00%	17.887%
11	12.727	1819	1826	1838	rBV	426033	713567	74.22%	13.276%
12	13.668	1979	1986	1996	rBV	461513	760062	79.06%	14.141%
13	13.833	2008	2014	2017	rBV3	15774	24426	2.54%	0.454%
14	13.868	2017	2020	2025	rVV	16407	26587	2.77%	0.495%
15	14.274	2083	2089	2093	rBV3	6687	10355	1.08%	0.193%
16	14.321	2093	2097	2104	rVB	27143	42048	4.37%	0.782%
17	14.533	2128	2133	2138	rBV	29278	46640	4.85%	0.868%
18	15.186	2235	2244	2249	rBV5	13887	28431	2.96%	0.529%
19	15.309	2256	2265	2271	rVB5	14501	34595	3.60%	0.644%
20	15.803	2343	2349	2352	rBV4	7358	12731	1.32%	0.237%


Sum of corrected areas: 5375027

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072600.D
Acq On : 24 May 2022 20:55
Operator : JC\MD
Sample : N2968-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

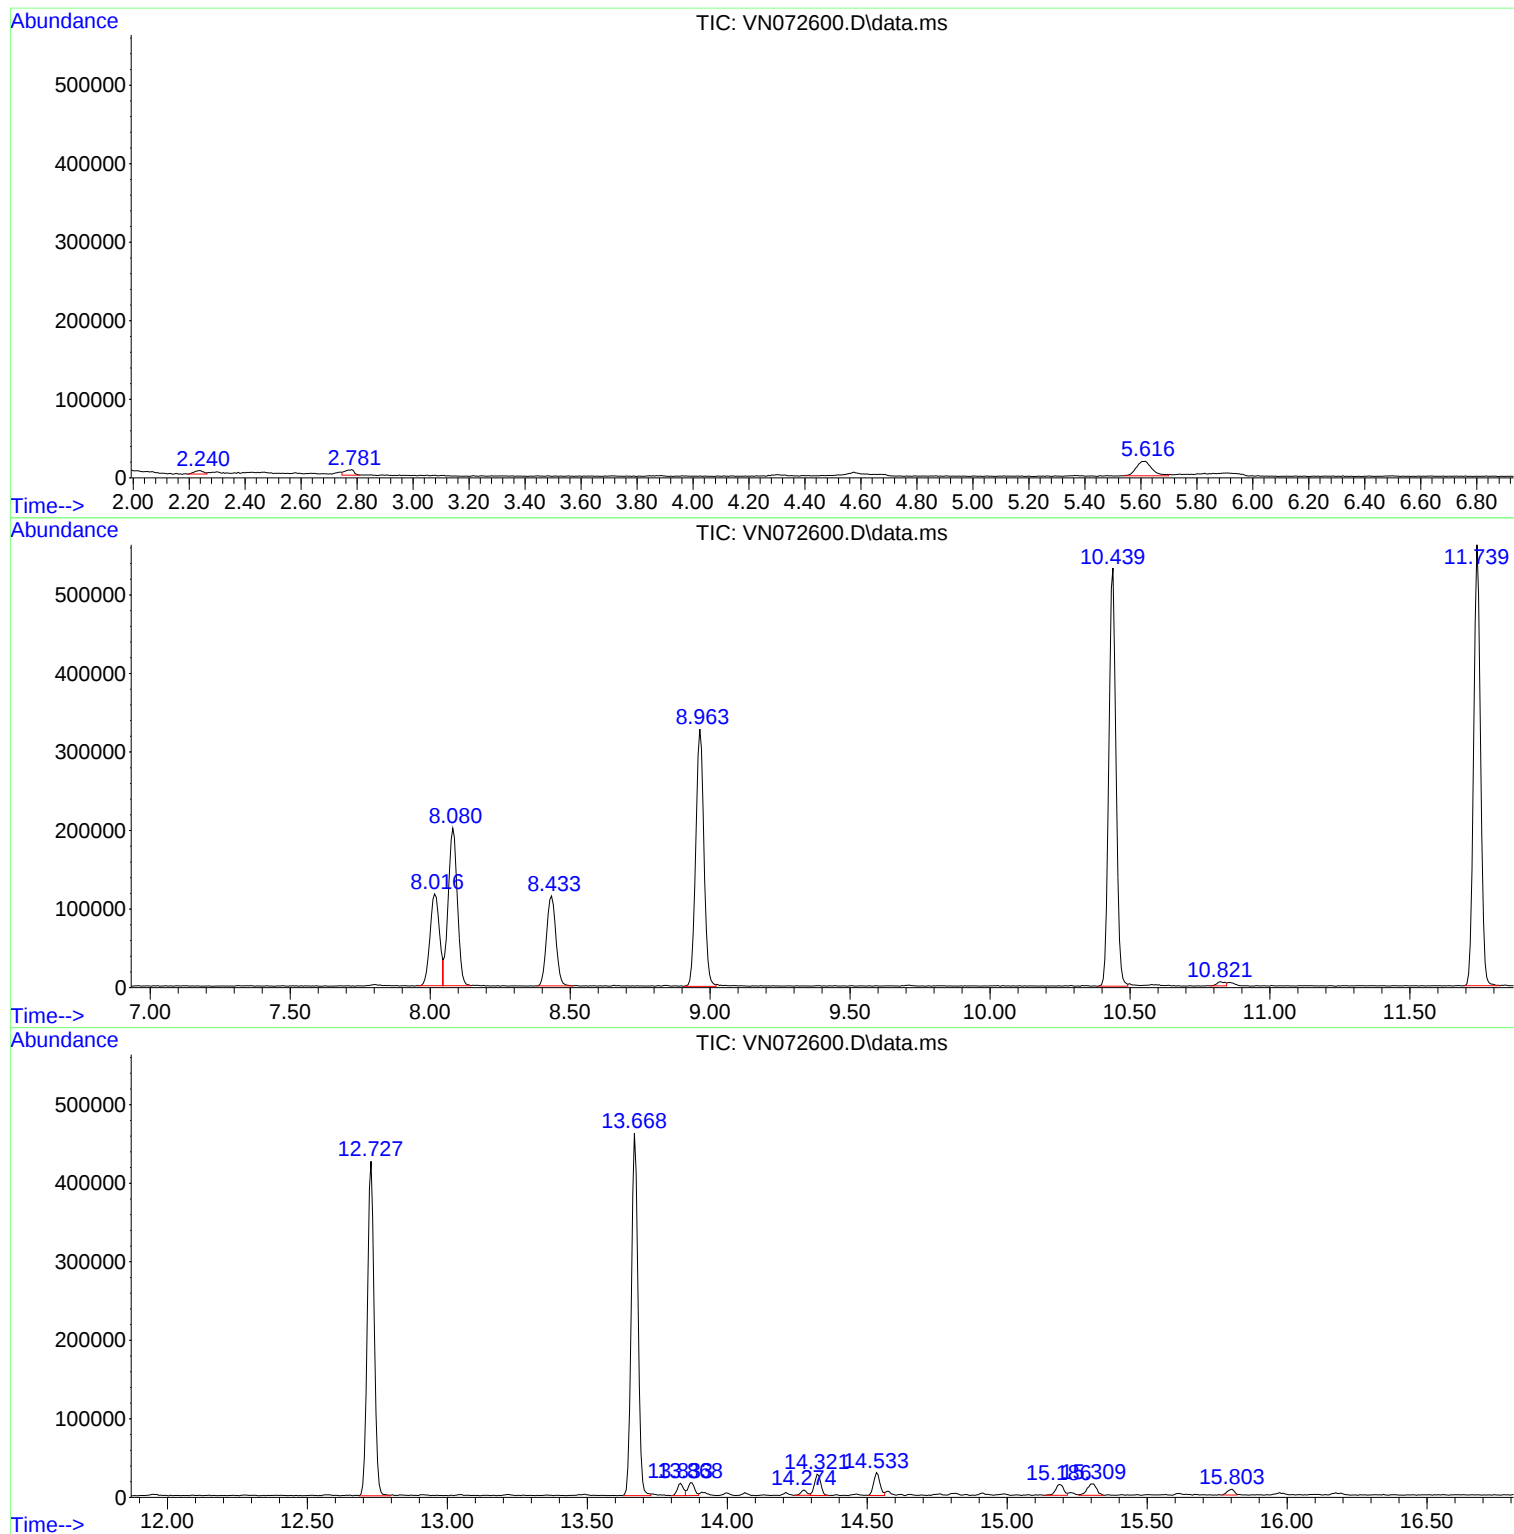

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072600.D
Acq On : 24 May 2022 20:55
Operator : JC\MD
Sample : N2968-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072600.D
Acq On : 24 May 2022 20:55
Operator : JC\MD
Sample : N2968-01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-24

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------