

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
 Data File : VN072602.D
 Acq On : 24 May 2022 21:43
 Operator : JC\MD
 Sample : N2968-03
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-40

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
 Title : SW846 8260

Signal : TIC: VN072602.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	560	573	589	rBV2	58954	212510	13.64%	2.983%
2	5.610	605	616	630	rBV2	28609	99950	6.41%	1.403%
3	6.487	756	765	780	rVB2	30499	97464	6.26%	1.368%
4	7.093	858	868	884	rBV4	10046	36571	2.35%	0.513%
5	8.016	1016	1025	1030	rBV	117004	272386	17.48%	3.823%
6	8.081	1030	1036	1047	rVB	196740	446633	28.66%	6.269%
7	8.451	1087	1099	1109	rBV2	604101	1558164	100.00%	21.869%
8	8.522	1109	1111	1119	rVB3	14788	27540	1.77%	0.387%
9	8.963	1177	1186	1196	rBV	318118	650277	41.73%	9.127%
10	10.192	1389	1395	1407	rVB2	18819	40424	2.59%	0.567%
11	10.439	1426	1437	1445	rBV	519309	963775	61.85%	13.527%
12	10.639	1465	1471	1477	rVB	29383	52352	3.36%	0.735%
13	10.710	1477	1483	1492	rVB	36155	64192	4.12%	0.901%
14	11.122	1548	1553	1562	rVB	36336	67336	4.32%	0.945%
15	11.580	1624	1631	1638	rBV2	11533	21984	1.41%	0.309%
16	11.739	1650	1658	1670	rVV	557000	975363	62.60%	13.690%
17	12.275	1743	1749	1759	rVB4	9133	17761	1.14%	0.249%
18	12.727	1816	1826	1837	rBV	430526	717359	46.04%	10.068%
19	13.669	1979	1986	1999	rBV	460369	775935	49.80%	10.891%
20	13.874	2016	2021	2032	rVB	14942	26882	1.73%	0.377%


Sum of corrected areas: 7124858

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072602.D
Acq On : 24 May 2022 21:43
Operator : JC\MD
Sample : N2968-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

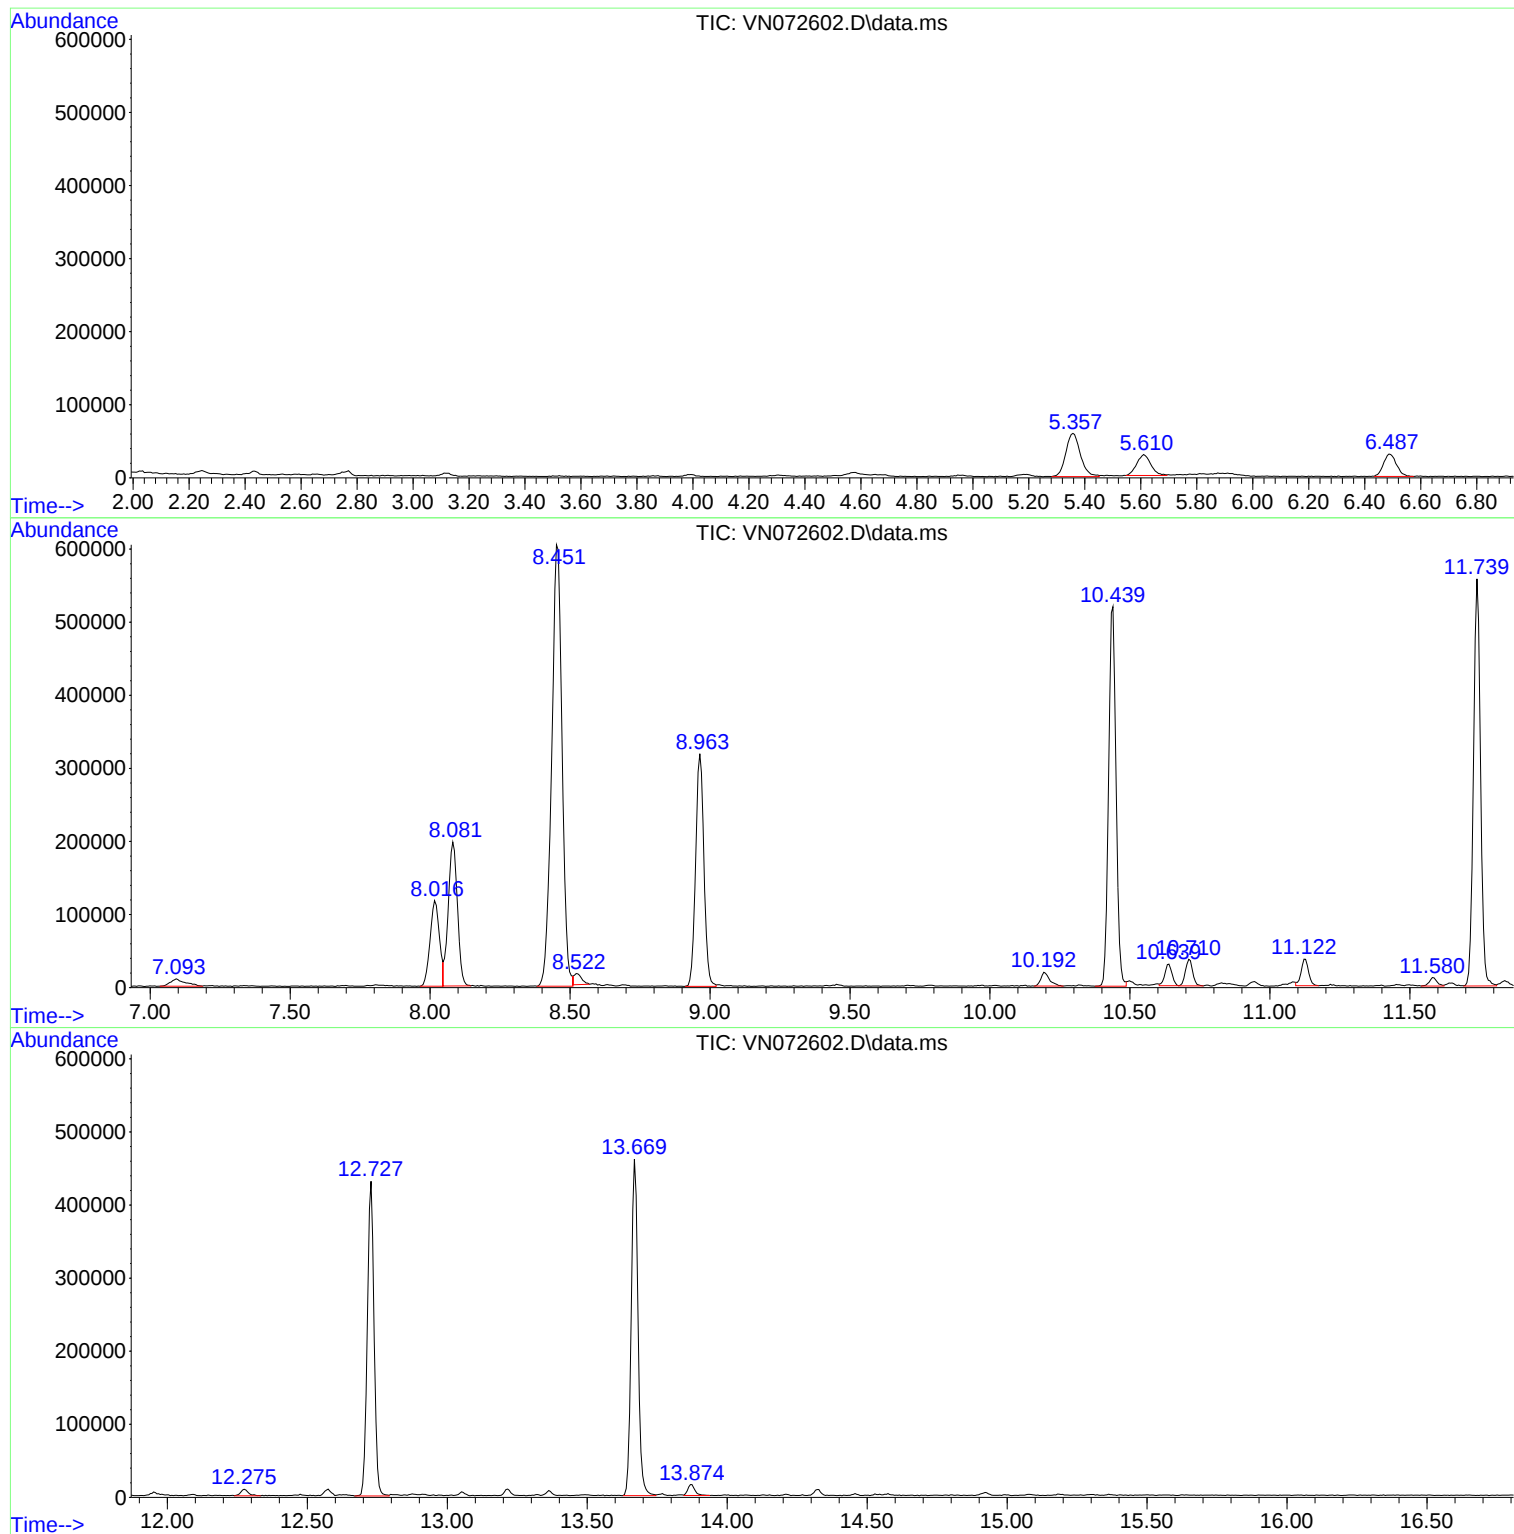

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072602.D
Acq On : 24 May 2022 21:43
Operator : JC\MD
Sample : N2968-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072602.D
Acq On : 24 May 2022 21:43
Operator : JC\MD
Sample : N2968-03
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc