
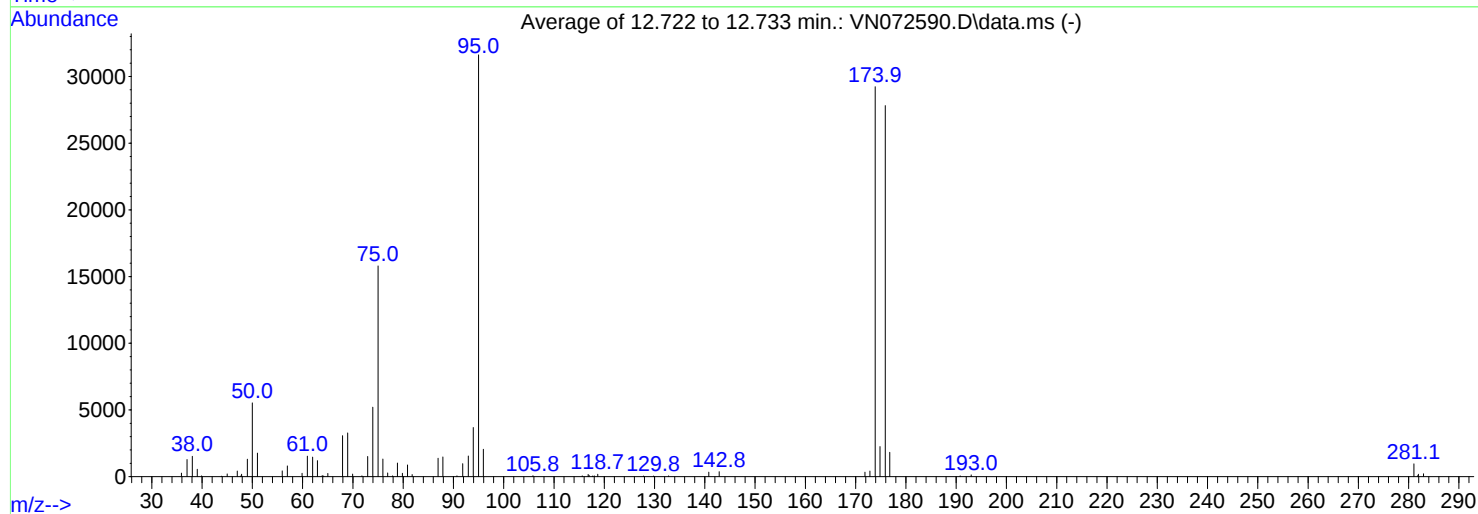


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052422\
Data File : VN072590.D
Acq On : 24 May 2022 16:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052422W.M
Title : SW846 8260
Last Update : Wed May 25 09:15:20 2022

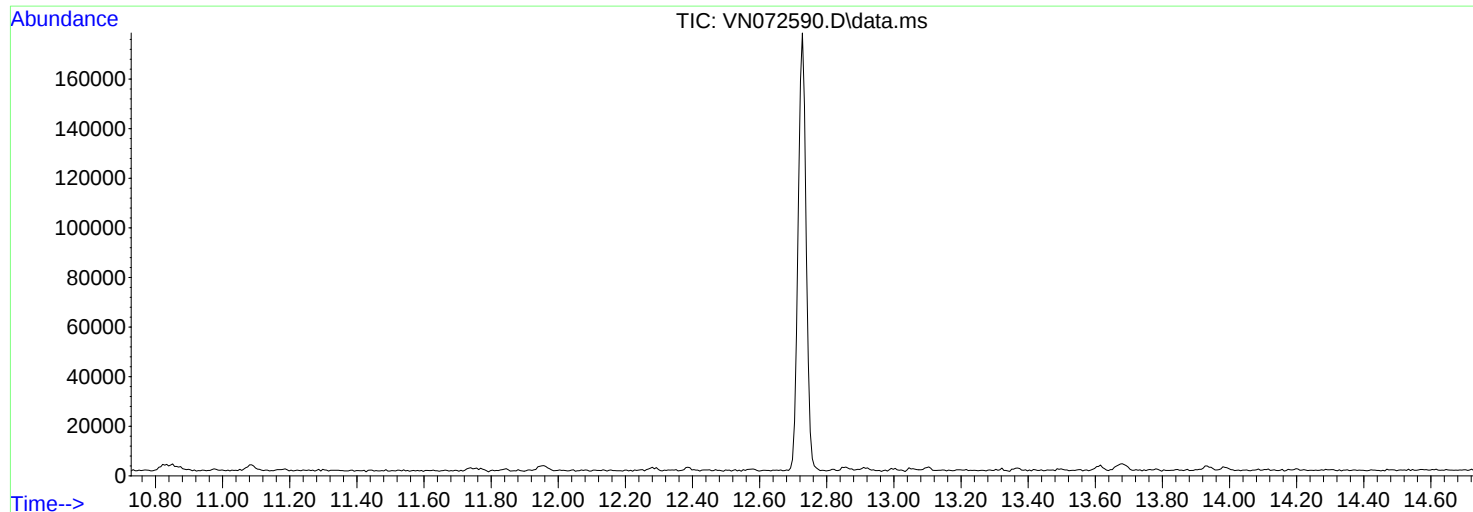

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	5531	PASS
75	95	30	60	49.9	15794	PASS
95	95	100	100	100.0	31624	PASS
96	95	5	9	6.5	2047	PASS
173	174	0.00	2	1.4	419	PASS
174	95	50	100	92.5	29237	PASS
175	174	5	9	7.7	2256	PASS
176	174	95	101	95.1	27819	PASS
177	176	5	9	6.6	1829	PASS