
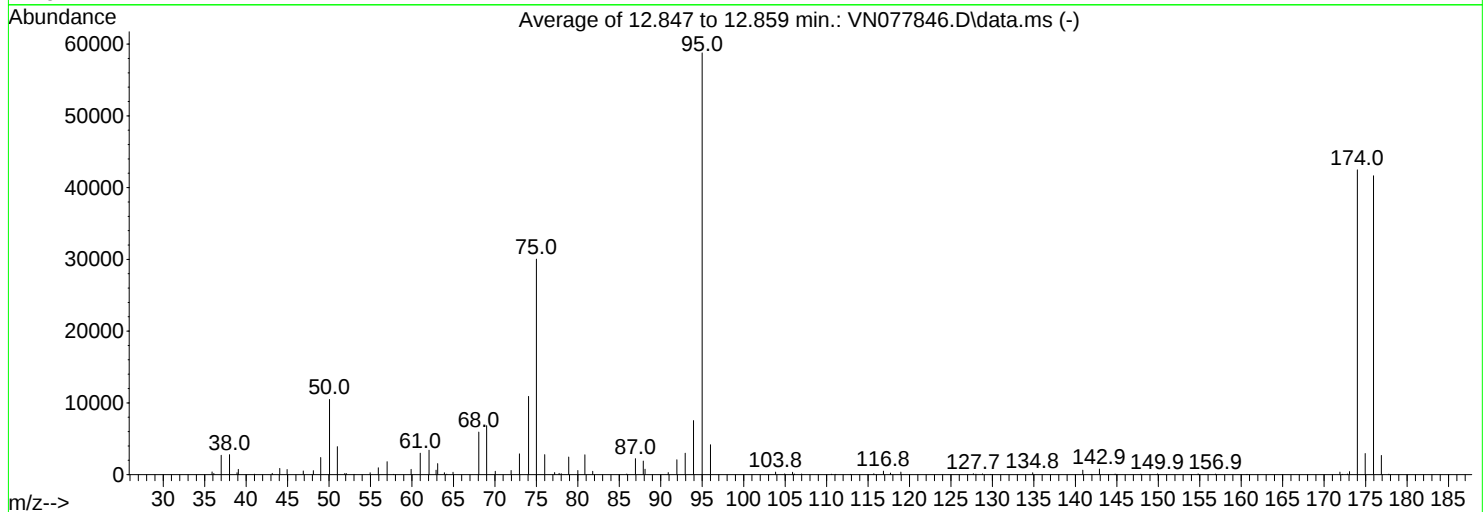


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052423\
Data File : VN077846.D
Acq On : 24 May 2023 08:55
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

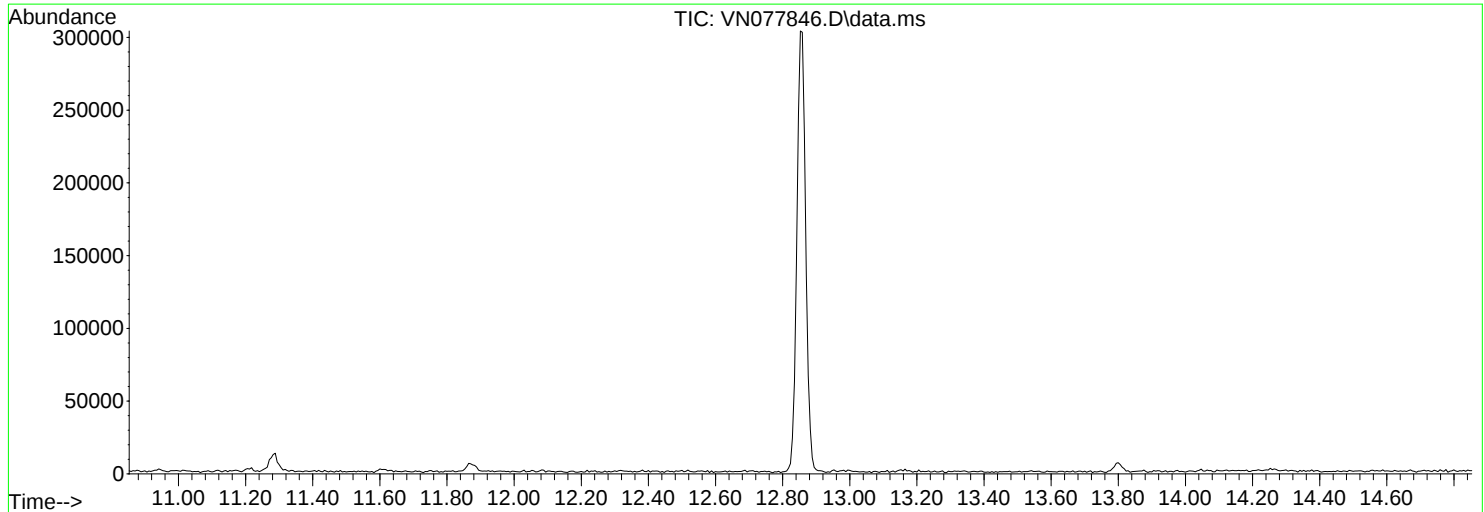

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	10491	PASS
75	95	30	60	51.1	30045	PASS
95	95	100	100	100.0	58781	PASS
96	95	5	9	7.1	4167	PASS
173	174	0.00	2	1.0	424	PASS
174	95	50	100	72.2	42469	PASS
175	174	5	9	6.9	2951	PASS
176	174	95	101	98.1	41648	PASS
177	176	5	9	6.4	2670	PASS

Average of 12.847 to 12.859 min.: VN077846.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	382	48.10	556	59.90	727	71.95	581
36.10	167	49.00	2385	61.00	2996	72.95	289
37.00	2696	50.05	10491	62.05	3416	74.05	1090
38.00	2791	51.00	3899	62.90	622	75.00	3004
38.90	258	51.90	189	63.10	1543	76.00	2796
39.05	729	52.10	126	63.90	274	77.20	285
41.00	69	53.00	56	64.20	67	77.75	171
43.15	176	54.95	278	64.95	329	78.00	129
44.05	876	55.95	968	68.05	5940	78.90	2450
44.95	720	57.00	1799	69.00	6833	80.00	573
46.90	523	57.80	51	70.05	474	80.85	2774

Average of 12.847 to 12.859 min.: VN077846.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.80	459	103.85	366	118.95	353	147.90	77
85.90	87	104.95	112	127.70	143	149.90	116
86.95	2232	105.90	336	128.00	60	154.80	110
87.90	1891	106.10	101	128.80	104	156.90	97
88.10	766	107.00	82	129.80	54	160.70	52
90.90	280	110.60	58	134.85	270	171.90	349
91.95	2070	111.10	51	140.90	623	172.20	53
92.95	2996	112.90	50	141.90	55	172.80	98
93.95	7530	115.70	143	142.90	786	173.05	424
95.00	58781	116.85	502	144.80	80	174.00	42469
96.00	4167	117.70	223	145.00	56	174.95	2951

Average of 12.847 to 12.859 min.: VN077846.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
175.95	41648						
176.90	2670						
177.80	68						

Instrument :
MSVOA_N
ClientSampleId :
BFB