
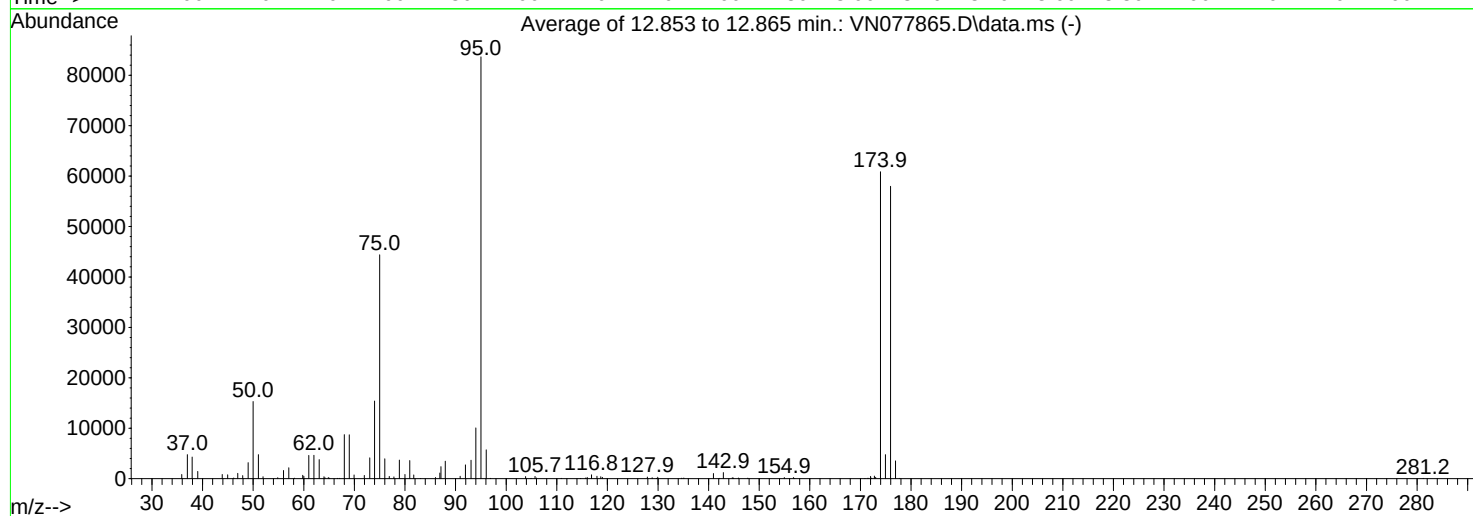


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052423\
Data File : VN077865.D
Acq On : 24 May 2023 22:13
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

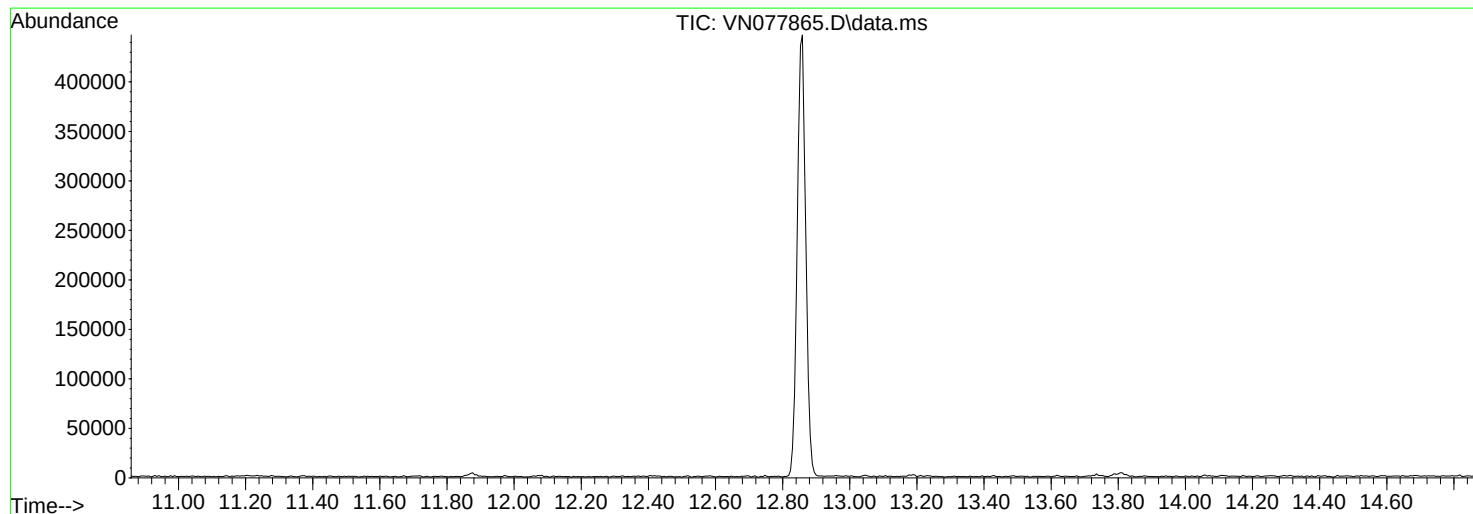

AutoFind: Scans 1853, 1854, 1855; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	15307	PASS
75	95	30	60	53.1	44405	PASS
95	95	100	100	100.0	83656	PASS
96	95	5	9	6.8	5718	PASS
173	174	0.00	2	0.8	498	PASS
174	95	50	100	72.8	60875	PASS
175	174	5	9	7.8	4754	PASS
176	174	95	101	95.3	57995	PASS
177	176	5	9	6.0	3508	PASS

Average of 12.853 to 12.865 min.: VN077865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	819	51.05	4760	64.00	388	74.00	1540
37.00	4751	51.95	373	64.20	197	75.00	4440
37.95	4273	54.85	179	64.85	216	76.00	393
39.05	1429	56.00	1607	65.10	104	76.90	45
43.90	839	57.05	2149	66.70	82	77.80	337
44.95	759	58.15	112	67.10	52	78.90	3670
46.15	121	59.80	660	68.00	8734	80.00	841
46.95	1064	60.00	474	69.00	8699	80.95	3572
47.95	592	61.00	4617	69.95	732	81.75	729
49.00	3161	62.00	4626	71.95	623	83.10	50
50.00	15307	63.05	3786	73.05	4119	86.05	215

Average of 12.853 to 12.865 min.: VN077865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.90	1100	104.90	67	127.90	320	145.90	116
87.10	2373	105.70	433	128.85	203	147.75	114
87.95	3467	106.00	141	129.70	78	154.95	237
90.90	478	110.90	80	129.95	287	156.75	233
91.95	2747	114.70	50	134.70	96	157.00	70
93.05	3646	115.70	140	135.10	118	170.90	50
94.00	10078	116.00	262	140.95	1023	171.50	91
95.00	83656	116.85	748	142.10	52	172.00	435
96.05	5718	117.95	492	142.90	1202	172.20	86
96.90	80	118.70	396	144.70	184	172.75	498
103.85	416	119.00	268	144.90	122	173.00	260

Average of 12.853 to 12.865 min.: VN077865.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
173.95	60875						
174.95	4754						
175.95	57995						
176.95	3508						
177.80	78						
281.20	52						

Instrument :

MSVOA_N

ClientSampleId :

BFB