

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052523\
 Data File : VN077900.D
 Acq On : 25 May 2023 14:27
 Operator : JC\MD
 Sample : 02897-02 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 OILY-WATER-0523

Quant Time: May 26 04:31:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.236	168	450282	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	808958	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	718090	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	285604	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	293423	43.552	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	87.100%		
35) Dibromofluoromethane	8.171	113	248634	47.133	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	94.260%		
50) Toluene-d8	10.571	98	1010464	49.766	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	99.540%		
62) 4-Bromofluorobenzene	12.853	95	353324	49.271	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.540%		
Target Compounds						
					Qvalue	
3) Chloromethane	2.371	50	1264	Below Cal	#	1
13) Acrolein	4.177	56	303	Below Cal	#	1
16) Acetone	4.442	43	52570	24.801	ug/l	94
17) Carbon Disulfide	4.712	76	5552	0.435	ug/l #	75
18) Methyl Acetate	5.036	43	2155	0.242	ug/l #	42
20) Methylene Chloride	5.283	84	9949	Below Cal		92
25) 2-Butanone	7.494	43	3976	1.199	ug/l #	86
27) cis-1,2-Dichloroethene	7.489	96	1476	0.231	ug/l	36
29) Tetrahydrofuran	7.847	42	11062	5.095	ug/l #	78
31) Cyclohexane	8.230	56	10195	1.113	ug/l #	22
36) 1,1-Dichloropropene	8.236	75	36407	4.719	ug/l #	49
37) Ethyl Acetate	7.571	43	52305	7.606	ug/l	97
38) Carbon Tetrachloride	8.236	117	50280	6.453	ug/l #	15
41) Methacrylonitrile	7.847	41	6846	1.869	ug/l #	34
44) Trichloroethene	9.365	130	1627	0.282	ug/l	55
51) 4-Methyl-2-Pentanone	10.459	43	2467	0.369	ug/l #	71
52) Toluene	10.635	92	4584	0.323	ug/l	88
59) 2-Hexanone	11.200	43	1535	0.311	ug/l #	45
64) Tetrachloroethene	11.106	164	1565	0.312	ug/l	92
67) Ethyl Benzene	11.971	91	5935	0.213	ug/l #	75
68) m/p-Xylenes	12.071	106	8974	0.849	ug/l	93
69) o-Xylene	12.412	106	5078	0.488	ug/l	95
76) 1,2,3-Trichloropropane	12.853	75	183031	25.590	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.176	105	10045	0.485	ug/l	94
81) trans-1,4-Dichloro-2-b...	12.853	75	183031	81.798	ug/l #	15
84) 1,2,4-Trimethylbenzene	13.488	105	27889	1.370	ug/l	93
86) p-Isopropyltoluene	13.735	119	1785983	87.266	ug/l	99
87) 1,3-Dichlorobenzene	13.741	146	2515	0.242	ug/l #	51
89) n-Butylbenzene	13.953	91	5459	0.290	ug/l	90
90) Hexachloroethane	14.335	117	1966	0.585	ug/l #	21
95) Naphthalene	15.647	128	326665	16.732	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: May 26 04:31:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.236 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion:168 Resp: 450282
Ion Ratio Lower Upper
168 100
99 60.5 53.0 79.6



#3
Chloromethane
Concen: Below Cal
RT: 2.371 min Scan# 71
Delta R.T. 0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 50 Resp: 1264
Ion Ratio Lower Upper
50 100
52 94.7 26.5 39.7#


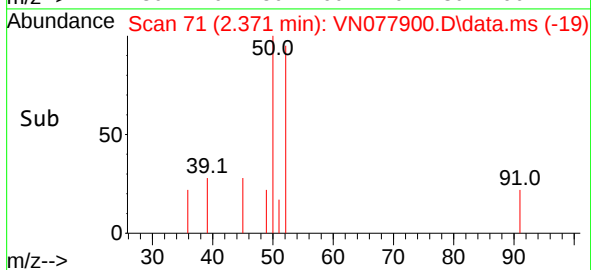






#13
Acrolein
Concen: Below Cal
RT: 4.177 min Scan# 31
Delta R.T. -0.012 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion: 56 Resp: 303
Ion Ratio Lower Upper
56 100
55 161.1 54.5 81.7#

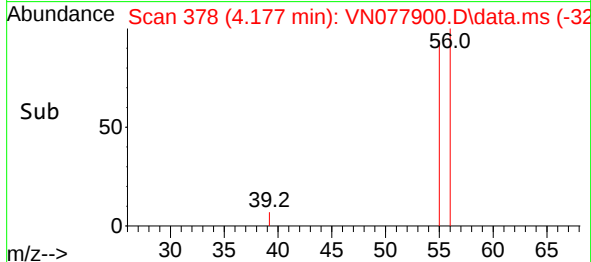

#16
Acetone
Concen: 24.801 ug/l
RT: 4.442 min Scan# 423
Delta R.T. 0.012 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 43 Resp: 52570
Ion Ratio Lower Upper
43 100
58 31.3 28.0 42.0

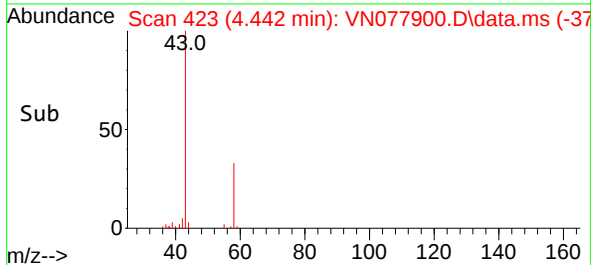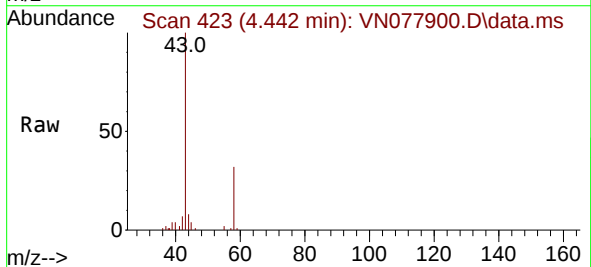



#17

Carbon Disulfide

Concen: 0.435 ug/l

RT: 4.712 min Scan# 4

Delta R.T. 0.000 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :





OILY-WATER-0523

Tgt Ion: 76 Resp: 5552

Ion Ratio Lower Upper

76 100

78 0.0 7.4 11.0#

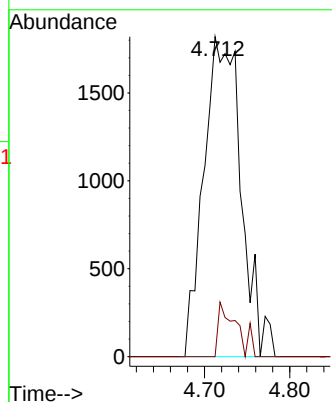

#18

Methyl Acetate

Concen: 0.242 ug/l

RT: 5.036 min Scan# 524

Delta R.T. -0.000 min

Lab File: VN077900.D




Acq: 25 May 2023 14:27


Tgt Ion: 43 Resp: 2155

Ion Ratio Lower Upper

43 100

74 0.0 26.2 39.4#

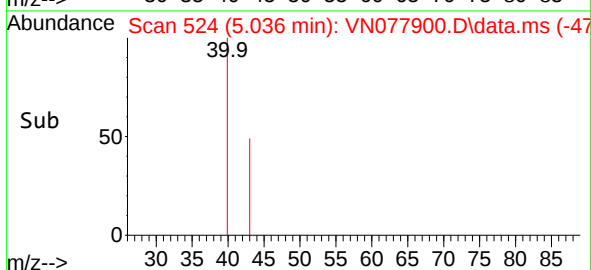



#25

2-Butanone

Concen: 1.199 ug/l

RT: 7.494 min Scan# 942

Delta R.T. 0.006 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :





OILY-WATER-0523

Tgt Ion: 43 Resp: 3976

Ion Ratio Lower Upper

43 100

72 29.5 30.2 45.2#

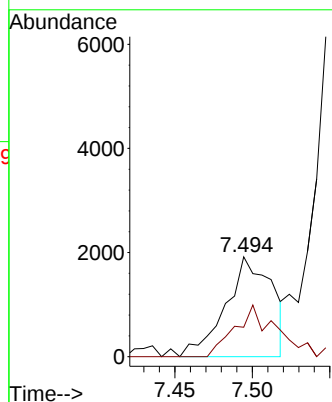

#27

cis-1,2-Dichloroethene

Concen: 0.231 ug/l

RT: 7.489 min Scan# 941

Delta R.T. 0.001 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27




Tgt Ion: 96 Resp: 1476


Ion Ratio Lower Upper

96 100

61 197.3 0.0 255.2

98 119.9 0.0 128.8

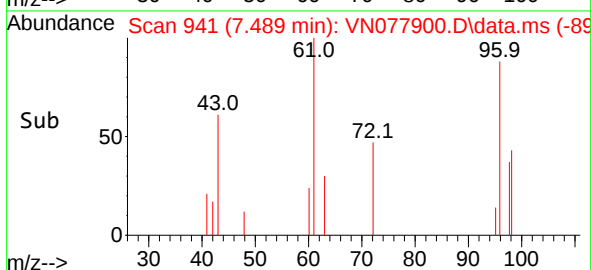

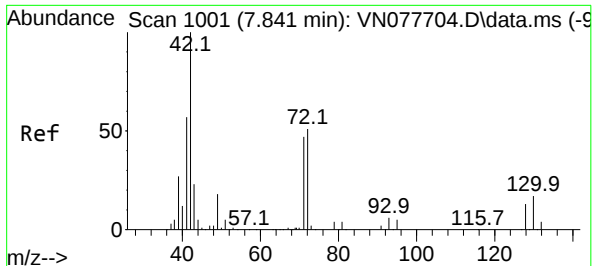

#29

Tetrahydrofuran

Concen: 5.095 ug/l

RT: 7.847 min Scan# 1062

Delta R.T. 0.006 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :

OILY-WATER-0523





Tgt Ion: 42 Resp: 11062

Ion Ratio Lower Upper

42 100

72 50.0 49.8 74.6

71 38.1 47.4 71.2#

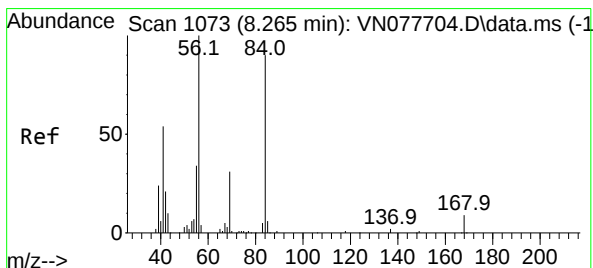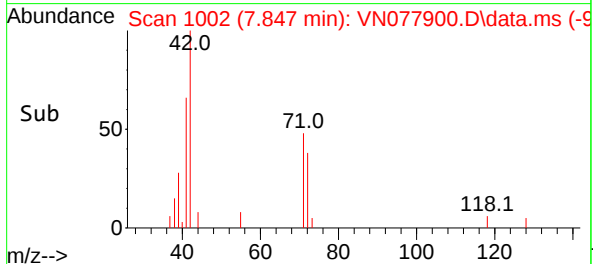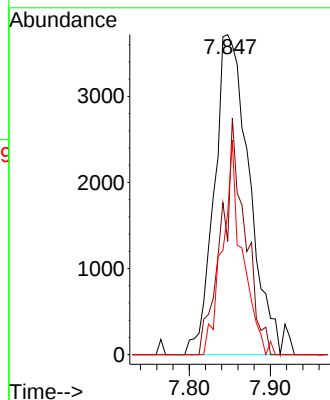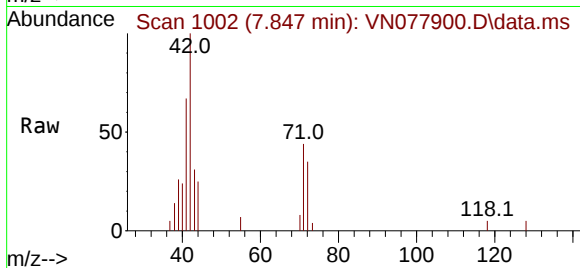

#31

Cyclohexane

Concen: 1.113 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.035 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27




Tgt Ion: 56 Resp: 10195


Ion Ratio Lower Upper

56 100

69 136.3 26.8 40.2#

84 147.4 81.8 122.6#

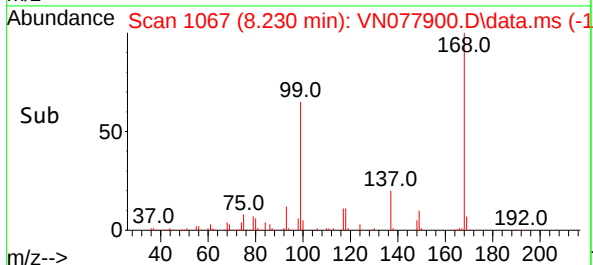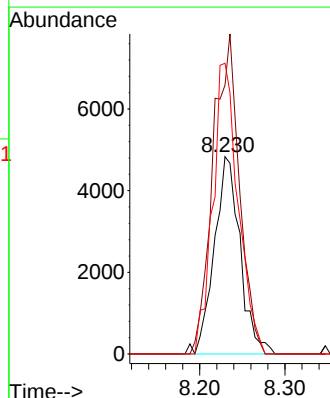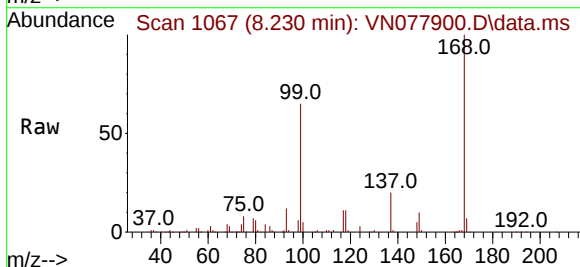

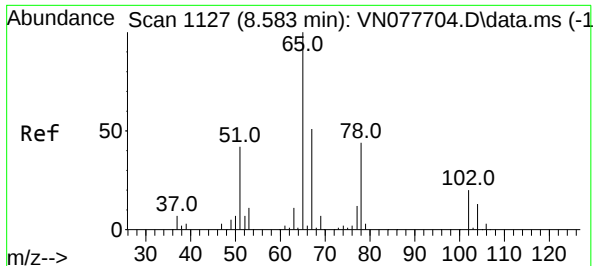

#33

1,2-Dichloroethane-d4

Concen: 43.552 ug/l

RT: 8.583 min Scan# 1127

Delta R.T. 0.001 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :





OILY-WATER-0523

Tgt Ion: 65 Resp: 293423

Ion Ratio Lower Upper

65 100

67 51.9 0.0 106.6

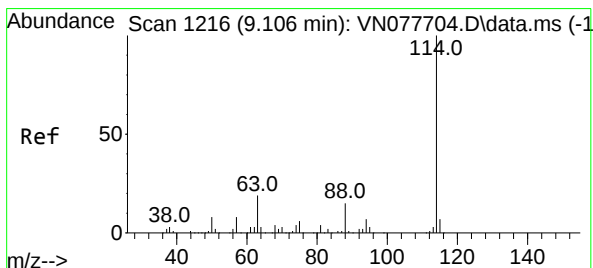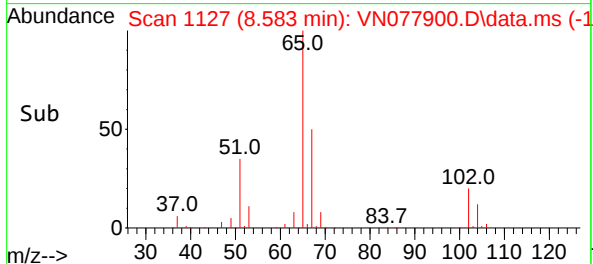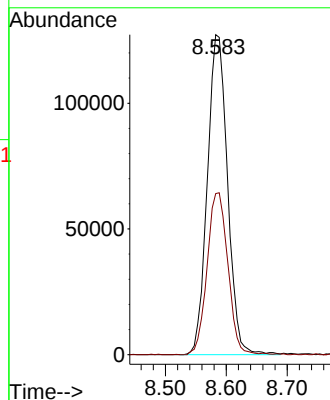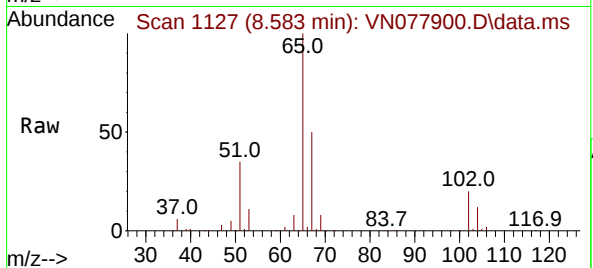

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1216

Delta R.T. 0.000 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27




Tgt Ion: 114 Resp: 808958


Ion Ratio Lower Upper

114 100

63 19.7 0.0 36.4

88 15.4 0.0 30.6

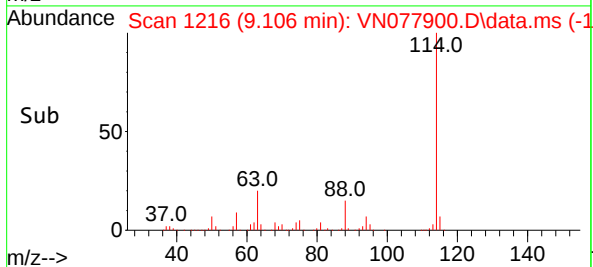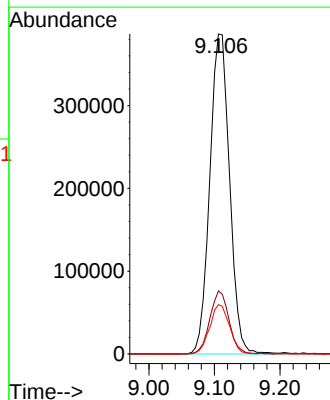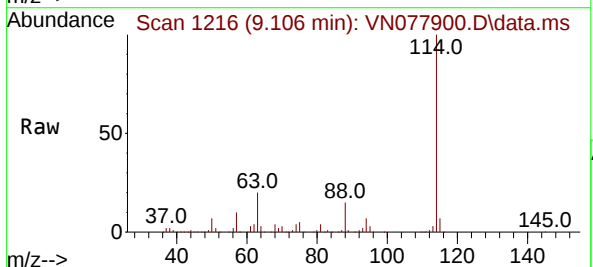

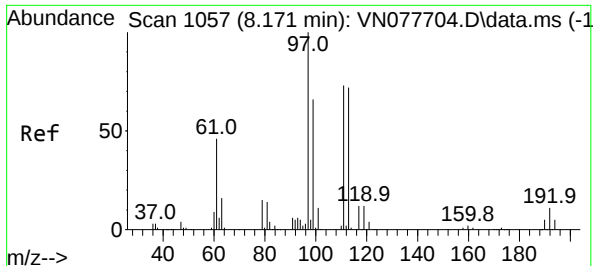

#35

Dibromofluoromethane

Concen: 47.133 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :

OILY-WATER-0523





Tgt Ion:113 Resp: 248634

Ion Ratio Lower Upper

113 100

111 103.2 82.6 123.8

192 17.0 12.7 19.1

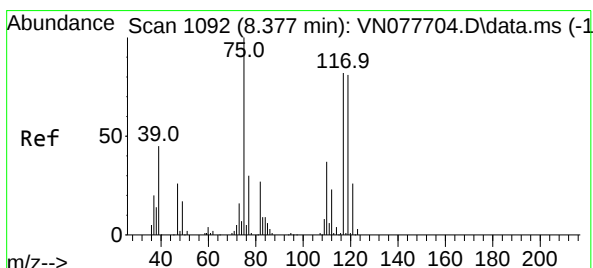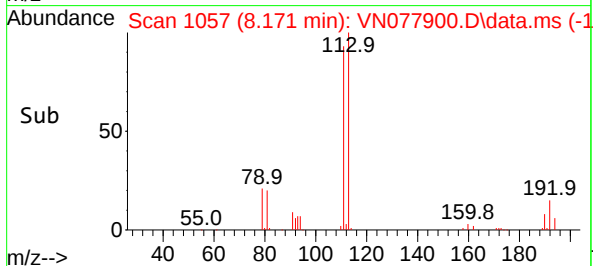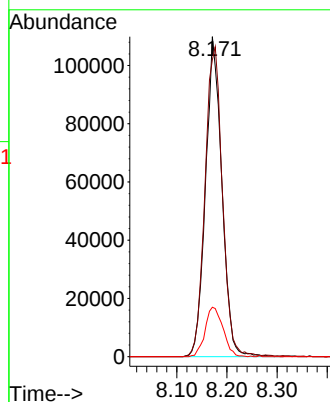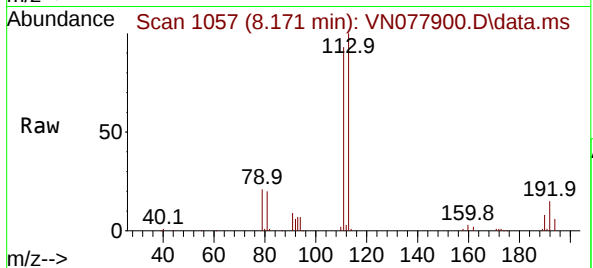

#36

1,1-Dichloropropene

Concen: 4.719 ug/l

RT: 8.236 min Scan# 1068

Delta R.T. -0.141 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27




Tgt Ion: 75 Resp: 36407


Ion Ratio Lower Upper

75 100

110 10.1 19.1 57.3#

77 0.0 25.0 37.4#

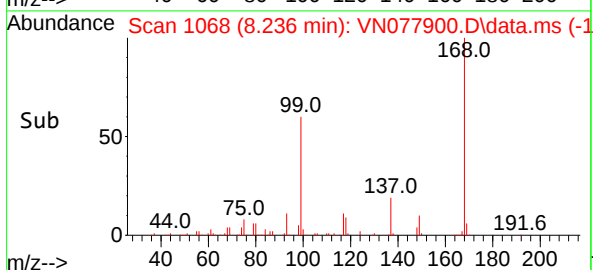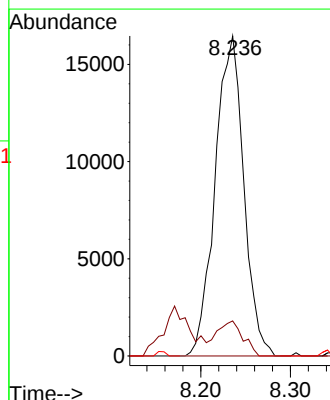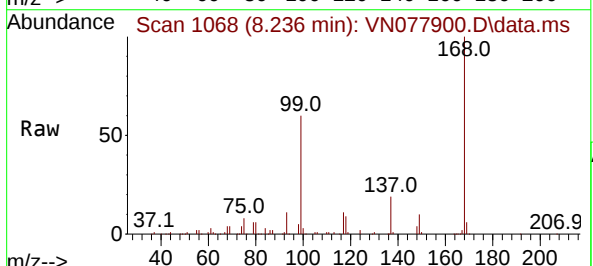



#37

Ethyl Acetate

Concen: 7.606 ug/l

RT: 7.571 min Scan# 91

Delta R.T. 0.006 min

Lab File: VN077900.D


Acq: 25 May 2023 14:27

Instrument :




MSVOA_N

ClientSampleId :

OILY-WATER-0523

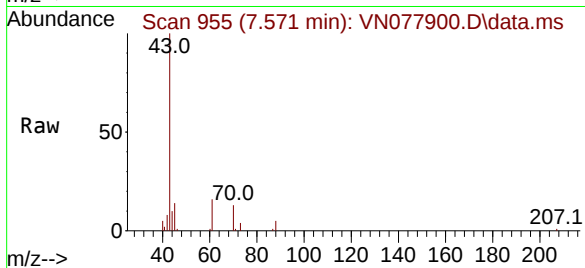

Tgt Ion:	43	Resp:	52305
Ion	Ratio	Lower	Upper
43	100		
61	16.8	13.2	19.8
70	11.8	11.3	16.9



#38

Carbon Tetrachloride

Concen: 6.453 ug/l




RT: 8.236 min Scan# 1068


Delta R.T. -0.135 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Tgt Ion:	117	Resp:	50280
Ion	Ratio	Lower	Upper
117	100		
119	4.6	77.3	115.9#
121	0.0	23.3	34.9#


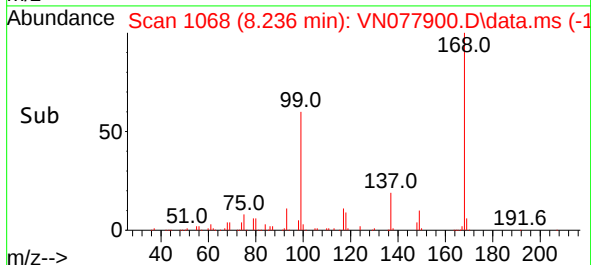
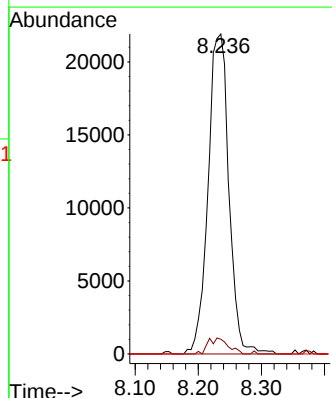
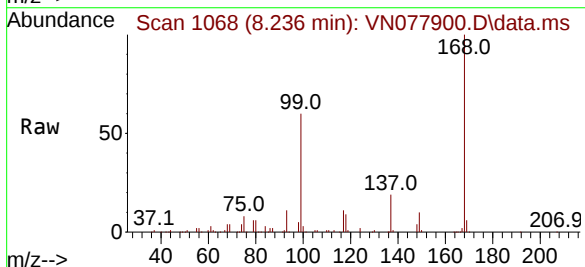




#41
Methacrylonitrile
Concen: 1.869 ug/l
RT: 7.847 min Scan# 1002
Delta R.T. 0.065 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion: 41	Resp: 6846
Ion Ratio	Lower Upper
41 100	
39 61.3	42.6 64.0
67 0.0	77.5 116.3#
52 0.0	28.9 43.3#

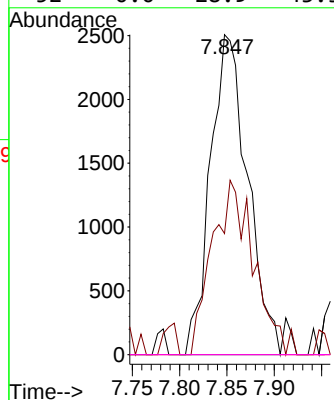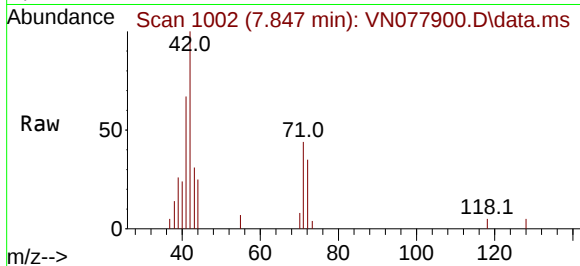

#44
Trichloroethene
Concen: 0.282 ug/l
RT: 9.365 min Scan# 1260
Delta R.T. 0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 130	Resp: 1627
Ion Ratio	Lower Upper
130 100	
95 56.2	0.0 204.6



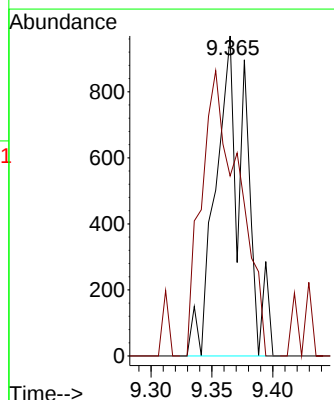
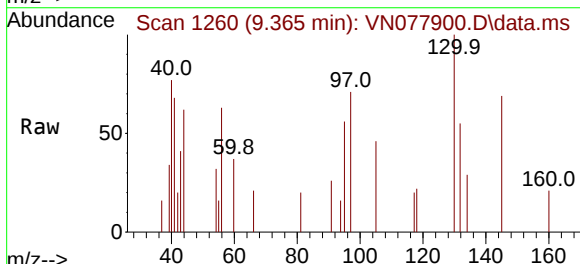




#50
Toluene-d8
Concen: 49.766 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion: 98 Resp: 1010464
Ion Ratio Lower Upper
98 100
100 62.6 52.0 78.0

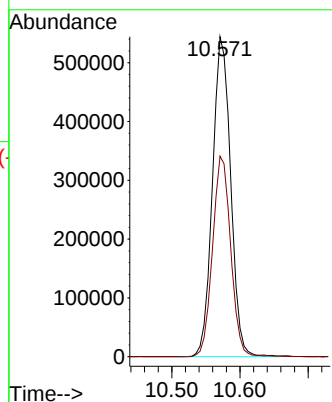

#51
4-Methyl-2-Pentanone
Concen: 0.369 ug/l
RT: 10.459 min Scan# 1446
Delta R.T. 0.012 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 43 Resp: 2467
Ion Ratio Lower Upper
43 100
58 26.7 36.6 54.8#


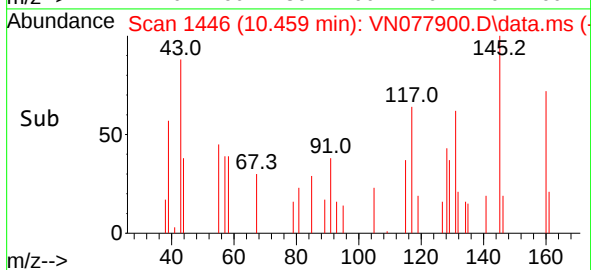
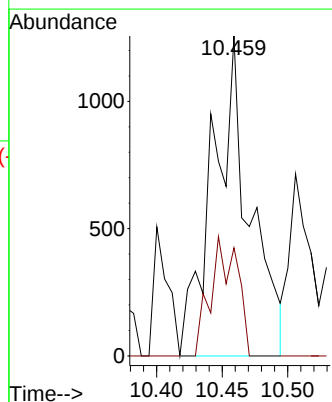
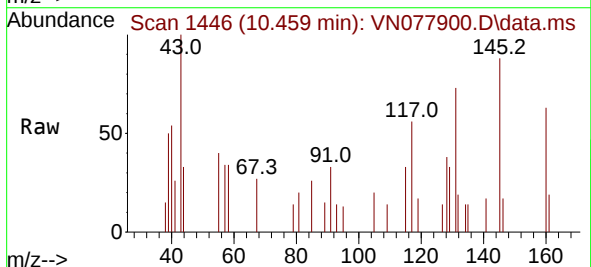




#52
Toluene
Concen: 0.323 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion: 92 Resp: 4584
Ion Ratio Lower Upper
92 100
91 188.2 137.4 206.0



#59
2-Hexanone
Concen: 0.311 ug/l
RT: 11.200 min Scan# 1572
Delta R.T. 0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 43 Resp: 1535
Ion Ratio Lower Upper
43 100
58 20.3 31.7 95.1#




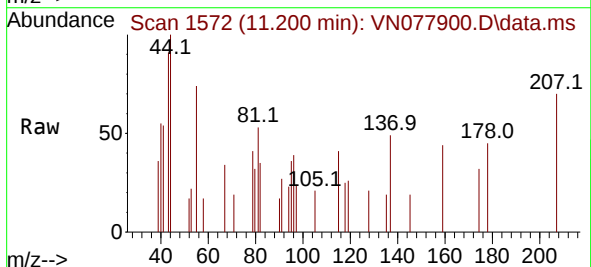


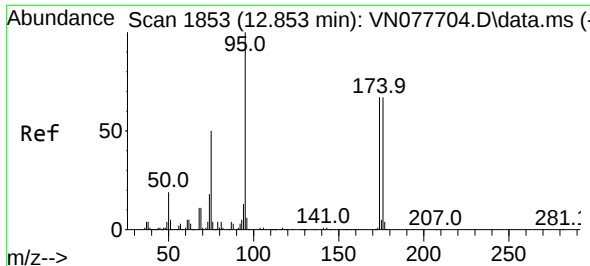

#62
4-Bromofluorobenzene
Concen: 49.271 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion: 95 Resp: 353324
Ion Ratio Lower Upper
95 100
174 73.6 0.0 143.8
176 69.8 0.0 135.8

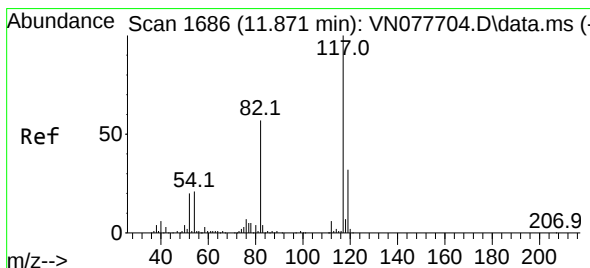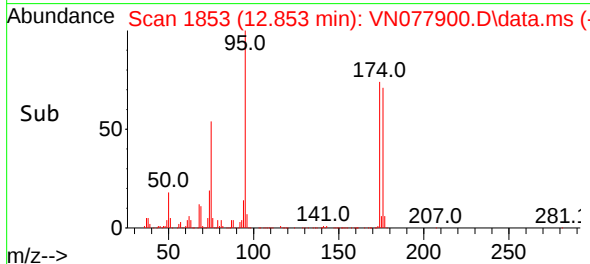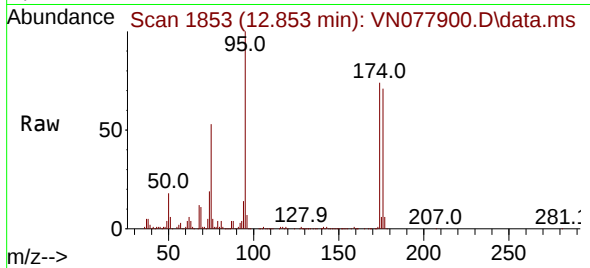

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1686
Delta R.T. 0.001 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27


Tgt Ion: 117 Resp: 718090
Ion Ratio Lower Upper
117 100
82 55.5 44.0 66.0
119 31.8 25.6 38.4

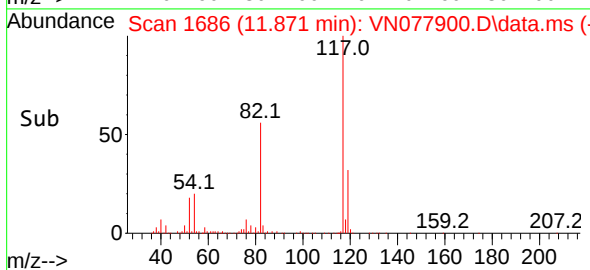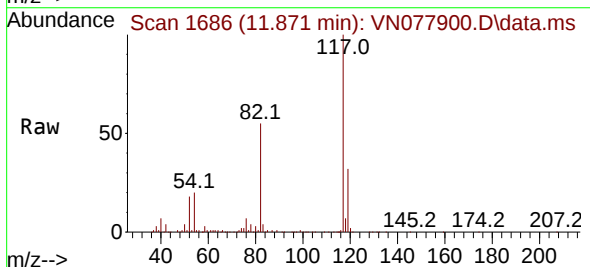



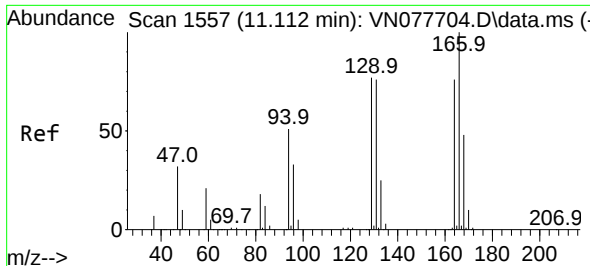


#64
Tetrachloroethene
Concen: 0.312 ug/l
RT: 11.106 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523



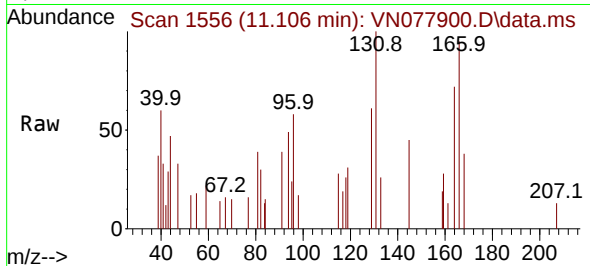



Tgt Ion:164	Resp:	1565
Ion	Ratio	Lower Upper
164	100	
166	131.3	101.4 152.0
129	84.2	82.4 123.6
131	98.6	78.2 117.4

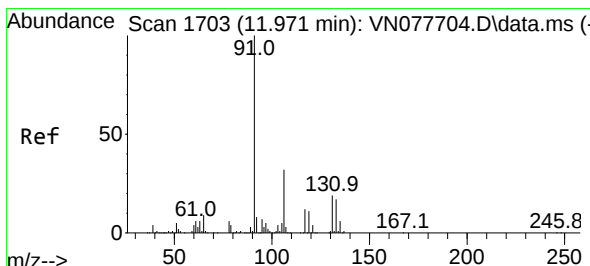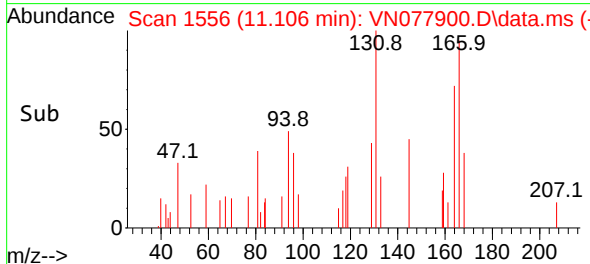

#67
Ethyl Benzene
Concen: 0.213 ug/l
RT: 11.971 min Scan# 1703
Delta R.T. 0.001 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 91	Resp:	5935
Ion	Ratio	Lower Upper
91	100	
106	18.3	25.6 38.4#


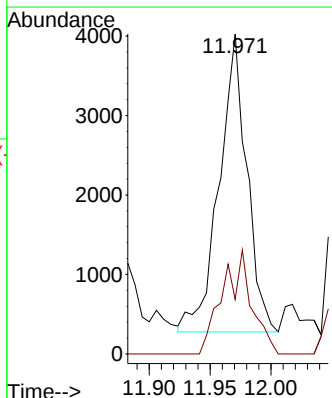
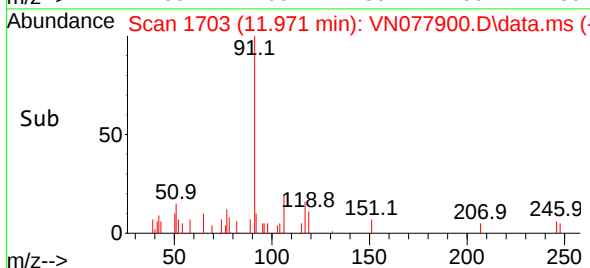
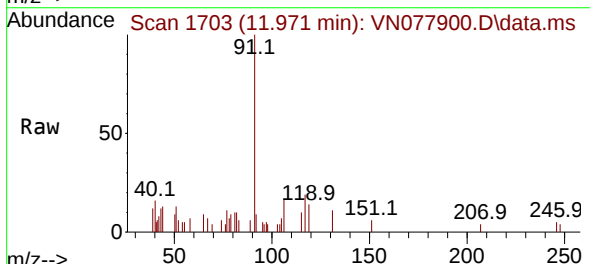




#68
m/p-Xylenes
Concen: 0.849 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. -0.005 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion:106 Resp: 8974
Ion Ratio Lower Upper
106 100
91 188.2 159.6 239.4

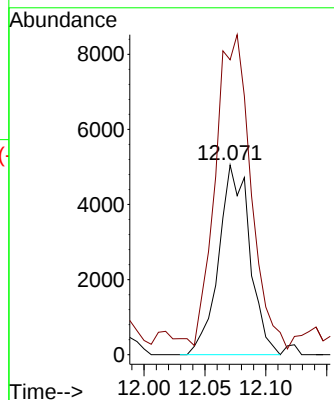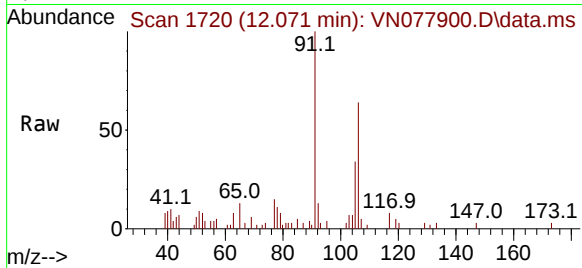

#69
o-Xylene
Concen: 0.488 ug/l
RT: 12.412 min Scan# 1778
Delta R.T. 0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion:106 Resp: 5078
Ion Ratio Lower Upper
106 100
91 202.3 105.2 315.5


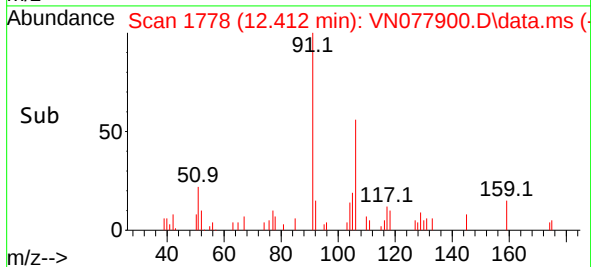
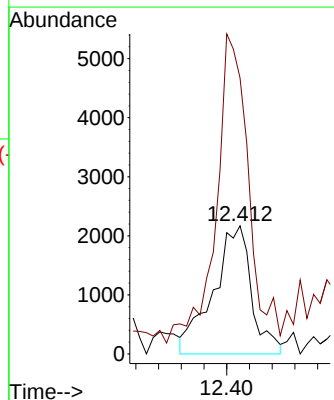
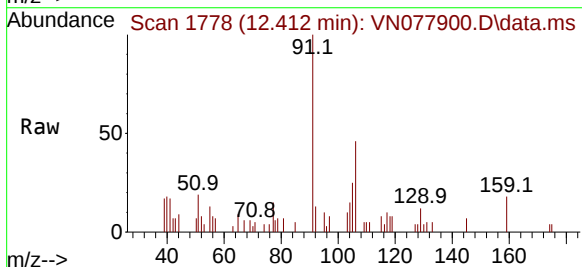


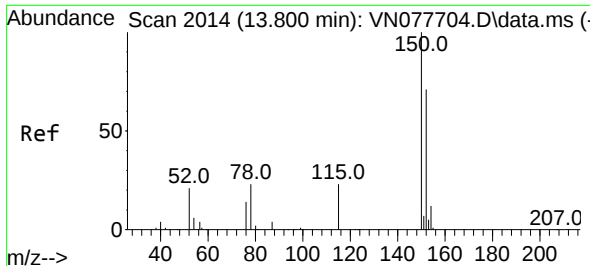

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.800 min Scan# 2014
 Delta R.T. -0.000 min
 Lab File: VN077900.D
 Acq: 25 May 2023 14:27




Instrument :
 MSVOA_N
 ClientSampleId :
 OILY-WATER-0523


Tgt Ion:152 Resp: 285604
 Ion Ratio Lower Upper
 152 100
 115 62.2 32.3 96.8
 150 154.0 0.0 355.8

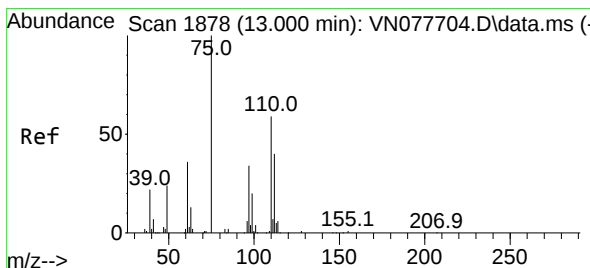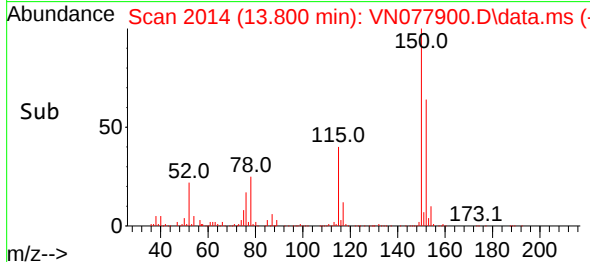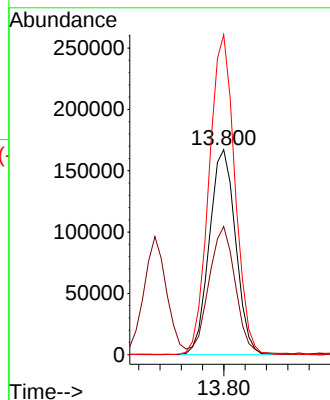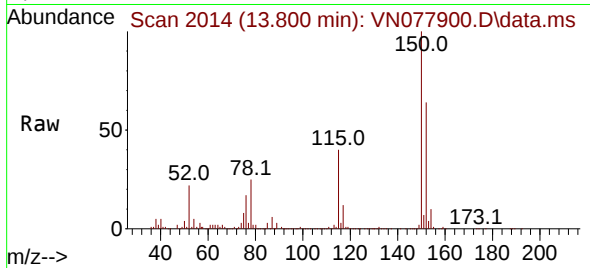

#76
 1,2,3-Trichloropropane
 Concen: 25.590 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.147 min
 Lab File: VN077900.D
 Acq: 25 May 2023 14:27

Tgt Ion: 75 Resp: 183031
 Ion Ratio Lower Upper
 75 100
 77 1.7 84.5 253.5#

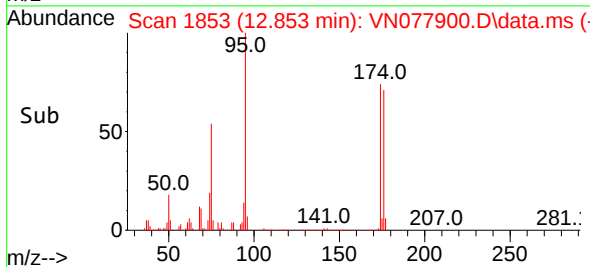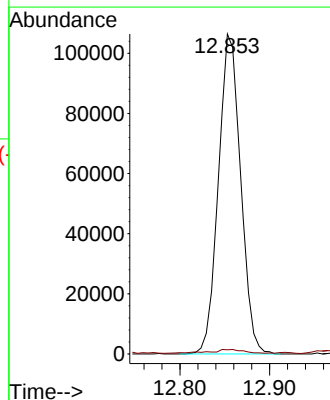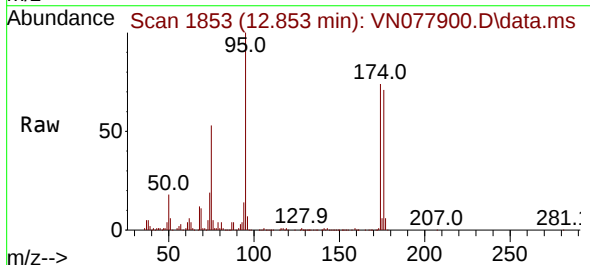



#80

1,3,5-Trimethylbenzene

Concen: 0.485 ug/l

RT: 13.176 min Scan# 1909

Delta R.T. -0.006 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27

Instrument :

MSVOA_N

ClientSampleId :





OILY-WATER-0523

Tgt Ion:105 Resp: 10045

Ion Ratio Lower Upper

105 100

120 52.6 24.1 72.3



#81

trans-1,4-Dichloro-2-butene

Concen: 81.798 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN077900.D

Acq: 25 May 2023 14:27




Tgt Ion: 75 Resp: 183031


Ion Ratio Lower Upper

75 100

53 0.2 67.4 101.2#

89 0.1 38.8 58.2#


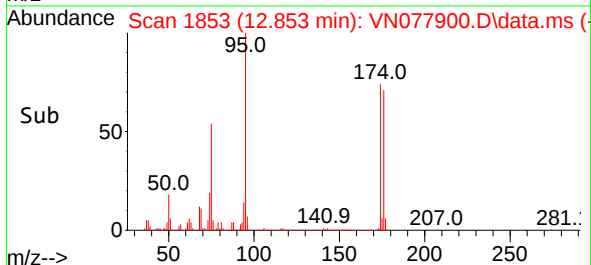
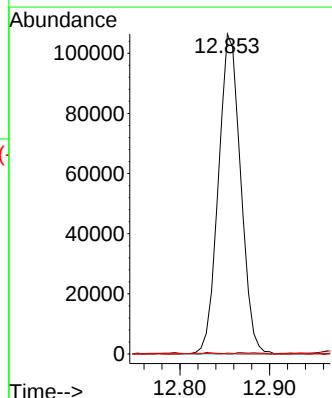
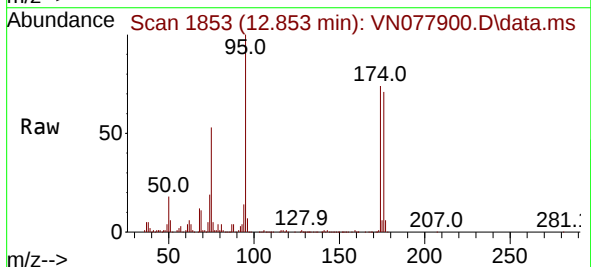




#84
1,2,4-Trimethylbenzene
Concen: 1.370 ug/l
RT: 13.488 min Scan# 1961
Delta R.T. 0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion:105 Resp: 27889
Ion Ratio Lower Upper
105 100
120 39.2 22.0 66.0

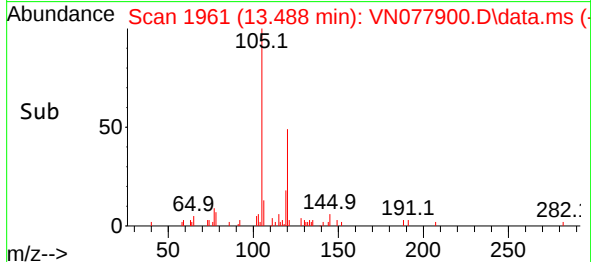

#86
p-Isopropyltoluene
Concen: 87.266 ug/l
RT: 13.735 min Scan# 2003
Delta R.T. 0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion:119 Resp: 1785983
Ion Ratio Lower Upper
119 100
134 25.8 12.6 37.8
91 24.9 12.4 37.2


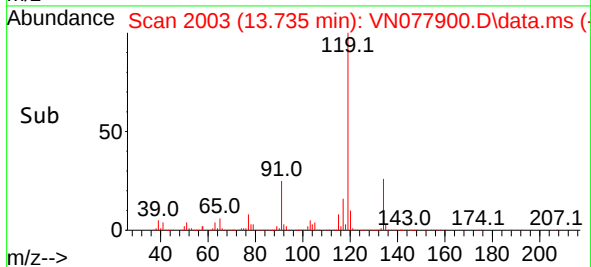

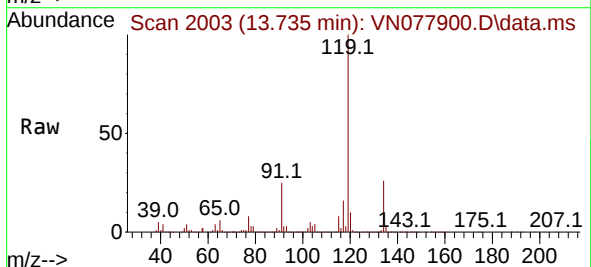




#87
1,3-Dichlorobenzene
Concen: 0.242 ug/l
RT: 13.741 min Scan# 2004
Delta R.T. 0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27




Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523


Tgt Ion:146 Resp: 2515
Ion Ratio Lower Upper
146 100
111 44.0 22.1 66.3
148 0.0 32.0 96.0#

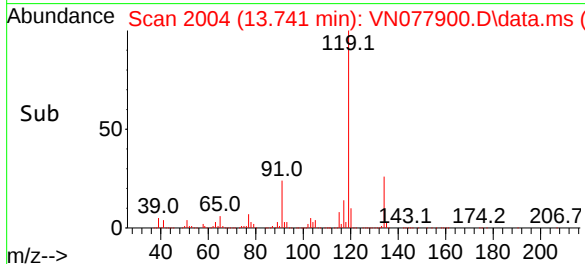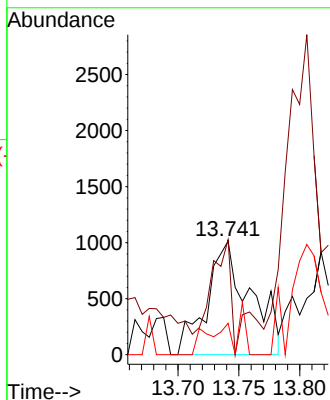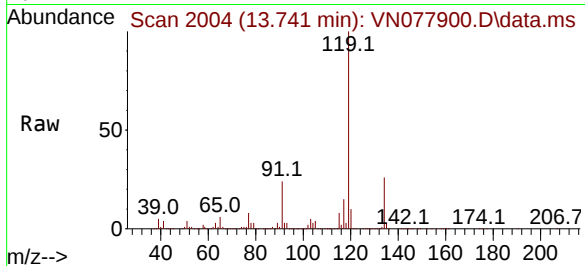

#89
n-Butylbenzene
Concen: 0.290 ug/l
RT: 13.953 min Scan# 2040
Delta R.T. -0.111 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion: 91 Resp: 5459
Ion Ratio Lower Upper
91 100
92 43.1 26.4 79.0
134 23.6 12.6 37.6


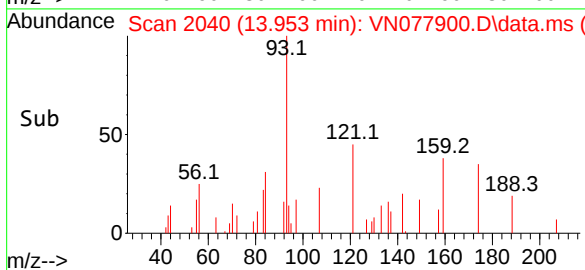
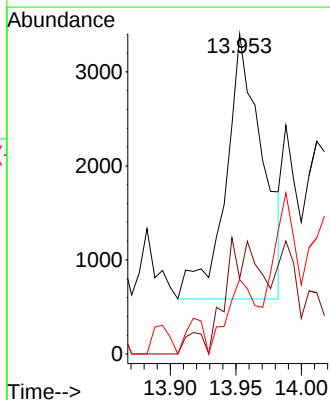
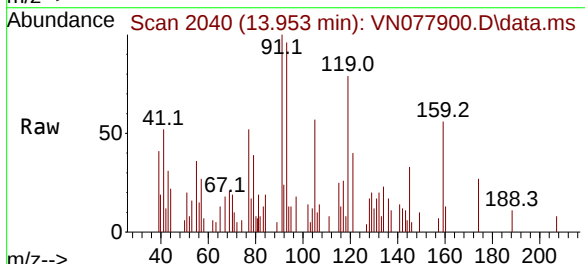




#90
Hexachloroethane
Concen: 0.585 ug/l
RT: 14.335 min Scan# 2106
Delta R.T. -0.006 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Instrument :
MSVOA_N
ClientSampleId :
OILY-WATER-0523

Tgt Ion:117 Resp: 1966
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

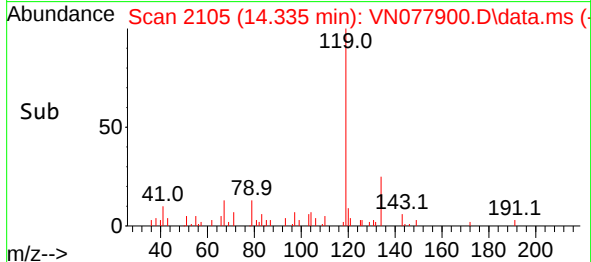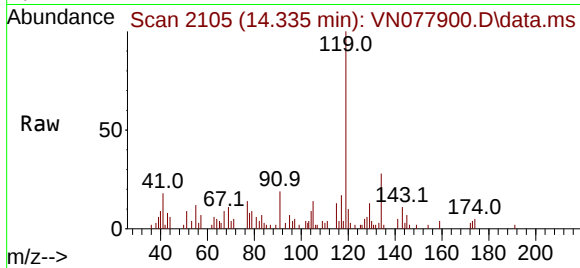

#95
Naphthalene
Concen: 16.732 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. -0.000 min
Lab File: VN077900.D
Acq: 25 May 2023 14:27

Tgt Ion:128 Resp: 326665
Ion Ratio Lower Upper
128 100
127 13.5 10.0 15.0
129 10.7 8.7 13.1

