

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052523\
 Data File : VN077904.D
 Acq On : 25 May 2023 16:02
 Operator : JC\MD
 Sample : 02944-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BP-VPB-RW11-GW-318-320

Quant Time: May 26 04:33:43 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 16 04:07:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	401636	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	741762	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	635125	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	198584	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	274544	45.685	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	91.360%
35) Dibromofluoromethane	8.171	113	233698	48.315	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.640%
50) Toluene-d8	10.576	98	904378	48.576	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	97.160%
62) 4-Bromofluorobenzene	12.859	95	292593	44.498	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	89.000%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052523\
Data File : VN077904.D
Acq On : 25 May 2023 16:02
Operator : JC\MD
Sample : 02944-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW11-GW-318-320

Quant Time: May 26 04:33:43 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Quant Title : SW846 8260
QLast Update : Tue May 16 04:07:42 2023
Response via : Initial Calibration




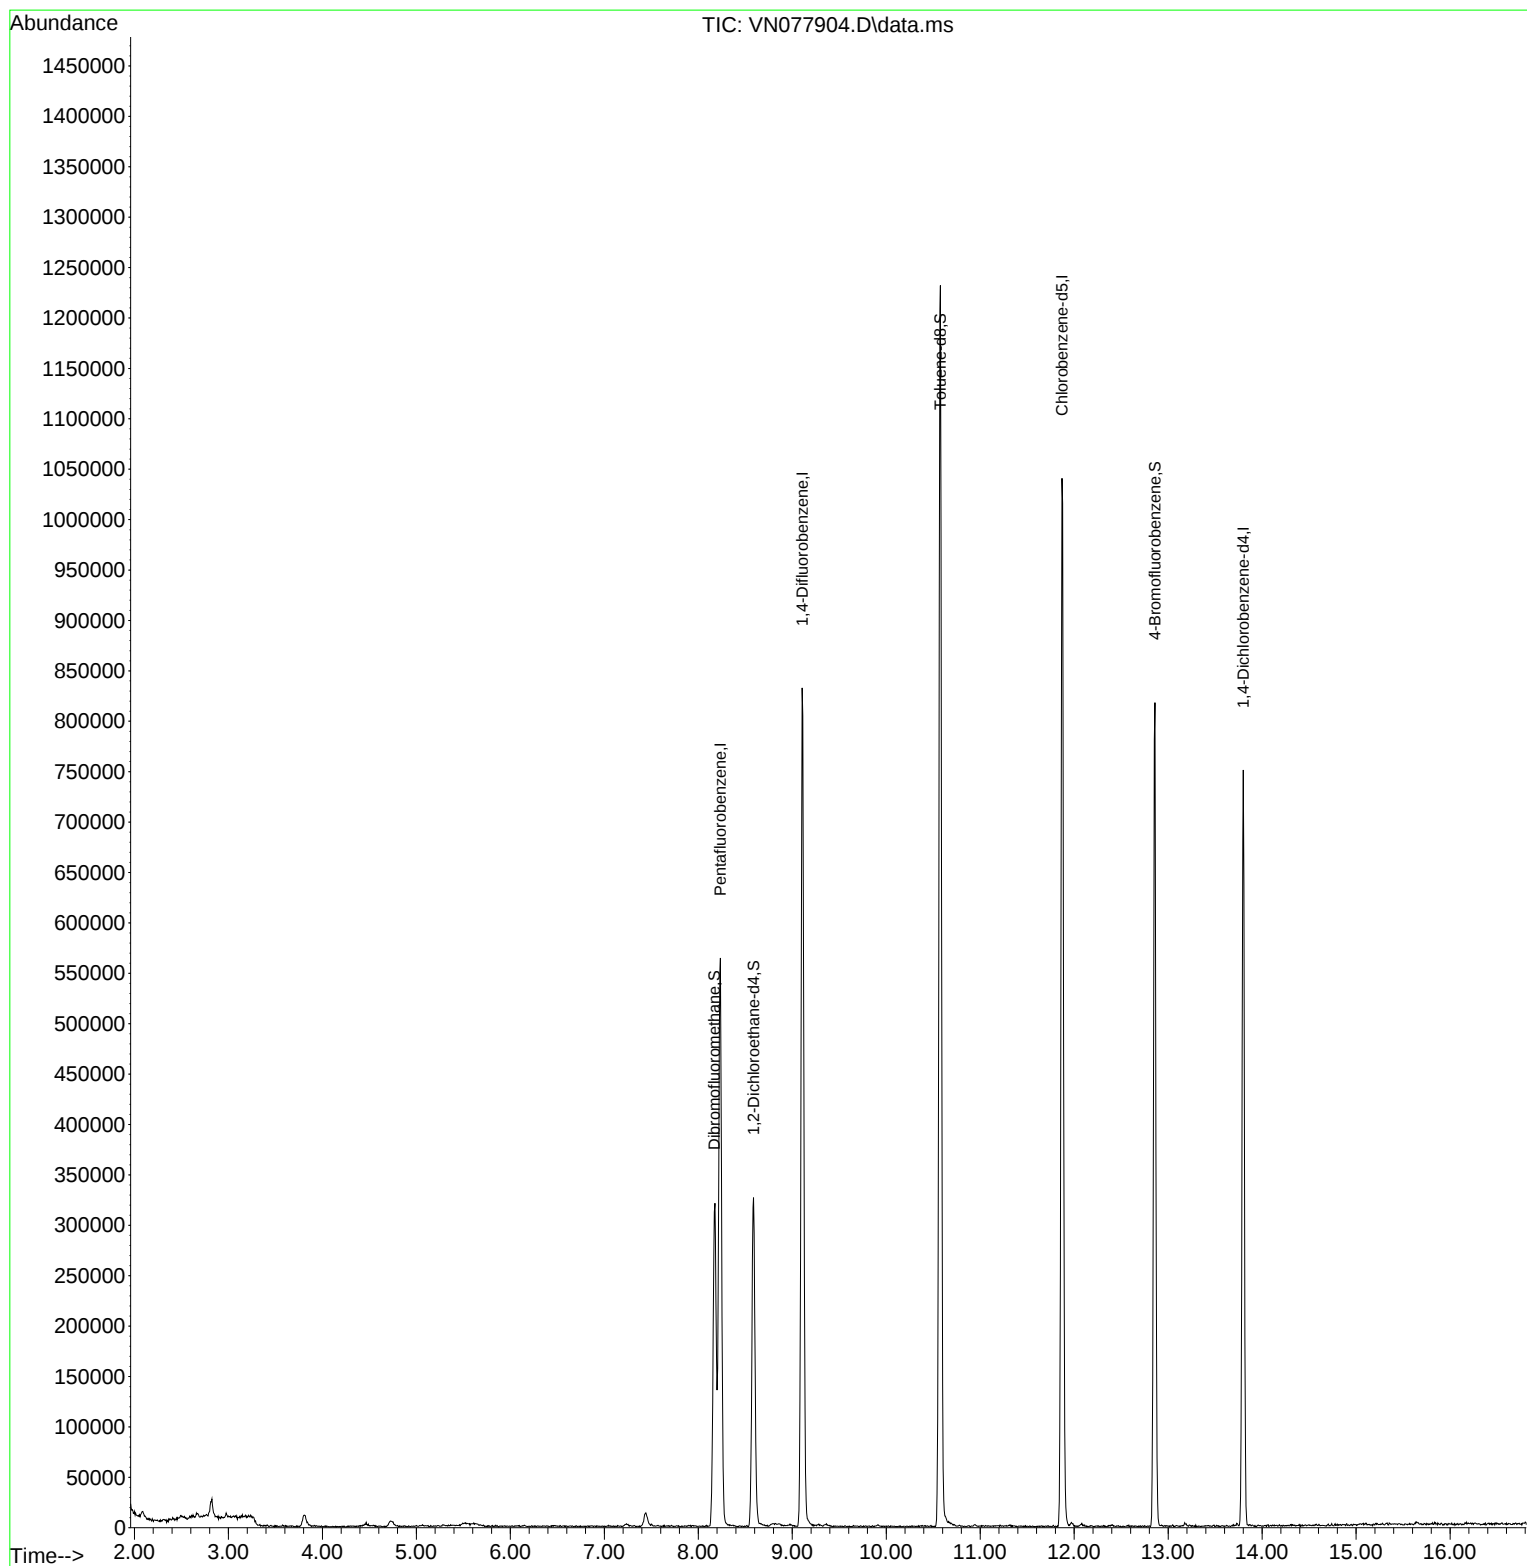


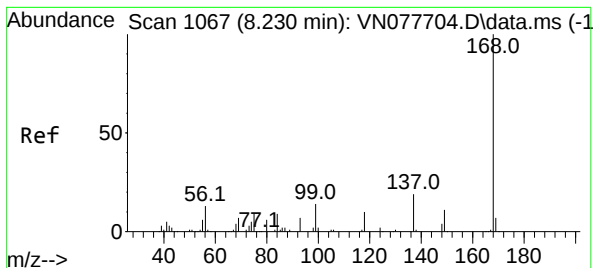

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1067
Delta R.T. 0.005 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW11-GW-318-320


Tgt Ion:168 Resp: 401636
Ion Ratio Lower Upper
168 100
99 66.4 53.0 79.6

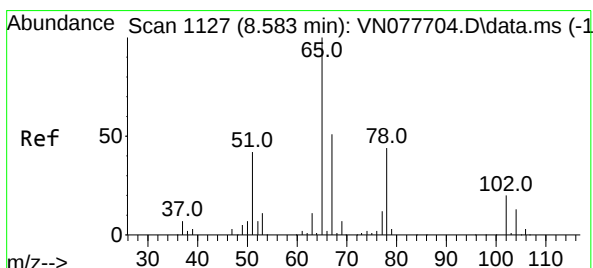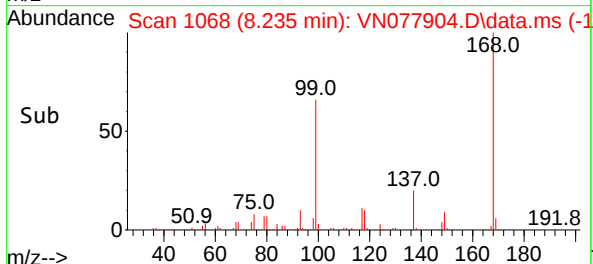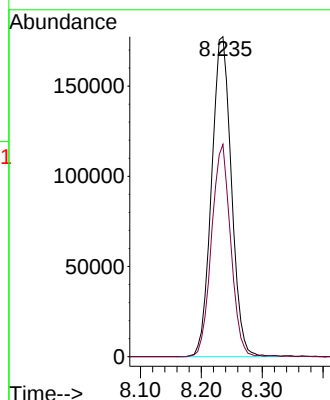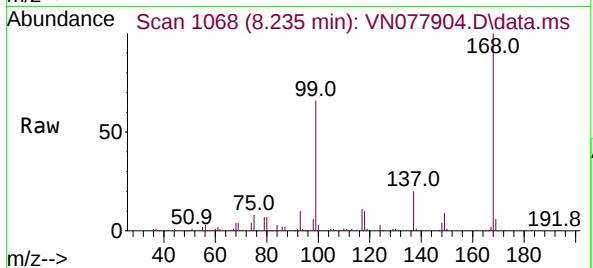

#33
1,2-Dichloroethane-d4
Concen: 45.685 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.006 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02

Tgt Ion: 65 Resp: 274544
Ion Ratio Lower Upper
65 100
67 52.3 0.0 106.6

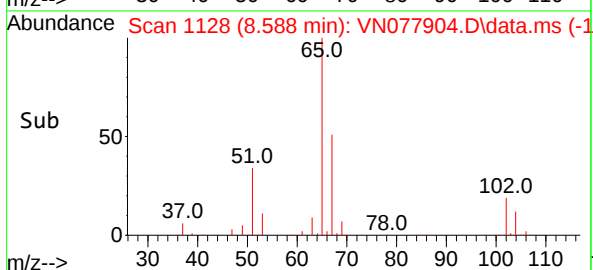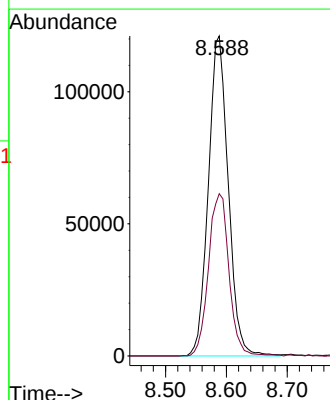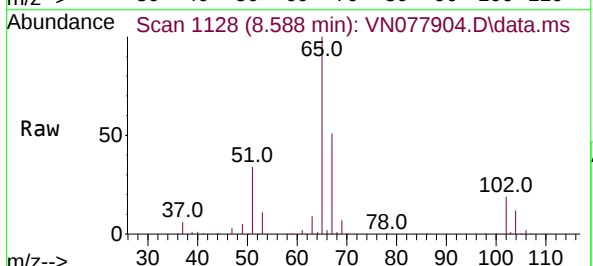

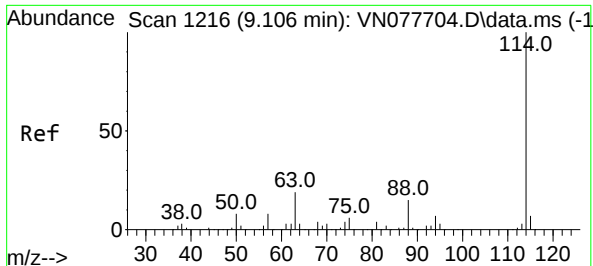

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN077904.D

Acq: 25 May 2023 16:02

Instrument :

MSVOA_N

ClientSampleId :

BP-VPB-RW11-GW-318-320





Tgt Ion:114 Resp: 741762

Ion Ratio Lower Upper

114 100

63 18.9 0.0 36.4

88 15.5 0.0 30.6

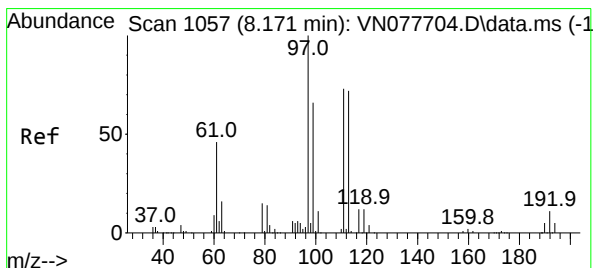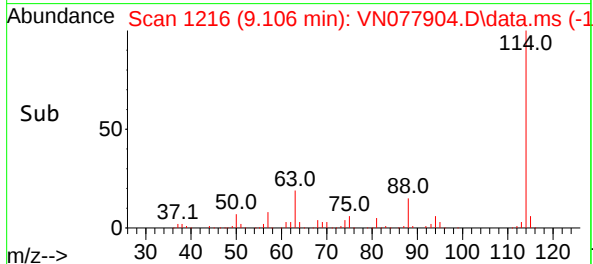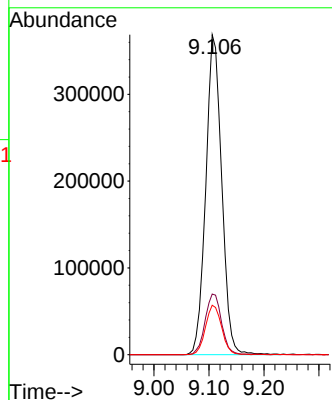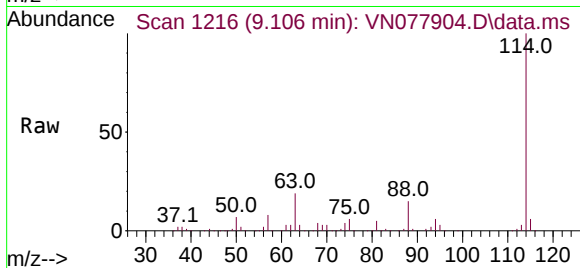

#35

Dibromofluoromethane

Concen: 48.315 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VN077904.D

Acq: 25 May 2023 16:02




Tgt Ion:113 Resp: 233698


Ion Ratio Lower Upper

113 100

111 103.4 82.6 123.8

192 16.3 12.7 19.1


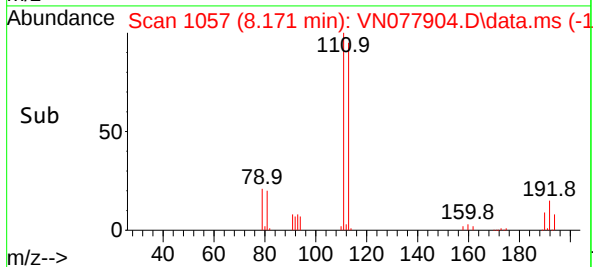
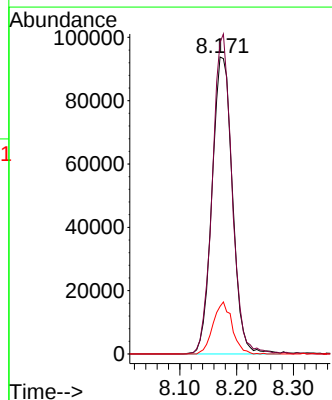
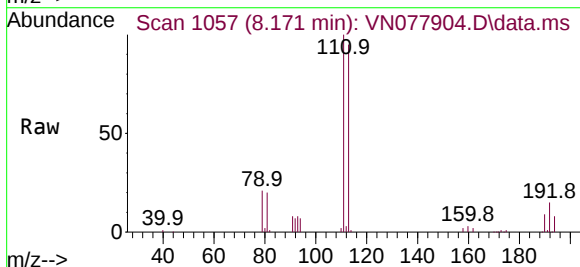


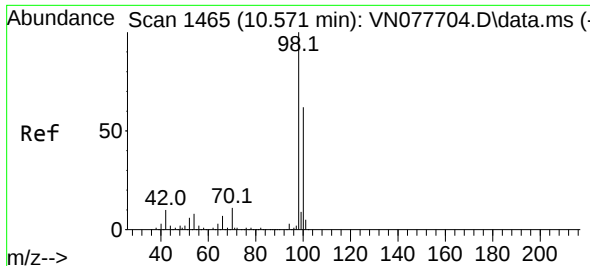

#50
Toluene-d8
Concen: 48.576 ug/l
RT: 10.576 min Scan# 1465
Delta R.T. 0.005 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02




Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW11-GW-318-320


Tgt Ion: 98 Resp: 904378
Ion Ratio Lower Upper
98 100
100 63.3 52.0 78.0

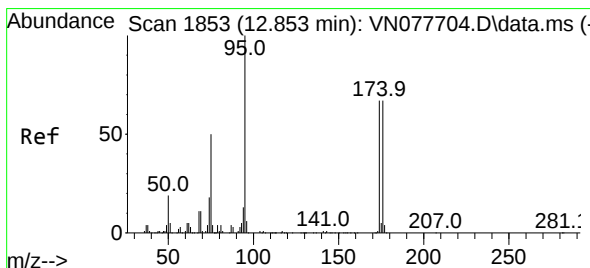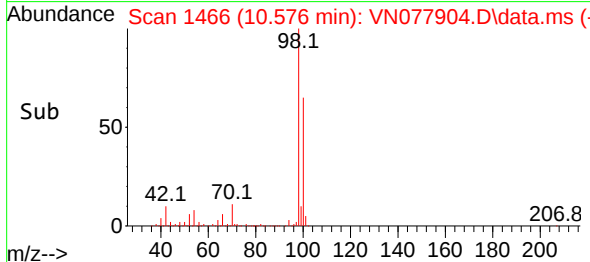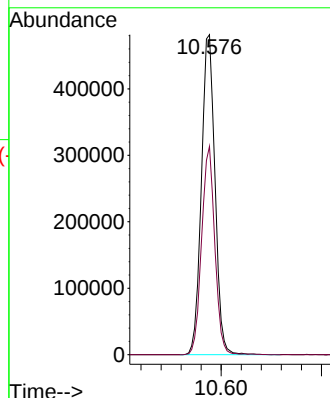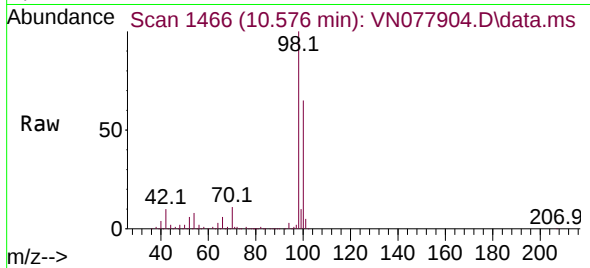

#62
4-Bromofluorobenzene
Concen: 44.498 ug/l
RT: 12.859 min Scan# 1854
Delta R.T. 0.006 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02

Tgt Ion: 95 Resp: 292593
Ion Ratio Lower Upper
95 100
174 71.5 0.0 143.8
176 69.9 0.0 135.8


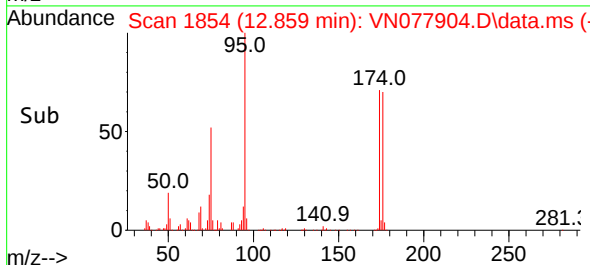
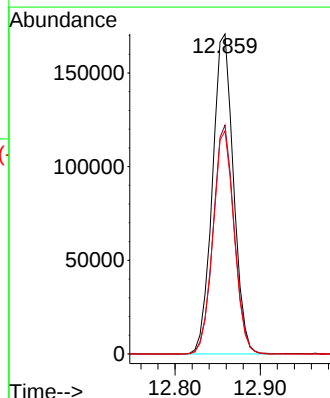
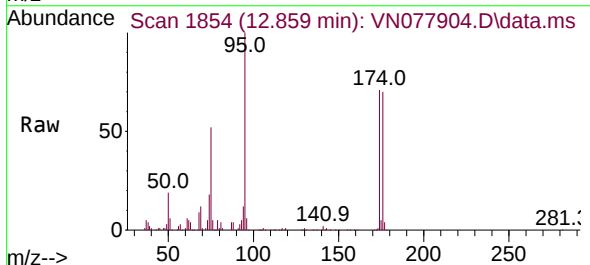


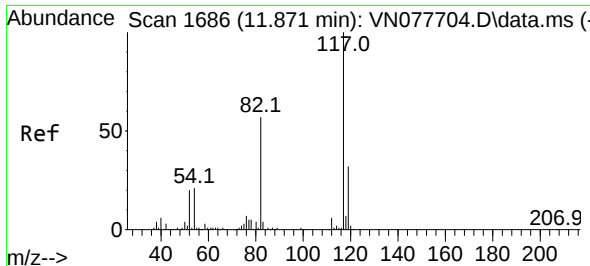

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02

Instrument :
MSVOA_N
ClientSampleId :
BP-VPB-RW11-GW-318-320

Tgt Ion:117 Resp: 635125
Ion Ratio Lower Upper
117 100
82 57.5 44.0 66.0
119 31.2 25.6 38.4

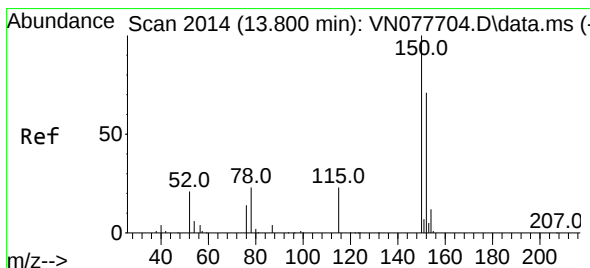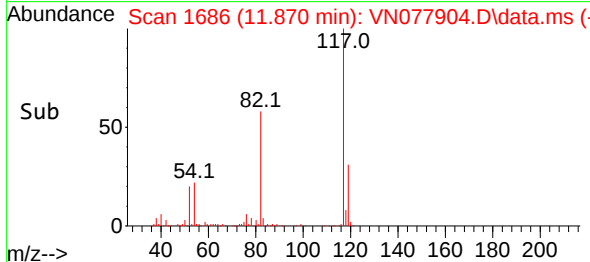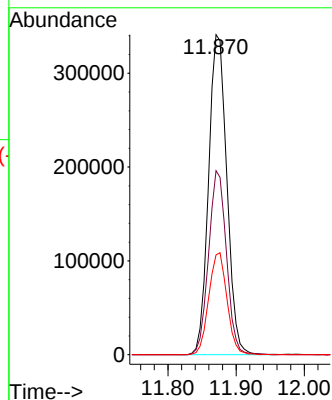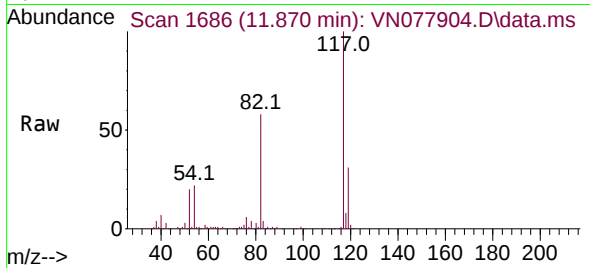

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN077904.D
Acq: 25 May 2023 16:02

Tgt Ion:152 Resp: 198584
Ion Ratio Lower Upper
152 100
115 64.7 32.3 96.8
150 160.1 0.0 355.8

