
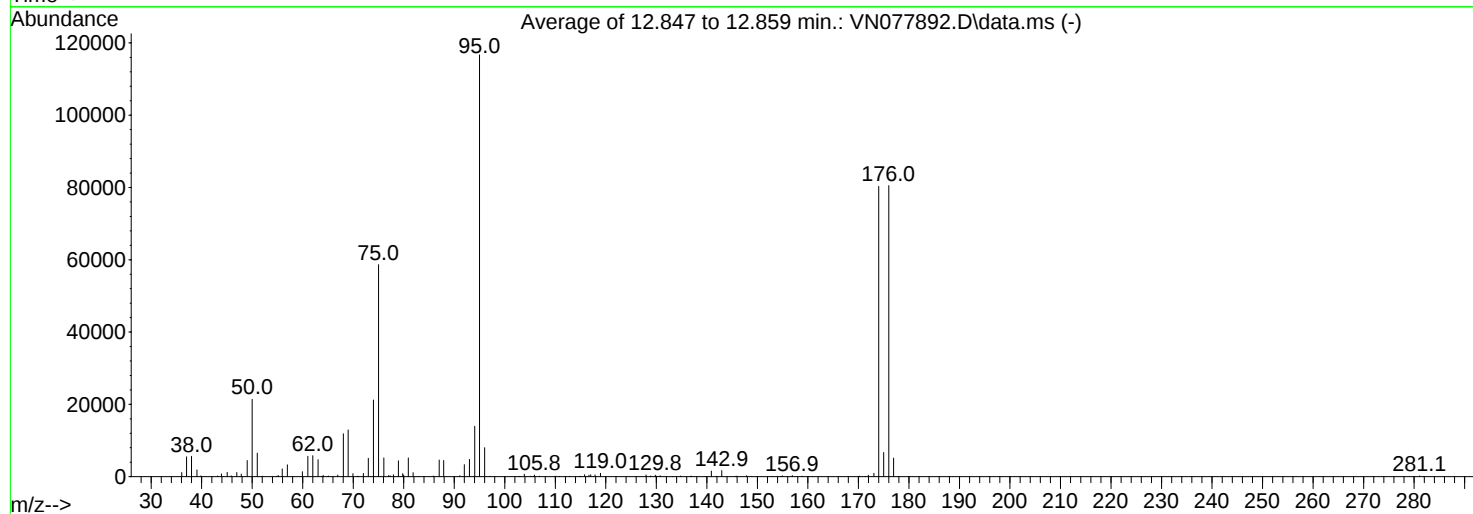


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052523\
Data File : VN077892.D
Acq On : 25 May 2023 09:33
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

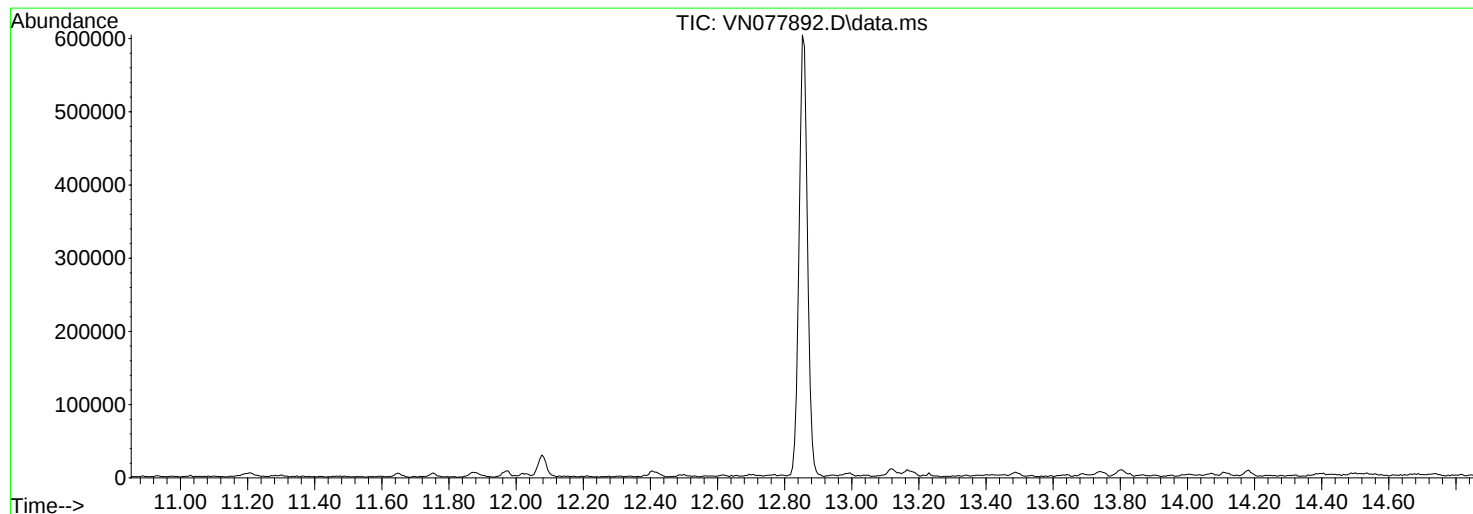

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1841

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	21405	PASS
75	95	30	60	50.3	58664	PASS
95	95	100	100	100.0	116701	PASS
96	95	5	9	6.9	8011	PASS
173	174	0.00	2	1.1	923	PASS
174	95	50	100	68.8	80312	PASS
175	174	5	9	8.3	6673	PASS
176	174	95	101	100.3	80520	PASS
177	176	5	9	6.4	5120	PASS

Average of 12.847 to 12.859 min.: VN077892.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	1168	49.00	4464	62.00	5787	70.90	111
37.00	5502	50.00	21405	63.05	4677	71.10	5
38.00	5612	51.00	6519	63.80	79	72.00	87
39.05	1870	51.95	118	64.05	369	73.00	509
39.85	243	54.90	151	64.80	112	74.00	21224
43.15	175	55.15	304	65.10	188	75.00	58664
43.90	759	55.95	2129	65.90	57	76.05	5164
45.05	1211	56.95	3295	66.95	447	77.00	320
45.85	205	58.00	60	68.05	11877	77.30	217
46.95	1145	59.95	1382	69.00	12947	77.95	530
47.85	723	61.00	5611	69.95	840	78.95	4366

Average of 12.847 to 12.859 min.: VN077892.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.80	857	94.05	13924	109.95	132	128.85	202
80.00	465	95.00	116701	110.80	96	129.80	383
80.90	5187	96.00	8011	112.80	91	130.10	152
81.85	1118	97.10	74	114.80	64	130.75	268
83.00	64	102.80	71	115.00	85	133.20	67
85.85	200	103.00	67	115.80	515	134.80	166
87.00	4619	103.85	679	116.65	414	135.00	56
87.90	4452	105.15	133	117.00	526	136.70	98
91.10	270	105.70	108	117.85	505	136.95	152
92.00	3315	105.85	434	118.95	948	139.70	61
93.00	4797	106.90	116	127.95	472	140.90	1553

Average of 12.847 to 12.859 min.: VN077892.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.85	153	160.90	50	281.80	101		
142.95	1705	170.25	128				
145.80	201	171.40	85				
147.85	271	171.95	386				
148.90	91	173.05	923				
150.00	54	174.00	80312				
153.00	62	175.00	6673				
154.70	113	176.00	80520				
154.95	220	176.95	5120				
156.90	325	177.80	60				
158.85	142	281.10	210				