


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052621\
 Data File : VN067165.D
 Acq On : 26 May 2021 9:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
 Title : SW846 8260
 Last Update : Fri May 21 17:24:08 2021

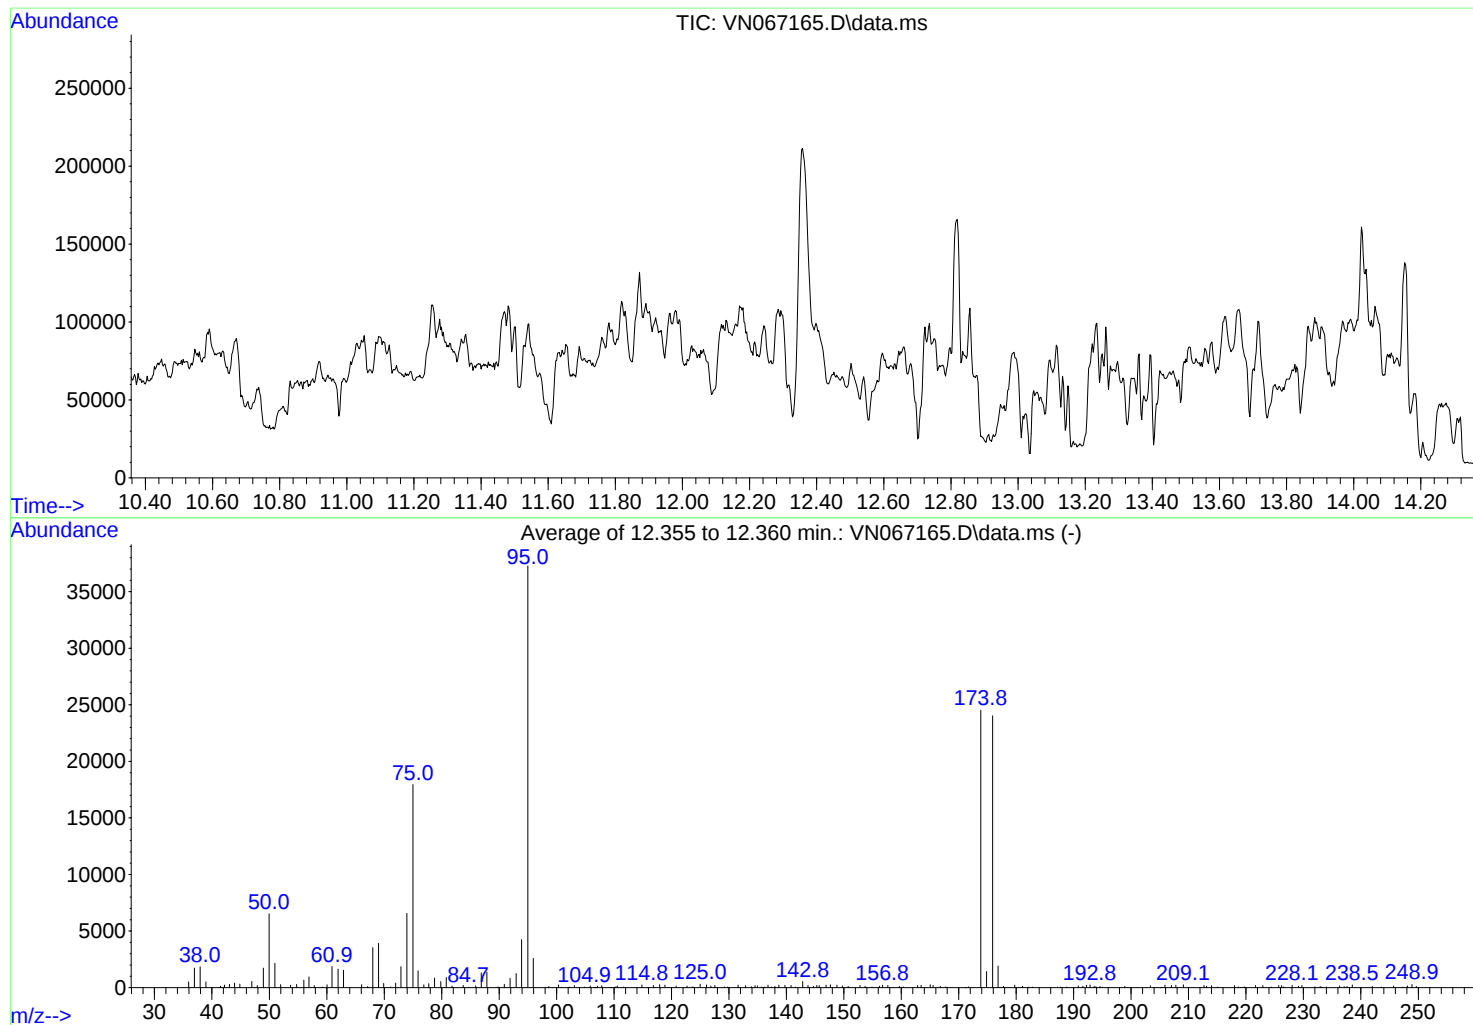

AutoFind: Scans 3958, 3959, 3960; Background Corrected with Scan 3941

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6521	PASS
75	95	30	60	48.1	17949	PASS
95	95	100	100	100.0	37282	PASS
96	95	5	9	6.9	2591	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	65.8	24525	PASS
175	174	5	9	5.8	1434	PASS
176	174	95	101	98.0	24027	PASS
177	176	5	9	7.9	1906	PASS