

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052622\
 Data File : VN072641.D
 Acq On : 26 May 2022 20:41
 Operator : JC\MD
 Sample : N3029-01 10X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 DSN-001-SEWER-OUTLET-001

Integration Parameters: RTEINT3.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M

Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VN072641.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	35	42	47	rBV3	7079	15933	2.59%	0.729%
2	2.751	124	130	134	rVB5	3842	7895	1.28%	0.361%
3	4.575	431	440	450	rBV3	5661	19494	3.16%	0.892%
4	7.304	897	904	913	rBV2	11037	30547	4.96%	1.397%
5	7.651	954	963	974	rBV3	79961	206392	33.50%	9.439%
6	7.810	982	990	1002	rVB4	10003	25647	4.16%	1.173%
7	8.433	1087	1096	1107	rBV	103167	229678	37.28%	10.504%
8	8.963	1178	1186	1197	rBV	181764	372074	60.39%	17.017%
9	10.439	1427	1437	1446	rBV	340868	616167	100.00%	28.181%
10	11.739	1650	1658	1673	rVB	224684	397170	64.46%	18.165%
11	12.727	1819	1826	1835	rBV	156177	265494	43.09%	12.142%


Sum of corrected areas: 2186491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052622\
Data File : VN072641.D
Acq On : 26 May 2022 20:41
Operator : JC\MD
Sample : N3029-01 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

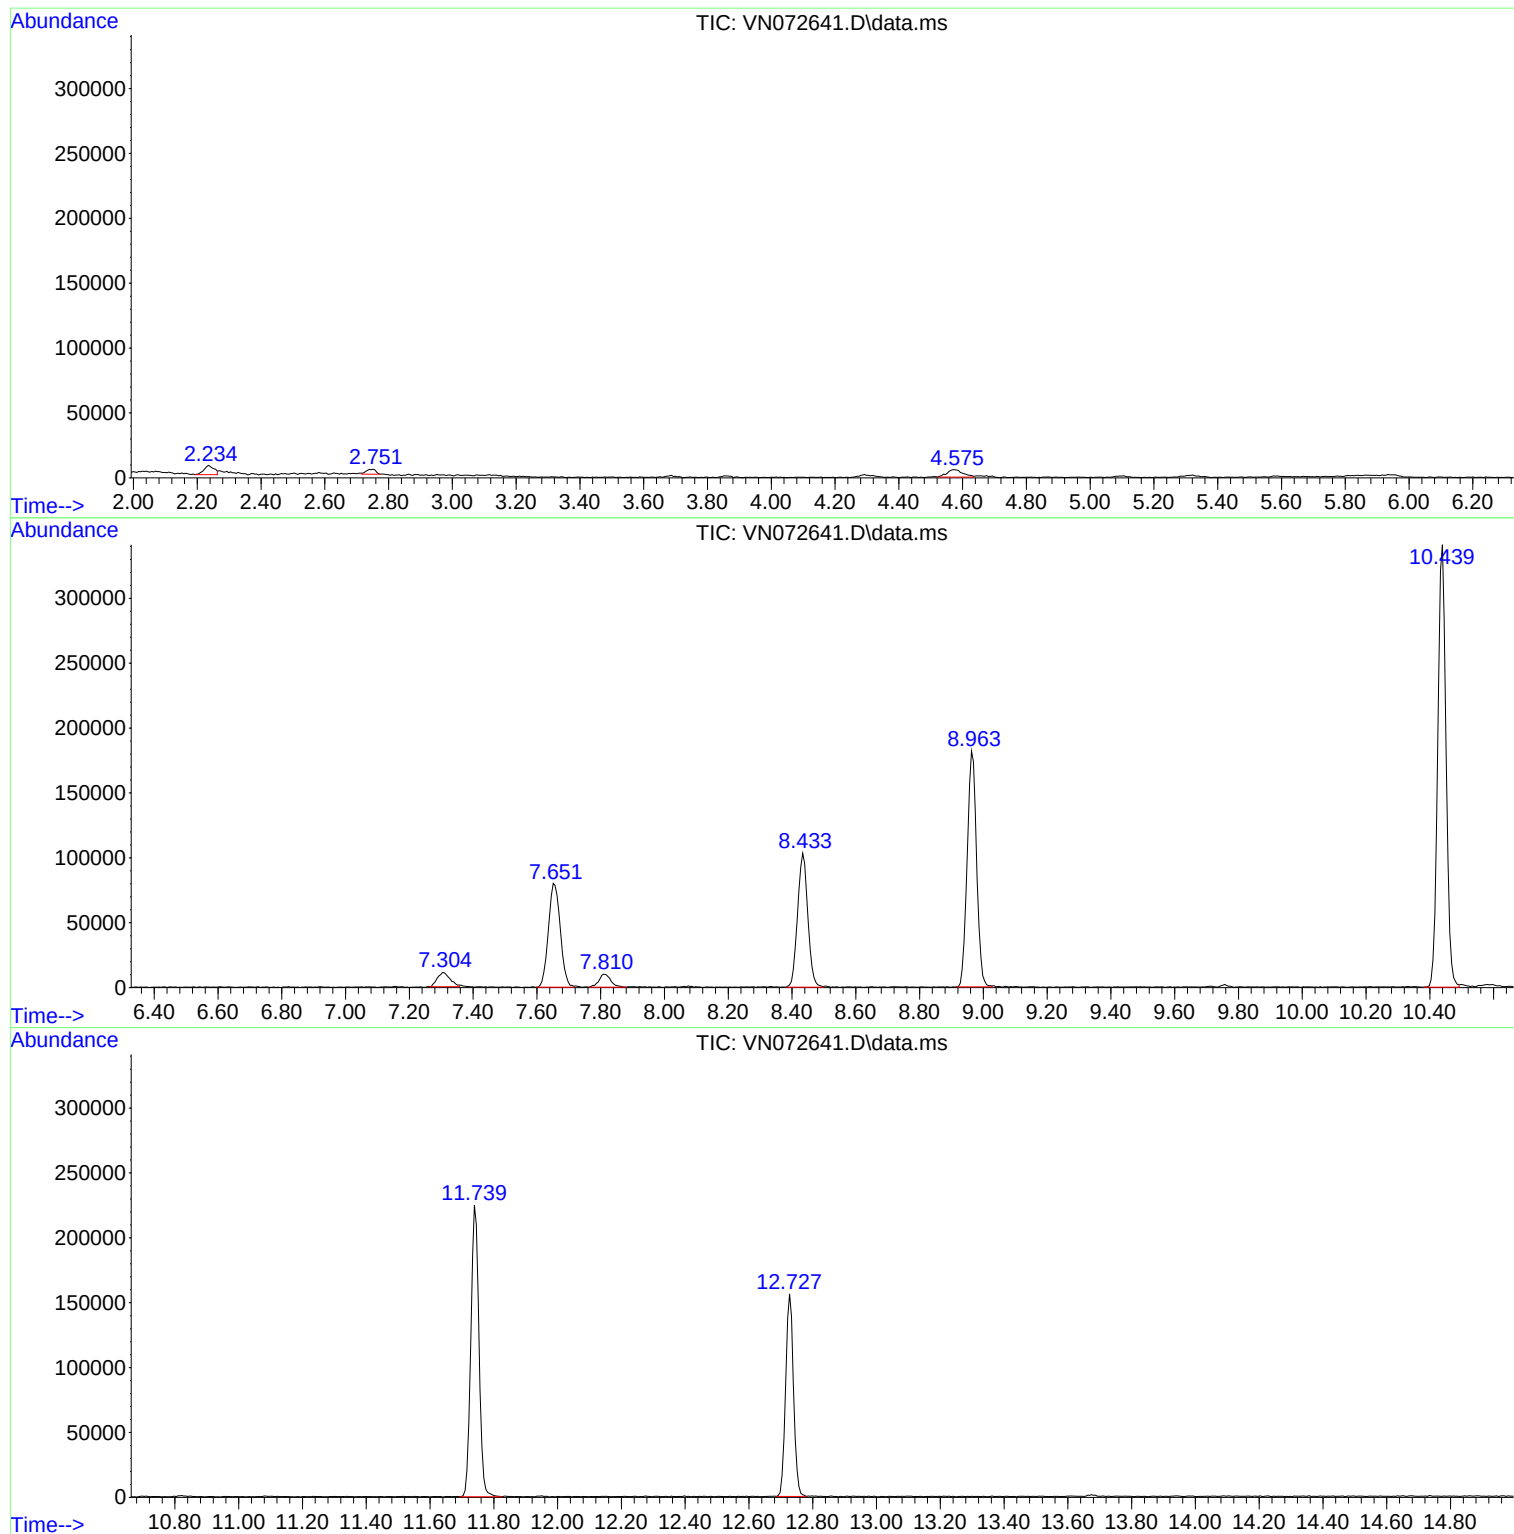

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052622\
Data File : VN072641.D
Acq On : 26 May 2022 20:41
Operator : JC\MD
Sample : N3029-01 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052622\
Data File : VN072641.D
Acq On : 26 May 2022 20:41
Operator : JC\MD
Sample : N3029-01 10X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc