
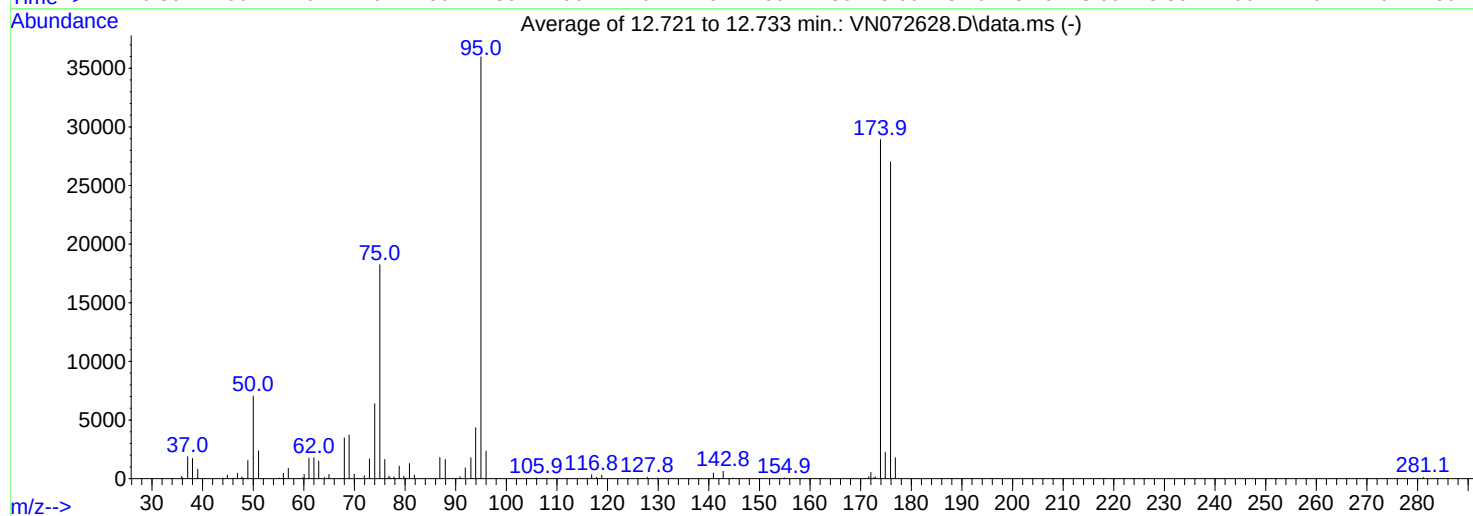


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052622\
 Data File : VN072628.D
 Acq On : 26 May 2022 13:35
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052622W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri May 27 05:07:24 2022

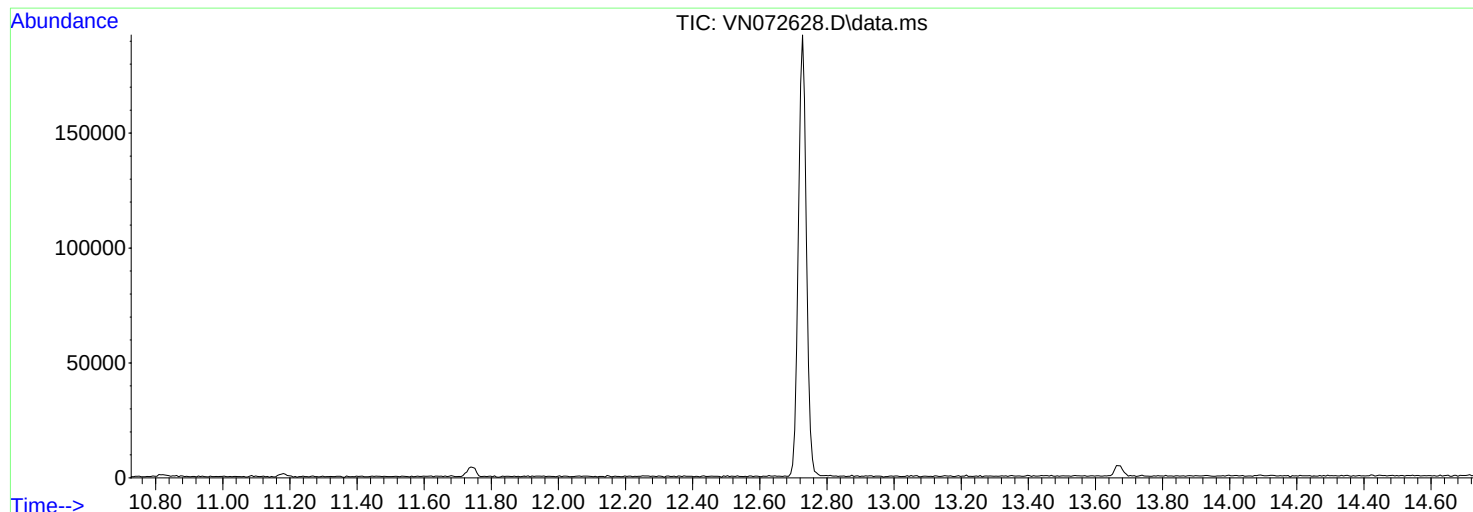

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	7047	PASS
75	95	30	60	50.7	18248	PASS
95	95	100	100	100.0	35973	PASS
96	95	5	9	6.5	2349	PASS
173	174	0.00	2	0.5	157	PASS
174	95	50	100	80.4	28912	PASS
175	174	5	9	7.8	2242	PASS
176	174	95	101	93.5	27027	FAIL*
177	176	5	9	6.6	1792	PASS