
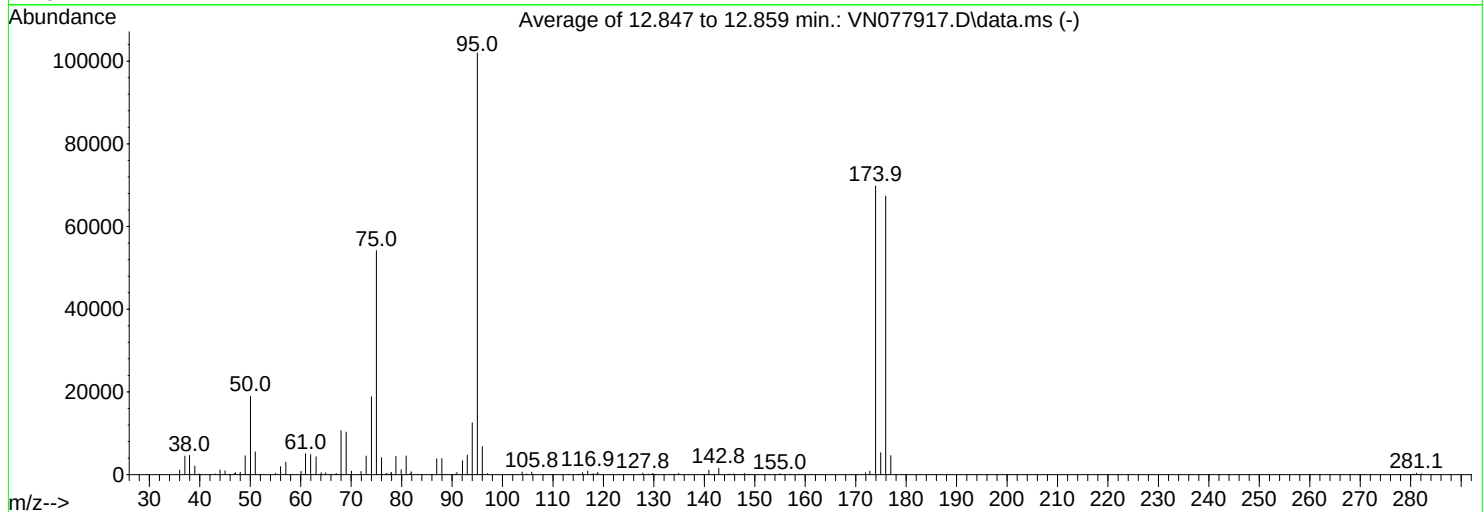


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052623\
Data File : VN077917.D
Acq On : 26 May 2023 08:10
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

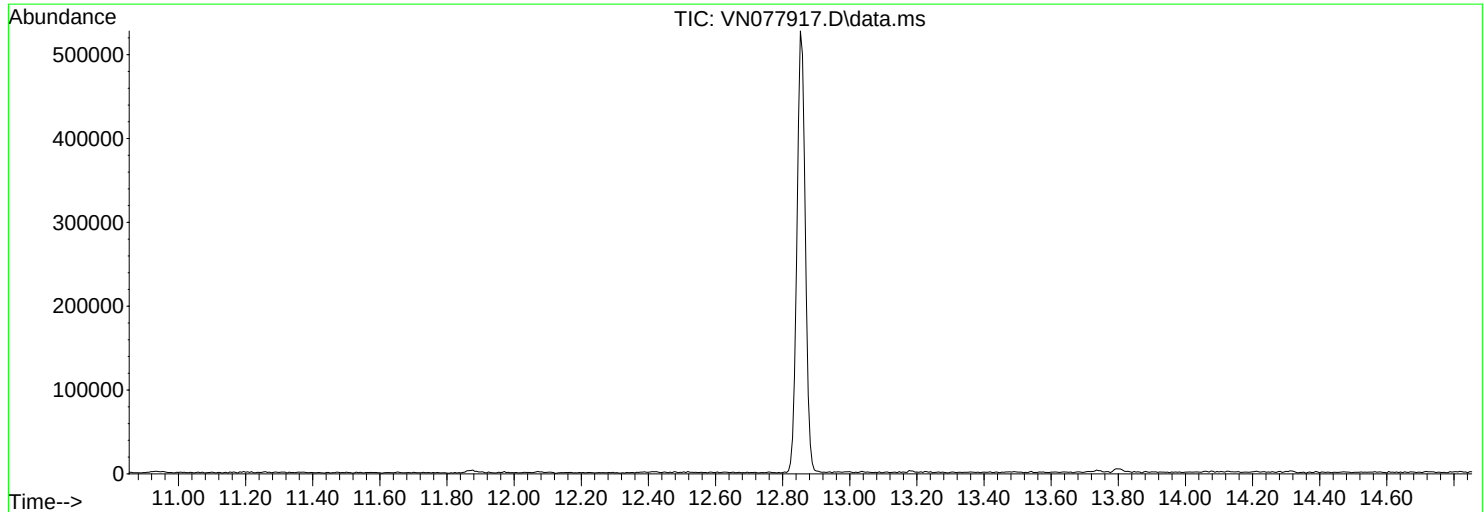

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	18976	PASS
75	95	30	60	53.1	54165	PASS
95	95	100	100	100.0	102008	PASS
96	95	5	9	6.6	6781	PASS
173	174	0.00	2	1.2	848	PASS
174	95	50	100	68.4	69792	PASS
175	174	5	9	7.6	5314	PASS
176	174	95	101	96.5	67368	PASS
177	176	5	9	6.9	4621	PASS

Average of 12.847 to 12.859 min.: VN077917.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1090	48.00	594	63.05	4350	76.00	411
37.05	4507	49.00	4553	64.05	472	76.90	14
37.95	4633	50.05	18976	64.95	435	77.10	33
39.00	2037	51.00	5491	67.05	260	77.80	22
39.90	189	51.90	122	68.00	10636	77.95	568
43.10	164	55.00	309	69.00	10291	78.85	4428
44.00	1117	56.00	1924	70.05	860	79.90	1222
45.00	932	57.05	3005	71.95	761	80.90	4540
45.80	103	60.05	816	72.95	4502	81.70	257
46.90	259	60.95	5050	74.00	18847	81.90	696
47.05	469	61.95	4822	75.00	54165	83.10	66

Average of 12.847 to 12.859 min.: VN077917.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	62	97.05	256	118.70	208	142.85	1558
86.95	3840	103.90	645	118.90	530	143.70	55
87.95	3916	104.75	143	127.80	379	144.90	170
88.80	85	105.80	631	128.90	110	145.80	195
90.70	102	109.70	58	129.75	293	147.70	71
90.95	496	113.00	60	130.00	169	147.95	260
92.05	3353	115.10	102	134.90	320	148.90	65
93.00	4711	115.85	461	136.80	85	152.10	56
94.00	12520	116.90	880	139.80	85	152.90	53
95.00	102008	117.70	117	140.90	1087	154.90	64
96.00	6781	118.00	290	141.90	106	155.00	249

Average of 12.847 to 12.859 min.: VN077917.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
157.00	114	280.90	58				
158.80	51	281.15	336				
160.90	83	282.10	187				
171.95	480						
172.80	848						
173.95	69792						
174.95	5314						
175.95	67368						
176.95	4621						
177.90	57						
280.50	138						

Instrument :

MSVOA_N

ClientSampleId :

BFB