
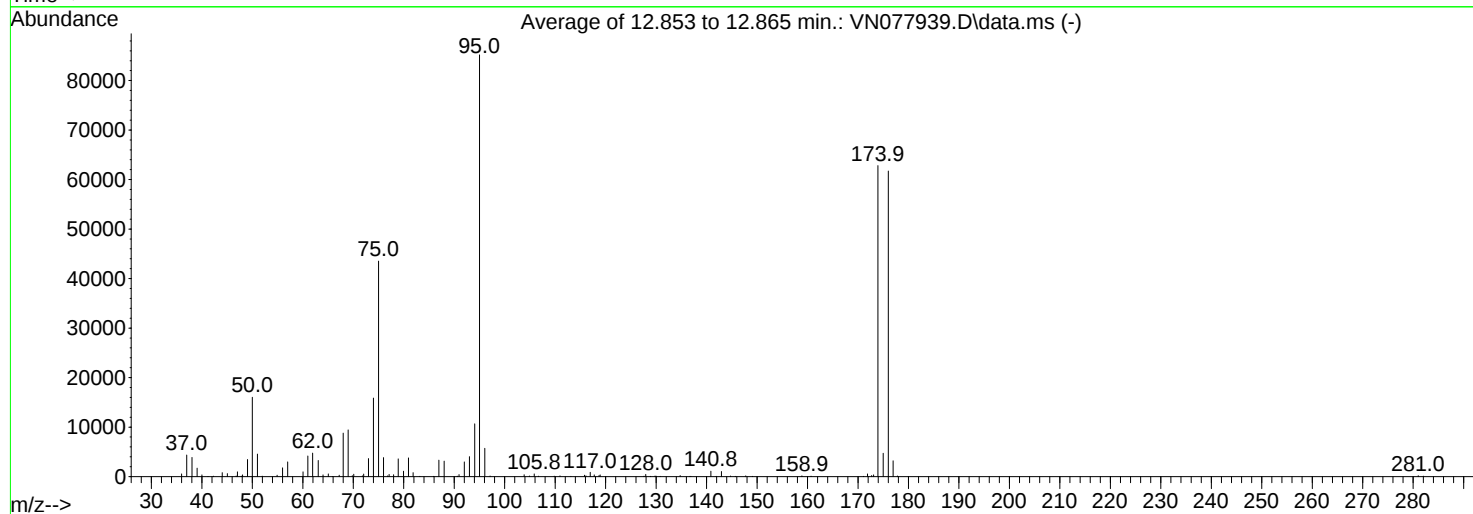


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052623\
Data File : VN077939.D
Acq On : 26 May 2023 20:36
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051523W.M
Title : SW846 8260
Last Update : Tue May 16 04:07:42 2023

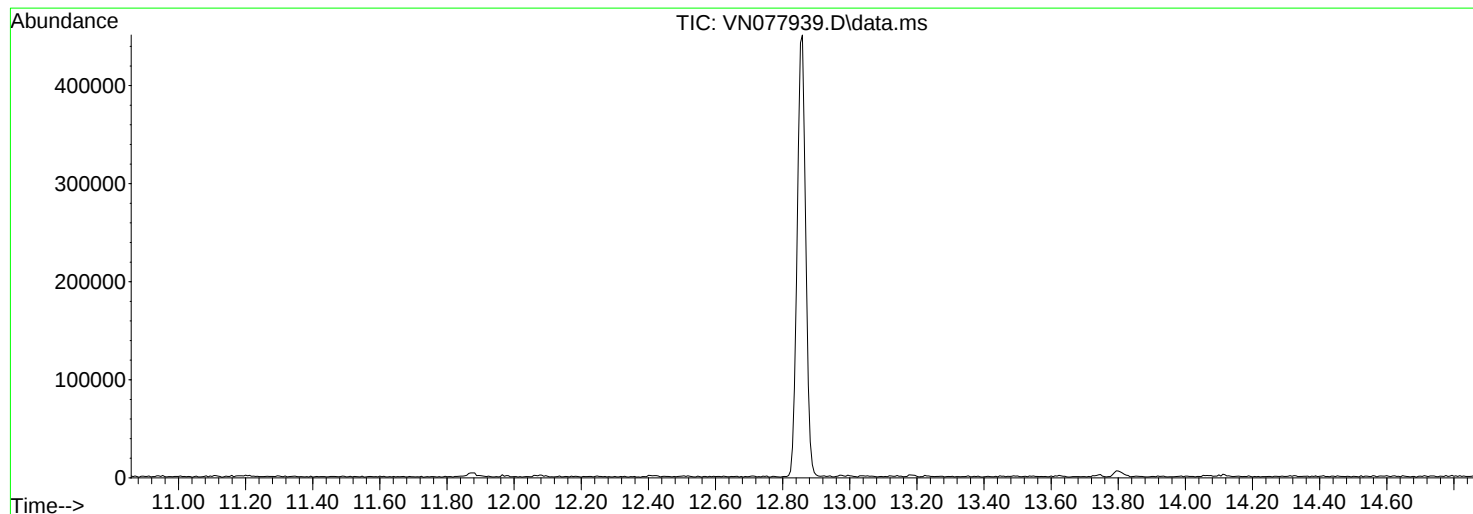

AutoFind: Scans 1853, 1854, 1855; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	16032	PASS
75	95	30	60	51.1	43520	PASS
95	95	100	100	100.0	85187	PASS
96	95	5	9	6.7	5709	PASS
173	174	0.00	2	0.6	349	PASS
174	95	50	100	73.8	62827	PASS
175	174	5	9	7.5	4735	PASS
176	174	95	101	98.3	61739	PASS
177	176	5	9	5.2	3186	PASS

Average of 12.853 to 12.865 min.: VN077939.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	562	47.80	85	61.95	4740	72.05	521
37.00	4372	48.05	361	63.05	3269	73.00	365
38.05	3868	49.05	3456	64.00	373	74.00	1588
39.05	1710	50.00	16032	65.05	560	75.00	4352
40.00	375	51.00	4550	65.90	51	76.00	3860
41.20	51	51.95	112	67.20	307	76.80	177
42.30	95	54.90	276	68.00	8776	77.10	460
44.05	804	56.00	1786	69.00	9424	78.00	391
45.05	607	57.00	2966	69.80	180	78.90	3575
46.80	124	60.05	971	70.10	474	79.95	1087
47.05	982	61.00	4174	71.80	152	80.95	3773

Average of 12.853 to 12.865 min.: VN077939.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.85	827	96.05	5709	116.95	874	136.70	75
83.20	57	97.10	116	117.75	362	136.90	53
85.90	52	103.85	399	118.70	238	140.85	1112
86.95	3335	104.90	144	118.90	355	141.90	56
88.00	3130	105.85	558	127.60	96	142.95	1026
90.60	85	106.70	94	127.95	451	144.75	133
90.95	436	109.80	100	128.90	68	145.70	56
92.00	2973	110.95	150	129.80	117	147.75	172
93.00	4059	113.10	71	130.00	111	149.10	72
94.05	10653	115.80	281	130.80	67	158.90	175
95.00	85187	116.10	166	134.75	214	160.70	85

Average of 12.853 to 12.865 min.: VN077939.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.10	79						
171.90	567						
172.70	236						
173.10	349						
173.95	62827						
175.00	4735						
176.00	61739						
176.95	3186						
177.80	142						
281.00	197						
282.00	86						