

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052725\
 Data File : VN086777.D
 Acq On : 27 May 2025 11:55
 Operator : JC\MD
 Sample : VN0527MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0527MBL01

Quant Time: May 29 01:45:07 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
 Quant Title : SW846 8260
 QLast Update : Sat May 17 00:46:13 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.218	168	193269	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	359485	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	342093	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	154068	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	119554	44.766	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	89.540%
35) Dibromofluoromethane	8.165	113	109232	51.022	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	102.040%
50) Toluene-d8	10.565	98	454547	51.234	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	102.460%
62) 4-Bromofluorobenzene	12.847	95	165518	52.837	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	105.680%


Target Compounds				Qvalue		
3) Chloromethane	2.365	50	1651	0.523	ug/l	98
5) Bromomethane	2.965	94	936	0.573	ug/l	92
10) Methyl Iodide	4.589	142	1432	0.568	ug/l #	80
13) Acrolein	4.183	56	760	1.462	ug/l	98
15) Acrylonitrile	5.712	53	549	0.456	ug/l #	65
16) Acetone	4.430	43	902	0.903	ug/l #	42
17) Carbon Disulfide	4.706	76	3126	0.524	ug/l #	75
21) trans-1,2-Dichloroethene	5.783	96	472	0.207	ug/l #	25
23) Vinyl Acetate	6.606	43	1276	0.231	ug/l #	69
25) 2-Butanone	7.488	43	641	0.415	ug/l #	46
29) Tetrahydrofuran	7.841	42	664	0.659	ug/l #	59
31) Cyclohexane	8.218	56	3658	0.913	ug/l #	1
38) Carbon Tetrachloride	8.218	117	18235	5.861	ug/l #	17
43) Isopropyl Acetate	8.694	43	2255	0.353	ug/l #	54
51) 4-Methyl-2-Pentanone	10.447	43	975	0.302	ug/l	88
59) 2-Hexanone	11.194	43	1688	0.717	ug/l	88
68) m/p-Xylenes	12.071	106	1368	0.281	ug/l #	72
76) 1,2,3-Trichloropropane	12.847	75	76349	21.912	ug/l #	1
77) Bromobenzene	12.982	156	627	0.209	ug/l	85
81) trans-1,4-Dichloro-2-b...	12.847	75	76349	55.298	ug/l #	15
82) 4-Chlorotoluene	13.218	91	2419	0.275	ug/l	93
85) sec-Butylbenzene	13.612	105	3976	0.357	ug/l	93
86) p-Isopropyltoluene	13.729	119	3167	0.347	ug/l	95
87) 1,3-Dichlorobenzene	13.729	146	1741	0.336	ug/l	95
88) 1,4-Dichlorobenzene	13.729	146	1741	0.339	ug/l	95
89) n-Butylbenzene	14.053	91	4652	0.614	ug/l	97
90) Hexachloroethane	14.329	117	311	0.205	ug/l #	18
91) 1,2-Dichlorobenzene	14.106	146	1808	0.367	ug/l	92
93) 1,2,4-Trichlorobenzene	15.394	180	2868	1.378	ug/l	97
94) Hexachlorobutadiene	15.494	225	1310	1.517	ug/l	91
95) Naphthalene	15.641	128	16305	2.257	ug/l	98
96) 1,2,3-Trichlorobenzene	15.835	180	3181	1.561	ug/l	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052725\
Data File : VN086777.D
Acq On : 27 May 2025 11:55
Operator : JC\MD
Sample : VN0527MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01

Quant Time: May 29 01:45:07 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Quant Title : SW846 8260
QLast Update : Sat May 17 00:46:13 2025
Response via : Initial Calibration




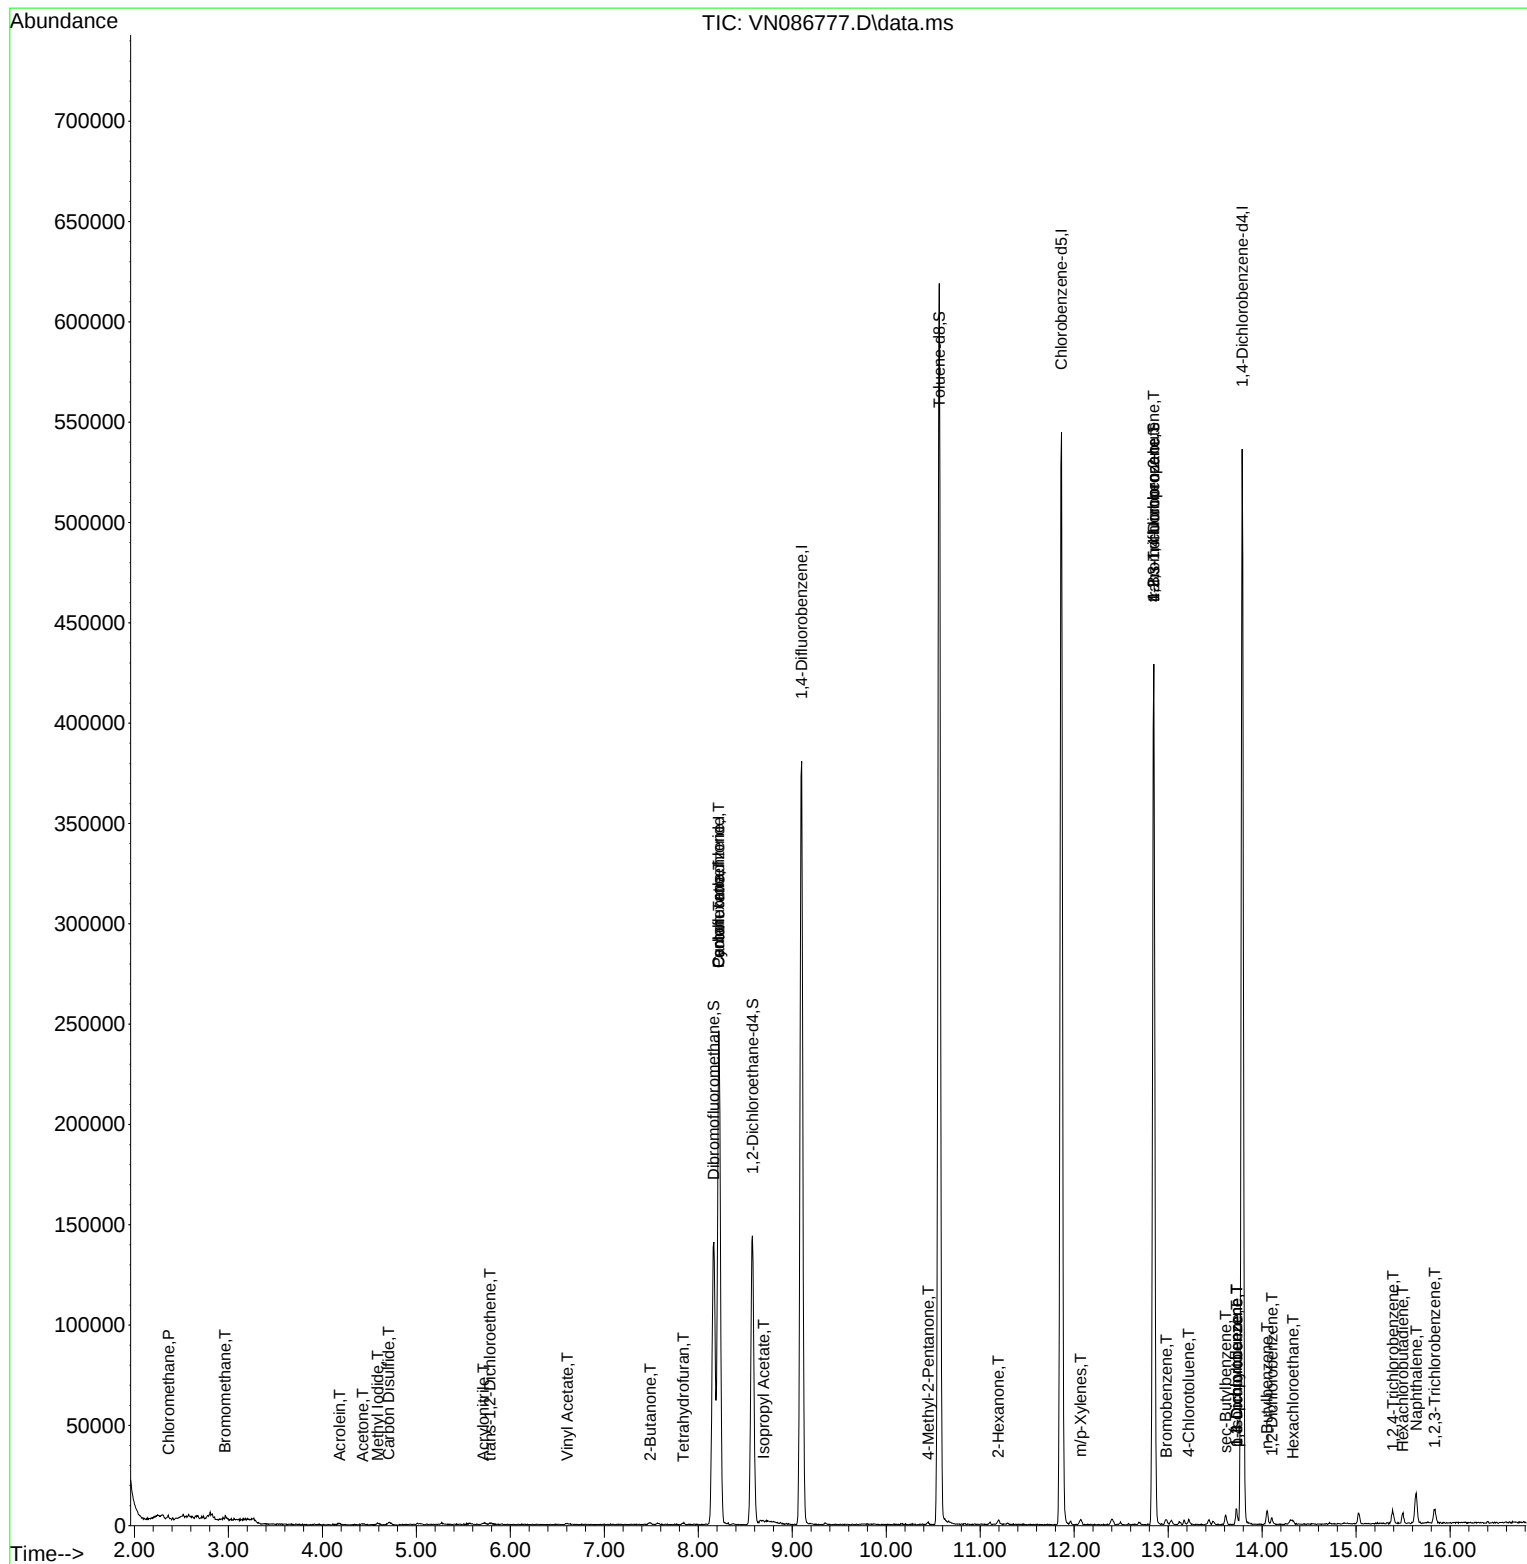




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.218 min Scan# 1
Delta R.T. -0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion:168 Resp: 193269
Ion Ratio Lower Upper
168 100
99 56.8 47.0 70.4



#3
Chloromethane
Concen: 0.523 ug/l
RT: 2.365 min Scan# 70
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 50 Resp: 1651
Ion Ratio Lower Upper
50 100
52 31.3 25.9 38.9









#5
Bromomethane
Concen: 0.573 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 94 Resp: 936
Ion Ratio Lower Upper
94 100
96 96.9 71.2 106.8

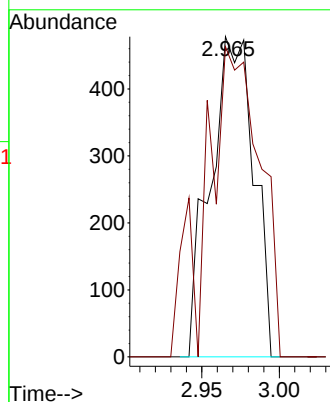

#10
Methyl Iodide
Concen: 0.568 ug/l
RT: 4.589 min Scan# 448
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion:142 Resp: 1432
Ion Ratio Lower Upper
142 100
127 31.0 32.4 48.6#
141 0.0 11.4 17.2#


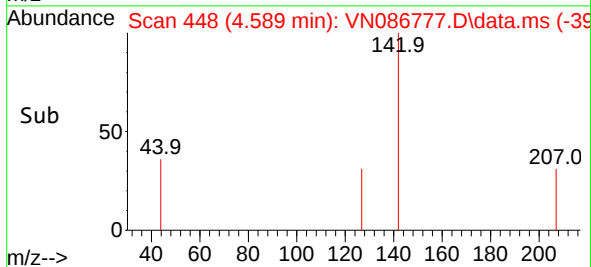

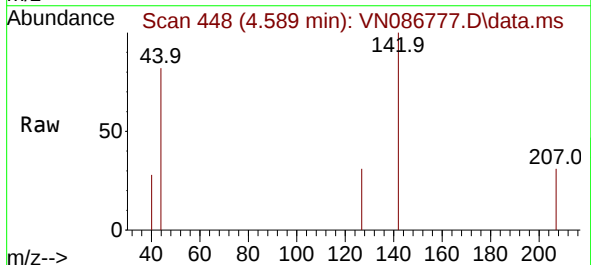




#13
Acrolein
Concen: 1.462 ug/l
RT: 4.183 min Scan# 31
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 56 Resp: 760
Ion Ratio Lower Upper
56 100
55 68.2 55.7 83.5



#15
Acrylonitrile
Concen: 0.456 ug/l
RT: 5.712 min Scan# 639
Delta R.T. -0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 53 Resp: 549
Ion Ratio Lower Upper
53 100
52 60.3 65.4 98.2#
51 0.0 27.9 41.9#


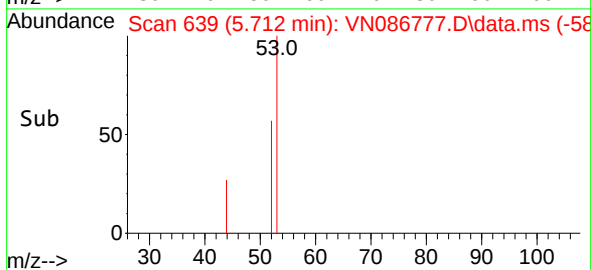






#16
Acetone
Concen: 0.903 ug/l
RT: 4.430 min Scan# 41
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 43 Resp: 902
Ion Ratio Lower Upper
43 100
58 0.0 25.8 38.6#

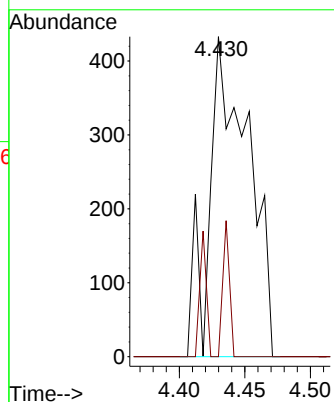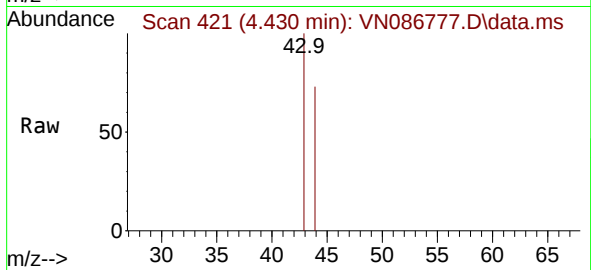

#17
Carbon Disulfide
Concen: 0.524 ug/l
RT: 4.706 min Scan# 468
Delta R.T. -0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 76 Resp: 3126
Ion Ratio Lower Upper
76 100
78 0.0 7.3 10.9#


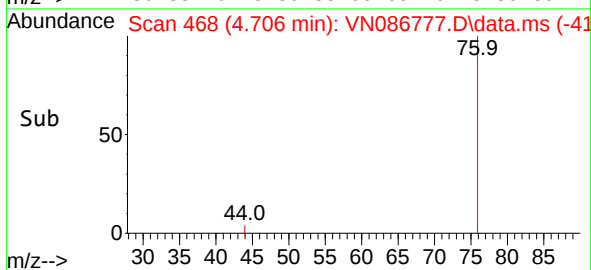
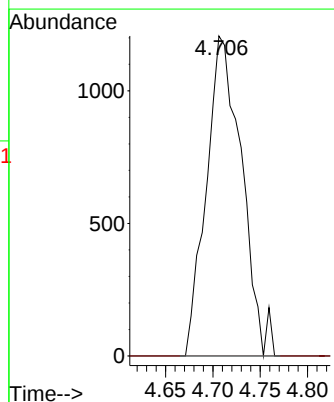
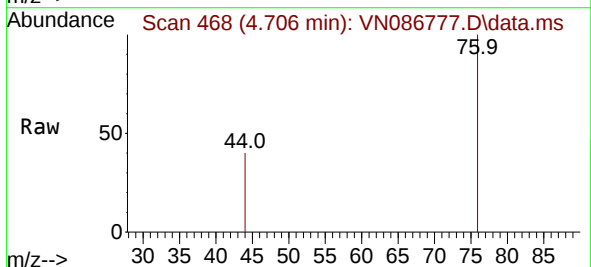




#21
trans-1,2-Dichloroethene
Concen: 0.207 ug/l
RT: 5.783 min Scan# 61
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 96 Resp: 472
Ion Ratio Lower Upper
96 100
61 47.4 105.7 158.5#
98 0.0 51.0 76.6#



#23
Vinyl Acetate
Concen: 0.231 ug/l
RT: 6.606 min Scan# 791
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 43 Resp: 1276
Ion Ratio Lower Upper
43 100
86 0.0 9.5 14.3#


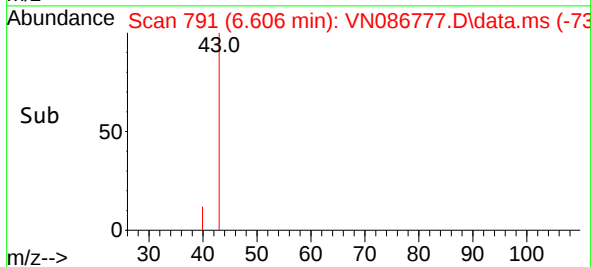

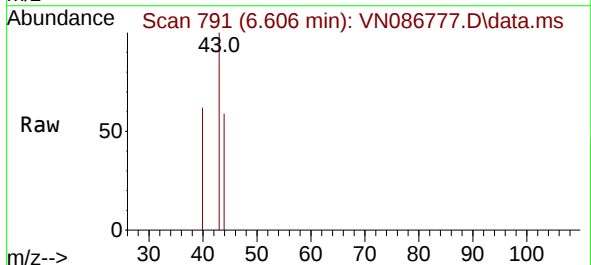




#25
2-Butanone
Concen: 0.415 ug/l
RT: 7.488 min Scan# 941
Delta R.T. 0.012 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 43 Resp: 641
Ion Ratio Lower Upper
43 100
72 0.0 23.1 34.7#



#29
Tetrahydrofuran
Concen: 0.659 ug/l
RT: 7.841 min Scan# 1001
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55


Tgt Ion: 42 Resp: 664
Ion Ratio Lower Upper
42 100
72 29.1 38.7 58.1#
71 9.6 36.2 54.4#

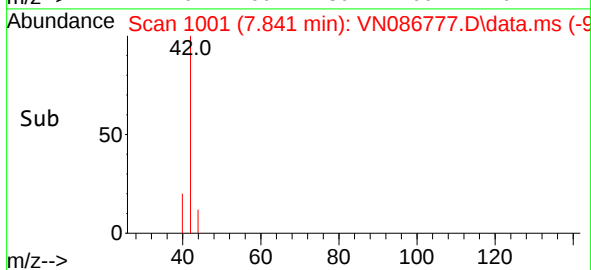



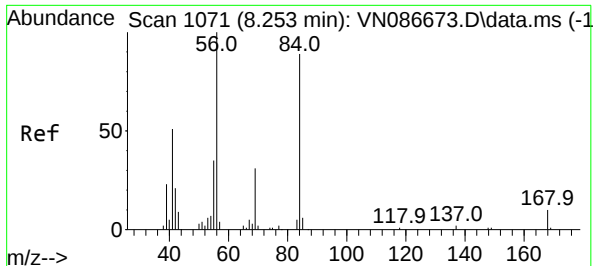


#31
Cyclohexane
Concen: 0.913 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.035 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01



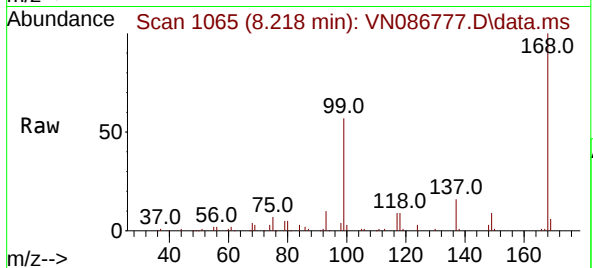



Tgt Ion: 56 Resp: 3658
Ion Ratio Lower Upper
56 100
69 153.9 25.0 37.6#
84 149.5 71.0 106.4#

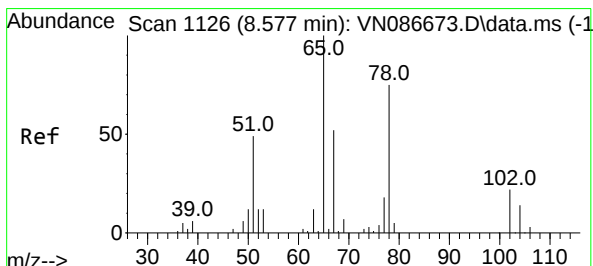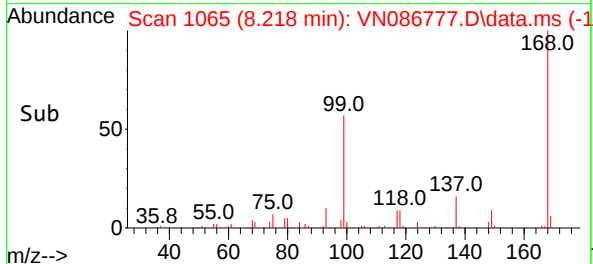

#33
1,2-Dichloroethane-d4
Concen: 44.766 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 65 Resp: 119554
Ion Ratio Lower Upper
65 100
67 54.7 0.0 106.4

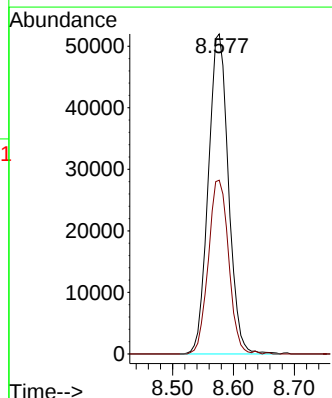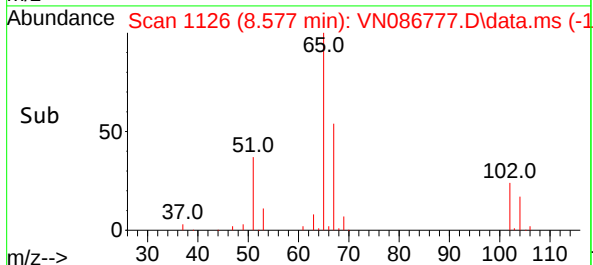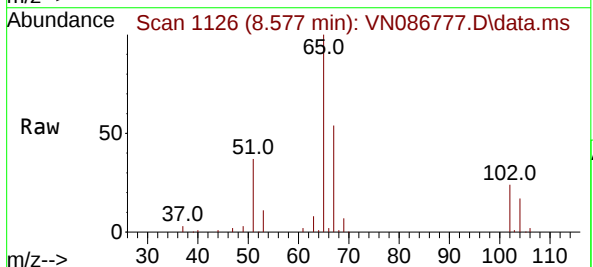

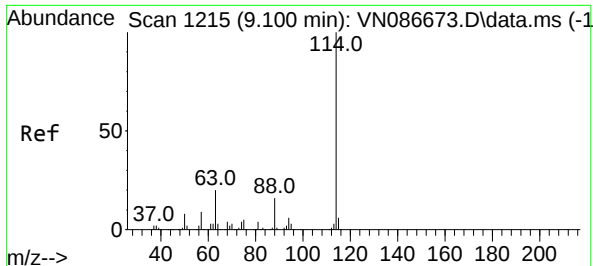

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55

Instrument :

MSVOA_N

ClientSampleId :

VN0527MBL01





Tgt Ion:114 Resp: 359485

Ion Ratio Lower Upper

114 100

63 19.5 0.0 40.2

88 15.4 0.0 31.2

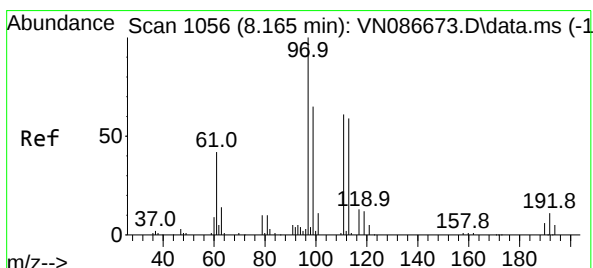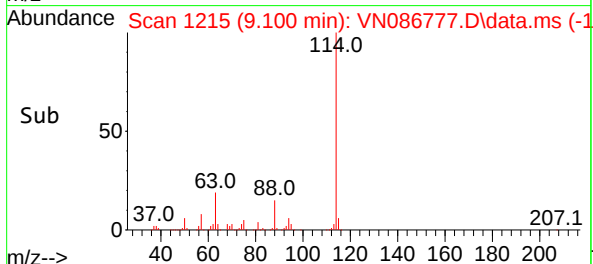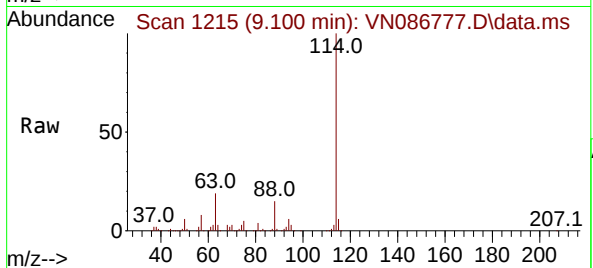

#35

Dibromofluoromethane

Concen: 51.022 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55




Tgt Ion:113 Resp: 109232


Ion Ratio Lower Upper

113 100

111 103.5 82.2 123.2


192 18.1 13.8 20.8

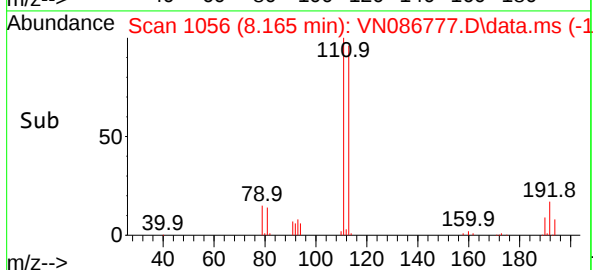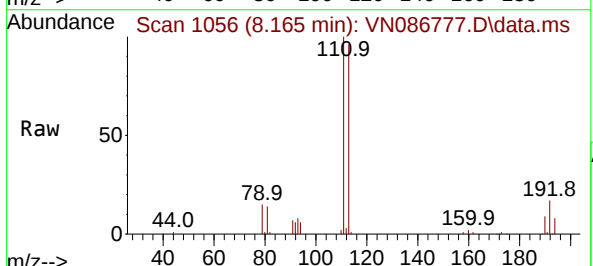



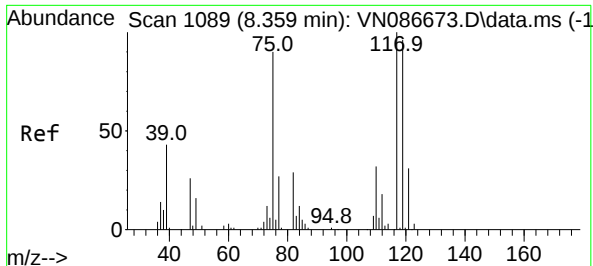


#38
Carbon Tetrachloride
Concen: 5.861 ug/l
RT: 8.218 min Scan# 1065
Delta R.T. -0.141 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01



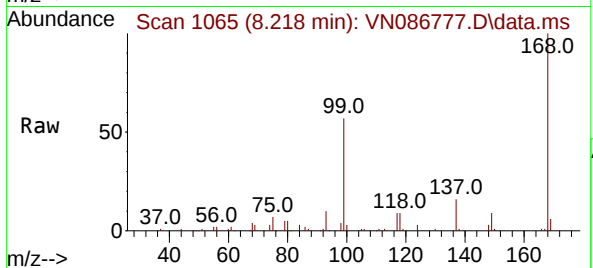



Tgt Ion:117 Resp: 18235
Ion Ratio Lower Upper
117 100
119 6.7 77.0 115.6#
121 0.0 25.0 37.6#

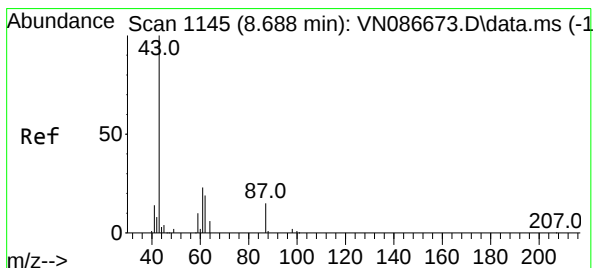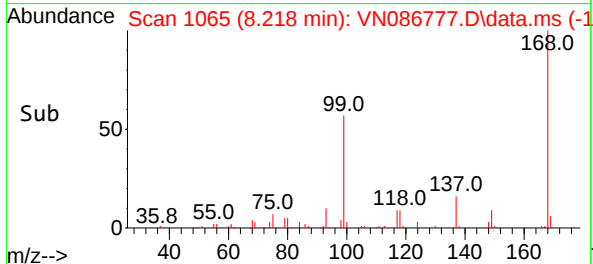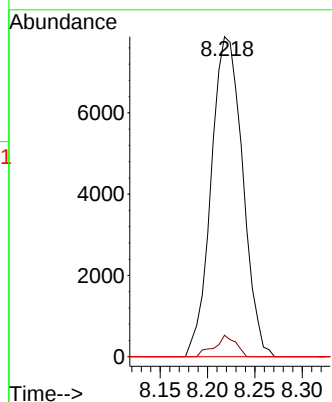

#43
Isopropyl Acetate
Concen: 0.353 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 43 Resp: 2255
Ion Ratio Lower Upper
43 100
61 0.0 21.4 32.2#
87 0.0 11.1 16.7#


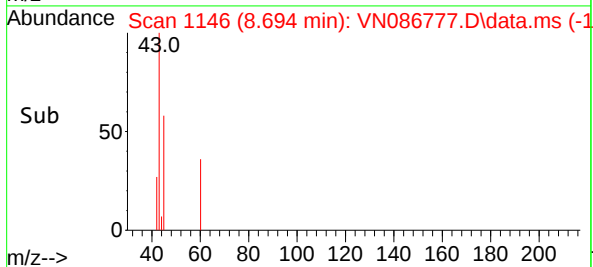

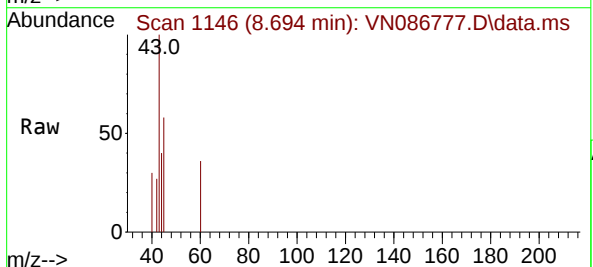




#50
Toluene-d8
Concen: 51.234 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 98 Resp: 454547
Ion Ratio Lower Upper
98 100
100 65.7 52.9 79.3

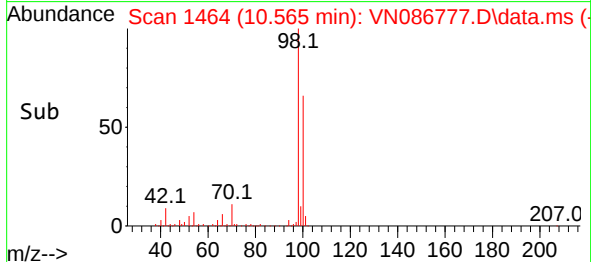

#51
4-Methyl-2-Pentanone
Concen: 0.302 ug/l
RT: 10.447 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 43 Resp: 975
Ion Ratio Lower Upper
43 100
58 35.0 33.9 50.9


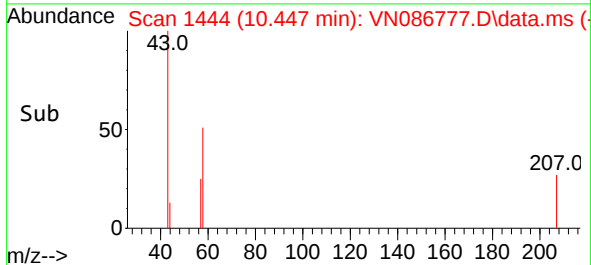

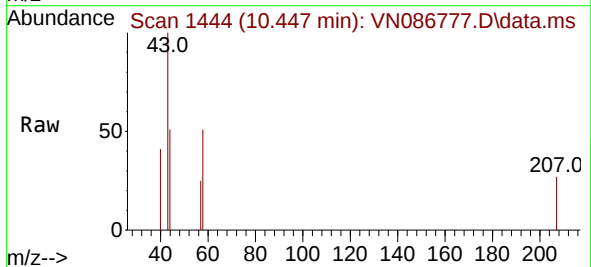




#59
2-Hexanone
Concen: 0.717 ug/l
RT: 11.194 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 43 Resp: 1688
Ion Ratio Lower Upper
43 100
58 50.5 29.8 89.5

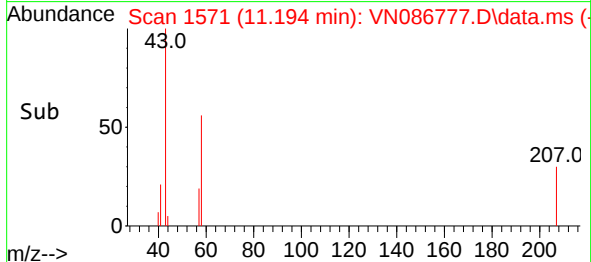

#62
4-Bromofluorobenzene
Concen: 52.837 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 95 Resp: 165518
Ion Ratio Lower Upper
95 100
174 73.9 0.0 145.4
176 70.2 0.0 137.8


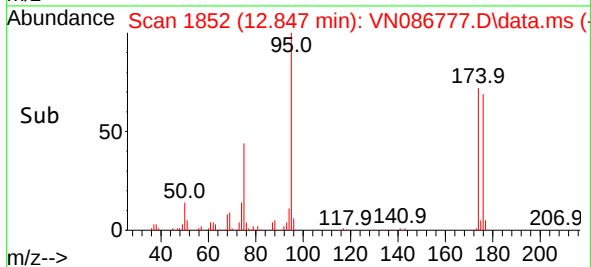

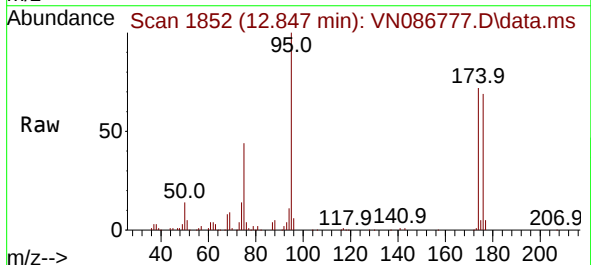




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion:117 Resp: 342093
Ion Ratio Lower Upper
117 100
82 53.4 44.2 66.2
119 32.0 25.4 38.2

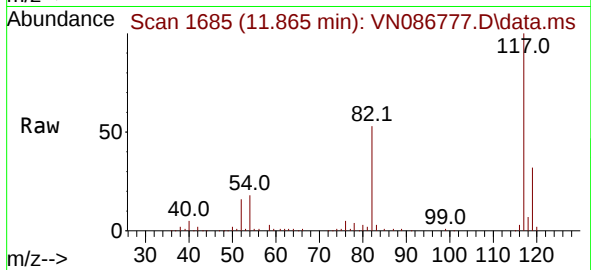

#68
m/p-Xylenes
Concen: 0.281 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion:106 Resp: 1368
Ion Ratio Lower Upper
106 100
91 160.5 162.4 243.6#




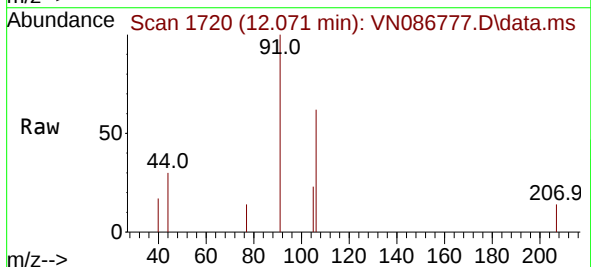


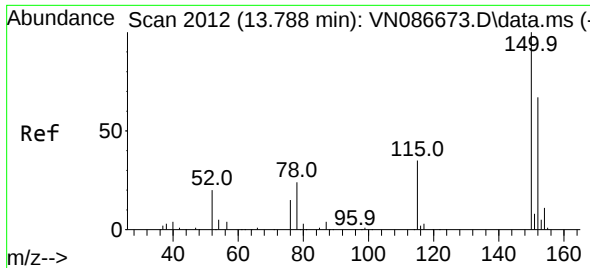

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.788 min Scan# 2012
 Delta R.T. -0.000 min
 Lab File: VN086777.D
 Acq: 27 May 2025 11:55




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0527MBL01


Tgt Ion:152 Resp: 154068
 Ion Ratio Lower Upper
 152 100
 115 59.7 30.0 90.1
 150 158.3 0.0 347.8

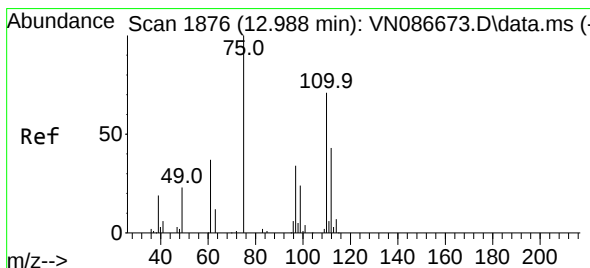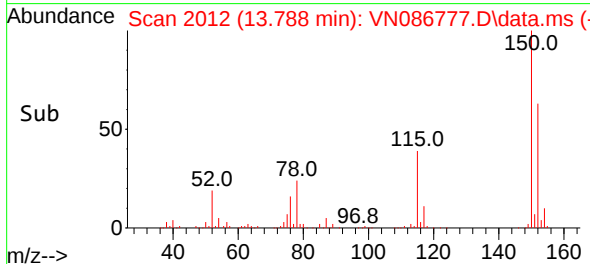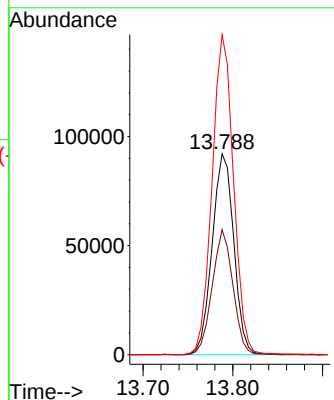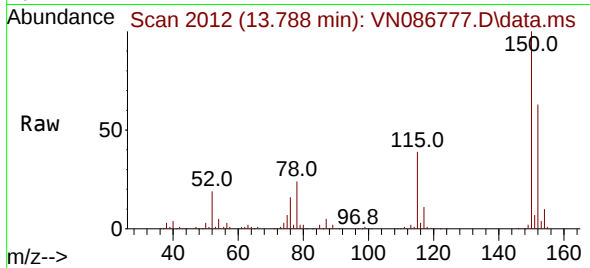

#76
 1,2,3-Trichloropropane
 Concen: 21.912 ug/l
 RT: 12.847 min Scan# 1852
 Delta R.T. -0.141 min
 Lab File: VN086777.D
 Acq: 27 May 2025 11:55

Tgt Ion: 75 Resp: 76349
 Ion Ratio Lower Upper
 75 100
 77 1.3 96.0 288.1#

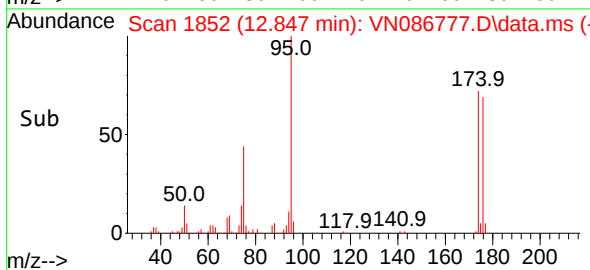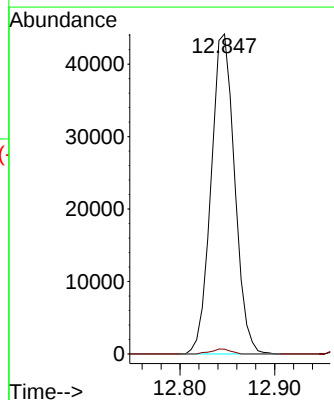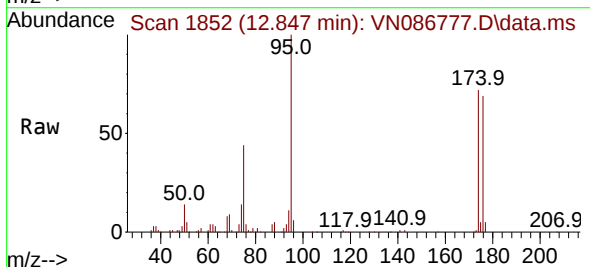

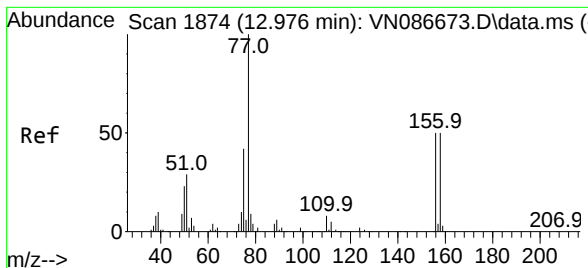

#77

Bromobenzene

Concen: 0.209 ug/l

RT: 12.982 min Scan# 1875

Delta R.T. 0.006 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55

Instrument :

MSVOA_N

ClientSampleId :

VN0527MBL01





Tgt Ion:156 Resp: 627

Ion Ratio Lower Upper

156 100

77 256.8 113.1 339.2

158 102.1 48.6 145.9

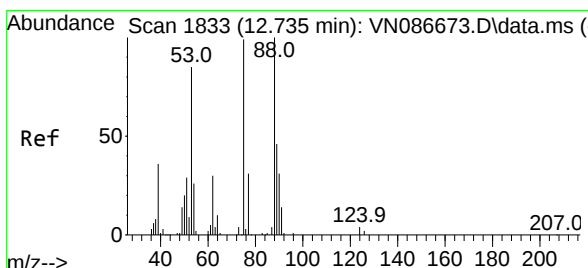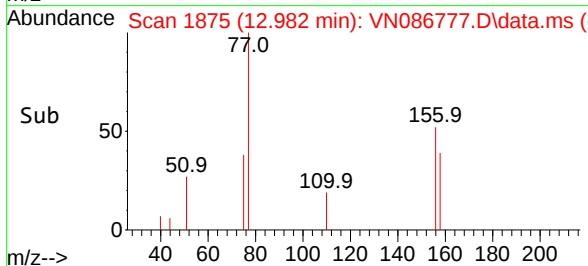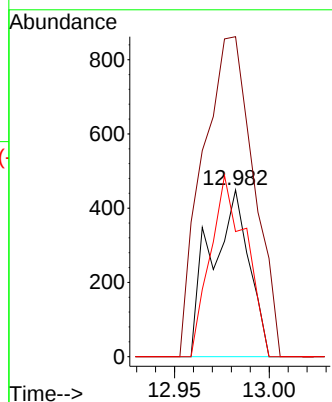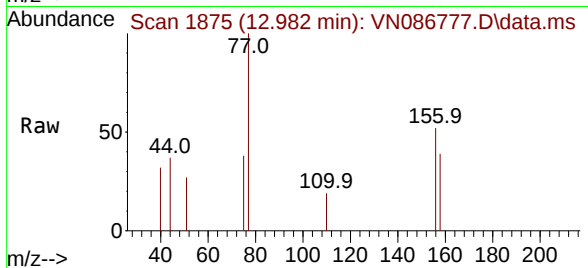

#81

trans-1,4-Dichloro-2-butene

Concen: 55.298 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.112 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55




Tgt Ion: 75 Resp: 76349


Ion Ratio Lower Upper

75 100

53 0.0 70.4 105.6#

89 0.0 32.4 48.6#


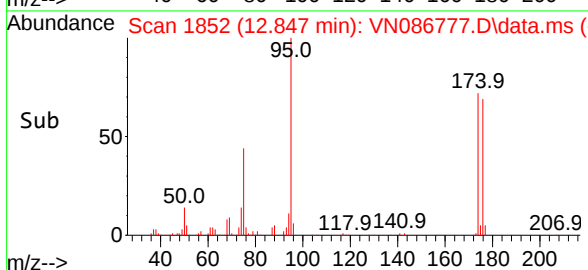

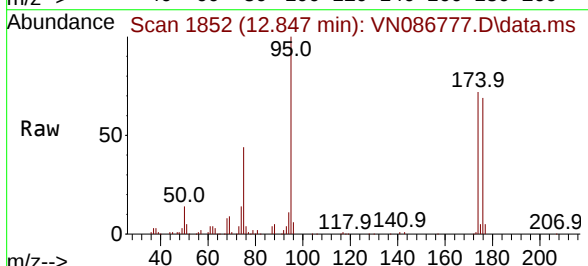




#82
4-Chlorotoluene
Concen: 0.275 ug/l
RT: 13.218 min Scan# 1915
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion: 91 Resp: 2419
Ion Ratio Lower Upper
91 100
126 30.1 17.0 50.9

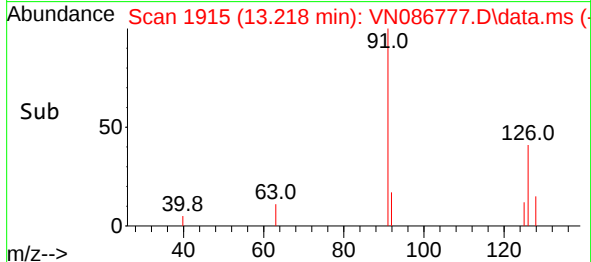

#85
sec-Butylbenzene
Concen: 0.357 ug/l
RT: 13.612 min Scan# 1982
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 105 Resp: 3976
Ion Ratio Lower Upper
105 100
134 17.0 10.1 30.1

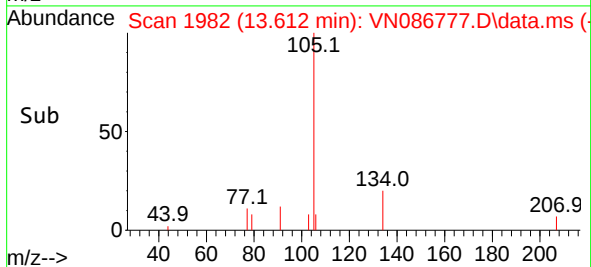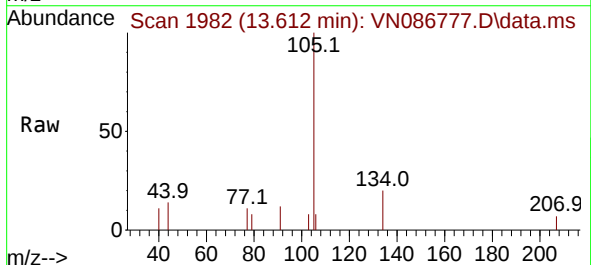



#86

p-Isopropyltoluene

Concen: 0.347 ug/l

RT: 13.729 min Scan# 2001

Delta R.T. 0.006 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55

Instrument :

MSVOA_N

ClientSampleId :

VN0527MBL01





Tgt Ion:119 Resp: 3167

Ion Ratio Lower Upper

119 100

134 22.7 13.1 39.1

91 21.0 11.5 34.5

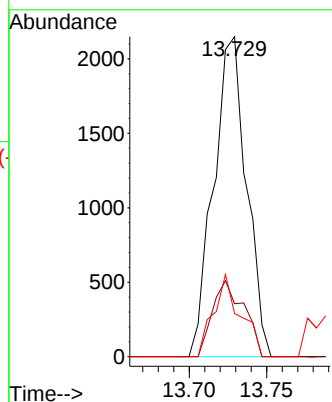

#87

1,3-Dichlorobenzene

Concen: 0.336 ug/l

RT: 13.729 min Scan# 2002

Delta R.T. -0.000 min

Lab File: VN086777.D

Acq: 27 May 2025 11:55




Tgt Ion:146 Resp: 1741


Ion Ratio Lower Upper

146 100

111 35.0 20.9 62.7

148 62.8 31.8 95.4


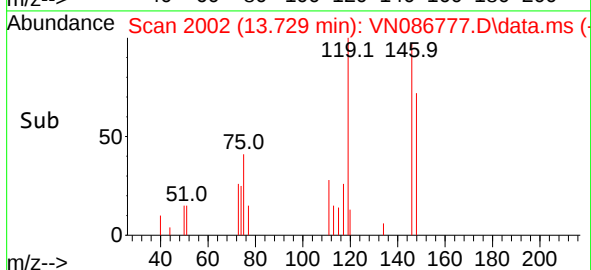






#88
1,4-Dichlorobenzene
Concen: 0.339 ug/l
RT: 13.729 min Scan# 2015
Delta R.T. -0.077 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion:146 Resp: 1741
Ion Ratio Lower Upper
146 100
111 35.0 20.6 61.8
148 62.8 32.0 96.0

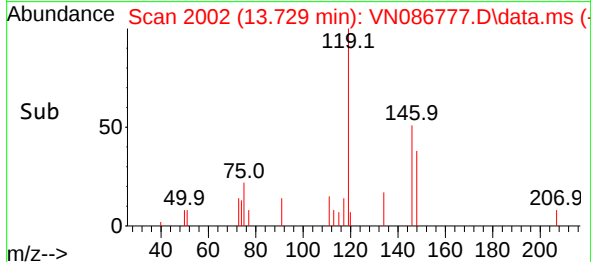

#89
n-Butylbenzene
Concen: 0.614 ug/l
RT: 14.053 min Scan# 2057
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion: 91 Resp: 4652
Ion Ratio Lower Upper
91 100
92 52.6 27.4 82.0
134 26.7 12.8 38.4


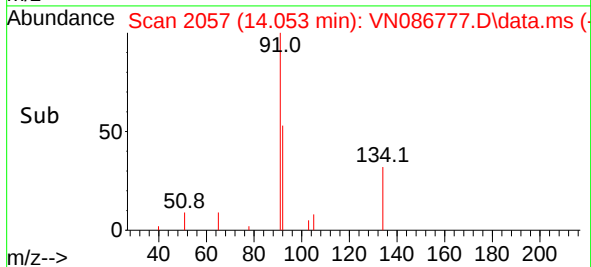

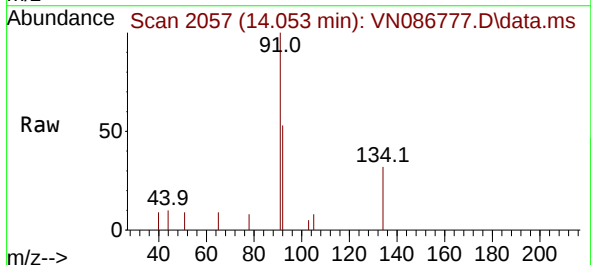




#90
Hexachloroethane
Concen: 0.205 ug/l
RT: 14.329 min Scan# 2104
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion:117 Resp: 311
Ion Ratio Lower Upper
117 100
201 0.0 32.0 96.0#

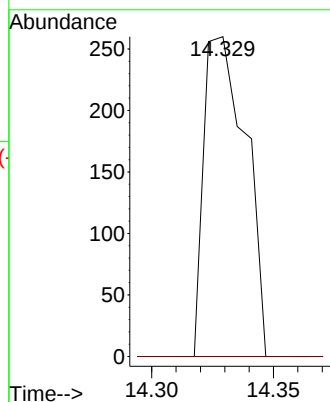

#91
1,2-Dichlorobenzene
Concen: 0.367 ug/l
RT: 14.106 min Scan# 2066
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion:146 Resp: 1808
Ion Ratio Lower Upper
146 100
111 38.3 21.6 65.0
148 70.1 31.7 95.1


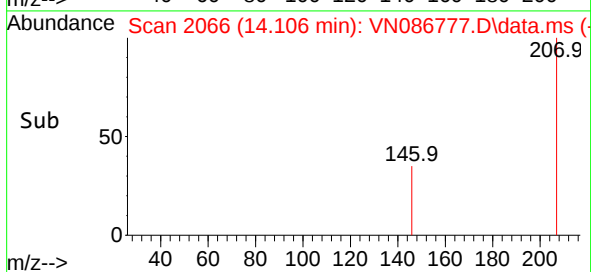
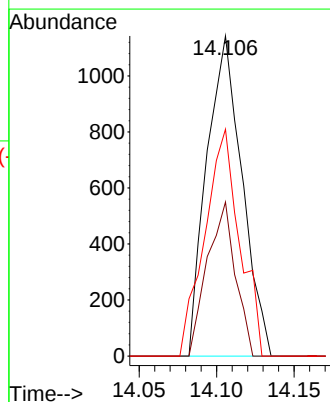
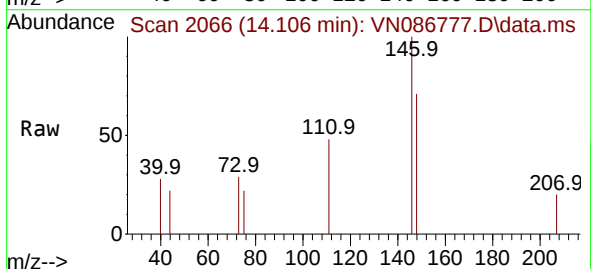




#93
1,2,4-Trichlorobenzene
Concen: 1.378 ug/l
RT: 15.394 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55




Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01


Tgt Ion:180 Resp: 2868
Ion Ratio Lower Upper
180 100
182 92.2 47.1 141.3
145 27.0 15.6 46.8



#94
Hexachlorobutadiene
Concen: 1.517 ug/l
RT: 15.494 min Scan# 2302
Delta R.T. -0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion:225 Resp: 1310
Ion Ratio Lower Upper
225 100
223 70.5 32.9 98.6
227 55.8 32.4 97.2


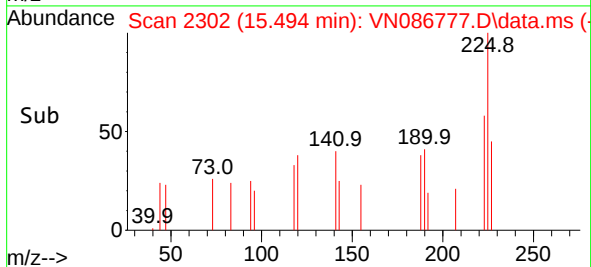

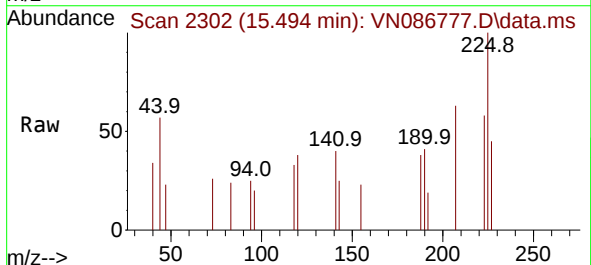


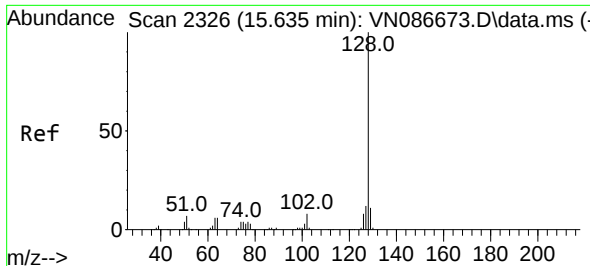

#95
Naphthalene
Concen: 2.257 ug/l
RT: 15.641 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Instrument :
MSVOA_N
ClientSampleId :
VN0527MBL01

Tgt Ion:	128	Resp:	16305
Ion Ratio	Lower	Upper	
128	100		
127	12.9	10.1	15.1
129	9.6	8.6	13.0

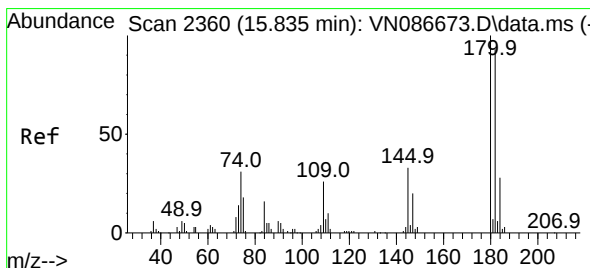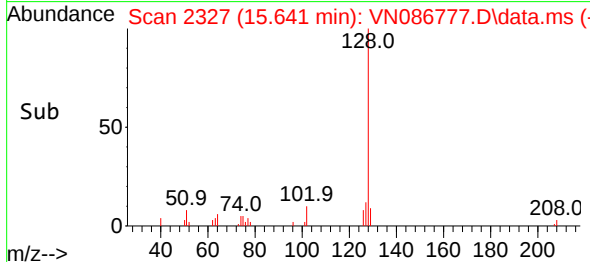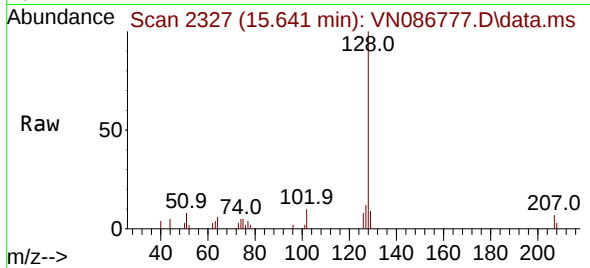

#96
1,2,3-Trichlorobenzene
Concen: 1.561 ug/l
RT: 15.835 min Scan# 2360
Delta R.T. -0.000 min
Lab File: VN086777.D
Acq: 27 May 2025 11:55

Tgt Ion:	180	Resp:	3181
Ion Ratio	Lower	Upper	
180	100		
182	100.7	47.0	141.2
145	33.4	16.7	50.1

