


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052725\
Data File : VN086775.D
Acq On : 27 May 2025 10:12
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

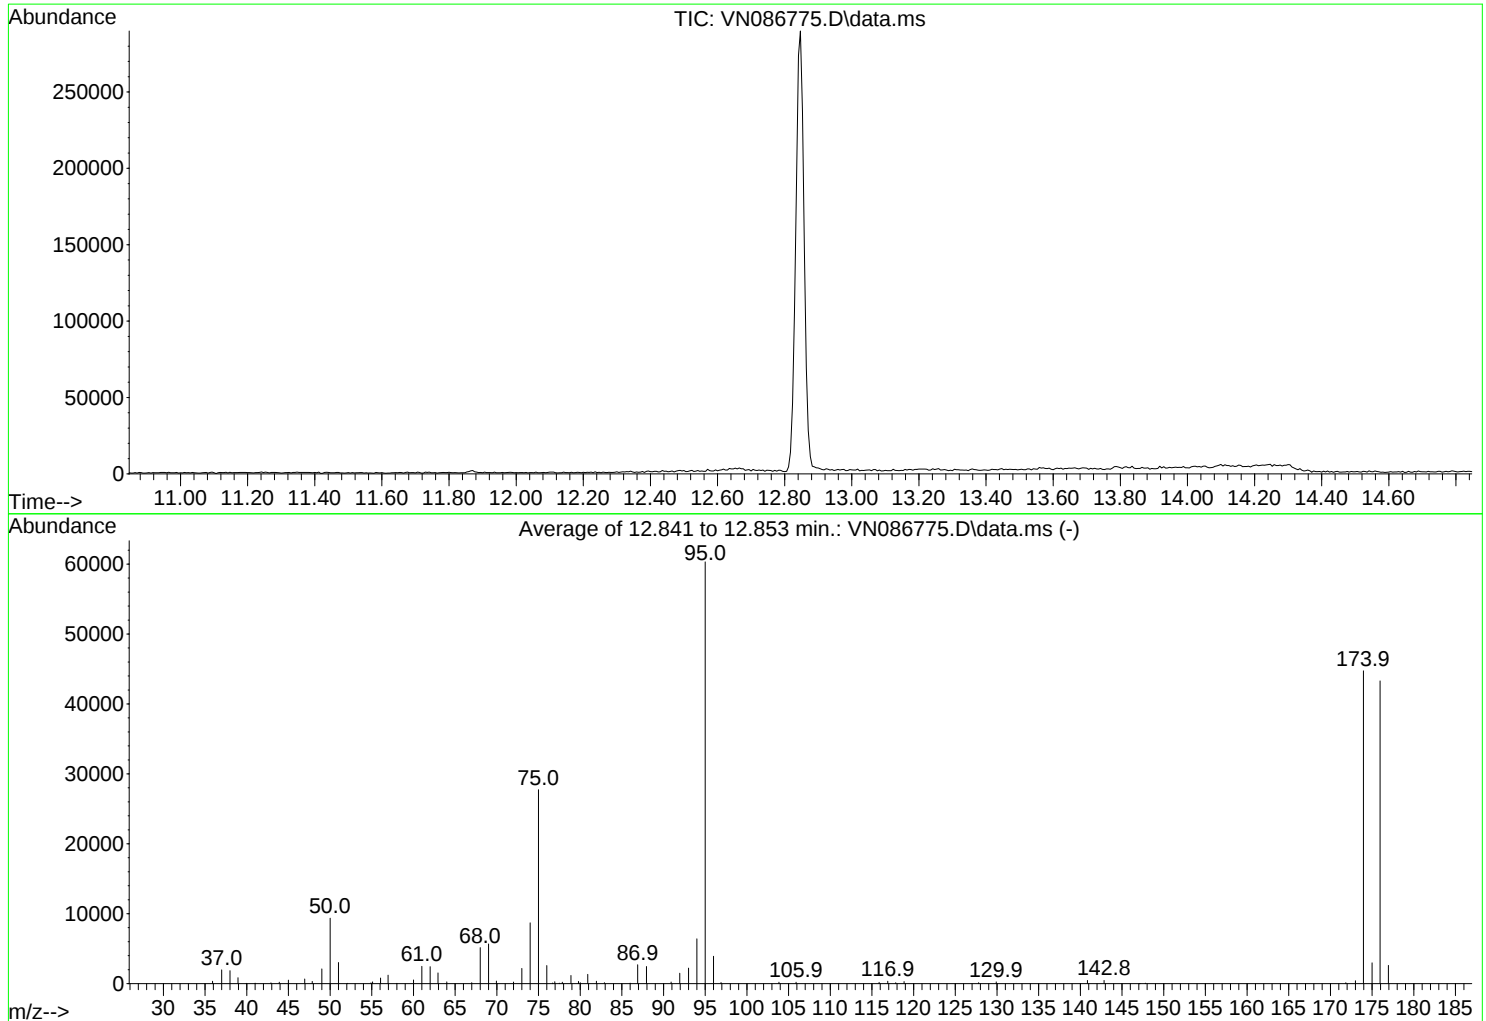

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.5	9366	PASS
75	95	30	60	46.0	27744	PASS
95	95	100	100	100.0	60325	PASS
96	95	5	9	6.5	3918	PASS
173	174	0.00	2	0.9	413	PASS
174	95	50	100	74.2	44736	PASS
175	174	5	9	6.6	2970	PASS
176	174	95	101	96.8	43304	PASS
177	176	5	9	6.0	2608	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	350	49.00	2099	62.00	2423	76.00	2581
37.00	1977	50.00	9366	62.95	1529	76.70	101
38.00	1855	51.00	3025	64.00	256	76.95	26
38.95	851	52.10	54	67.00	144	77.50	7
39.95	49	54.90	121	68.00	5147	77.85	201
41.00	75	55.10	263	69.00	5676	78.90	1173
42.90	109	56.05	808	69.95	356	79.80	327
43.90	198	56.95	1210	72.00	239	80.00	133
45.00	498	58.00	56	73.00	2186	80.90	1321
46.95	661	60.00	525	74.00	8692	81.95	351
47.85	315	61.00	2473	75.00	27744	82.90	139

Average of 12.841 to 12.853 min.: VN086775.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	66	105.90	210	171.85	140		
86.90	2693	115.85	191	173.00	413		
87.95	2449	116.90	335	173.95	44736		
90.90	224	117.85	145	175.00	2970		
91.95	1483	118.85	307	175.95	43304		
93.00	2217	127.80	134	176.95	2608		
94.00	6419	129.90	245				
95.00	60325	140.85	449				
96.00	3918	142.85	463				
96.90	163	147.05	2				
103.85	209	147.80	73				

Instrument :

MSVOA_N

ClientSampleId :

BFB