


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN052819\
Data File : VN055837.D
Acq On : 28 May 2019 8:24
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
Title : SW846 8260
Last Update : Fri May 24 06:41:54 2019

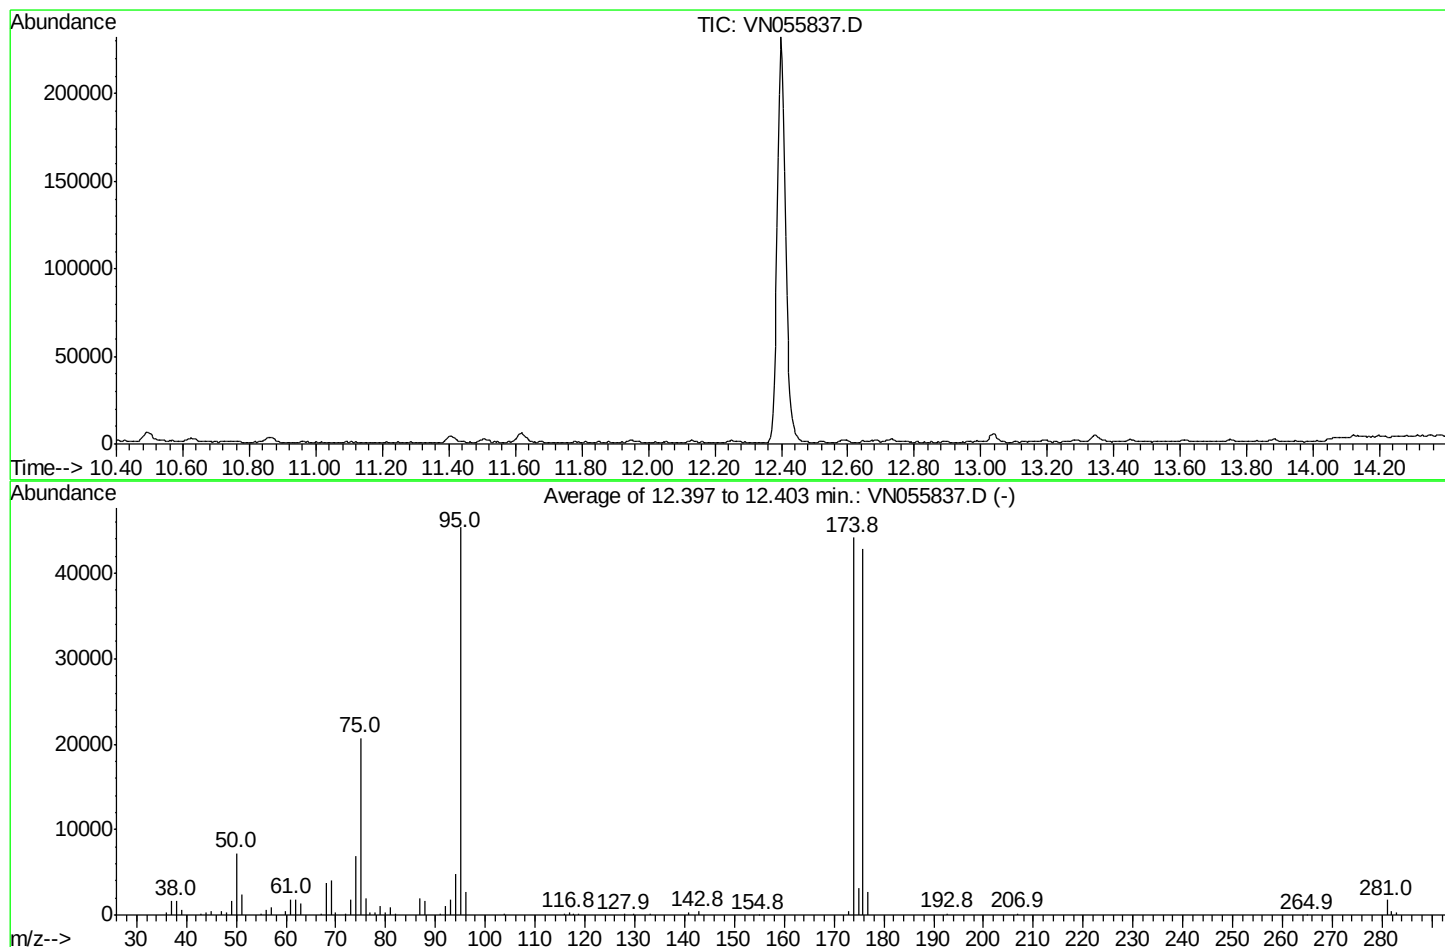

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	7229	PASS
75	95	30	60	45.6	20709	PASS
95	95	100	100	100.0	45384	PASS
96	95	5	9	6.1	2769	PASS
173	174	0.00	2	0.9	414	PASS
174	95	50	100	97.4	44184	PASS
175	174	5	9	7.2	3194	PASS
176	174	95	101	97.0	42866	PASS
177	176	5	9	6.3	2690	PASS