



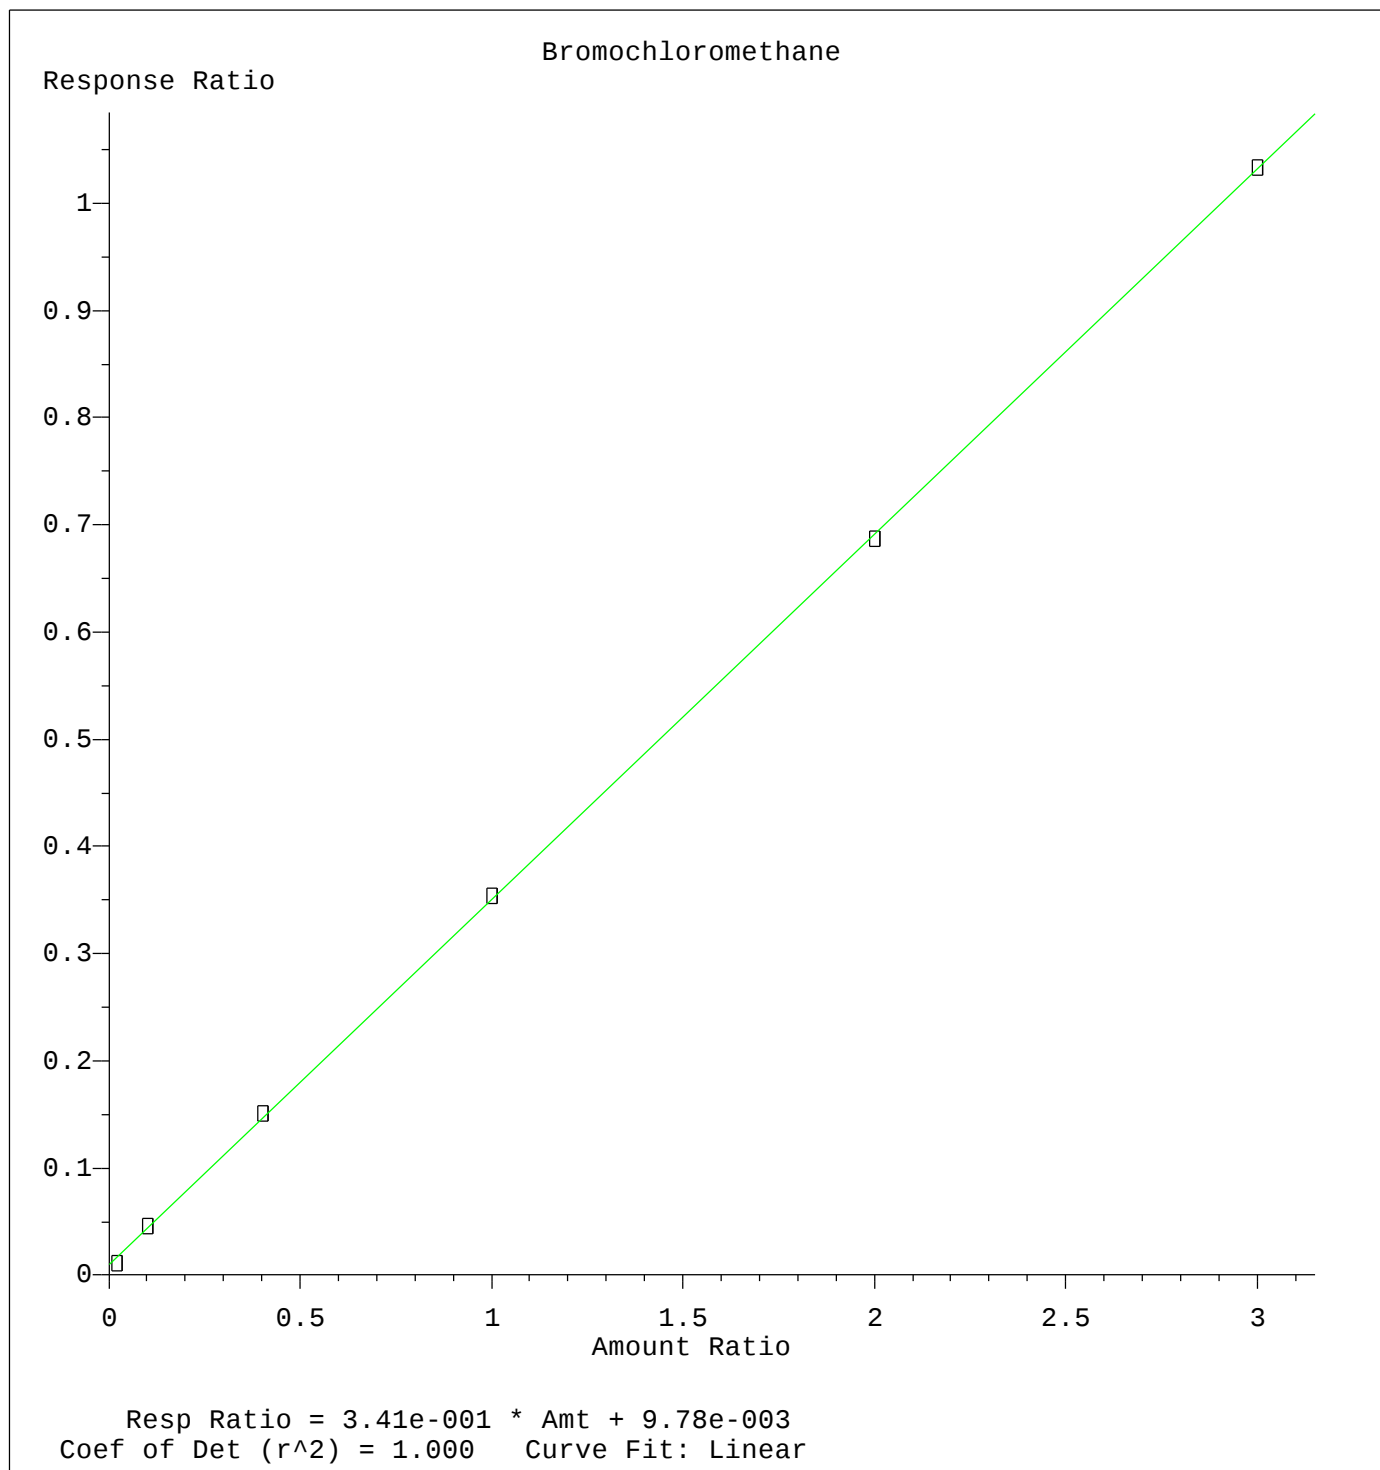

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Calibration Table Last Updated: Fri May 29 02:14:10 2020


Dichlorodifluoromethane

Response Ratio

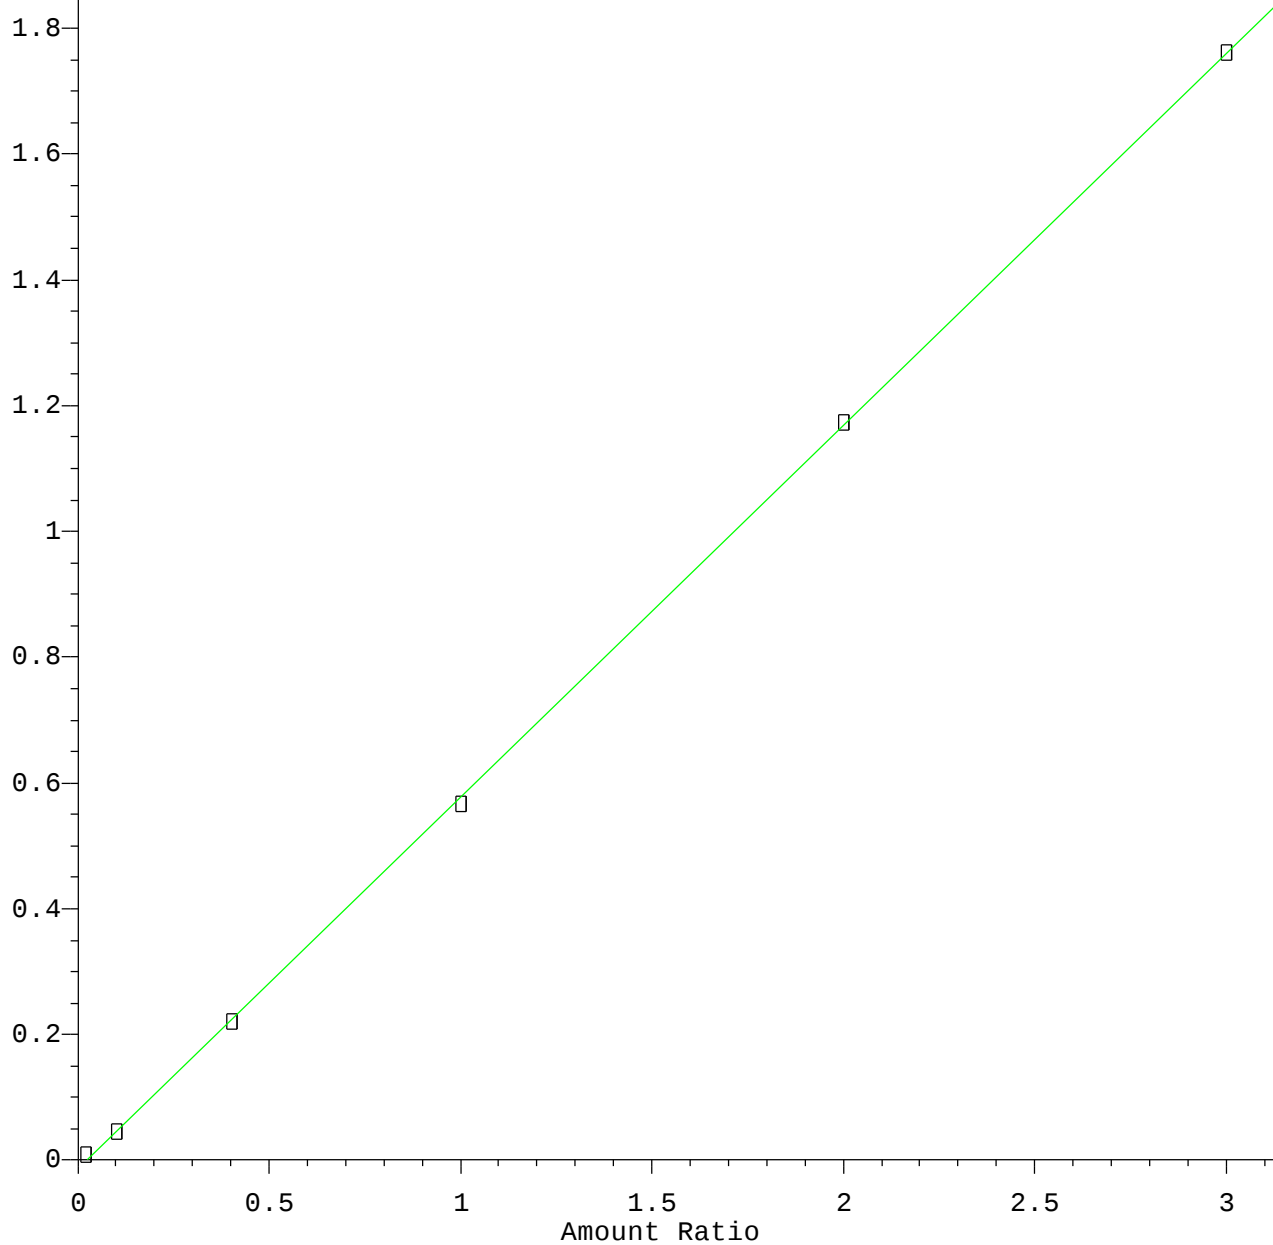

Resp Ratio = $5.91 \times 10^{-1} \times \text{Amt} - 1.36 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Calibration Table Last Updated: Fri May 29 02:14:10 2020

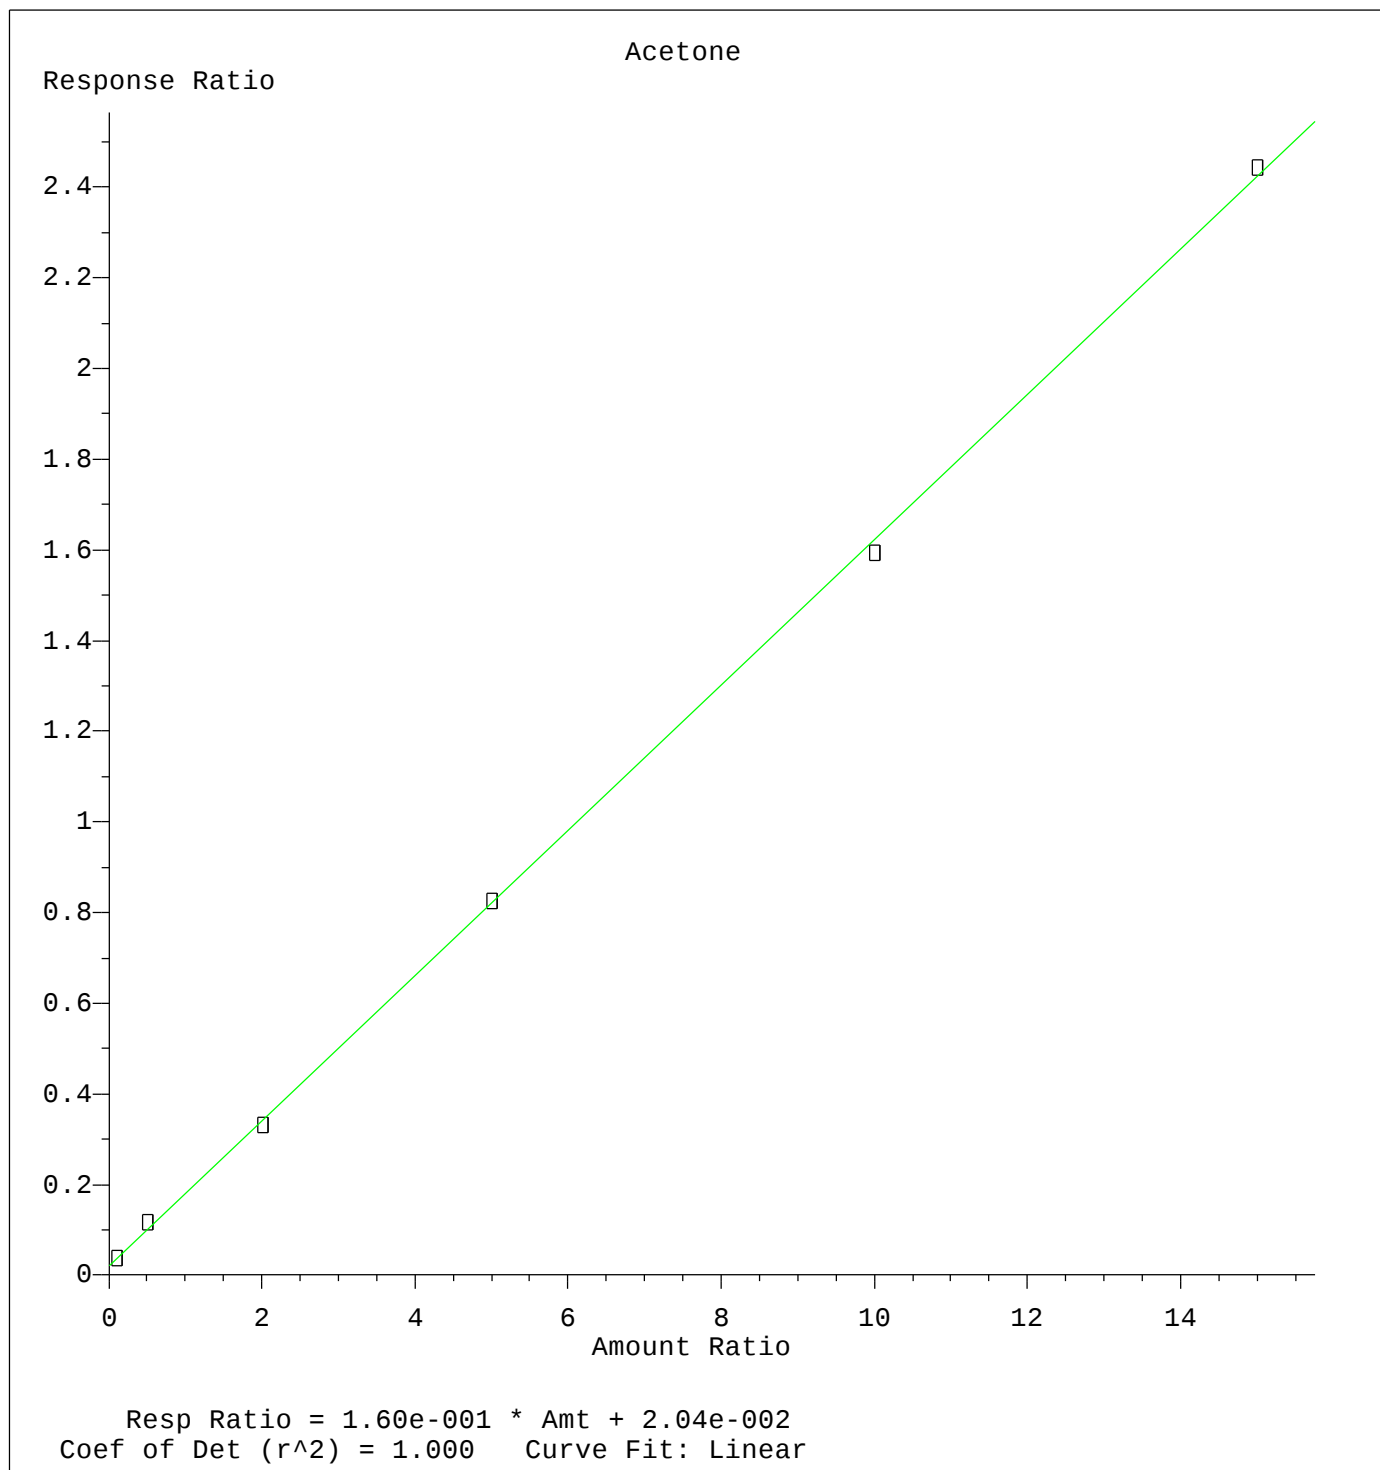

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Calibration Table Last Updated: Fri May 29 02:14:10 2020

Methylene Chloride

Response Ratio

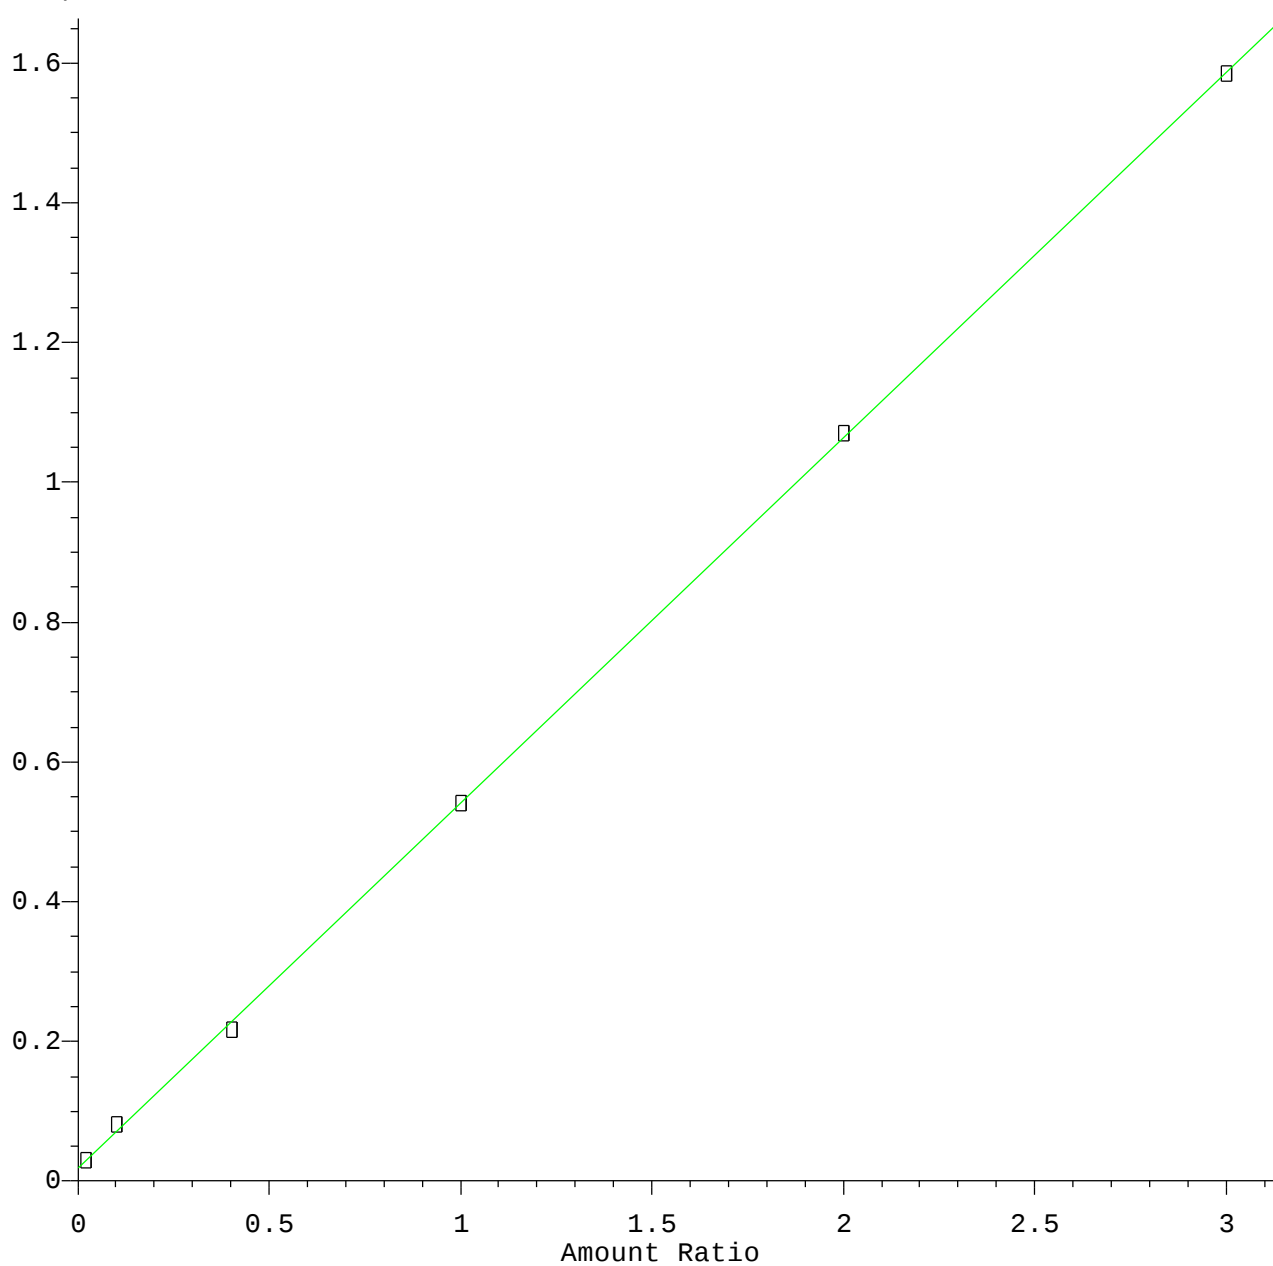

Resp Ratio = 5.23e-001 * Amt + 1.88e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Calibration Table Last Updated: Fri May 29 02:14:10 2020