

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052821\
 Data File : VN067183.D
 Acq On : 28 May 2021 15:15
 Operator : JC/MD
 Sample : PB136697TB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB136697TB

Quant Time: May 29 02:23:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
 Quant Title : SW846 8260
 QLast Update : Fri May 21 17:24:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.581	168	251932	50.00	ug/l	#-0.02
34) 1,4-Difluorobenzene	8.509	114	459527	50.00	ug/l	-0.02
63) Chlorobenzene-d5	11.344	117	411220	50.00	ug/l	-0.01
72) 1,4-Dichlorobenzene-d4	13.285	152	148849	50.00	ug/l	-0.01

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.943	65	184049	47.07	ug/l	-0.02
Spiked Amount	50.000	Range	61 - 141	Recovery	=	94.14%
35) Dibromofluoromethane	7.503	113	142727	50.61	ug/l	-0.02
Spiked Amount	50.000	Range	69 - 133	Recovery	=	101.22%
50) Toluene-d8	10.022	98	568177	52.35	ug/l	-0.01
Spiked Amount	50.000	Range	65 - 126	Recovery	=	104.70%
62) 4-Bromofluorobenzene	12.341	95	194327	52.38	ug/l	-0.01
Spiked Amount	50.000	Range	58 - 135	Recovery	=	104.76%


Target Compounds						Qvalue
3) Chloromethane	2.032	50	1498	0.33	ug/l	# 88
11) Tert butyl alcohol	4.679	59	302	0.37	ug/l	# 87
13) Acrolein	3.537	56	392	0.57	ug/l	# 70
16) Acetone	3.746	43	24651	15.34	ug/l	92
18) Methyl Acetate	4.245	43	1785	0.40	ug/l	# 58
20) Methylene Chloride	4.462	84	23400	5.92	ug/l	# 86
25) 2-Butanone	6.741	43	2287	0.90	ug/l	# 82
29) Tetrahydrofuran	7.114	42	387	0.23	ug/l	# 43
31) Cyclohexane	7.581	56	5712	0.94	ug/l	# 1
36) 1,1-Dichloropropene	7.581	75	22147	4.77	ug/l	# 43
38) Carbon Tetrachloride	7.581	117	27193	6.01	ug/l	# 15
43) Isopropyl Acetate	8.085	43	38178	4.30	ug/l	# 84
45) 1,2-Dichloropropane	9.198	63	2132	0.55	ug/l	# 45
48) Methyl methacrylate	9.112	41	8134	2.06	ug/l	# 9
49) 1,4-Dioxane	9.193	88	86	62.00	ug/l	# 1
51) 4-Methyl-2-Pentanone	9.914	43	3871	0.79	ug/l	# 55
54) cis-1,3-Dichloropropene	9.836	75	56777	9.63	ug/l	# 63
56) Ethyl methacrylate	10.367	69	49	2.80	ug/l	# 1
57) 1,3-Dichloropropane	10.700	76	28161	4.90	ug/l	# 43
59) 2-Hexanone	10.700	43	411987	120.95	ug/l	# 46
70) Styrene	11.918	104	940	2.59	ug/l	# 86
76) 1,2,3-Trichloropropane	12.341	75	98434	23.76	ug/l	# 100
80) 1,3,5-Trimethylbenzene	12.682	105	2899	0.24	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.341	75	98434	67.30	ug/l	# 15
86) p-Isopropyltoluene	13.235	119	2223	0.21	ug/l	89
87) 1,3-Dichlorobenzene	13.229	146	1445	0.29	ug/l	69
88) 1,4-Dichlorobenzene	13.304	146	2639	0.50	ug/l	# 52
92) 1,2-Dibromo-3-Chloropr...	14.238	75	198	0.25	ug/l	59
93) 1,2,4-Trichlorobenzene	14.871	180	1965	3.98	ug/l	84
94) Hexachlorobutadiene	14.954	225	436	0.34	ug/l	84
95) Naphthalene	15.082	128	4239	4.38	ug/l	# 78
96) 1,2,3-Trichlorobenzene	15.259	180	3146	1.48	ug/l	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052821\
Data File : VN067183.D
Acq On : 28 May 2021 15:15
Operator : JC/MD
Sample : PB136697TB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB136697TB

Quant Time: May 29 02:23:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
Quant Title : SW846 8260
QLast Update : Fri May 21 17:24:08 2021
Response via : Initial Calibration




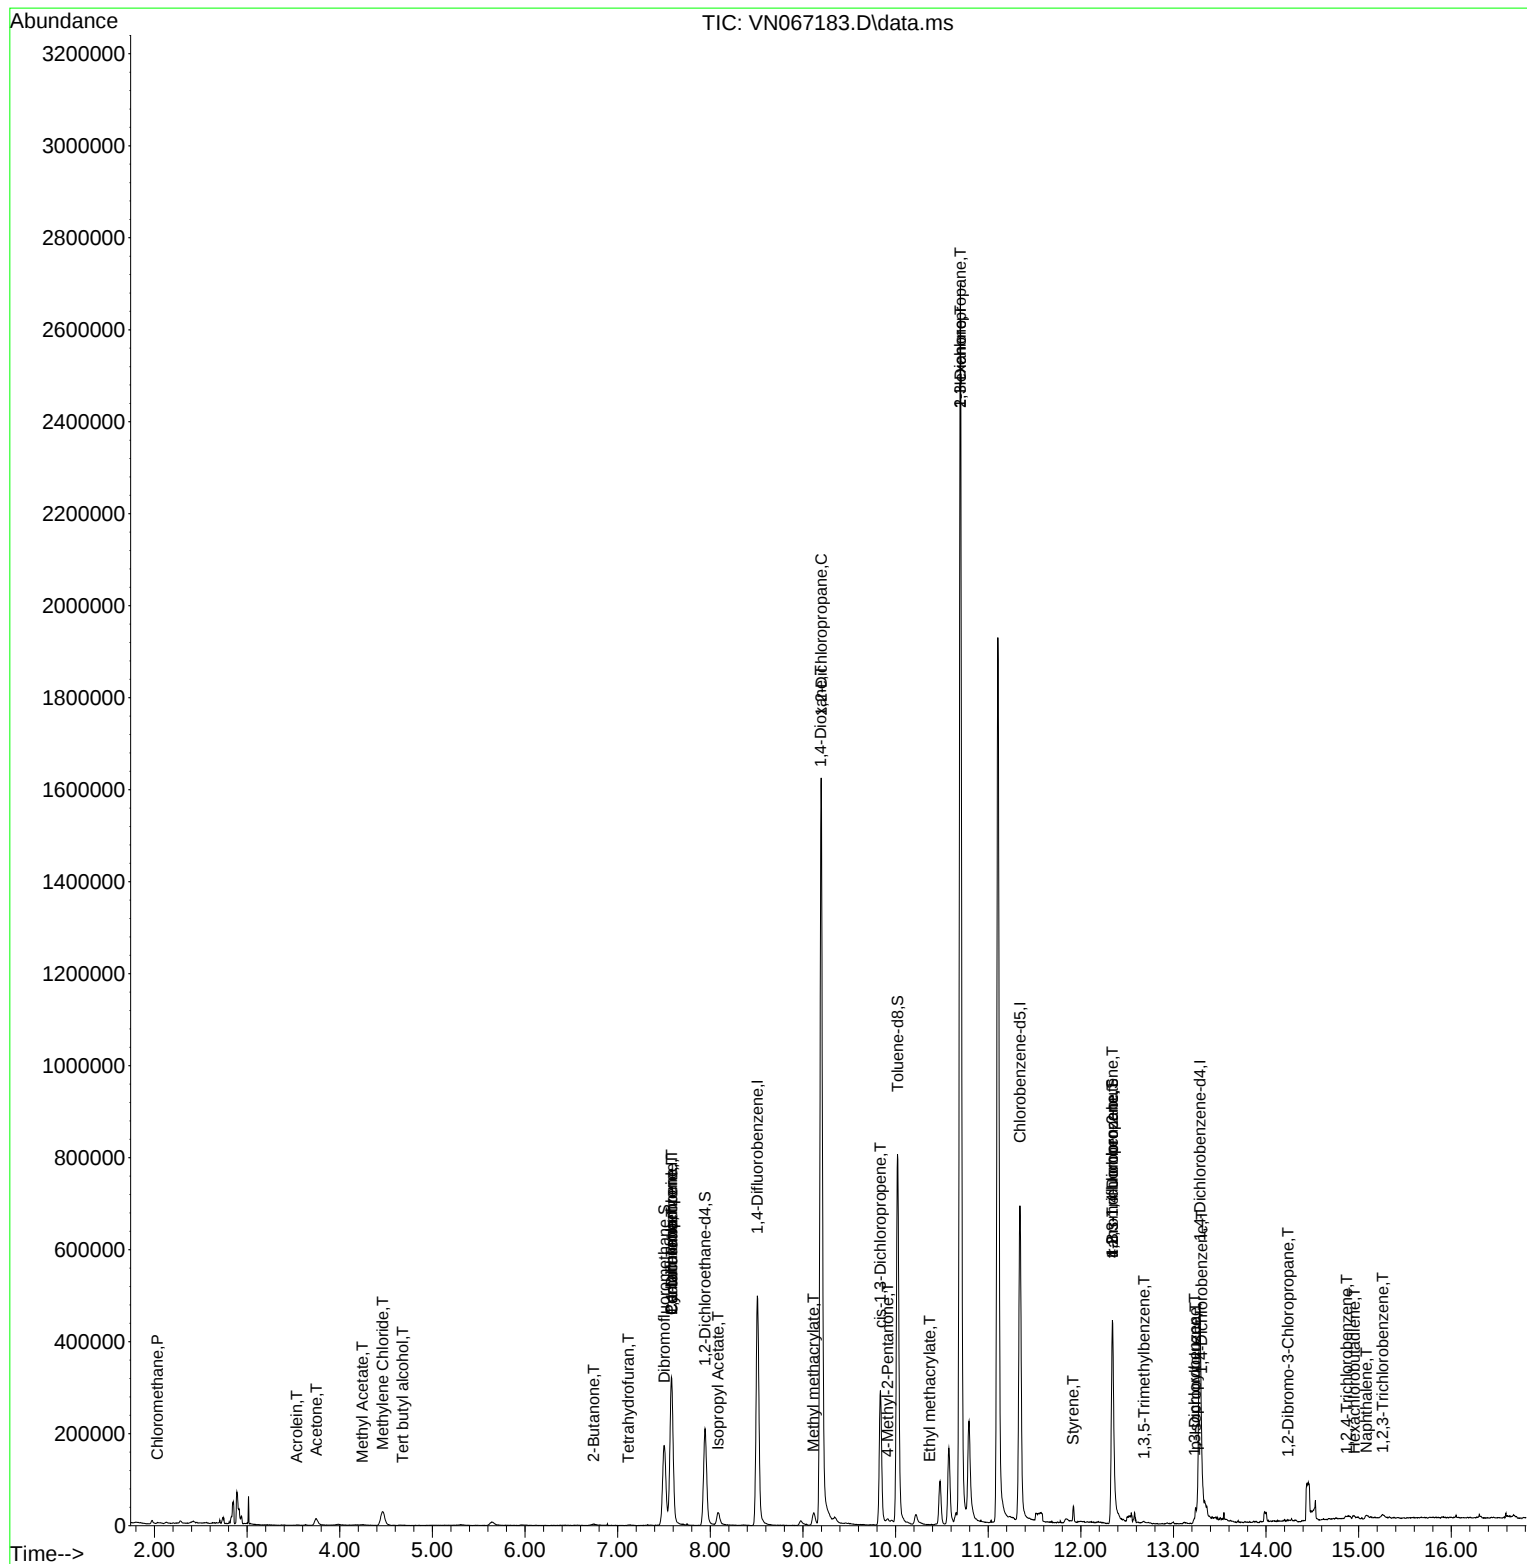


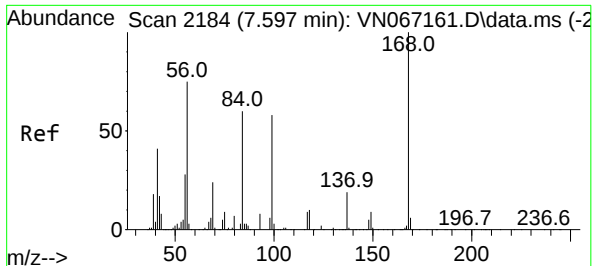

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.581 min Scan# 2178
Delta R.T. -0.016 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampled :
PB136697TB


Tgt Ion:168 Resp: 251932
Ion Ratio Lower Upper
168 100
99 64.4 38.5 57.7#

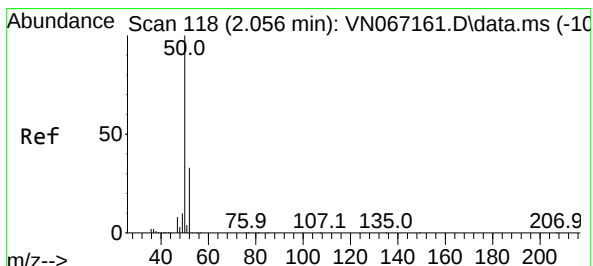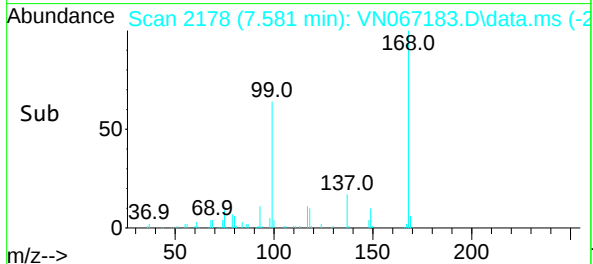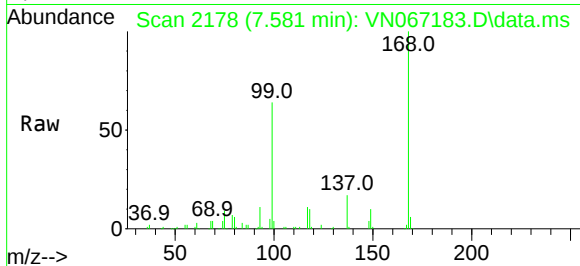

#3
Chloromethane
Concen: 0.33 ug/l
RT: 2.032 min Scan# 109
Delta R.T. -0.024 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 50 Resp: 1498
Ion Ratio Lower Upper
50 100
52 26.5 26.5 39.7#

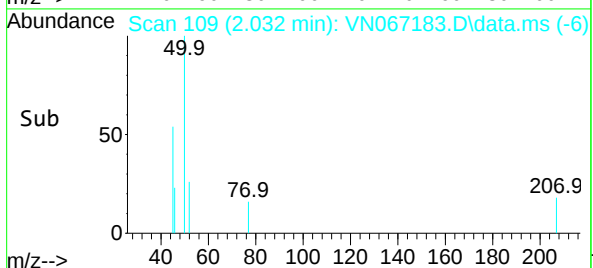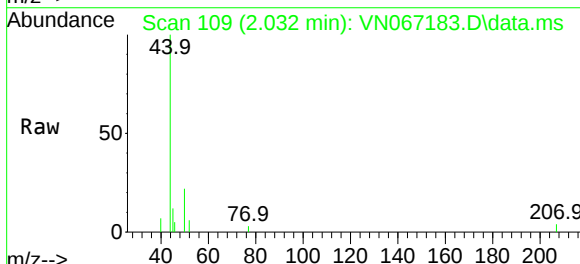







#11

Tert butyl alcohol
Concen: 0.37 ug/l
RT: 4.679 min Scan# 1096
Delta R.T. -0.043 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Instrument :
MSVOA_N
ClientSampleId :
PB136697TB




Tgt Ion: 59 Resp: 302
Ion Ratio Lower Upper
59 100
57 0.0 3.5 5.3#




#13

Acrolein
Concen: 0.57 ug/l
RT: 3.537 min Scan# 670
Delta R.T. -0.021 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 56 Resp: 392
Ion Ratio Lower Upper
56 100
55 43.1 53.8 80.6#


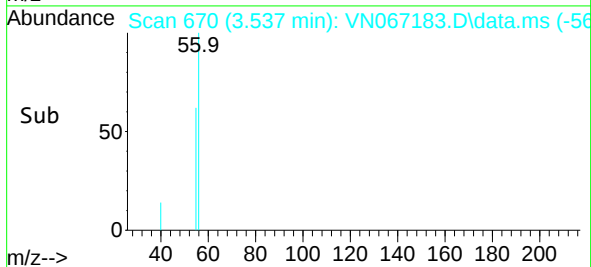

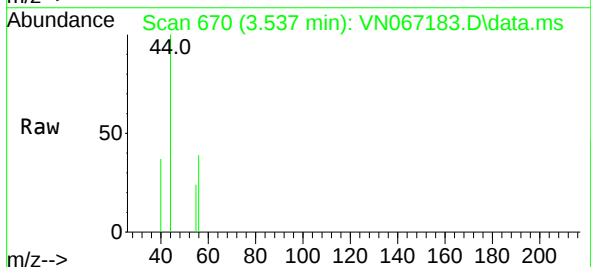




#16
Acetone
Concen: 15.34 ug/l
RT: 3.746 min Scan# 748
Delta R.T. -0.021 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion: 43 Resp: 24651
Ion Ratio Lower Upper
43 100
58 29.2 27.2 40.8

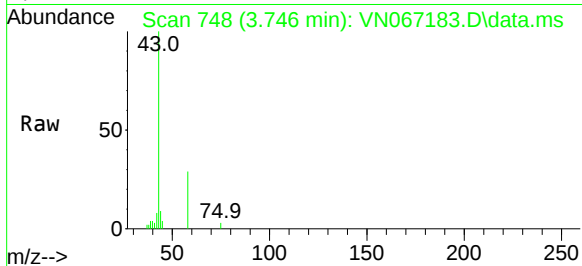

#18
Methyl Acetate
Concen: 0.40 ug/l
RT: 4.245 min Scan# 934
Delta R.T. -0.018 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 43 Resp: 1785
Ion Ratio Lower Upper
43 100
74 4.9 21.4 32.2#

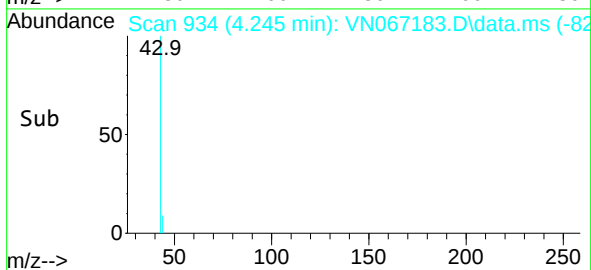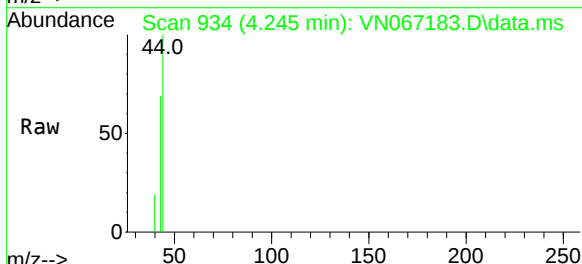



#20

Methylene Chloride

Concen: 5.92 ug/l

RT: 4.462 min Scan# 1015

Delta R.T. -0.021 min

Lab File: VN067183.D

Acq: 28 May 2021 15:15

Tgt Ion: 84 Resp: 23400





Ion Ratio Lower Upper

84 100

49 130.7 88.3 132.5

51 41.1 26.7 40.1#

86 58.6 51.1 76.7

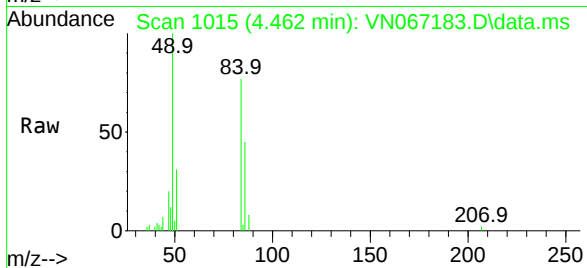

#25

2-Butanone

Concen: 0.90 ug/l

RT: 6.741 min Scan# 1865

Delta R.T. -0.014 min

Lab File: VN067183.D




Acq: 28 May 2021 15:15


Tgt Ion: 43 Resp: 2287

Ion Ratio Lower Upper

43 100

72 20.6 24.4 36.6#




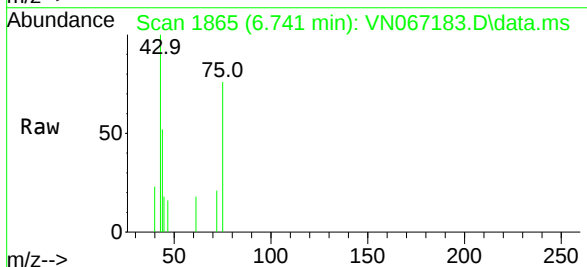


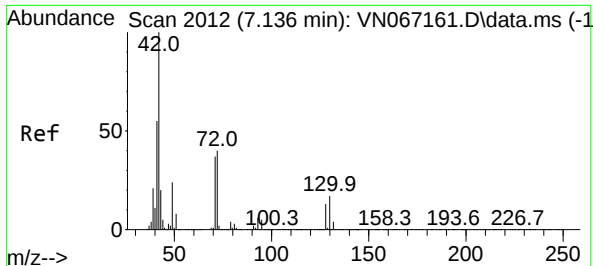

#29
Tetrahydrofuran
Concen: 0.23 ug/l
RT: 7.114 min Scan# 2004
Delta R.T. -0.022 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampled :
PB136697TB


Tgt Ion:	42	Resp:	387
Ion	Ratio	Lower	Upper
42	100		
72	13.4	40.1	60.1#
71	6.5	37.9	56.9#

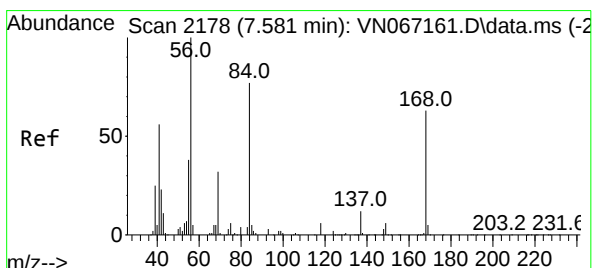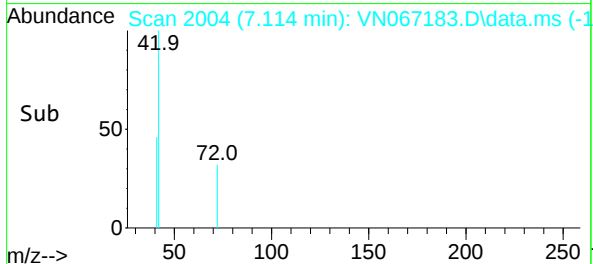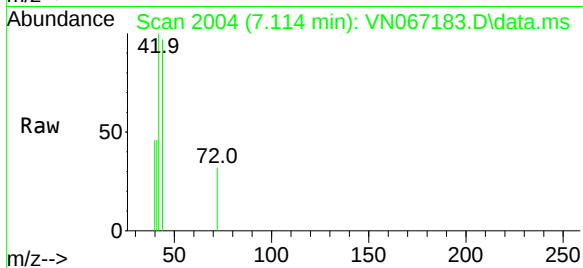

#31
Cyclohexane
Concen: 0.94 ug/l
RT: 7.581 min Scan# 2178
Delta R.T. -0.000 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion:	56	Resp:	5712
Ion	Ratio	Lower	Upper
56	100		
69	185.2	28.0	42.0#
84	146.2	74.2	111.2#


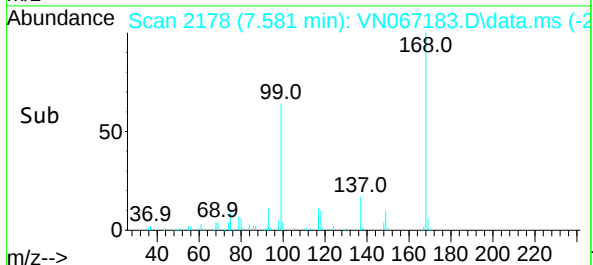

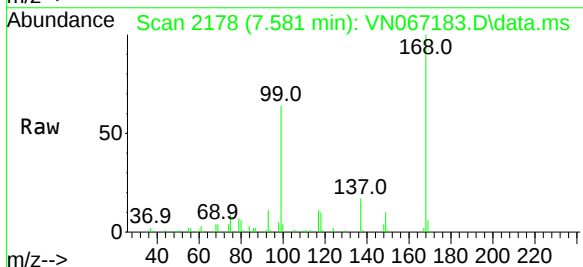




#33
1,2-Dichloroethane-d4
Concen: 47.07 ug/l
RT: 7.943 min Scan# 2313
Delta R.T. -0.016 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion: 65 Resp: 184049
Ion Ratio Lower Upper
65 100
67 54.7 0.0 110.4



#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.509 min Scan# 2524
Delta R.T. -0.016 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 114 Resp: 459527
Ion Ratio Lower Upper
114 100
63 22.4 0.0 35.8
88 16.6 0.0 30.4


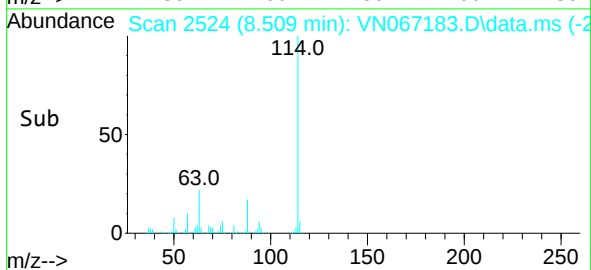






#35
Dibromofluoromethane
Concen: 50.61 ug/l
RT: 7.503 min Scan# 2149
Delta R.T. -0.016 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:113 Resp: 142727
Ion Ratio Lower Upper
113 100
111 105.2 82.6 124.0
192 17.0 18.2 27.4#

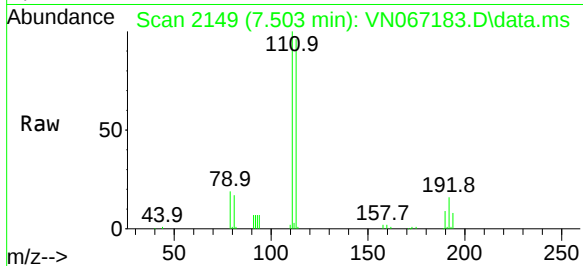

#36
1,1-Dichloropropene
Concen: 4.77 ug/l
RT: 7.581 min Scan# 2178
Delta R.T. -0.142 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 75 Resp: 22147
Ion Ratio Lower Upper
75 100
110 4.0 19.1 57.3#
77 0.0 24.8 37.2#


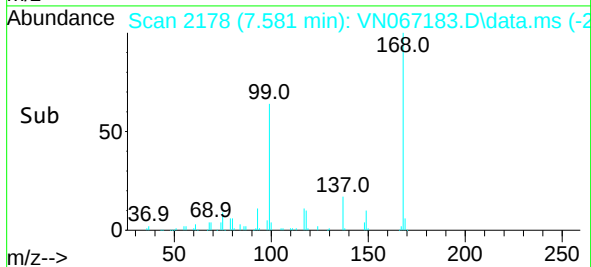

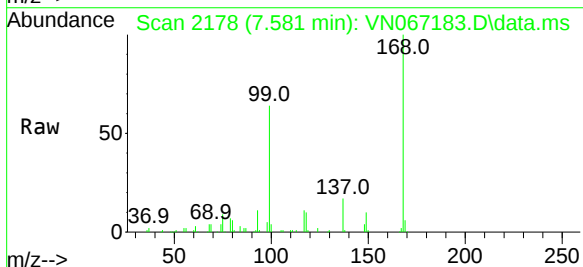




#38
Carbon Tetrachloride
Concen: 6.01 ug/l
RT: 7.581 min Scan# 2178
Delta R.T. -0.121 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion: 117 Resp: 27193
Ion Ratio Lower Upper
117 100
119 5.2 78.2 117.2#
121 0.0 24.7 37.1#

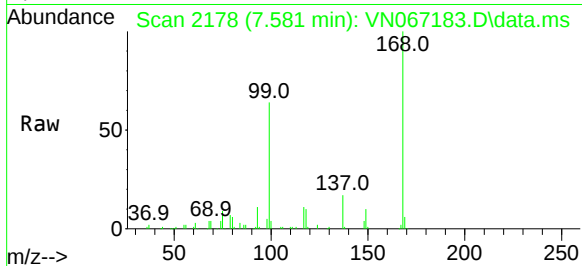

#43
Isopropyl Acetate
Concen: 4.30 ug/l
RT: 8.085 min Scan# 2366
Delta R.T. -0.016 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 43 Resp: 38178
Ion Ratio Lower Upper
43 100
61 18.8 23.4 35.0#
87 11.1 12.2 18.2#

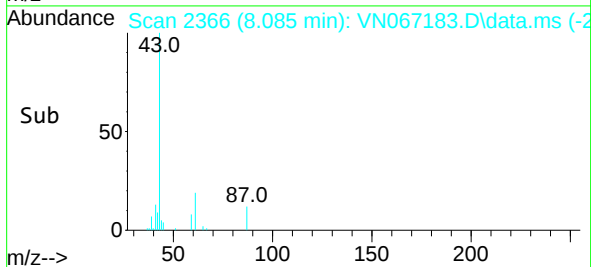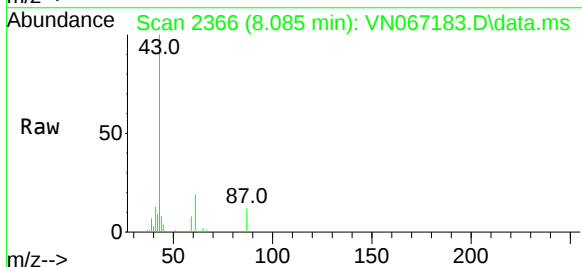



#45

1,2-Dichloropropane

Concen: 0.55 ug/l

RT: 9.198 min Scan# 2781

Delta R.T. 0.139 min

Lab File: VN067183.D

Acq: 28 May 2021 15:15

Tgt Ion: 63 Resp: 2132

Ion Ratio Lower Upper

63 100





65 0.0 23.9 35.9#

Instrument :

MSVOA_N

ClientSampleId :

PB136697TB

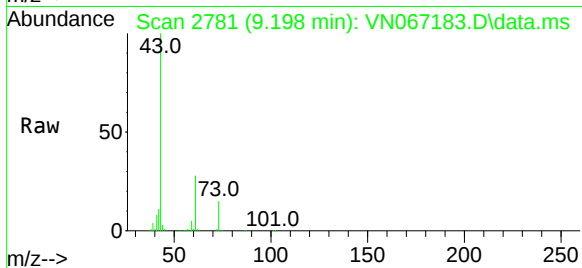

#48

Methyl methacrylate

Concen: 2.06 ug/l

RT: 9.112 min Scan# 2749

Delta R.T. -0.033 min

Lab File: VN067183.D

Acq: 28 May 2021 15:15




Tgt Ion: 41 Resp: 8134


Ion Ratio Lower Upper

41 100

69 0.7 80.5 120.7#

39 0.0 41.4 62.0#


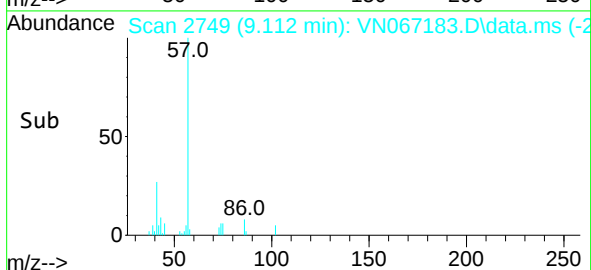

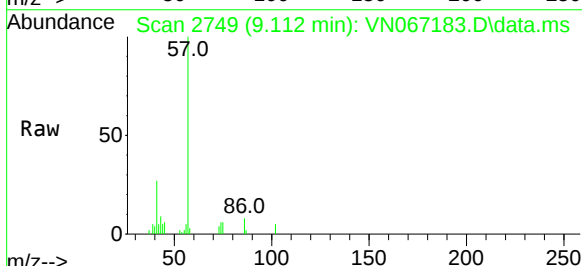




#49
1,4-Dioxane
Concen: 62.00 ug/l
RT: 9.193 min Scan# 2779
Delta R.T. 0.048 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion: 88 Resp: 86
Ion Ratio Lower Upper
88 100
43 2034286.0 21.8 32.8#
58 7782.6 50.8 76.2#

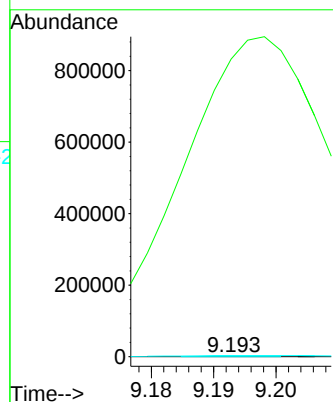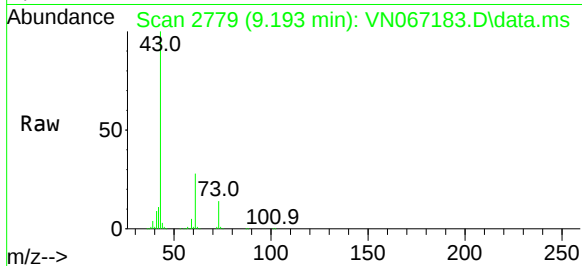

#50
Toluene-d8
Concen: 52.35 ug/l
RT: 10.022 min Scan# 3088
Delta R.T. -0.014 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 98 Resp: 568177
Ion Ratio Lower Upper
98 100
100 66.0 51.8 77.8


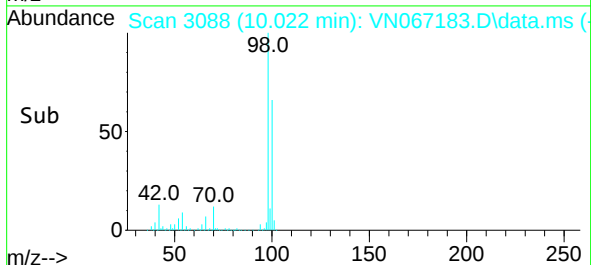
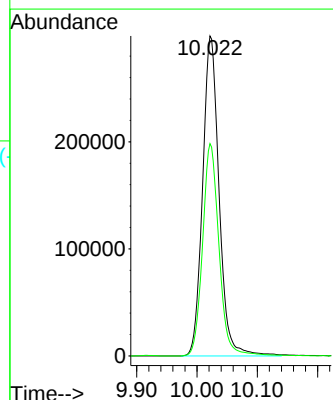
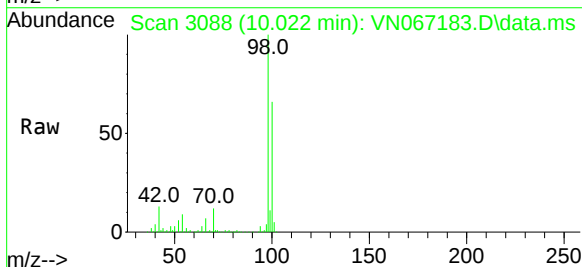


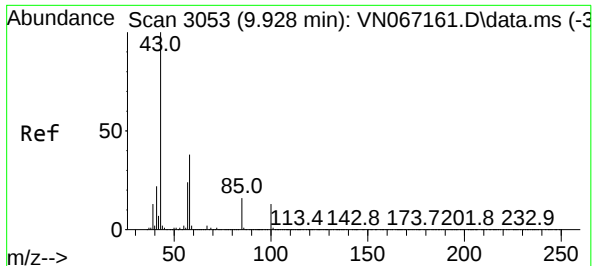

#51
4-Methyl-2-Pentanone
Concen: 0.79 ug/l
RT: 9.914 min Scan# 3048
Delta R.T. -0.014 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampled :
PB136697TB


Tgt Ion: 43 Resp: 3871
Ion Ratio Lower Upper
43 100
58 72.1 34.5 51.7#

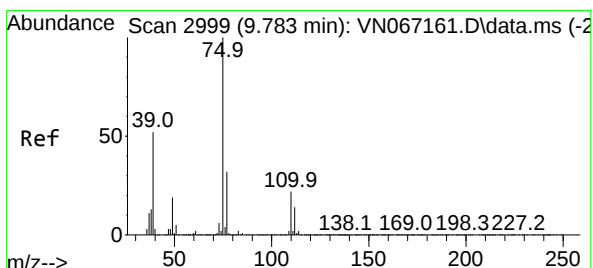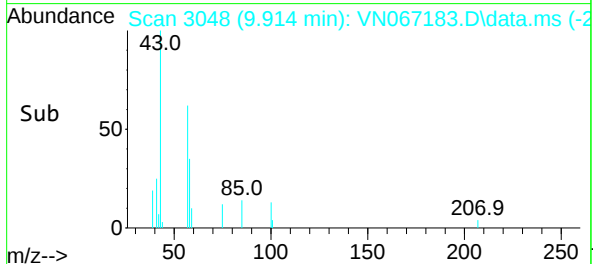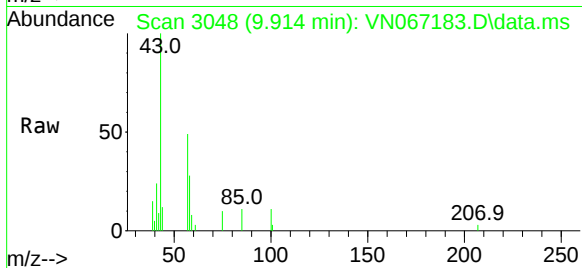

#54
cis-1,3-Dichloropropene
Concen: 9.63 ug/l
RT: 9.836 min Scan# 3019
Delta R.T. 0.053 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 75 Resp: 56777
Ion Ratio Lower Upper
75 100
77 0.0 25.1 37.7#
39 25.9 30.9 46.3#


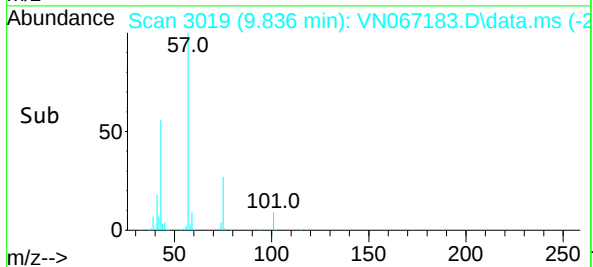

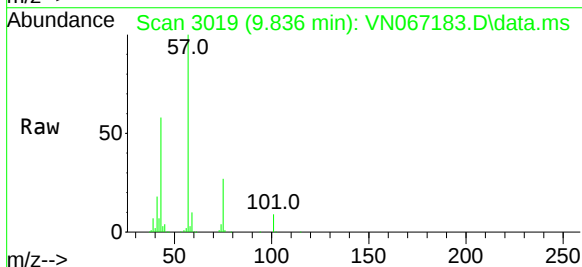




#56
Ethyl methacrylate
Concen: 2.80 ug/l
RT: 10.367 min Scan# 3217
Delta R.T. -0.011 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion: 69 Resp: 49
Ion Ratio Lower Upper
69 100
41 0.0 45.5 68.3#
39 606.1 22.9 34.3#

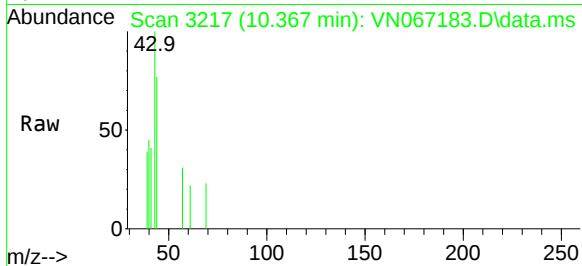

#57
1,3-Dichloropropane
Concen: 4.90 ug/l
RT: 10.700 min Scan# 3341
Delta R.T. 0.045 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 76 Resp: 28161
Ion Ratio Lower Upper
76 100
78 0.8 26.3 39.5#


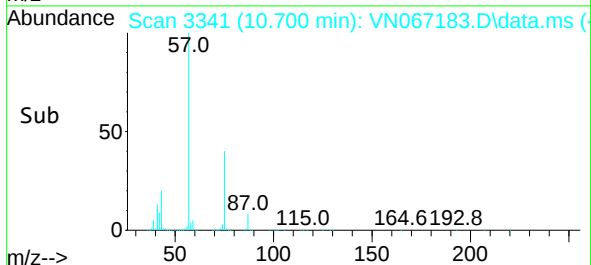

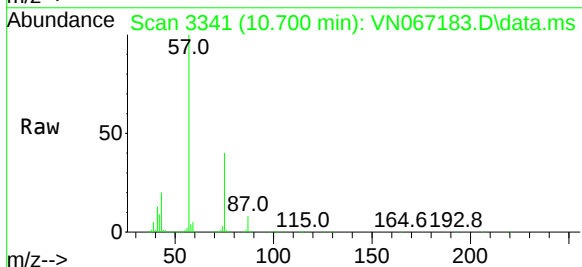




#59
2-Hexanone
Concen: 120.95 ug/l
RT: 10.700 min Scan# 3341
Delta R.T. 0.000 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampled :
PB136697TB


Tgt Ion: 43 Resp: 411987
Ion Ratio Lower Upper
43 100
58 19.1 29.8 89.5#

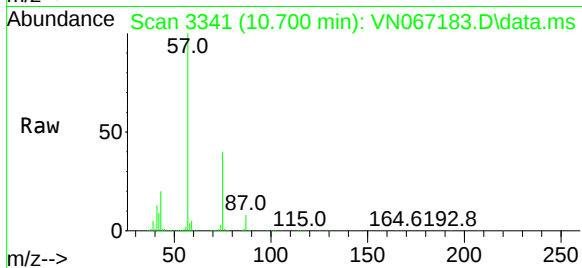

#62
4-Bromofluorobenzene
Concen: 52.38 ug/l
RT: 12.341 min Scan# 3953
Delta R.T. -0.014 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 95 Resp: 194327
Ion Ratio Lower Upper
95 100
174 67.0 0.0 182.8
176 64.5 0.0 176.6


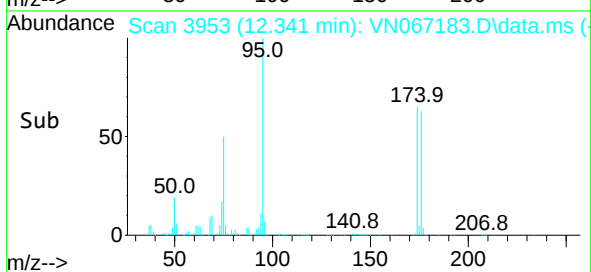

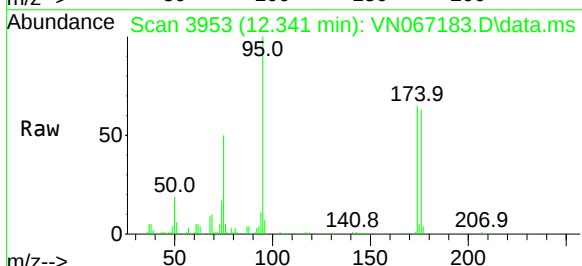




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.344 min Scan# 3581
Delta R.T. -0.013 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:117 Resp: 411220
Ion Ratio Lower Upper
117 100
82 60.1 42.2 63.2
119 32.0 25.8 38.6

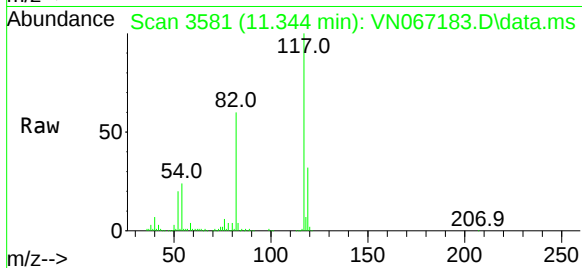

#70
Styrene
Concen: 2.59 ug/l
RT: 11.918 min Scan# 3795
Delta R.T. -0.000 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion:104 Resp: 940
Ion Ratio Lower Upper
104 100
78 50.5 37.7 56.5
103 70.9 44.2 66.4#


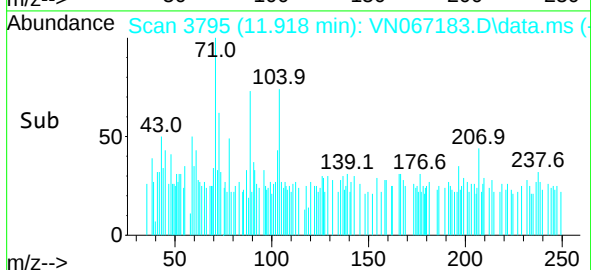

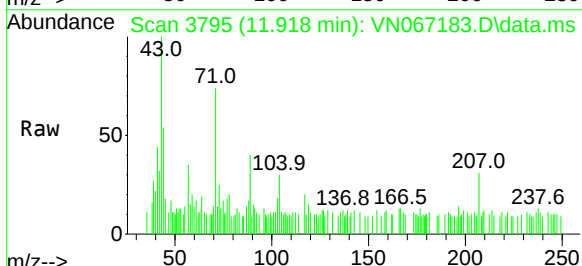


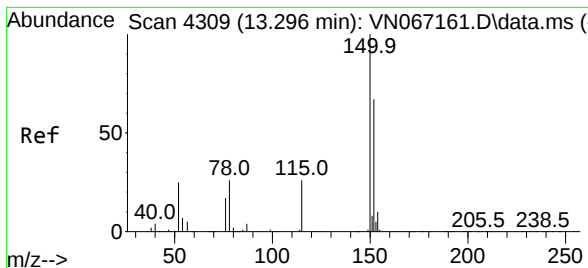

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.285 min Scan# 4305
Delta R.T. -0.011 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:152 Resp: 148849
Ion Ratio Lower Upper
152 100
115 66.3 27.0 80.8
150 166.4 0.0 350.2

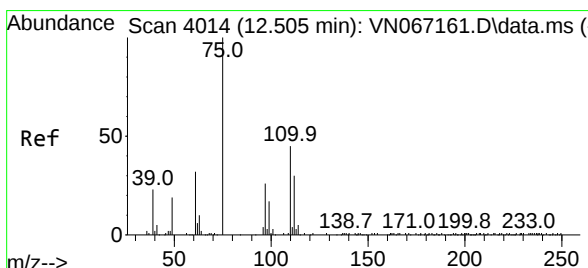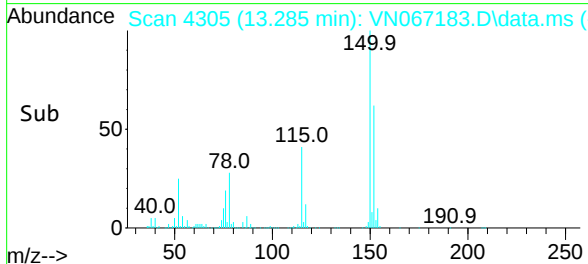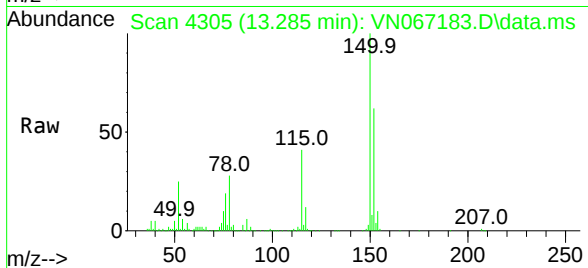

#76
1,2,3-Trichloropropane
Concen: 23.76 ug/l
RT: 12.341 min Scan# 3953
Delta R.T. -0.164 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 75 Resp: 98434
Ion Ratio Lower Upper
75 100
77 0.9 0.0 0.0#


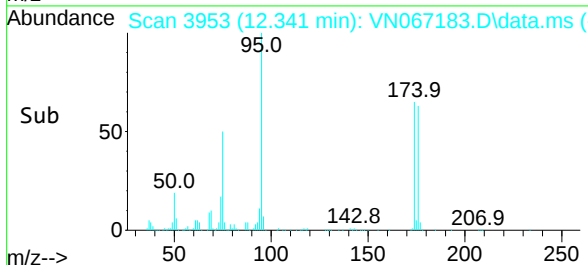

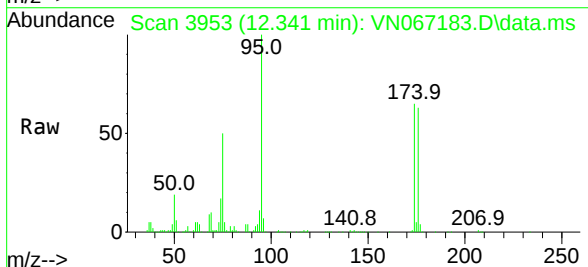


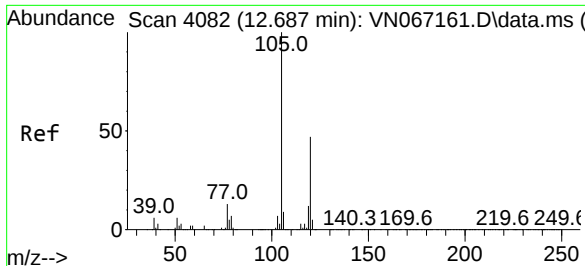

#80
1,3,5-Trimethylbenzene
Concen: 0.24 ug/l
RT: 12.682 min Scan# 4080
Delta R.T. -0.005 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:105 Resp: 2899
Ion Ratio Lower Upper
105 100
120 44.0 25.0 75.0

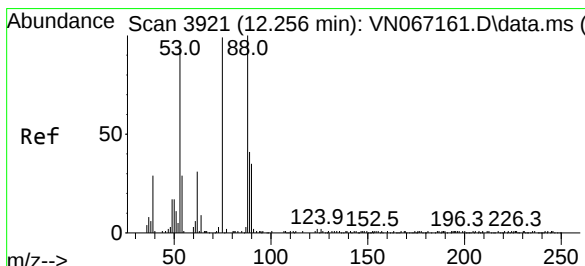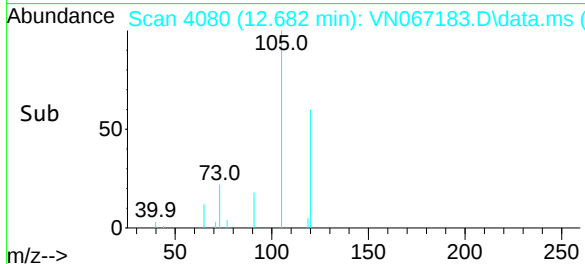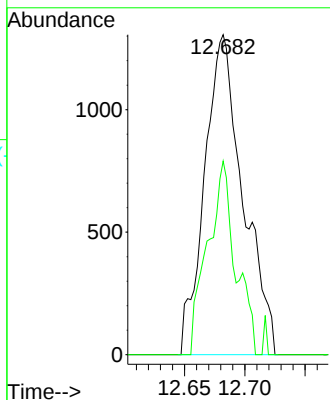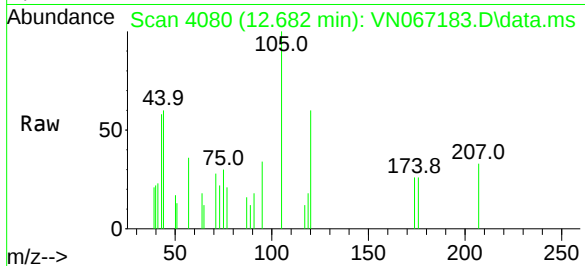

#81
trans-1,4-Dichloro-2-butene
Concen: 67.30 ug/l
RT: 12.341 min Scan# 3953
Delta R.T. 0.085 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 75 Resp: 98434
Ion Ratio Lower Upper
75 100
53 0.1 66.3 99.5#
89 0.1 39.5 59.3#


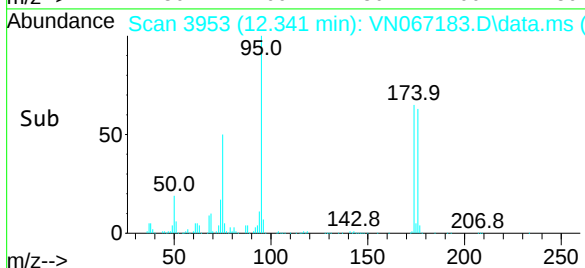
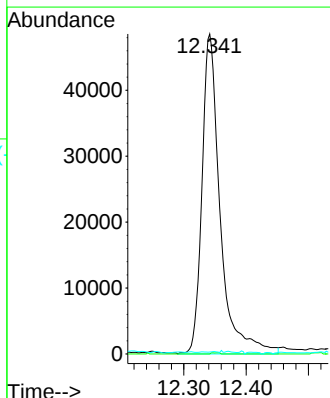
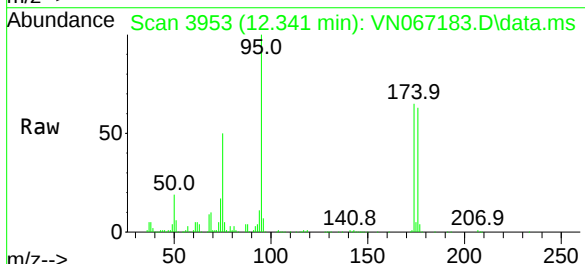




#86
p-Isopropyltoluene
Concen: 0.21 ug/l
RT: 13.235 min Scan# 4286
Delta R.T. -0.008 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:119 Resp: 2223
Ion Ratio Lower Upper
119 100
134 23.5 13.3 39.9
91 29.4 10.7 32.1

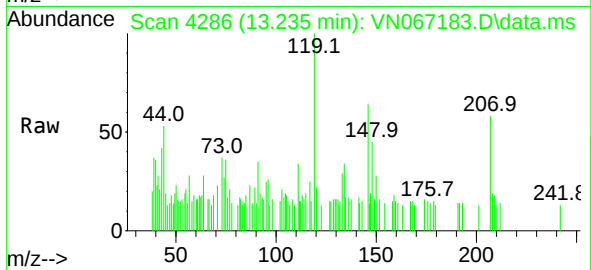

#87
1,3-Dichlorobenzene
Concen: 0.29 ug/l
RT: 13.229 min Scan# 4284
Delta R.T. -0.008 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion:146 Resp: 1445
Ion Ratio Lower Upper
146 100
111 57.1 19.3 57.8
148 88.4 32.0 96.2




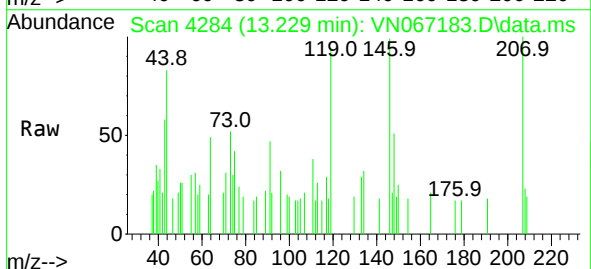


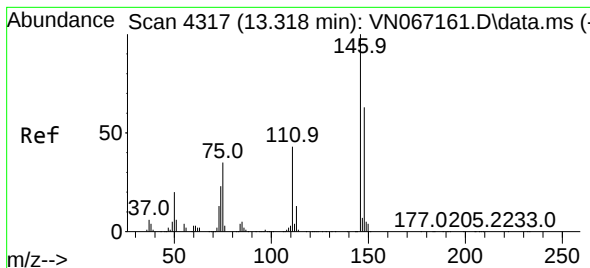

#88
1,4-Dichlorobenzene
Concen: 0.50 ug/l
RT: 13.304 min Scan# 4312
Delta R.T. -0.014 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:146 Resp: 2639
Ion Ratio Lower Upper
146 100
111 96.3 18.5 55.5#
148 77.2 31.4 94.3

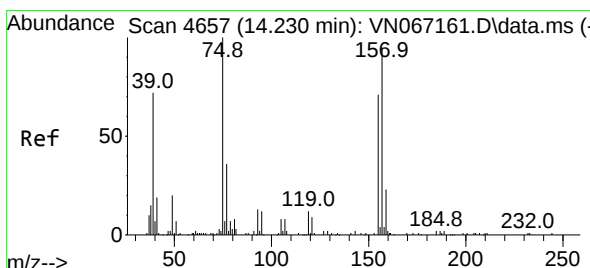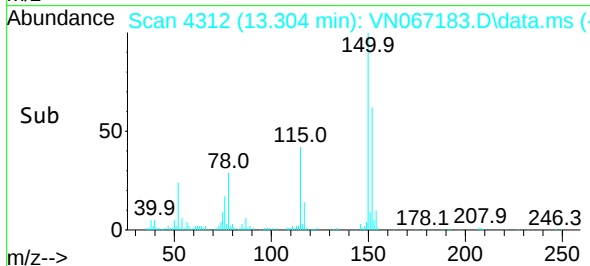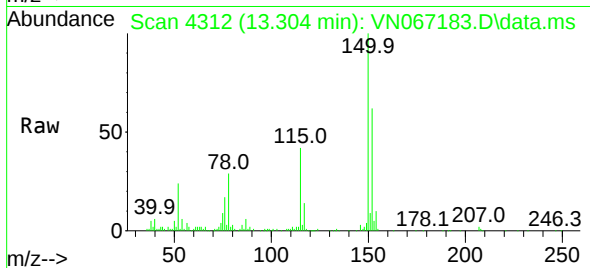

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.25 ug/l
RT: 14.238 min Scan# 4660
Delta R.T. 0.008 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion: 75 Resp: 198
Ion Ratio Lower Upper
75 100
155 72.7 49.9 149.7
157 68.2 63.8 191.4


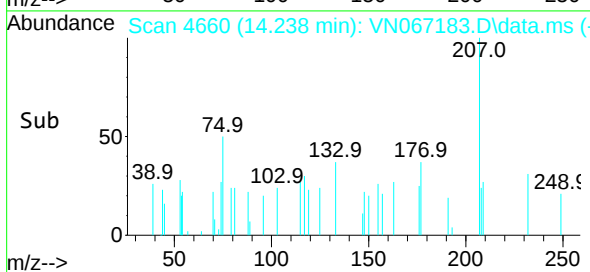

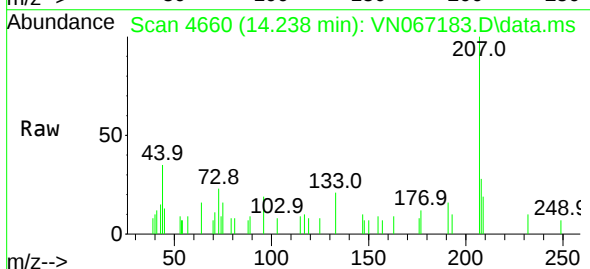




#93
1,2,4-Trichlorobenzene
Concen: 3.98 ug/l
RT: 14.871 min Scan# 4896
Delta R.T. 0.005 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15




Instrument :
MSVOA_N
ClientSampleId :
PB136697TB


Tgt Ion:180 Resp: 1965
Ion Ratio Lower Upper
180 100
182 113.8 47.3 141.8
145 29.0 14.0 42.0

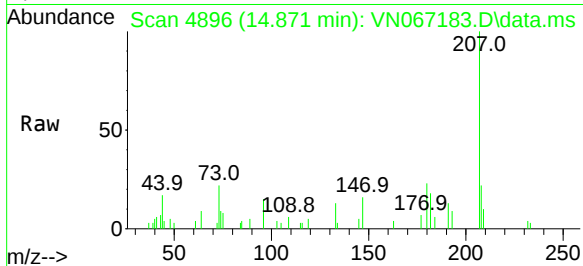

#94
Hexachlorobutadiene
Concen: 0.34 ug/l
RT: 14.954 min Scan# 4927
Delta R.T. -0.008 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion:225 Resp: 436
Ion Ratio Lower Upper
225 100
223 73.9 31.7 95.1
227 77.3 31.7 95.1



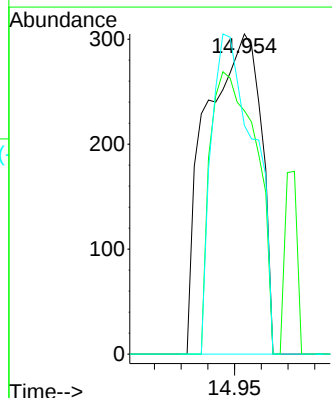
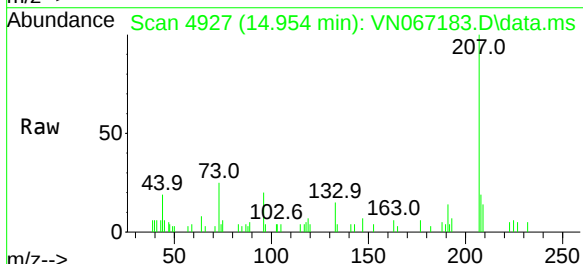


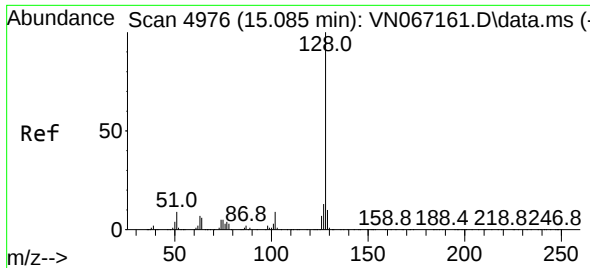

#95
Naphthalene
Concen: 4.38 ug/l
RT: 15.082 min Scan# 4975
Delta R.T. -0.003 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Instrument :
MSVOA_N
ClientSampleId :
PB136697TB

Tgt Ion:128 Resp: 4239
Ion Ratio Lower Upper
128 100
127 25.7 10.2 15.2#
129 14.4 8.6 13.0#

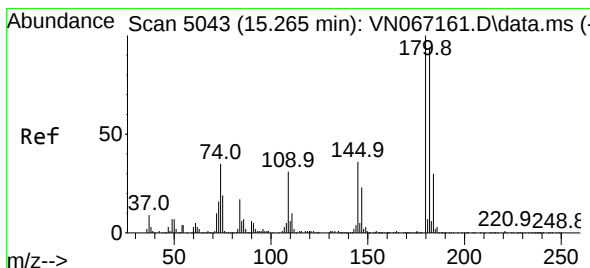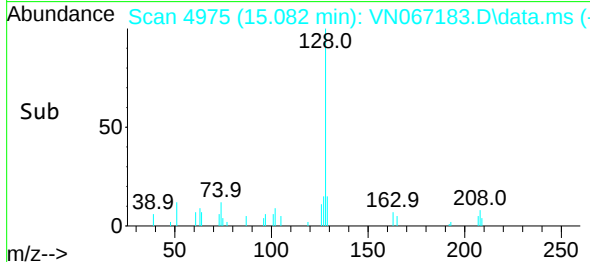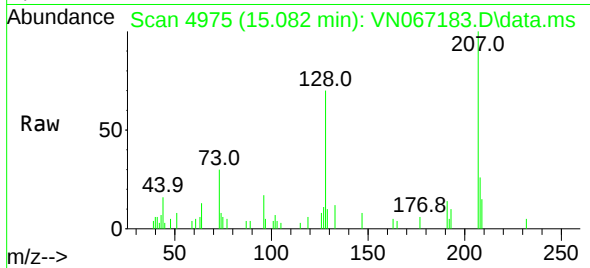

#96
1,2,3-Trichlorobenzene
Concen: 1.48 ug/l
RT: 15.259 min Scan# 5041
Delta R.T. -0.006 min
Lab File: VN067183.D
Acq: 28 May 2021 15:15

Tgt Ion:180 Resp: 3146
Ion Ratio Lower Upper
180 100
182 79.7 48.5 145.6
145 6.4 15.4 46.2#

