

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN052821\  
 Data File : VN067185.D  
 Acq On : 28 May 2021 16:02  
 Operator : JC/MD  
 Sample : PB136697ZHE#02  
 Misc : 5.00mL/MSVOA\_N/WATER  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB136697ZHE#02

Quant Time: May 29 02:24:09 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N052121W.M  
 Quant Title : SW846 8260  
 QLast Update : Fri May 21 17:24:08 2021  
 Response via : Initial Calibration


| Compound                      | R.T.           | QIon | Response   | Conc    | Units  | Dev(Min) |
|-------------------------------|----------------|------|------------|---------|--------|----------|
| -----                         |                |      |            |         |        |          |
| Internal Standards            |                |      |            |         |        |          |
| 1) Pentafluorobenzene         | 7.583          | 168  | 250090     | 50.00   | ug/l   | #-0.01   |
| 34) 1,4-Difluorobenzene       | 8.509          | 114  | 459640     | 50.00   | ug/l   | -0.02    |
| 63) Chlorobenzene-d5          | 11.344         | 117  | 399464     | 50.00   | ug/l   | -0.01    |
| 72) 1,4-Dichlorobenzene-d4    | 13.285         | 152  | 143352     | 50.00   | ug/l   | -0.01    |
|                               |                |      |            |         |        |          |
| System Monitoring Compounds   |                |      |            |         |        |          |
| 33) 1,2-Dichloroethane-d4     | 7.943          | 65   | 182690     | 47.07   | ug/l   | -0.02    |
| Spiked Amount 50.000          | Range 61 - 141 |      | Recovery = | 94.14%  |        |          |
| 35) Dibromofluoromethane      | 7.506          | 113  | 143024     | 50.70   | ug/l   | -0.01    |
| Spiked Amount 50.000          | Range 69 - 133 |      | Recovery = | 101.40% |        |          |
| 50) Toluene-d8                | 10.021         | 98   | 558891     | 51.48   | ug/l   | -0.01    |
| Spiked Amount 50.000          | Range 65 - 126 |      | Recovery = | 102.96% |        |          |
| 62) 4-Bromofluorobenzene      | 12.341         | 95   | 188753     | 50.86   | ug/l   | -0.01    |
| Spiked Amount 50.000          | Range 58 - 135 |      | Recovery = | 101.72% |        |          |
|                               |                |      |            |         |        |          |
| Target Compounds              |                |      |            |         | Qvalue |          |
| 3) Chloromethane              | 2.032          | 50   | 1454       | 0.32    | ug/l   | 90       |
| 11) Tert butyl alcohol        | 4.682          | 59   | 550        | 0.67    | ug/l # | 86       |
| 16) Acetone                   | 3.743          | 43   | 78913      | 49.46   | ug/l   | 92       |
| 18) Methyl Acetate            | 4.244          | 43   | 3753       | 0.84    | ug/l # | 81       |
| 20) Methylene Chloride        | 4.462          | 84   | 26242      | 6.69    | ug/l   | 89       |
| 25) 2-Butanone                | 6.741          | 43   | 5111       | 2.02    | ug/l # | 83       |
| 29) Tetrahydrofuran           | 7.119          | 42   | 431        | 0.26    | ug/l # | 72       |
| 31) Cyclohexane               | 7.581          | 56   | 6880       | 1.15    | ug/l # | 10       |
| 36) 1,1-Dichloropropene       | 7.578          | 75   | 22774      | 4.90    | ug/l # | 44       |
| 37) Ethyl Acetate             | 6.741          | 43   | 5111       | 1.00    | ug/l # | 65       |
| 38) Carbon Tetrachloride      | 7.583          | 117  | 27556      | 6.09    | ug/l # | 19       |
| 43) Isopropyl Acetate         | 8.085          | 43   | 36628      | 4.12    | ug/l # | 88       |
| 48) Methyl methacrylate       | 9.109          | 41   | 7288       | 1.85    | ug/l # | 11       |
| 49) 1,4-Dioxane               | 9.128          | 88   | 427        | 67.67   | ug/l # | 1        |
| 51) 4-Methyl-2-Pentanone      | 9.917          | 43   | 12245      | 2.49    | ug/l   | 99       |
| 54) cis-1,3-Dichloropropene   | 9.836          | 75   | 57004      | 9.67    | ug/l # | 64       |
| 56) Ethyl methacrylate        | 10.357         | 69   | 297        | 2.84    | ug/l # | 31       |
| 57) 1,3-Dichloropropane       | 10.700         | 76   | 29895      | 5.21    | ug/l # | 42       |
| 58) 2-Chloroethyl Vinyl ether | 9.608          | 63   | 221        | 7.01    | ug/l   | 94       |
| 59) 2-Hexanone                | 10.700         | 43   | 426042     | 124.40  | ug/l # | 46       |
| 70) Styrene                   | 11.920         | 104  | 209        | 2.52    | ug/l # | 83       |
| 76) 1,2,3-Trichloropropane    | 12.341         | 75   | 94074      | 23.57   | ug/l # | 100      |
| 80) 1,3,5-Trimethylbenzene    | 12.679         | 105  | 6541       | 0.57    | ug/l   | 82       |
| 81) trans-1,4-Dichloro-2-b... | 12.341         | 75   | 94074      | 66.84   | ug/l # | 15       |
| 93) 1,2,4-Trichlorobenzene    | 14.876         | 180  | 458        | 3.44    | ug/l # | 65       |
| 95) Naphthalene               | 15.082         | 128  | 433        | 3.92    | ug/l # | 2        |
| -----                         |                |      |            |         |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN052821\  
Data File : VN067185.D  
Acq On : 28 May 2021 16:02  
Operator : JC/MD  
Sample : PB136697ZHE#02  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02

Quant Time: May 29 02:24:09 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N052121W.M  
Quant Title : SW846 8260  
QLast Update : Fri May 21 17:24:08 2021  
Response via : Initial Calibration




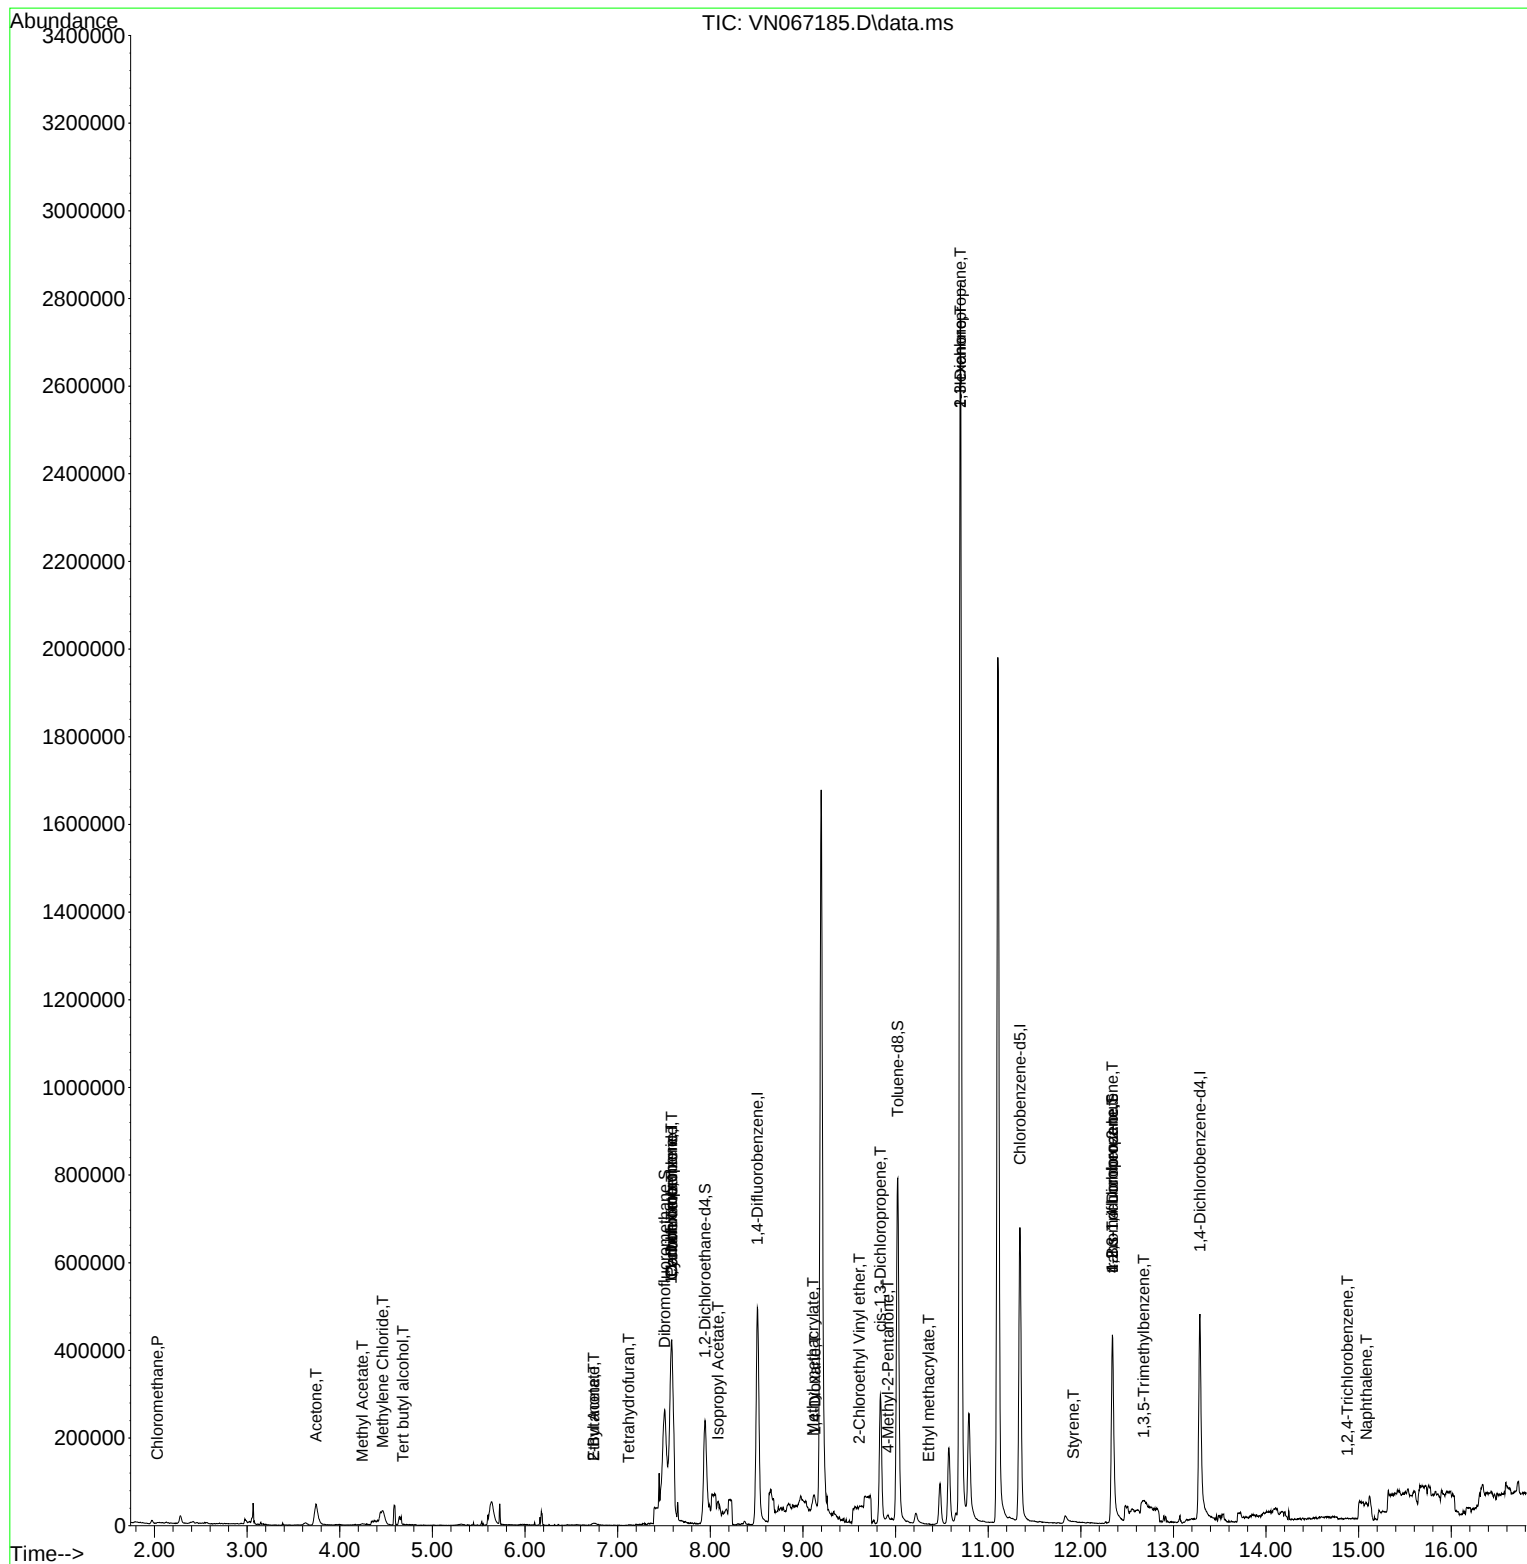


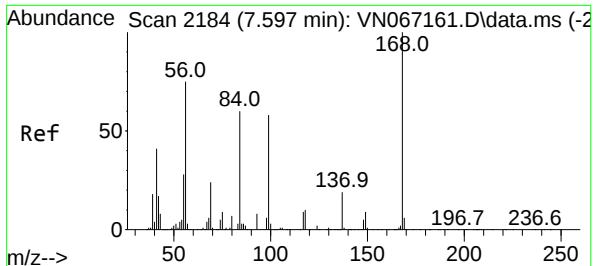

#1  
Pentafluorobenzene  
Concen: 50.00 ug/l  
RT: 7.583 min Scan# 2179  
Delta R.T. -0.014 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion:168 Resp: 250090  
Ion Ratio Lower Upper  
168 100  
99 63.0 38.5 57.7#

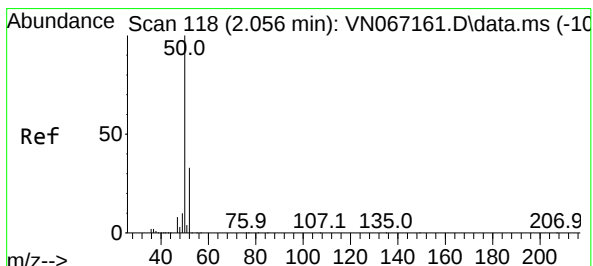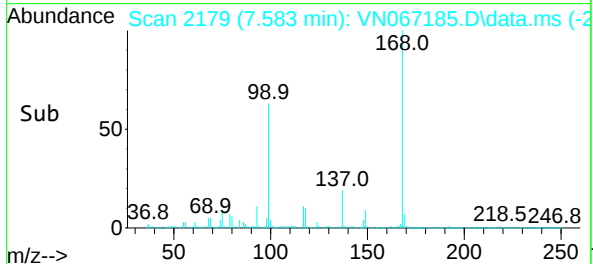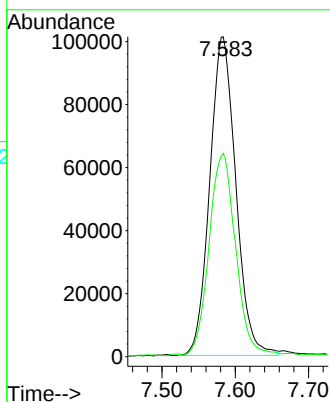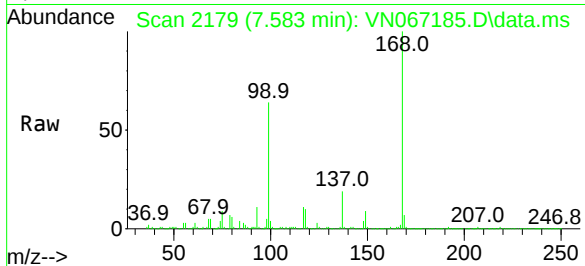

#3  
Chloromethane  
Concen: 0.32 ug/l  
RT: 2.032 min Scan# 109  
Delta R.T. -0.024 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 50 Resp: 1454  
Ion Ratio Lower Upper  
50 100  
52 38.5 26.5 39.7

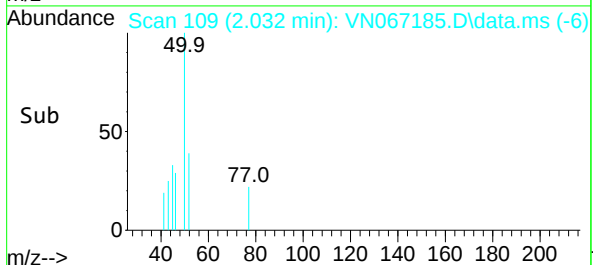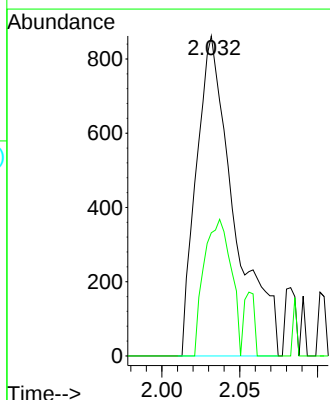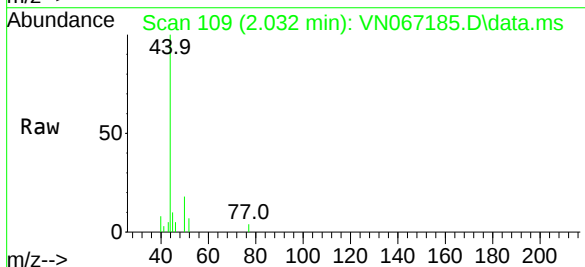







#11

Tert butyl alcohol  
Concen: 0.67 ug/l  
RT: 4.682 min Scan# 1097  
Delta R.T. -0.040 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02




Tgt Ion: 59 Resp: 550  
Ion Ratio Lower Upper  
59 100  
57 8.9 3.5 5.3#

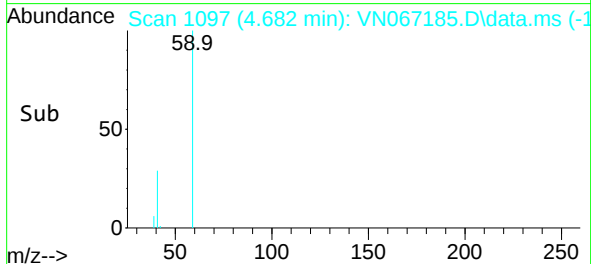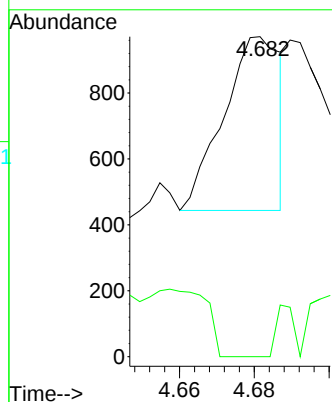


#16

Acetone  
Concen: 49.46 ug/l  
RT: 3.743 min Scan# 747  
Delta R.T. -0.024 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 43 Resp: 78913  
Ion Ratio Lower Upper  
43 100  
58 29.3 27.2 40.8


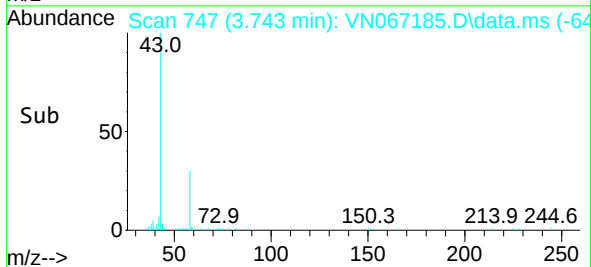
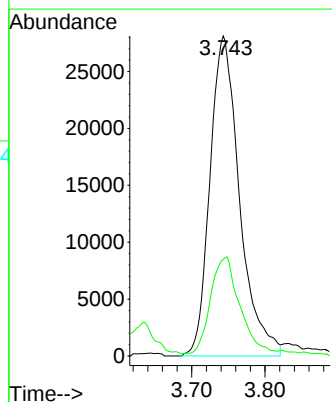
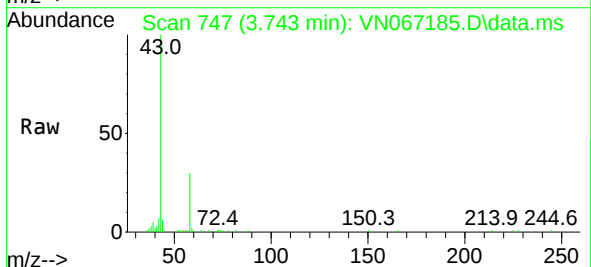


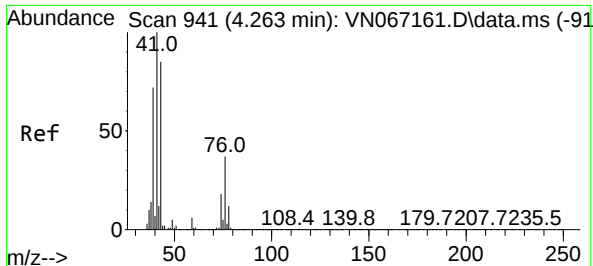

#18  
Methyl Acetate  
Concen: 0.84 ug/l  
RT: 4.244 min Scan# 934  
Delta R.T. -0.019 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 43 Resp: 3753  
Ion Ratio Lower Upper  
43 100  
74 17.1 21.4 32.2#

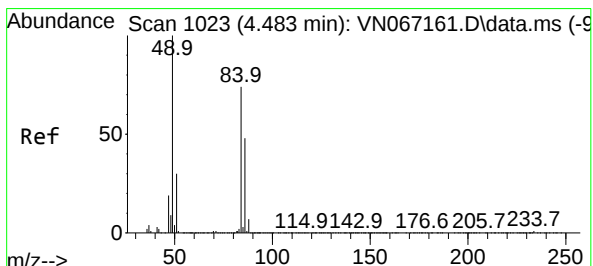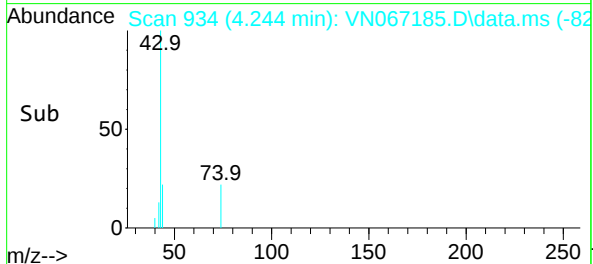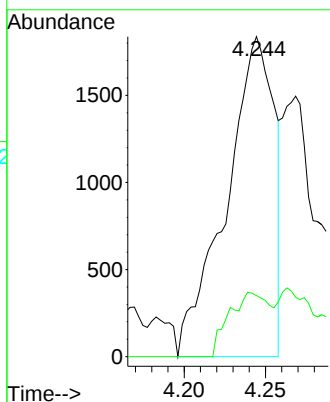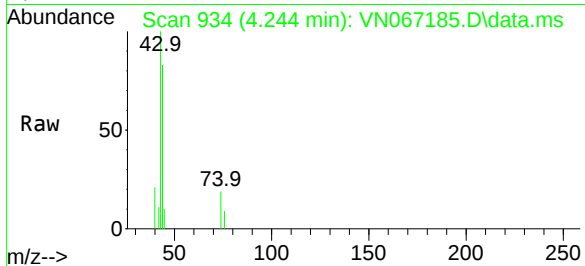

#20  
Methylene Chloride  
Concen: 6.69 ug/l  
RT: 4.462 min Scan# 1015  
Delta R.T. -0.021 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 84 Resp: 26242  
Ion Ratio Lower Upper  
84 100  
49 127.1 88.3 132.5  
51 40.0 26.7 40.1  
86 60.9 51.1 76.7


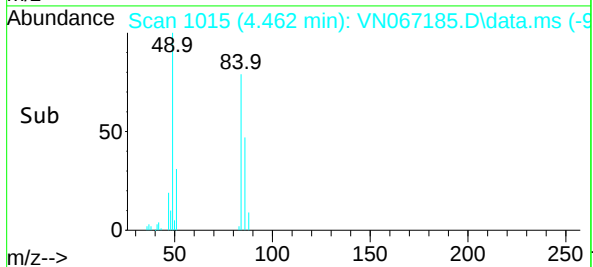
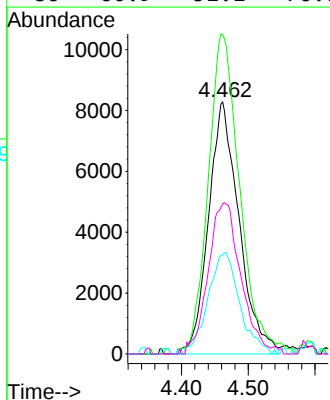
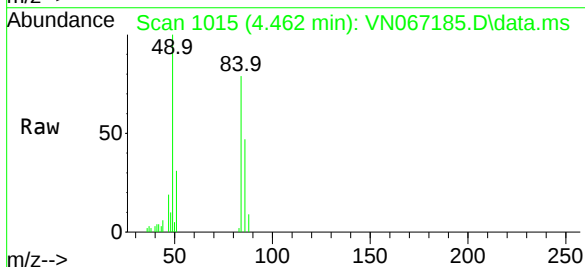


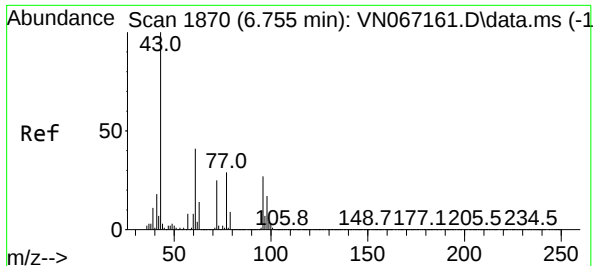

#25  
2-Butanone  
Concen: 2.02 ug/l  
RT: 6.741 min Scan# 1865  
Delta R.T. -0.014 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 43 Resp: 5111  
Ion Ratio Lower Upper  
43 100  
72 21.3 24.4 36.6#

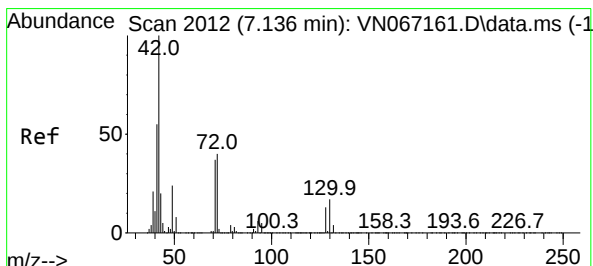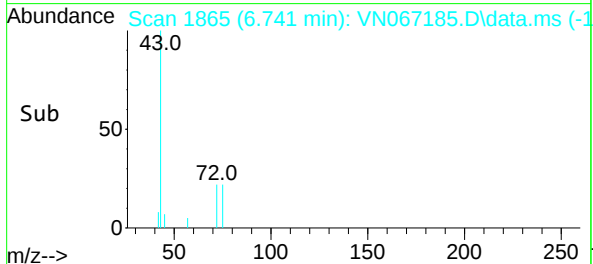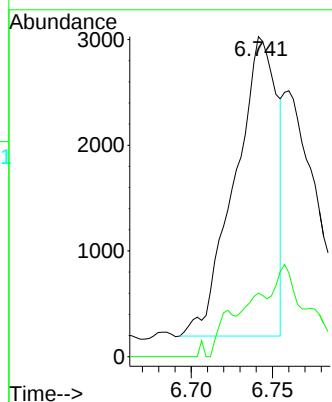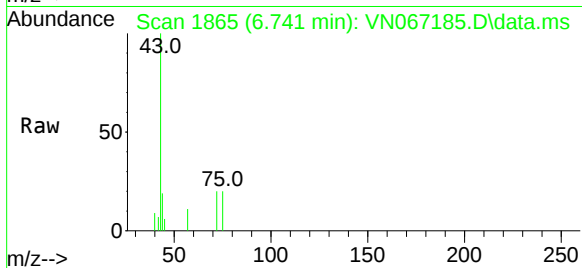

#29  
Tetrahydrofuran  
Concen: 0.26 ug/l  
RT: 7.119 min Scan# 2006  
Delta R.T. -0.017 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 42 Resp: 431  
Ion Ratio Lower Upper  
42 100  
72 18.8 40.1 60.1#  
71 41.1 37.9 56.9


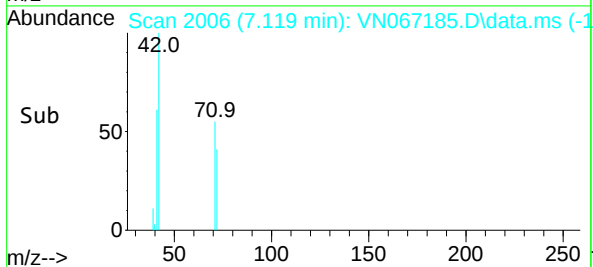

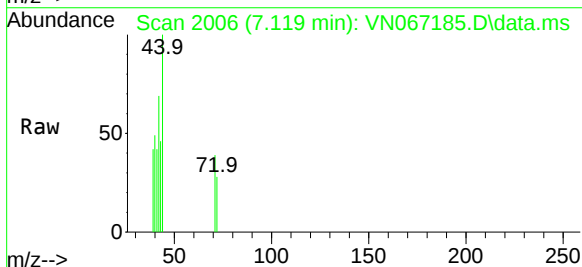




#31  
Cyclohexane  
Concen: 1.15 ug/l  
RT: 7.581 min Scan# 2178  
Delta R.T. -0.000 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 56 Resp: 6880  
Ion Ratio Lower Upper  
56 100  
69 156.9 28.0 42.0#  
84 135.5 74.2 111.2#

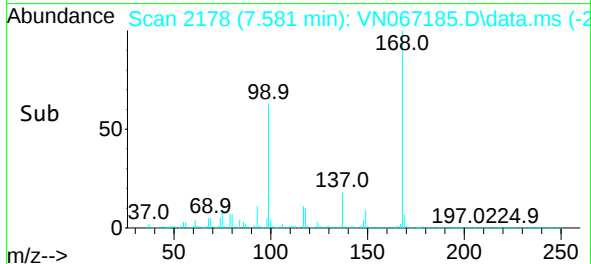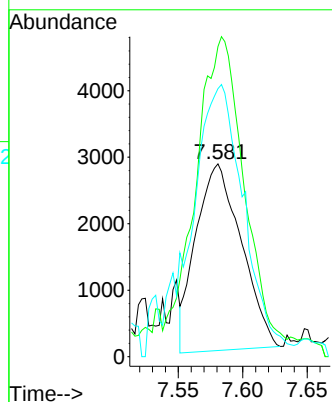

#33  
1,2-Dichloroethane-d4  
Concen: 47.07 ug/l  
RT: 7.943 min Scan# 2313  
Delta R.T. -0.016 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 65 Resp: 182690  
Ion Ratio Lower Upper  
65 100  
67 53.9 0.0 110.4




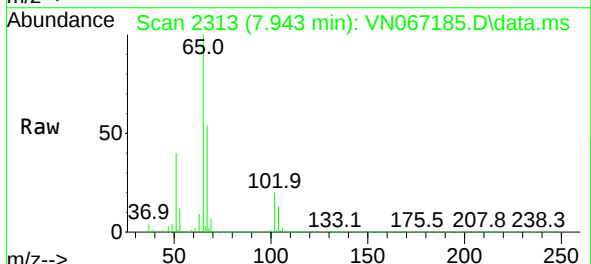




#34  
1,4-Difluorobenzene  
Concen: 50.00 ug/l  
RT: 8.509 min Scan# 2524  
Delta R.T. -0.016 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion:114 Resp: 459640  
Ion Ratio Lower Upper  
114 100  
63 23.0 0.0 35.8  
88 16.7 0.0 30.4

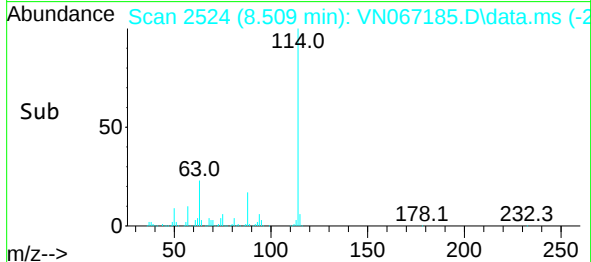

#35  
Dibromofluoromethane  
Concen: 50.70 ug/l  
RT: 7.506 min Scan# 2150  
Delta R.T. -0.013 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion:113 Resp: 143024  
Ion Ratio Lower Upper  
113 100  
111 104.4 82.6 124.0  
192 17.8 18.2 27.4#


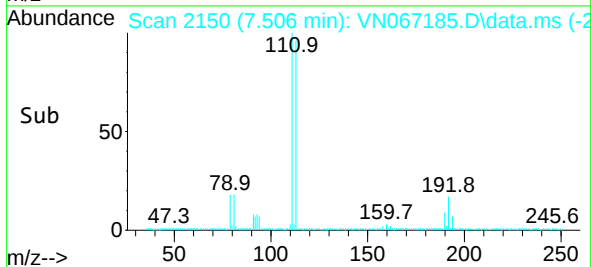

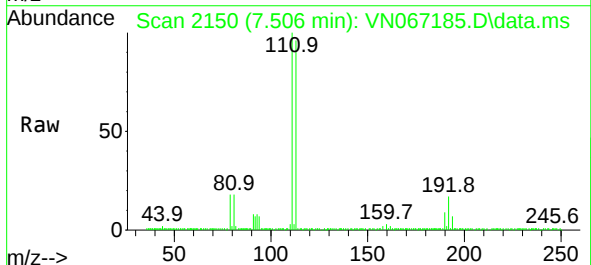


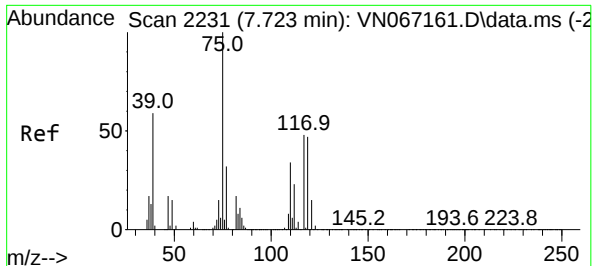

#36  
1,1-Dichloropropene  
Concen: 4.90 ug/l  
RT: 7.578 min Scan# 2177  
Delta R.T. -0.145 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 75 Resp: 22774  
Ion Ratio Lower Upper  
75 100  
110 2.1 19.1 57.3#  
77 3.0 24.8 37.2#

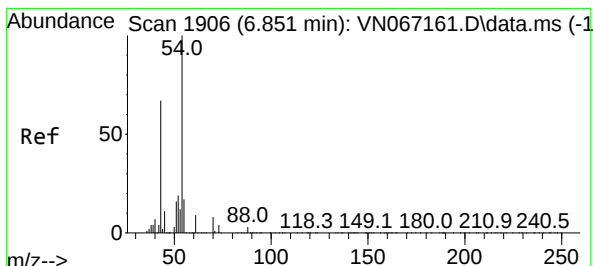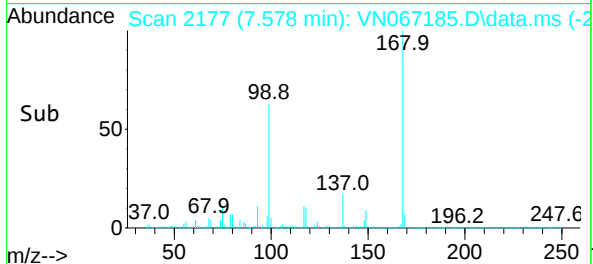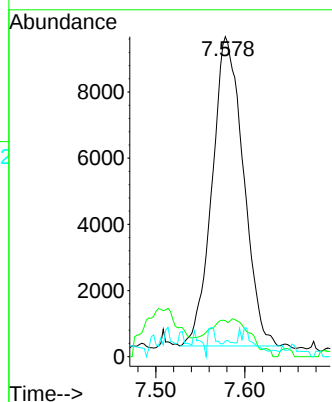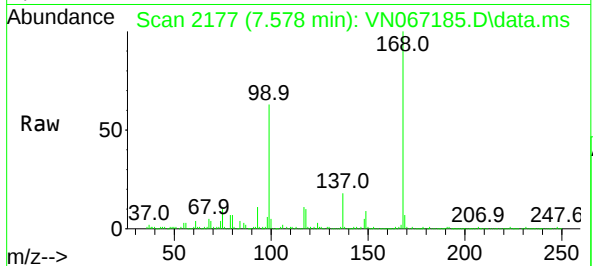

#37  
Ethyl Acetate  
Concen: 1.00 ug/l  
RT: 6.741 min Scan# 1865  
Delta R.T. -0.110 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 43 Resp: 5111  
Ion Ratio Lower Upper  
43 100  
61 0.0 13.0 19.4#  
70 0.0 9.2 13.8#


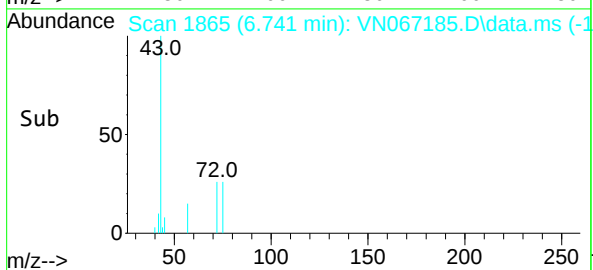

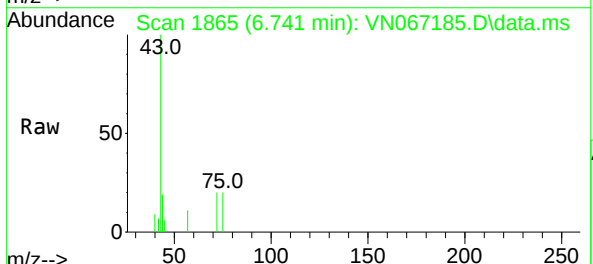




#38  
Carbon Tetrachloride  
Concen: 6.09 ug/l  
RT: 7.583 min Scan# 2179  
Delta R.T. -0.119 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion:117 Resp: 27556  
Ion Ratio Lower Upper  
117 100  
119 6.7 78.2 117.2#  
121 5.3 24.7 37.1#

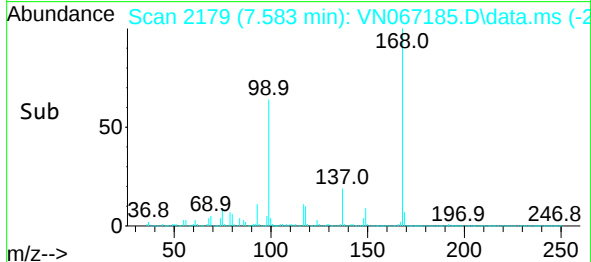

#43  
Isopropyl Acetate  
Concen: 4.12 ug/l  
RT: 8.085 min Scan# 2366  
Delta R.T. -0.016 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 43 Resp: 36628  
Ion Ratio Lower Upper  
43 100  
61 22.3 23.4 35.0#  
87 10.9 12.2 18.2#


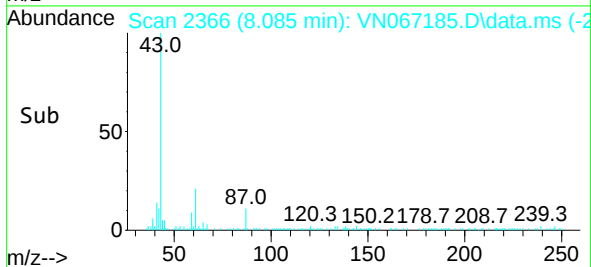

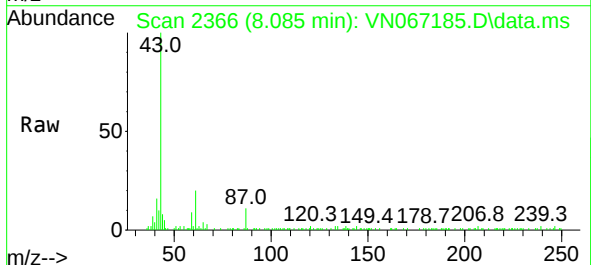




#48  
Methyl methacrylate  
Concen: 1.85 ug/l  
RT: 9.109 min Scan# 2748  
Delta R.T. -0.036 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 41 Resp: 7288  
Ion Ratio Lower Upper  
41 100  
69 3.5 80.5 120.7#  
39 0.0 41.4 62.0#

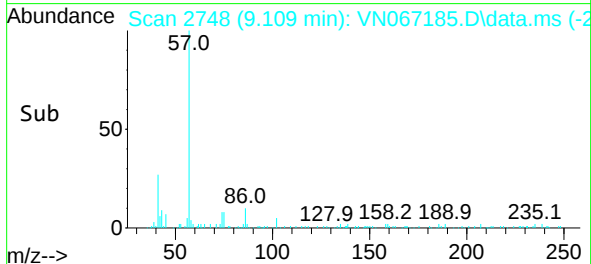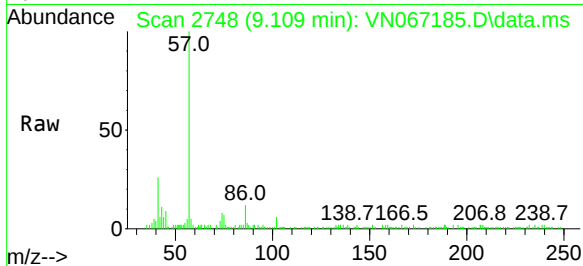

#49  
1,4-Dioxane  
Concen: 67.67 ug/l  
RT: 9.128 min Scan# 2755  
Delta R.T. -0.017 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 88 Resp: 427  
Ion Ratio Lower Upper  
88 100  
43 0.0 21.8 32.8#  
58 225.5 50.8 76.2#



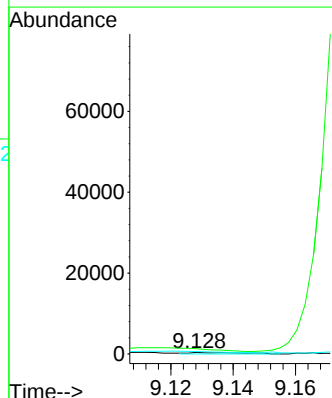
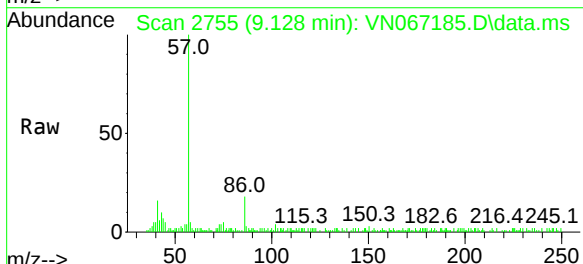




#50  
Toluene-d8  
Concen: 51.48 ug/l  
RT: 10.021 min Scan# 3088  
Delta R.T. -0.014 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 98 Resp: 558891  
Ion Ratio Lower Upper  
98 100  
100 64.9 51.8 77.8

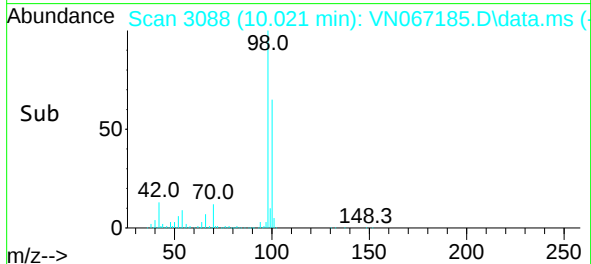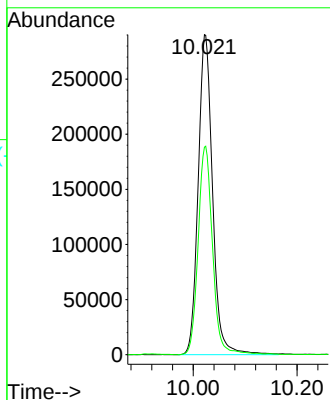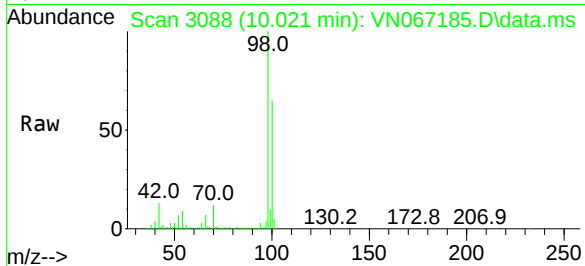

#51  
4-Methyl-2-Pentanone  
Concen: 2.49 ug/l  
RT: 9.917 min Scan# 3049  
Delta R.T. -0.011 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 43 Resp: 12245  
Ion Ratio Lower Upper  
43 100  
58 42.5 34.5 51.7


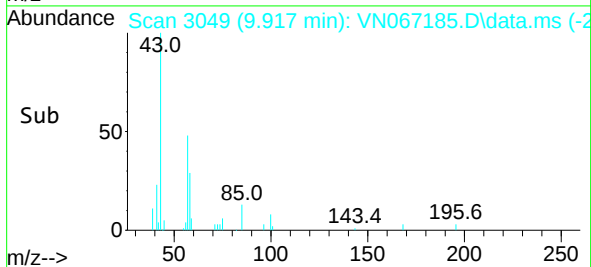
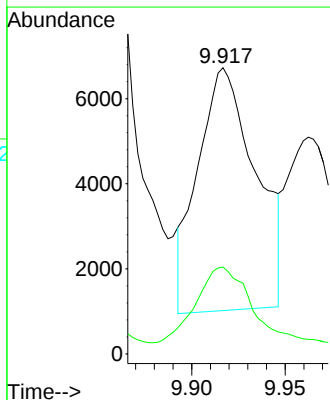
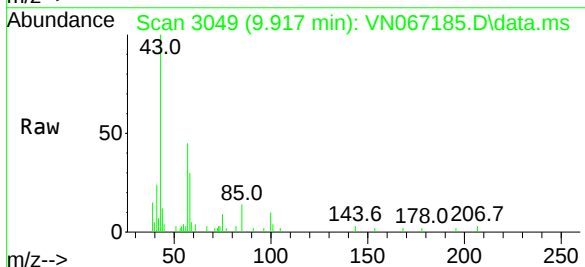




#54  
 cis-1,3-Dichloropropene  
 Concen: 9.67 ug/l  
 RT: 9.836 min Scan# 3019  
 Delta R.T. 0.053 min  
 Lab File: VN067185.D  
 Acq: 28 May 2021 16:02




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB136697ZHE#02


Tgt Ion: 75 Resp: 57004  
 Ion Ratio Lower Upper  
 75 100  
 77 0.9 25.1 37.7#  
 39 26.1 30.9 46.3#

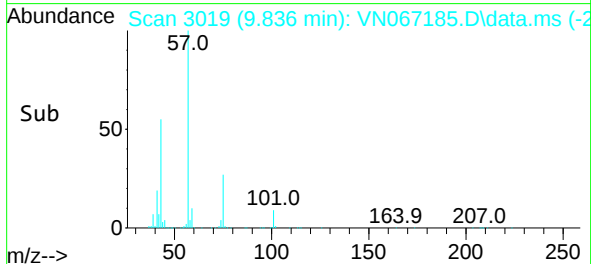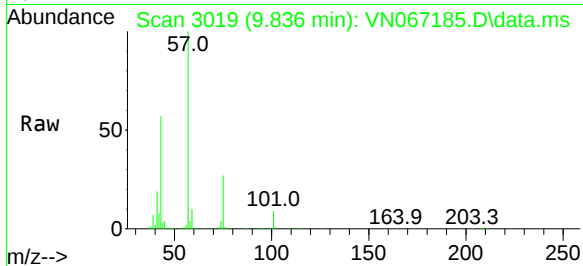

#56  
 Ethyl methacrylate  
 Concen: 2.84 ug/l  
 RT: 10.357 min Scan# 3213  
 Delta R.T. -0.021 min  
 Lab File: VN067185.D  
 Acq: 28 May 2021 16:02

Tgt Ion: 69 Resp: 297  
 Ion Ratio Lower Upper  
 69 100  
 41 0.0 45.5 68.3#  
 39 0.0 22.9 34.3#


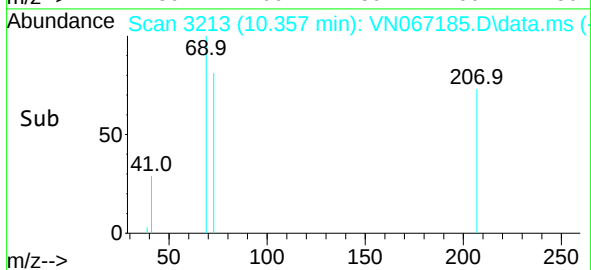

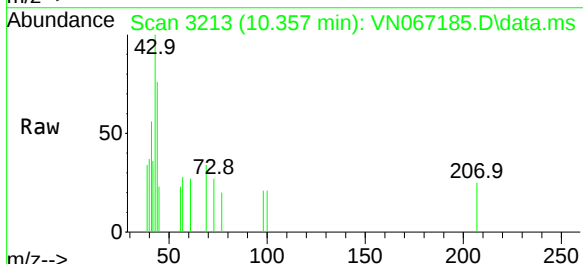




#57  
1,3-Dichloropropane  
Concen: 5.21 ug/l  
RT: 10.700 min Scan# 3341  
Delta R.T. 0.045 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 76 Resp: 29895  
Ion Ratio Lower Upper  
76 100  
78 0.3 26.3 39.5#

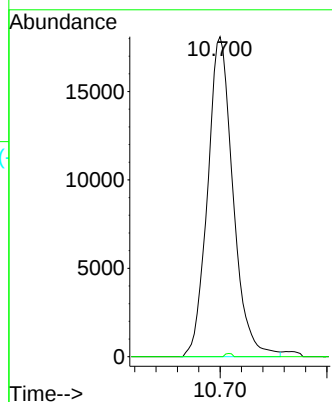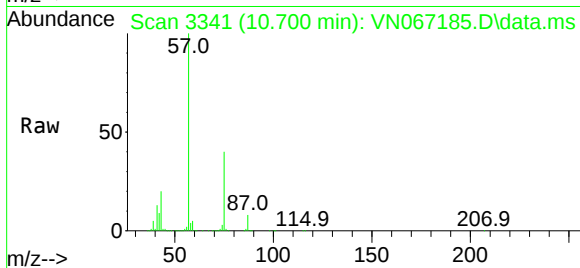

#58  
2-Chloroethyl Vinyl ether  
Concen: 7.01 ug/l  
RT: 9.608 min Scan# 2934  
Delta R.T. -0.033 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 63 Resp: 221  
Ion Ratio Lower Upper  
63 100  
106 33.0 23.9 35.9


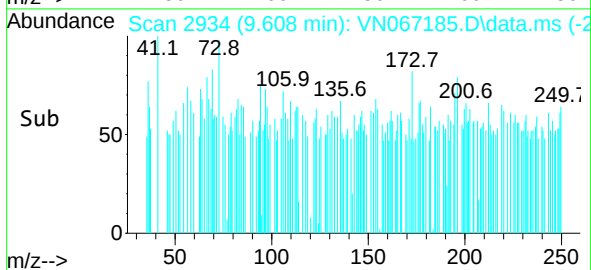
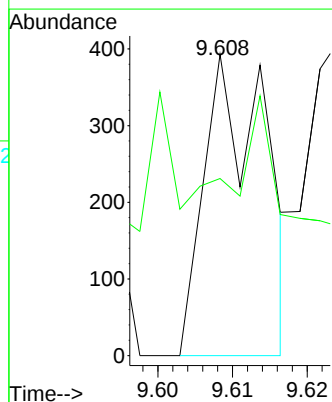
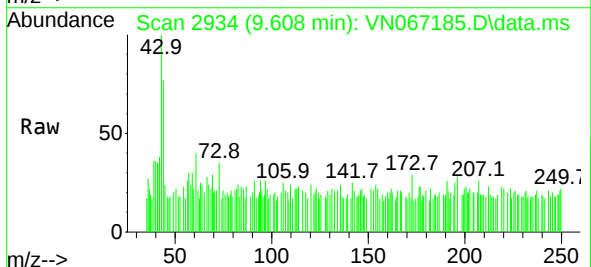




#59  
2-Hexanone  
Concen: 124.40 ug/l  
RT: 10.700 min Scan# 3341  
Delta R.T. -0.000 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion: 43 Resp: 426042  
Ion Ratio Lower Upper  
43 100  
58 19.1 29.8 89.5#

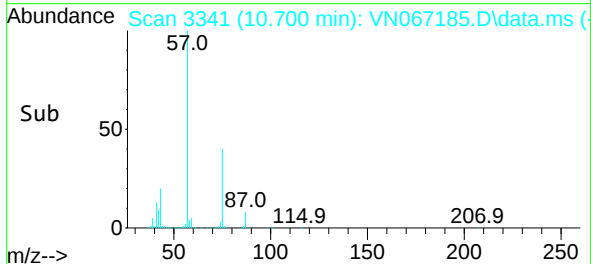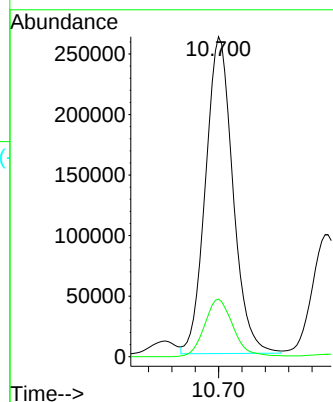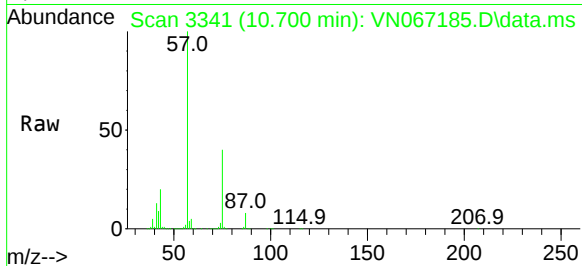

#62  
4-Bromofluorobenzene  
Concen: 50.86 ug/l  
RT: 12.341 min Scan# 3953  
Delta R.T. -0.014 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 95 Resp: 188753  
Ion Ratio Lower Upper  
95 100  
174 65.8 0.0 182.8  
176 63.8 0.0 176.6


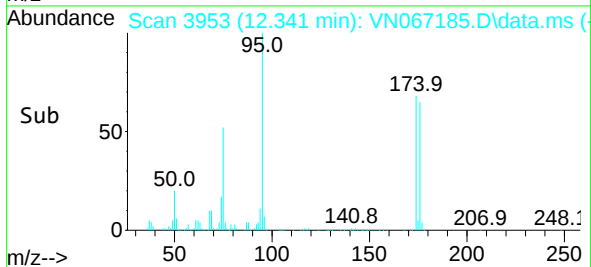
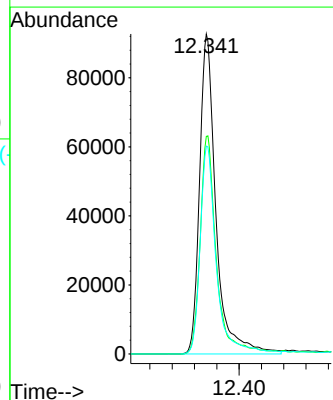
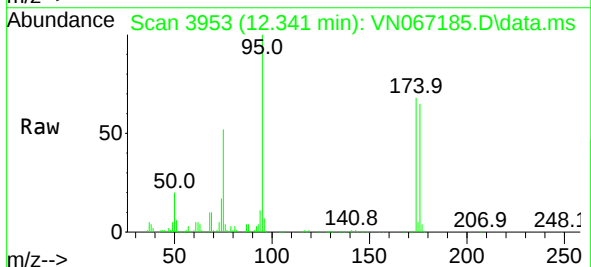




#63  
Chlorobenzene-d5  
Concen: 50.00 ug/l  
RT: 11.344 min Scan# 3581  
Delta R.T. -0.013 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


|          |       |       |        |
|----------|-------|-------|--------|
| Tgt Ion: | 117   | Resp: | 399464 |
| Ion      | Ratio | Lower | Upper  |
| 117      | 100   |       |        |
| 82       | 59.7  | 42.2  | 63.2   |
| 119      | 32.0  | 25.8  | 38.6   |

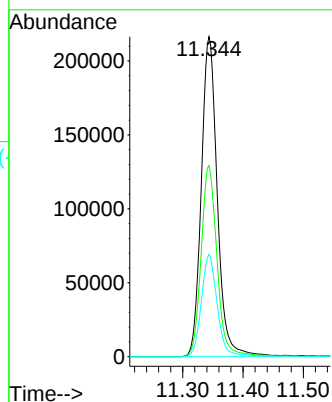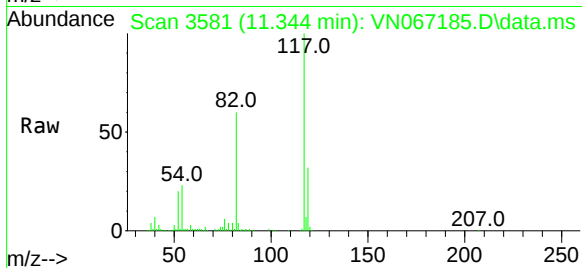

#70  
Styrene  
Concen: 2.52 ug/l  
RT: 11.920 min Scan# 3796  
Delta R.T. 0.002 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

|          |       |       |       |
|----------|-------|-------|-------|
| Tgt Ion: | 104   | Resp: | 209   |
| Ion      | Ratio | Lower | Upper |
| 104      | 100   |       |       |
| 78       | 39.7  | 37.7  | 56.5  |
| 103      | 71.3  | 44.2  | 66.4  |


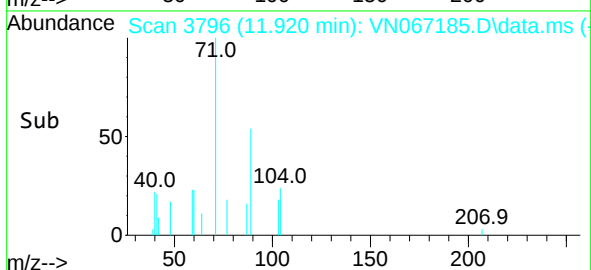

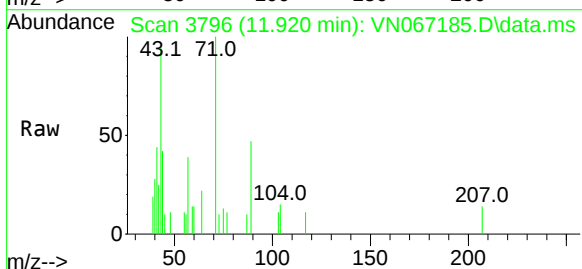


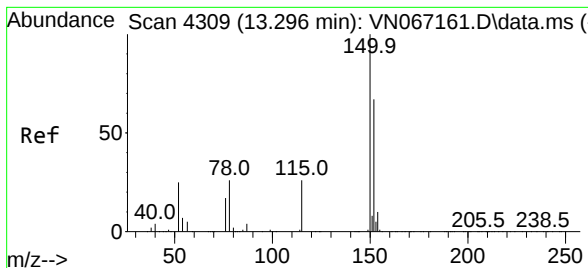

#72  
 1,4-Dichlorobenzene-d4  
 Concen: 50.00 ug/l  
 RT: 13.285 min Scan# 4305  
 Delta R.T. -0.011 min  
 Lab File: VN067185.D  
 Acq: 28 May 2021 16:02




Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 PB136697ZHE#02


Tgt Ion:152 Resp: 143352  
 Ion Ratio Lower Upper  
 152 100  
 115 64.4 27.0 80.8  
 150 166.1 0.0 350.2

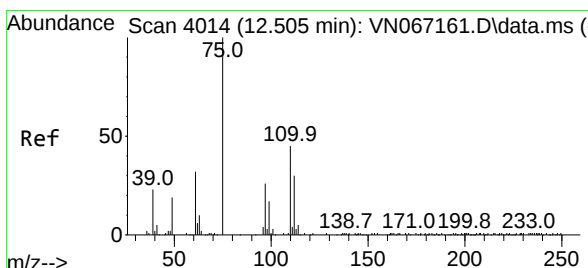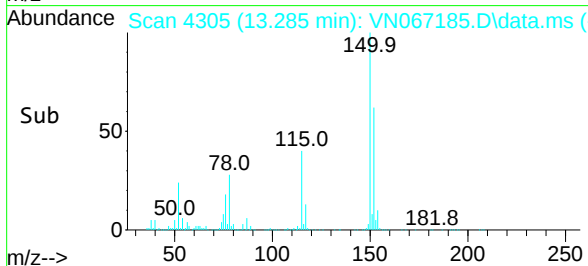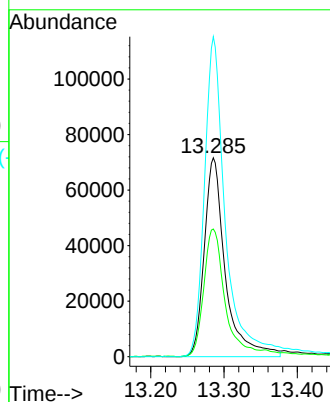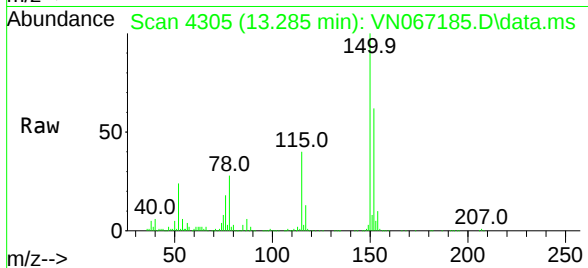

#76  
 1,2,3-Trichloropropane  
 Concen: 23.57 ug/l  
 RT: 12.341 min Scan# 3953  
 Delta R.T. -0.164 min  
 Lab File: VN067185.D  
 Acq: 28 May 2021 16:02

Tgt Ion: 75 Resp: 94074  
 Ion Ratio Lower Upper  
 75 100  
 77 0.2 0.0 0.0#


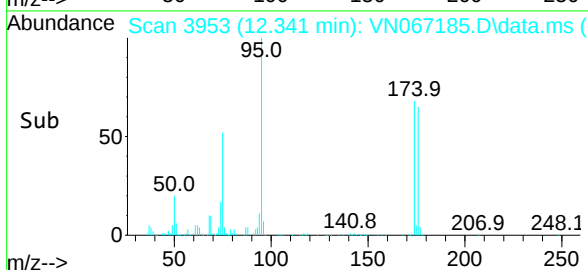
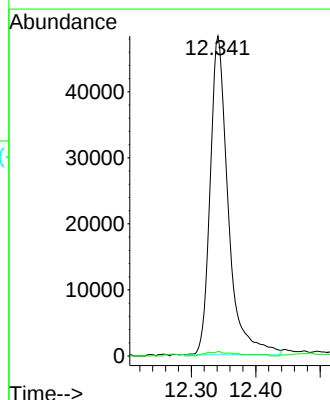
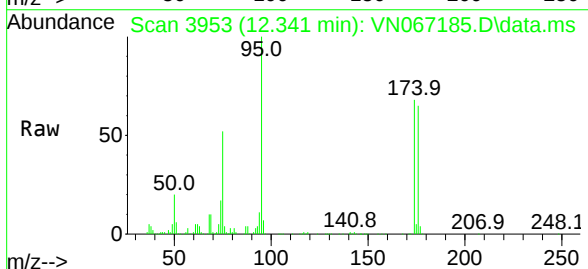


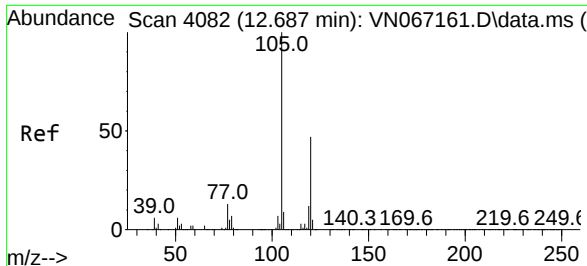

#80  
1,3,5-Trimethylbenzene  
Concen: 0.57 ug/l  
RT: 12.679 min Scan# 4079  
Delta R.T. -0.008 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02




Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02


Tgt Ion:105 Resp: 6541  
Ion Ratio Lower Upper  
105 100  
120 37.9 25.0 75.0

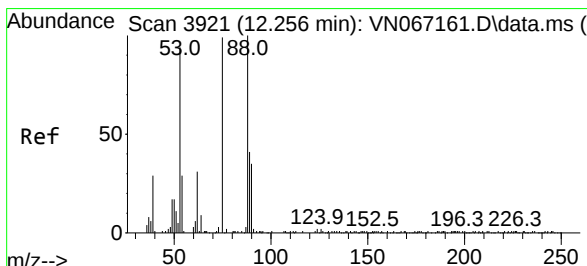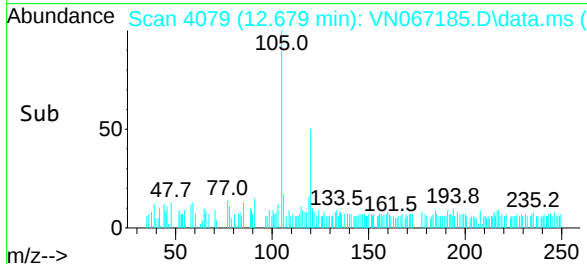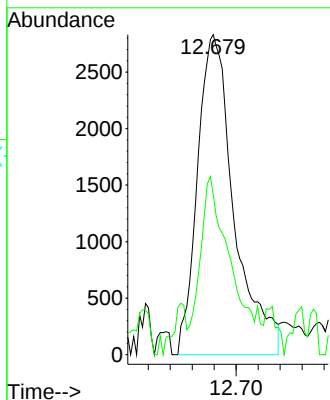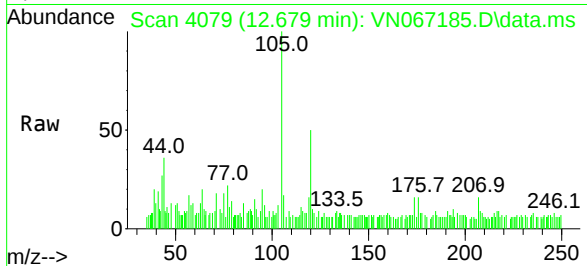

#81  
trans-1,4-Dichloro-2-butene  
Concen: 66.84 ug/l  
RT: 12.341 min Scan# 3953  
Delta R.T. 0.085 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion: 75 Resp: 94074  
Ion Ratio Lower Upper  
75 100  
53 0.1 66.3 99.5#  
89 0.2 39.5 59.3#


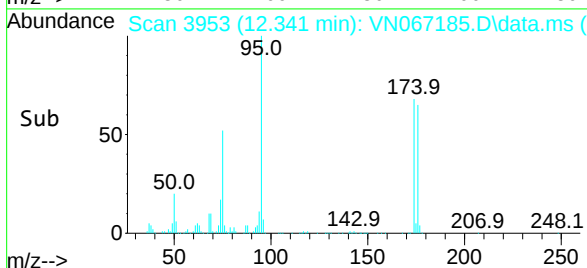
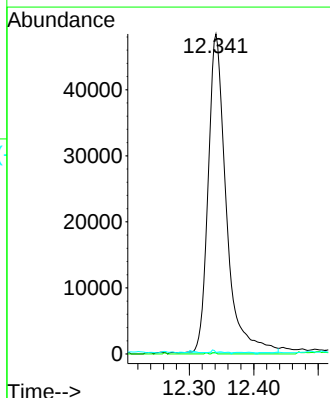
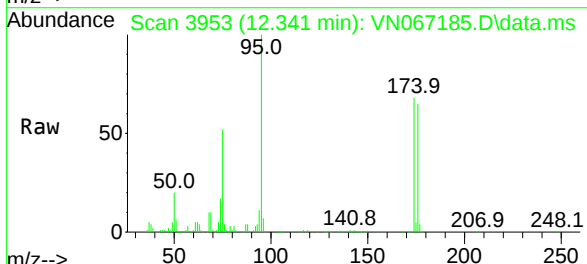




#93  
1,2,4-Trichlorobenzene  
Concen: 3.44 ug/l  
RT: 14.876 min Scan# 4898  
Delta R.T. 0.011 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Instrument :  
MSVOA\_N  
ClientSampleId :  
PB136697ZHE#02

Tgt Ion:180 Resp: 458  
Ion Ratio Lower Upper  
180 100  
182 63.1 47.3 141.8  
145 5.5 14.0 42.0#

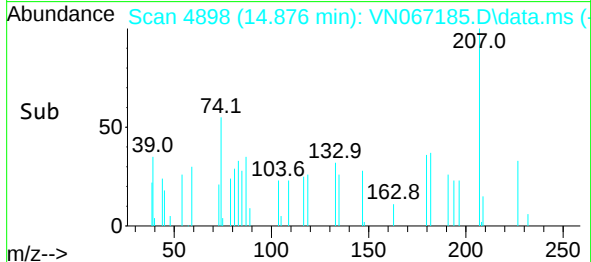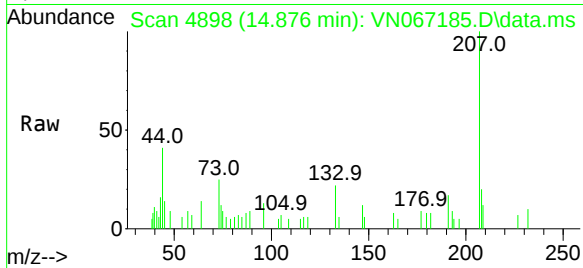

#95  
Naphthalene  
Concen: 3.92 ug/l  
RT: 15.082 min Scan# 4975  
Delta R.T. -0.003 min  
Lab File: VN067185.D  
Acq: 28 May 2021 16:02

Tgt Ion:128 Resp: 433  
Ion Ratio Lower Upper  
128 100  
127 75.1 10.2 15.2#  
129 0.0 8.6 13.0#

