
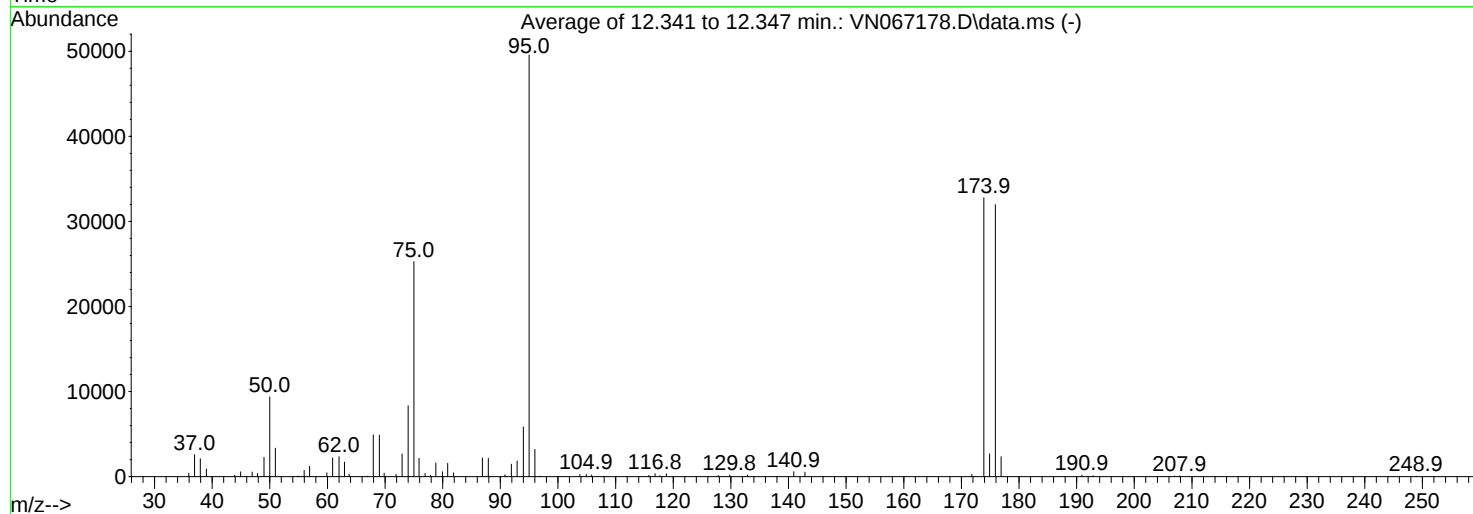


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052821\
Data File : VN067178.D
Acq On : 28 May 2021 12:34
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N052121W.M
Title : SW846 8260
Last Update : Fri May 21 17:24:08 2021

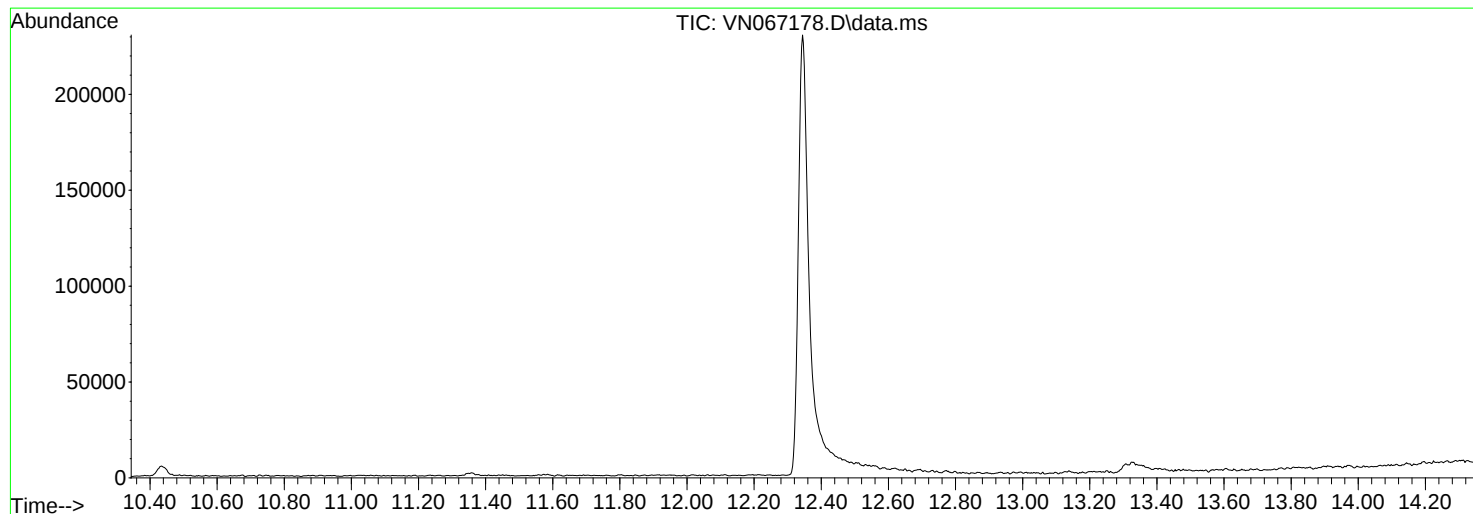

AutoFind: Scans 3953, 3954, 3955; Background Corrected with Scan 3937

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	9374	PASS
75	95	30	60	51.0	25280	PASS
95	95	100	100	100.0	49584	PASS
96	95	5	9	6.5	3220	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	66.1	32787	PASS
175	174	5	9	8.1	2671	PASS
176	174	95	101	97.5	31973	PASS
177	176	5	9	7.4	2360	PASS