
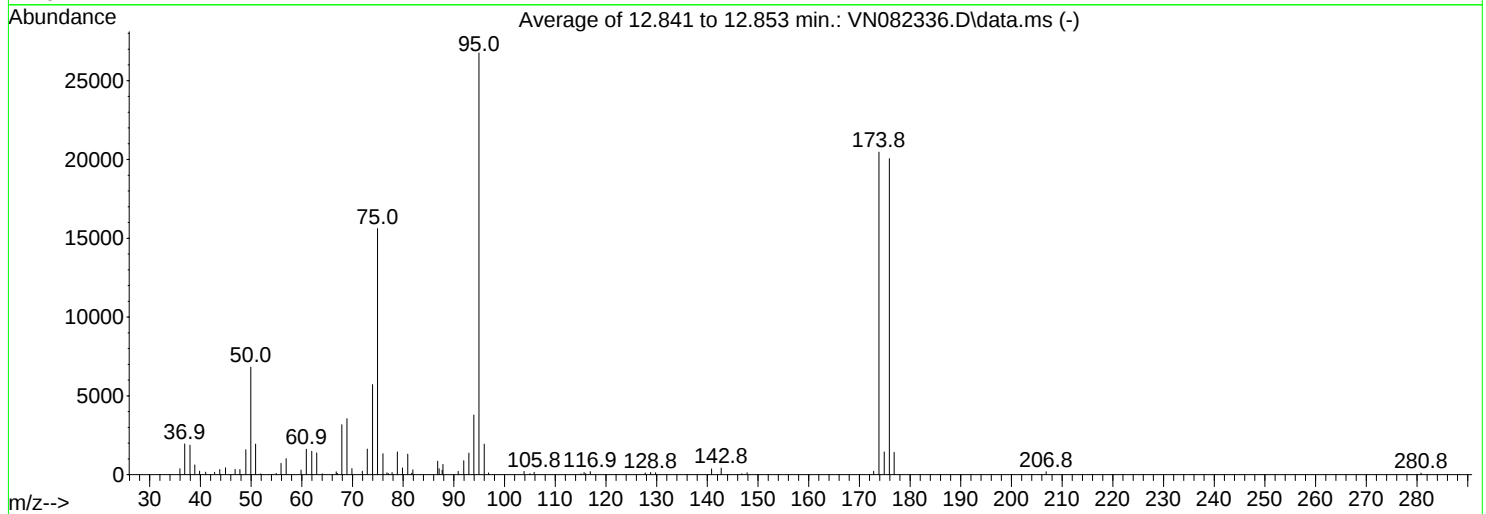


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052824\
Data File : VN082336.D
Acq On : 28 May 2024 08:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

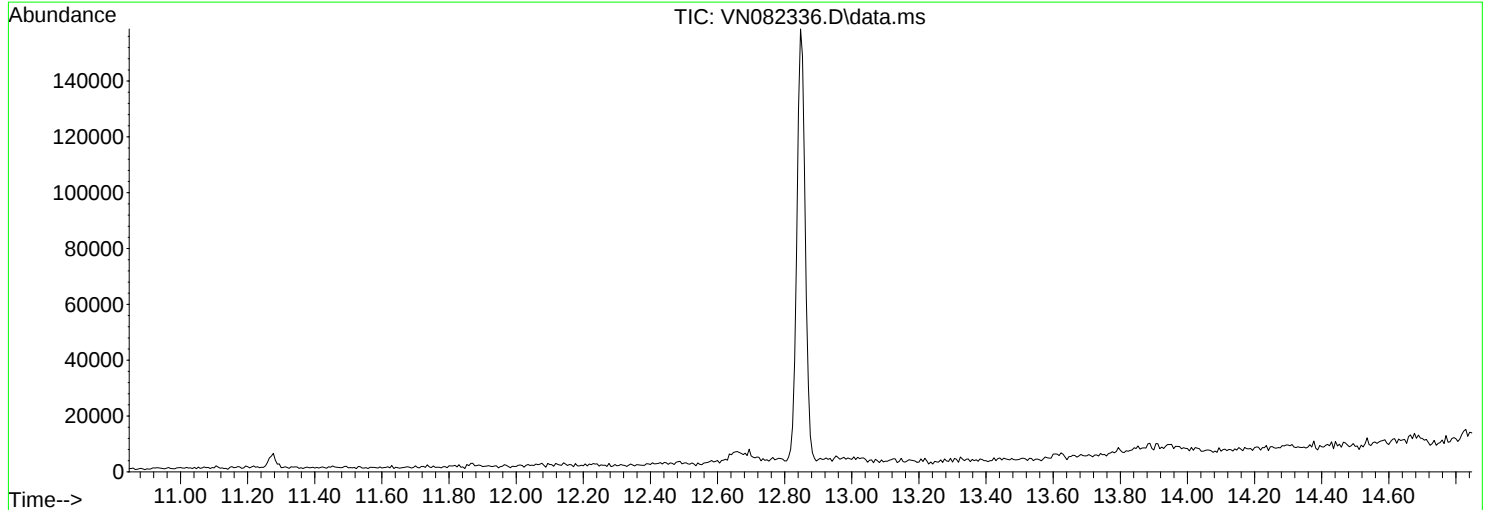

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.5	6826	PASS
75	95	30	60	58.4	15620	PASS
95	95	100	100	100.0	26765	PASS
96	95	5	9	7.3	1943	PASS
173	174	0.00	2	1.0	209	PASS
174	95	50	100	76.5	20464	PASS
175	174	5	9	7.0	1442	PASS
176	174	95	101	98.0	20050	PASS
177	176	5	9	7.1	1418	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	376	48.95	1588	64.10	50	76.80	12
36.90	1947	49.95	6826	66.80	179	77.10	5
37.95	1872	50.90	1942	67.00	77	77.80	13
38.90	624	51.90	52	67.90	3164	78.85	144
39.85	221	54.95	78	68.90	3557	79.85	424
41.05	166	55.90	719	69.90	383	80.90	1302
42.80	151	56.90	1011	71.95	222	81.70	94
43.80	322	59.85	295	72.90	1624	81.90	307
44.95	440	60.90	1619	73.95	5719	86.80	854
46.85	335	61.95	1485	74.95	15620	87.10	380
47.80	329	62.95	1379	76.00	1335	87.70	285

Average of 12.841 to 12.853 min.: VN082336.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.85	654	115.10	53	172.80	209		
90.85	211	115.70	130	173.85	20464		
91.95	884	116.00	64	174.90	1442		
92.95	1373	116.90	198	175.90	20050		
93.95	3789	127.75	117	176.85	1418		
94.95	26765	128.80	142	206.85	179		
96.00	1943	129.80	121	280.80	100		
96.85	112	140.85	369				
103.85	202	142.75	414				
105.00	60	146.80	59				
105.85	153	147.85	124				