


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052825\
Data File : VN086789.D
Acq On : 28 May 2025 08:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051625W.M
Title : SW846 8260
Last Update : Sat May 17 00:46:13 2025

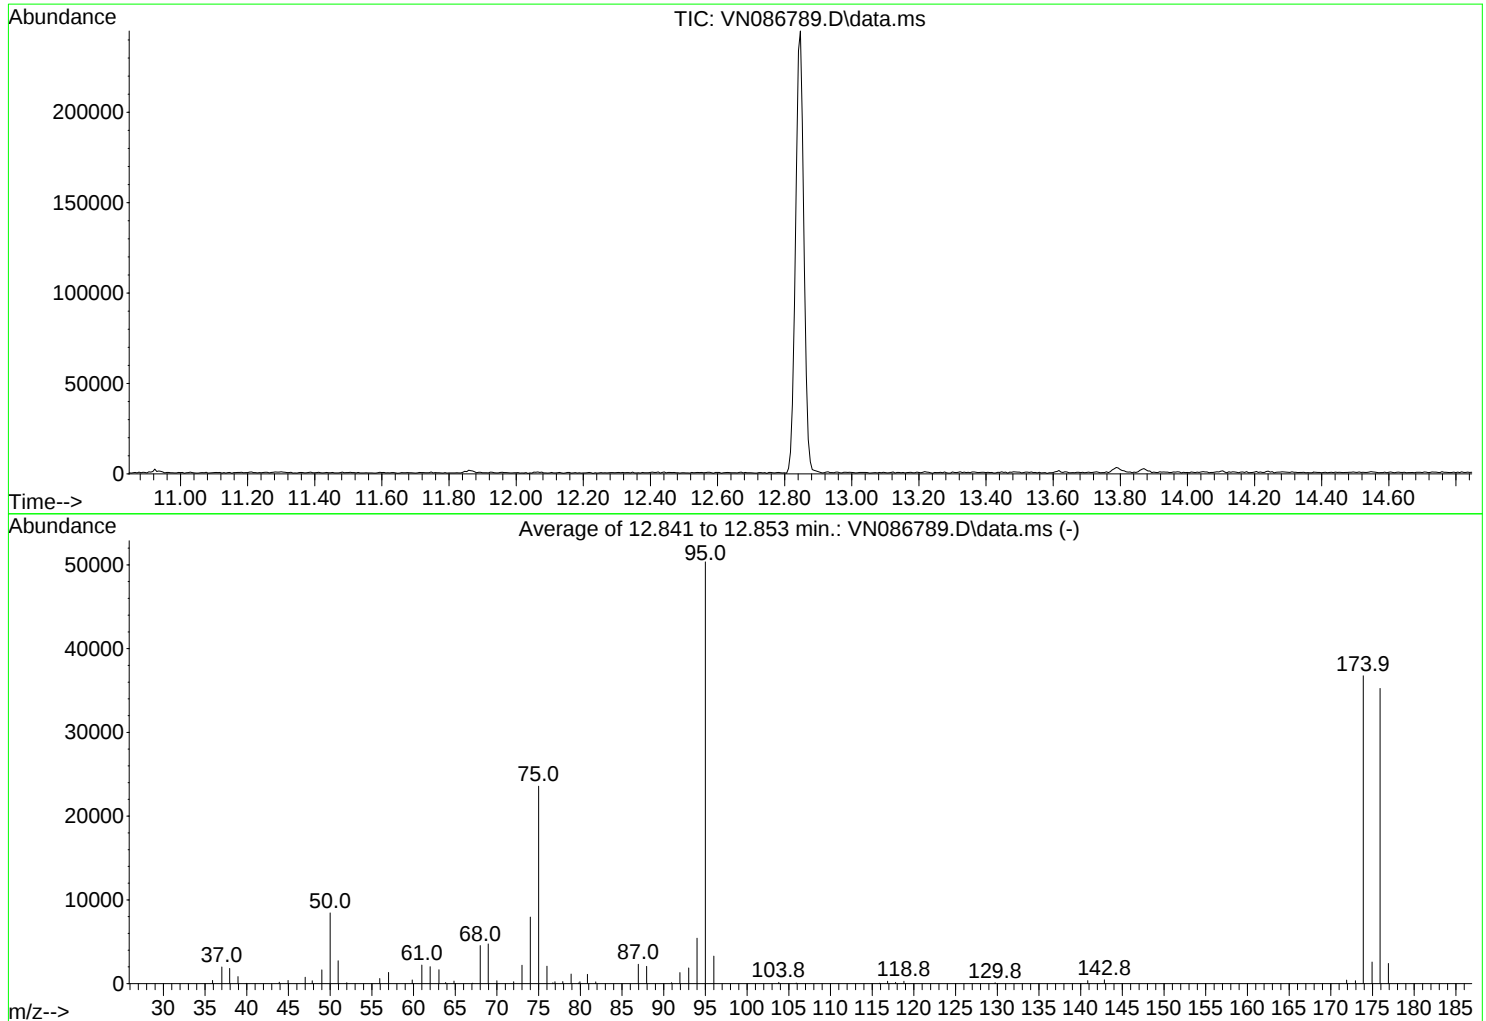

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	8445	PASS
75	95	30	60	46.8	23579	PASS
95	95	100	100	100.0	50363	PASS
96	95	5	9	6.5	3293	PASS
173	174	0.00	2	0.9	342	PASS
174	95	50	100	73.0	36752	PASS
175	174	5	9	7.0	2573	PASS
176	174	95	101	95.9	35243	PASS
177	176	5	9	6.8	2402	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	383	50.95	2740	68.00	4557	78.90	1151
37.00	1980	52.00	119	68.95	4732	79.80	81
37.95	1820	55.95	620	70.00	344	79.95	23
38.95	835	57.00	1344	72.00	232	80.85	110
39.95	48	59.85	434	73.00	2197	81.85	211
43.90	177	61.00	2217	74.00	7950	86.95	2311
44.95	376	62.00	2019	75.00	23579	87.95	2072
47.00	762	63.05	1654	76.00	2087	90.95	109
47.85	337	63.85	133	76.70	90	91.95	1312
49.00	1645	64.85	308	76.95	229	93.00	1869
50.00	8445	67.10	61	77.90	251	94.00	5429

Average of 12.841 to 12.853 min.: VN086789.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
95.00	50363	171.90	416				
96.00	3293	172.95	342				
103.80	155	173.90	36752				
105.90	68	174.95	2573				
115.90	62	175.90	35243				
116.85	283	176.90	2402				
117.80	147						
118.80	292						
129.75	123						
140.85	358						
142.85	453						

Instrument :

MSVOA_N

ClientSampleId :

BFB