

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052919\
 Data File : VN055883.D
 Acq On : 29 May 2019 17:28
 Operator : JC/SP
 Sample : K3082-03 10X
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 14B-3

Quant Time: May 30 07:27:22 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N052219W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu May 23 05:54:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.19	128	52383	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.59	114	276037	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	222274	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.03	65	106364	31.06	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	103.53%
60) 4-Bromofluorobenzene	12.40	95	79165	22.90	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	76.33%
63) Toluene-d8	10.09	98	322228	31.72	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	105.73%


Target Compounds					Ovalue
25) Chloroform	7.37	83	84409	15.653 ug/l	100
41) Bromodichloromethane	9.40	83	6727	1.585 ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN052919\
Data File : VN055883.D
Acq On : 29 May 2019 17:28
Operator : JC/SP
Sample : K3082-03 10X
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
14B-3

Quant Time: May 30 07:27:22 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA N\METHODS\624N052219W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu May 23 05:54:54 2019
Response via : Initial Calibration

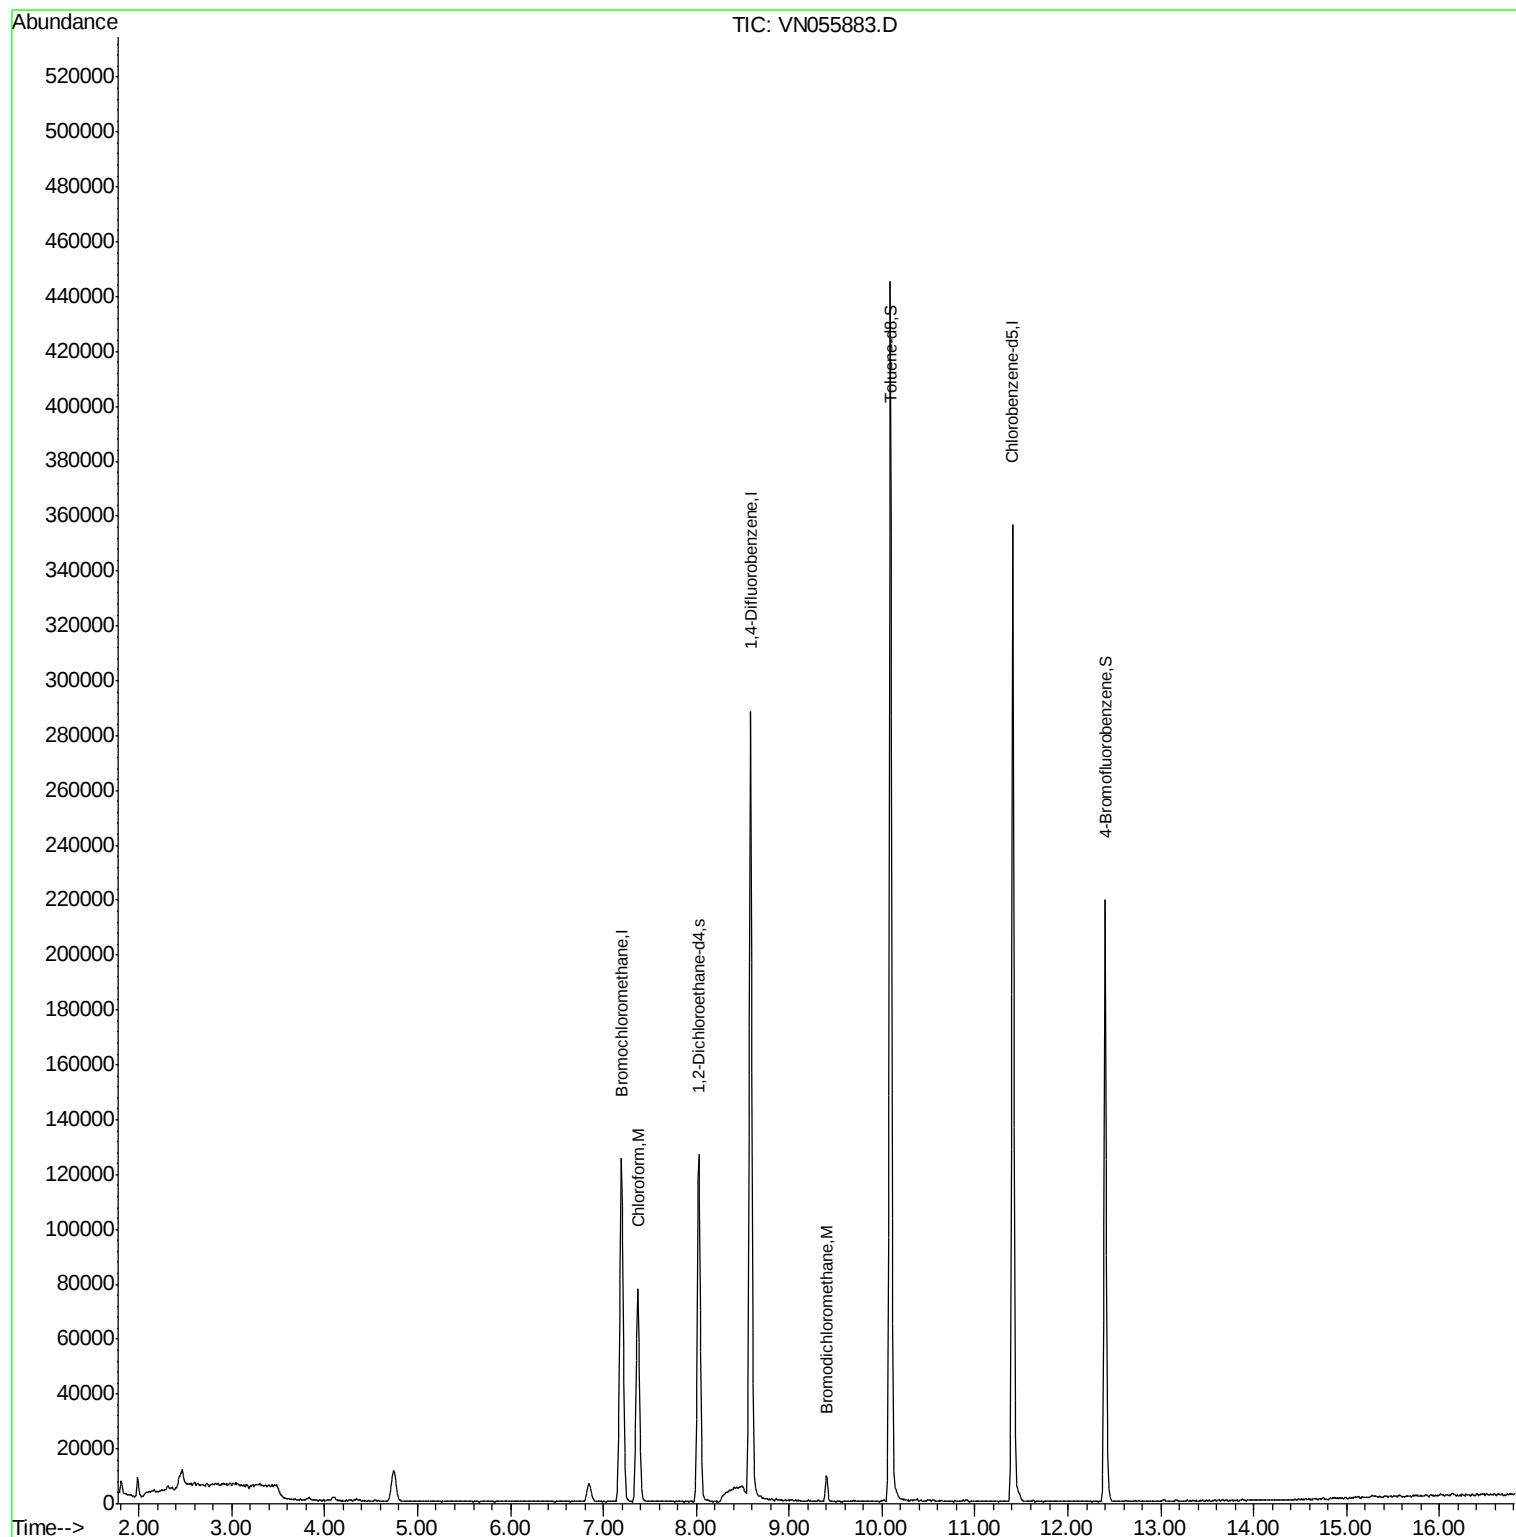


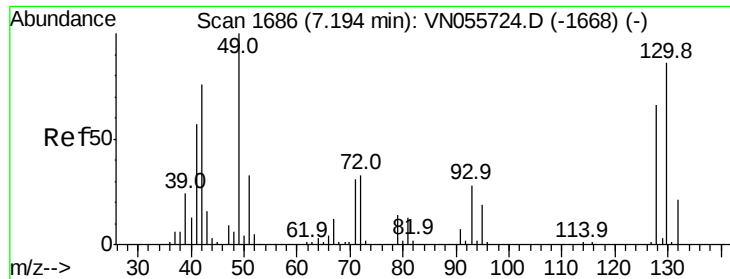




#1
 Bromochloromethane
 Concen: 30.000 ug/l
 RT: 7.19 min Scan# 1686
 Delta R.T. -0.00 min
 Lab File: VN055883.D
 Acq: 29 May 2019 17:28

Instrument :
 MSVOA_N
 ClientSampleId :
 14B-3

Tot Ion:128 Resp: 52383
 Ion Ratio Lower Upper
 128 100
 49 145.3 0.0 383.2
 130 130.5 0.0 326.3

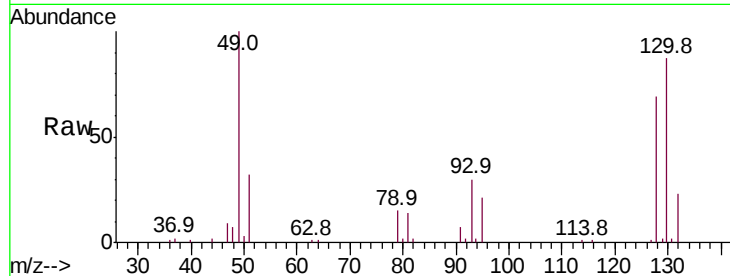


Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 49.00 (48.70 to 49.70): VN
 Ion 130.00 (129.70 to 130.70): V

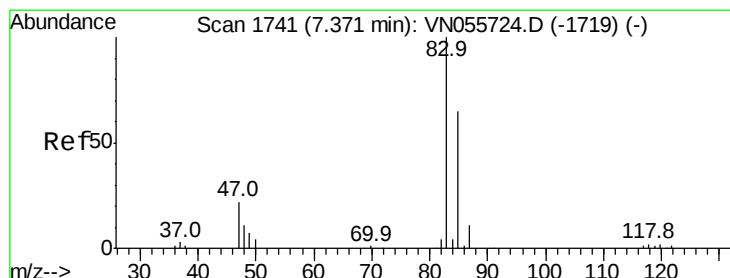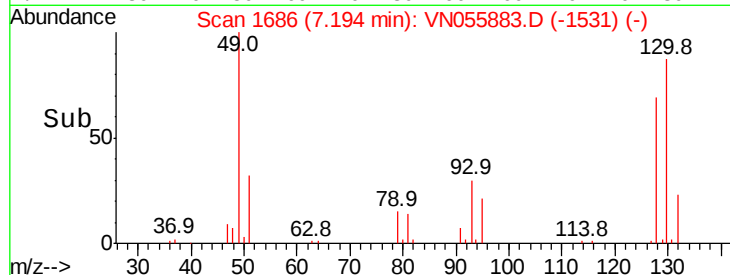
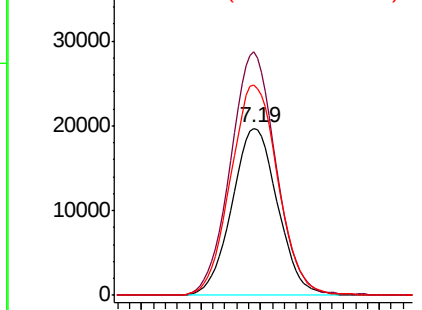



#25
 Chloroform
 Concen: 15.653 ug/l
 RT: 7.37 min Scan# 1741
 Delta R.T. -0.00 min
 Lab File: VN055883.D
 Acq: 29 May 2019 17:28

Tgt Ion: 83 Resp: 84409
 Ion Ratio Lower Upper
 83 100
 85 64.3 51.7 77.5

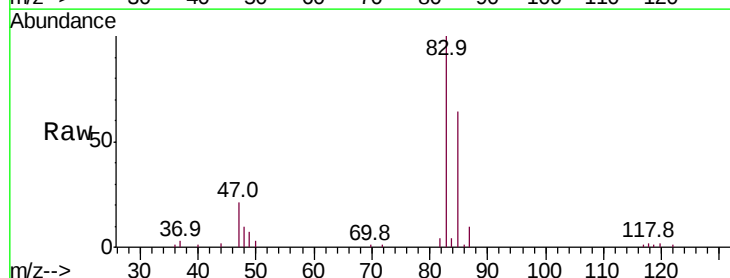

Abundance Ion 83.00 (82.70 to 83.70): VN
 Ion 85.00 (84.70 to 85.70): VN



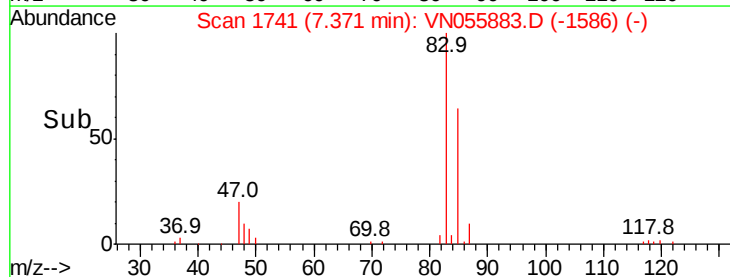
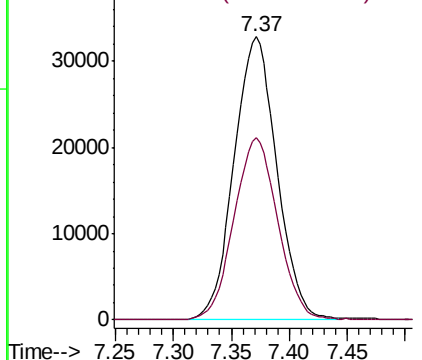


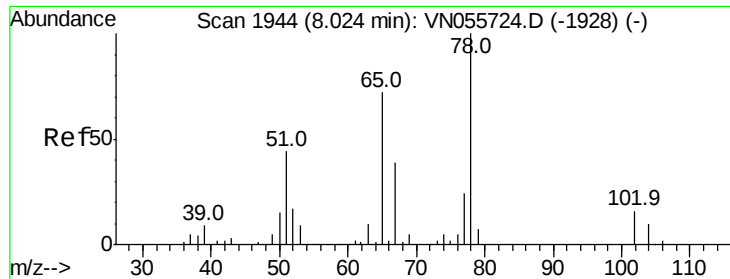

#27
 1,2-Dichloroethane-d4
 Concen: 31.065 ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN055883.D
 Acq: 29 May 2019 17:28




Instrument :
 MSVOA_N
 ClientSampled :
 14B-3


Tot Ion: 65 Resp: 106364
 Ion Ratio Lower Upper
 65 100
 67 54.7 43.5 65.3

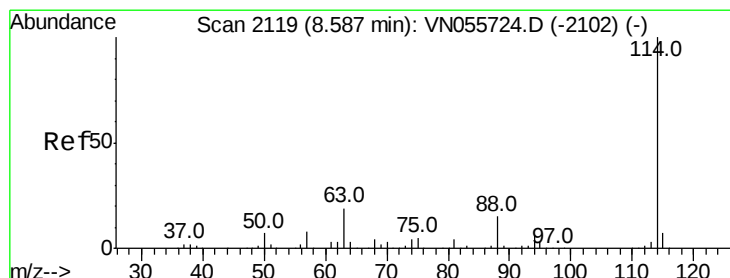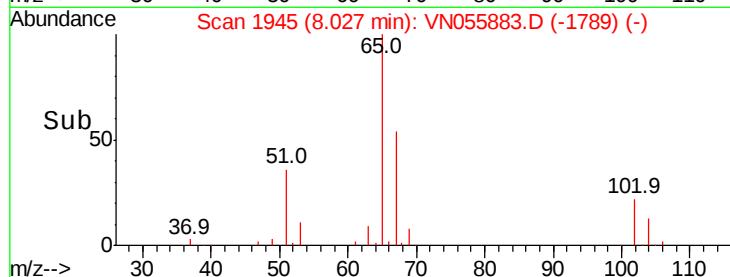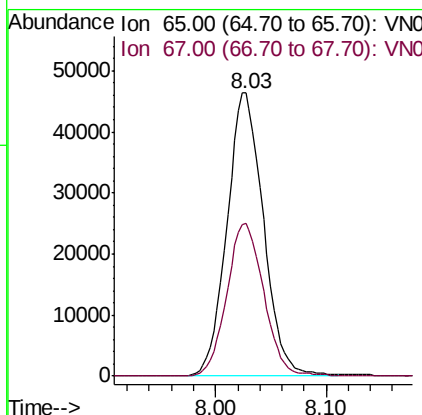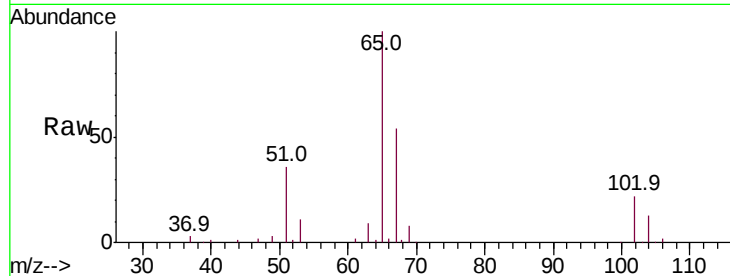

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. -0.00 min
 Lab File: VN055883.D
 Acq: 29 May 2019 17:28

Tgt Ion: 114 Resp: 276037
 Ion Ratio Lower Upper
 114 100
 63 19.3 15.6 23.4
 88 15.1 12.3 18.5

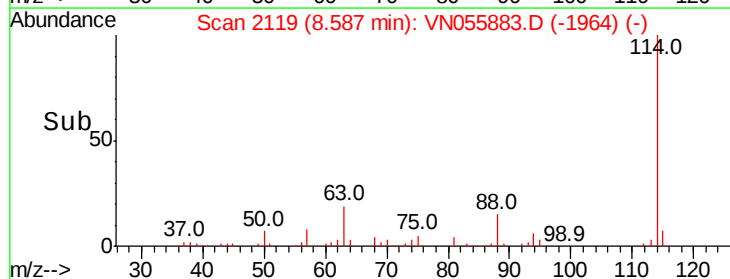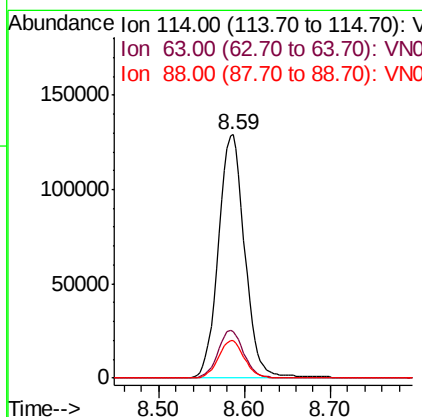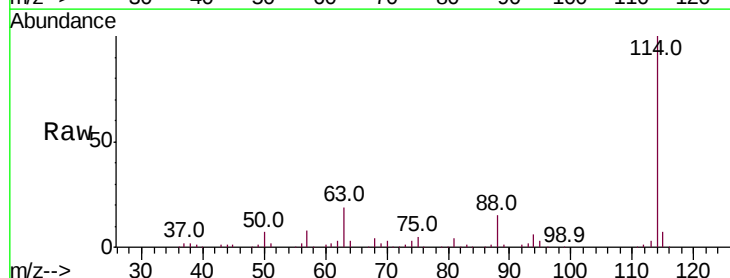

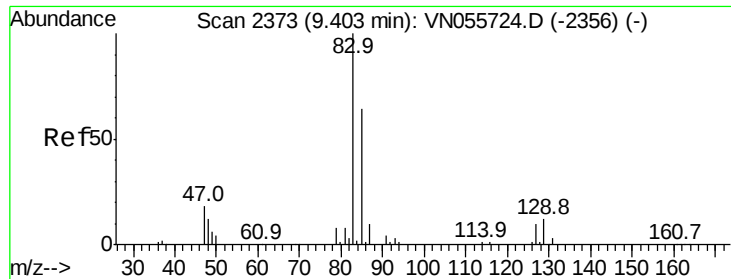

#41

Bromodichloromethane

Concen: 1.585 ug/l

RT: 9.40 min Scan# 2372

Delta R.T. -0.00 min

Lab File: VN055883.D

Acq: 29 May 2019 17:28

Instrument :

MSVOA_N

ClientSampled :

14B-3


Tot Ion: 83 Resp: 6727

Ion Ratio Lower Upper

83 100

85 66.6 51.4 77.0




127 9.5 7.7 11.5

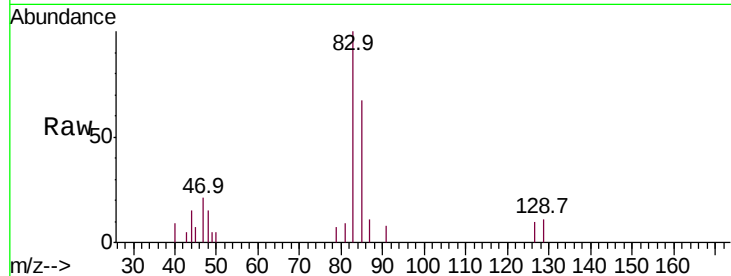

Abundance Ion 83.00 (82.70 to 83.70): VN0

Ion 85.00 (84.70 to 85.70): VN0

Ion 127.00 (126.70 to 127.70): V

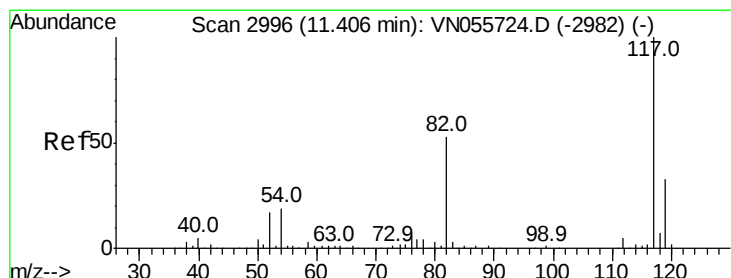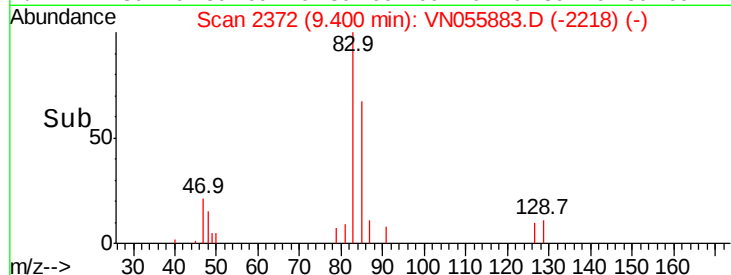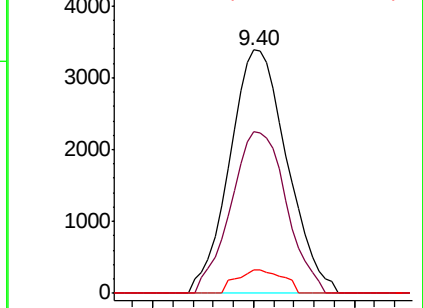

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.41 min Scan# 2996

Delta R.T. -0.00 min

Lab File: VN055883.D

Acq: 29 May 2019 17:28


Tgt Ion: 117 Resp: 222274

Ion Ratio Lower Upper

117 100

82 52.1 42.6 64.0



119 32.5 25.9 38.9

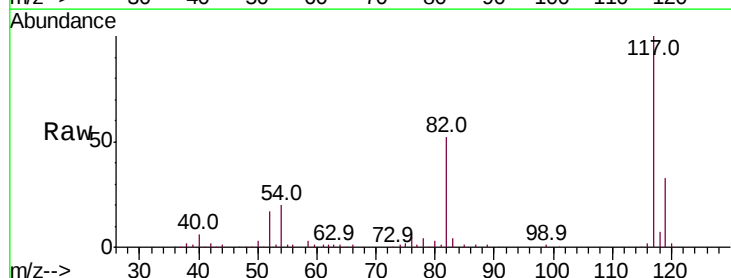


Abundance Ion 117.00 (116.70 to 117.70): V

Ion 82.00 (81.70 to 82.70): VN0

Ion 119.00 (118.70 to 119.70): V

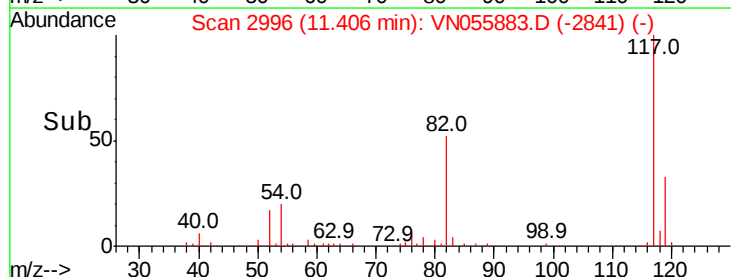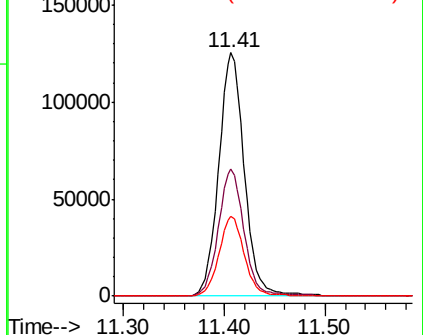

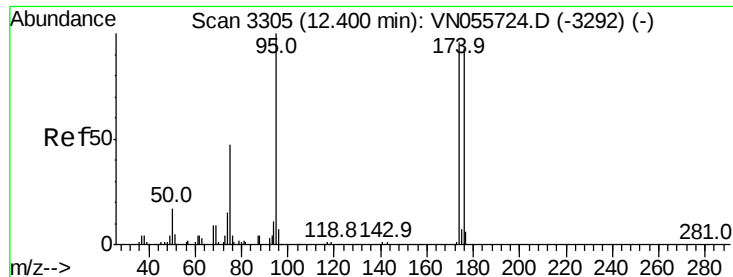

#60

4-Bromofluorobenzene

Concen: 22.895 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN055883.D

Acq: 29 May 2019 17:28

Instrument :

MSVOA_N

ClientSampled :

14B-3


Tot Ion: 95 Resp: 79165

Ion Ratio Lower Upper

95 100

174 92.0 75.7 113.5




176 88.2 74.1 111.1

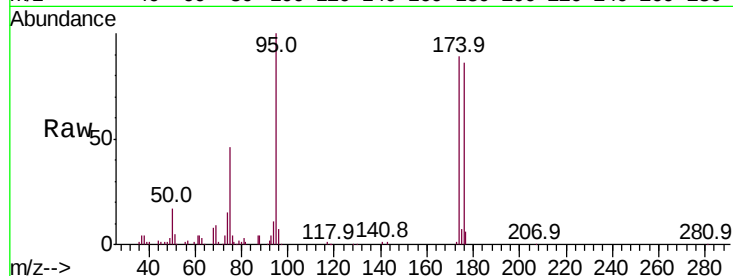

Abundance Ion 95.00 (94.70 to 95.70): VN055883.D (-3150) (-)

Ion 174.00 (173.70 to 174.70): VN055883.D (-3150) (-)

Ion 176.00 (175.70 to 176.70): VN055883.D (-3150) (-)

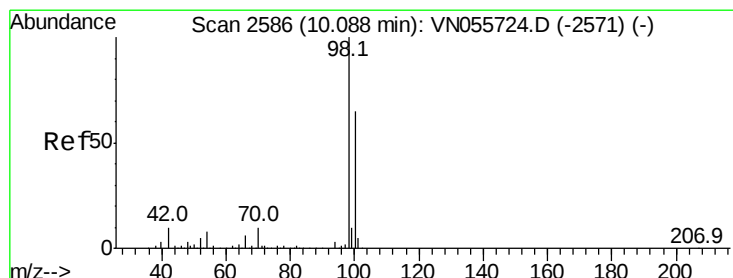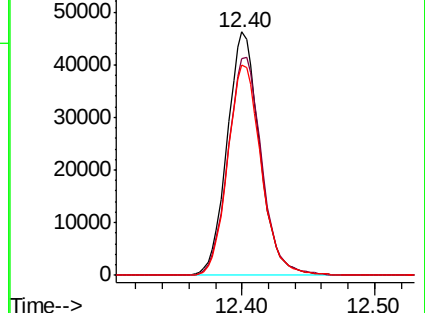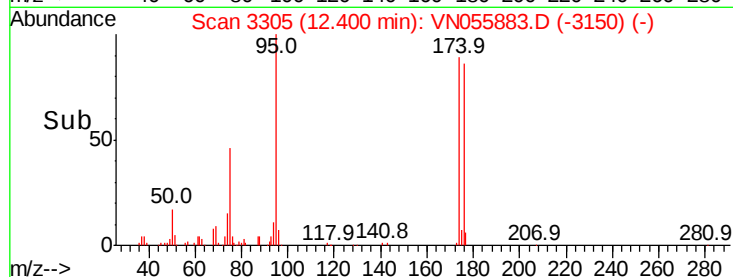

#63

Toluene-d8

Concen: 31.723 ug/l

RT: 10.09 min Scan# 2586

Delta R.T. -0.00 min

Lab File: VN055883.D


Acq: 29 May 2019 17:28

Tgt Ion: 98 Resp: 322228

Ion Ratio Lower Upper

98 100

100 64.8 51.6 77.4

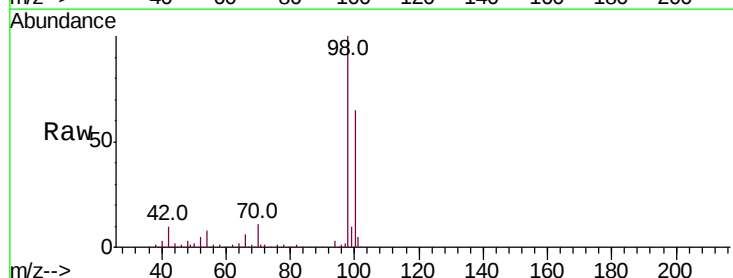

Abundance Ion 98.00 (97.70 to 98.70): VN055883.D (-2431) (-)

Ion 100.00 (99.70 to 100.70): VN055883.D (-2431) (-)

