


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN052919\
Data File : VN055863.D
Acq On : 29 May 2019 8:31
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N052219W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 23 05:54:54 2019

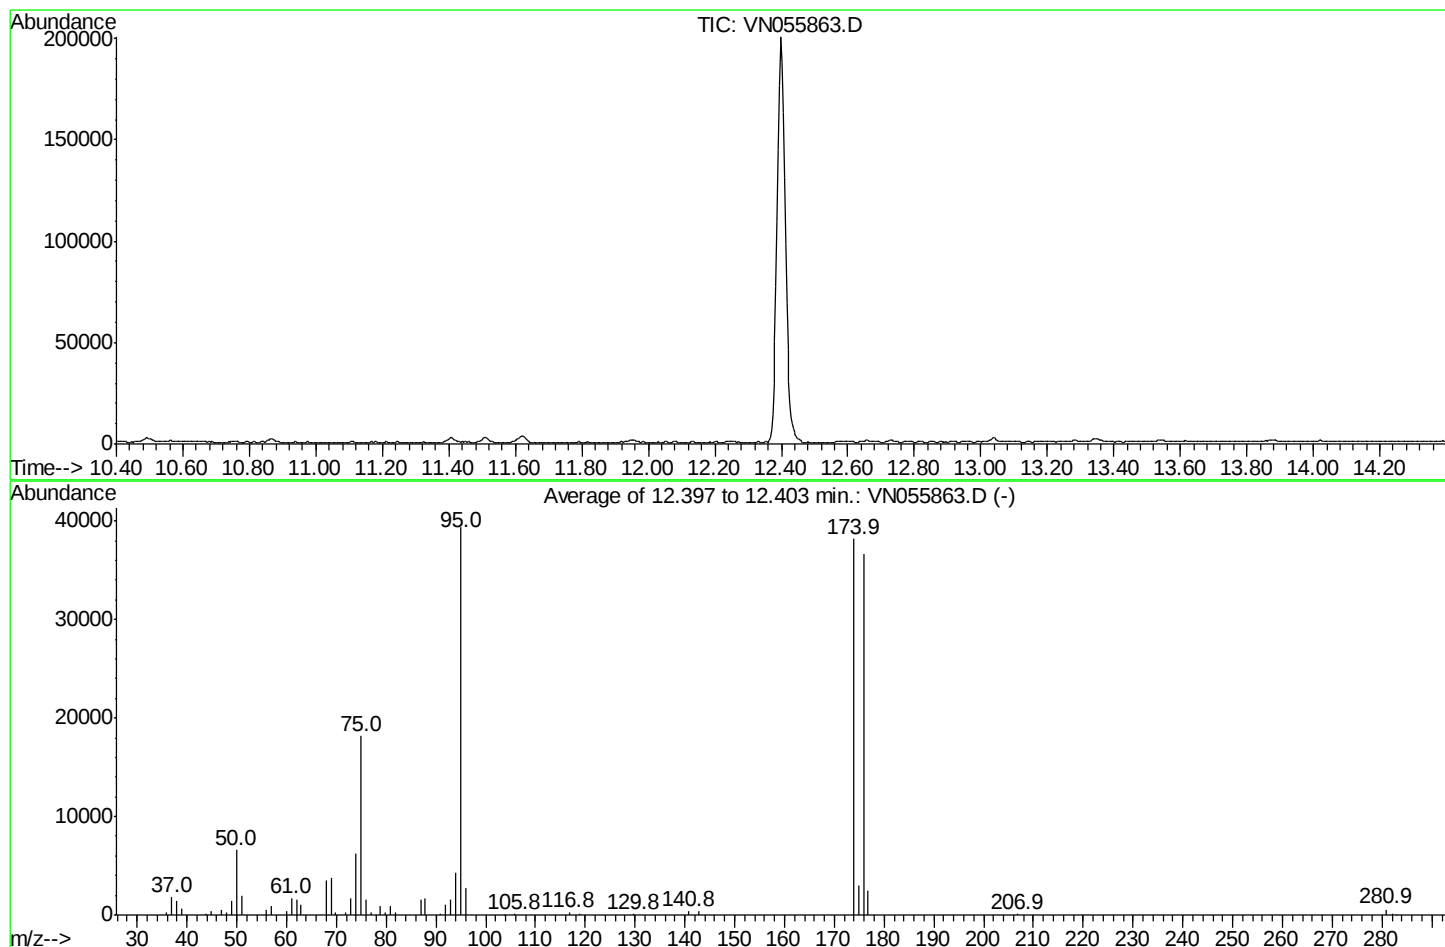

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	6616	PASS
75	95	30	60	46.2	18189	PASS
95	95	100	100	100.0	39368	PASS
96	95	5	9	6.8	2689	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	97.0	38168	PASS
175	174	5	9	7.8	2960	PASS
176	174	95	101	96.0	36632	PASS
177	176	5	9	6.8	2483	PASS