


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN052920\
Data File : VN061555.D
Acq On : 29 May 2020 9:55
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052820W.M
Title : SW846 8260
Last Update : Fri May 29 02:14:10 2020

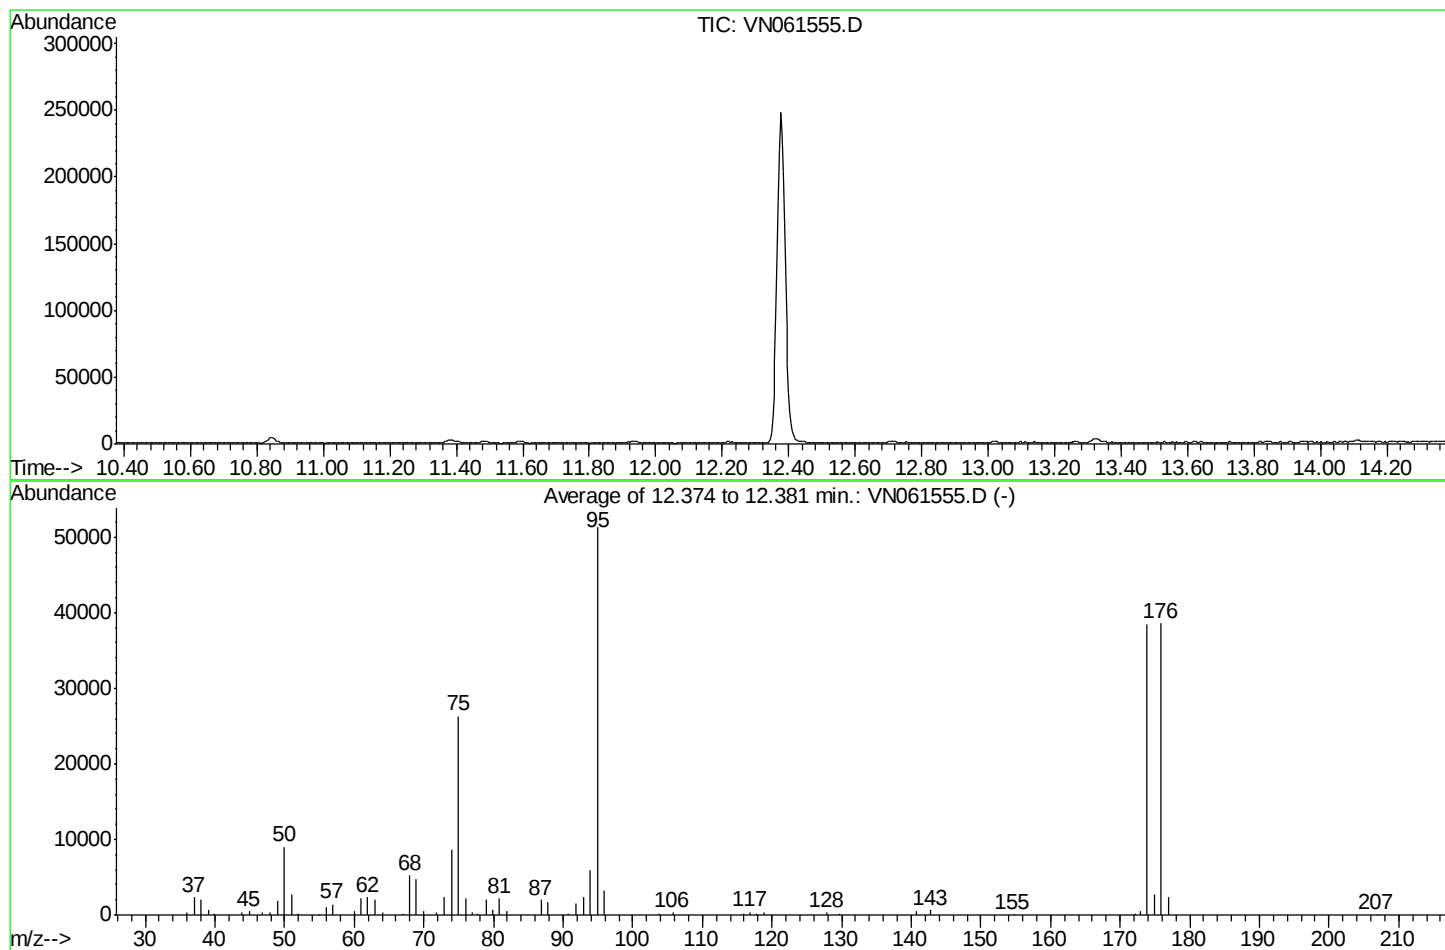

AutoFind: Scans 3297, 3298, 3299; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9033	PASS
75	95	30	60	51.3	26298	PASS
95	95	100	100	100.0	51293	PASS
96	95	5	9	6.3	3246	PASS
173	174	0.00	2	1.3	515	PASS
174	95	50	100	75.0	38450	PASS
175	174	5	9	7.0	2681	PASS
176	174	95	101	100.4	38608	PASS
177	176	5	9	6.1	2355	PASS