
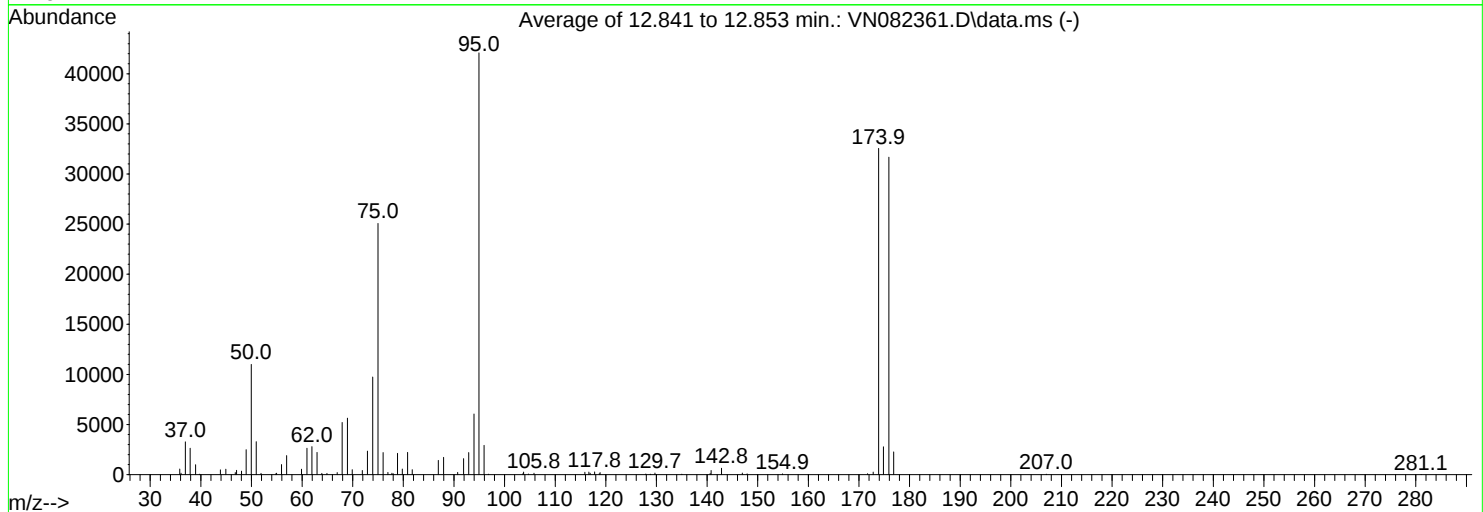


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052924\
Data File : VN082361.D
Acq On : 29 May 2024 09:07
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

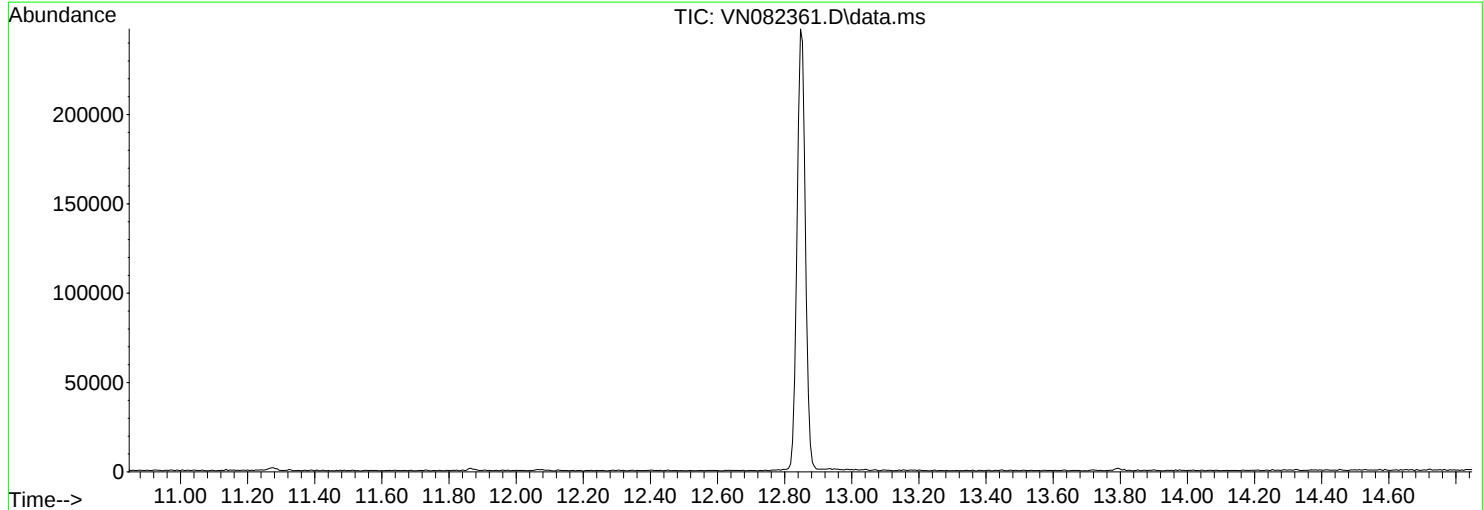

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	26.1	11003	PASS
75	95	30	60	59.6	25067	PASS
95	95	100	100	100.0	42088	PASS
96	95	5	9	7.0	2927	PASS
173	174	0.00	2	0.8	253	PASS
174	95	50	100	77.3	32549	PASS
175	174	5	9	8.5	2780	PASS
176	174	95	101	97.3	31683	PASS
177	176	5	9	7.2	2271	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	561	48.95	2493	62.95	2219	76.00	2201
36.10	150	49.95	11003	63.90	137	76.95	2201
36.95	3277	50.95	3293	64.90	132	77.75	143
37.90	2642	51.90	125	66.95	203	78.00	90
38.95	994	54.80	81	67.90	5209	78.85	2117
39.80	50	54.95	143	68.95	5637	79.80	552
43.85	472	55.95	1014	69.90	498	80.85	2220
44.95	543	56.95	1905	71.90	413	81.75	494
46.80	205	59.90	541	72.90	2346	86.90	1422
47.05	436	60.95	2640	73.95	9732	87.95	1723
48.05	352	61.95	2797	75.00	25067	90.75	231

Average of 12.841 to 12.853 min.: VN082361.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
91.90	1598	116.65	263	142.85	643	281.05	16
92.90	2203	116.90	151	146.95	164		
93.95	6055	117.80	270	147.90	81		
94.95	42088	118.70	99	154.90	83		
95.95	2927	118.85	215	171.70	90		
96.80	52	127.90	63	172.80	253		
103.60	83	128.80	56	173.90	32549		
103.75	260	129.70	163	174.85	2780		
104.70	63	135.00	55	175.90	31683		
105.80	150	140.60	108	176.85	2271		
115.85	244	140.80	419	207.00	50		

Instrument :

MSVOA_N

ClientSampleId :

BFB