
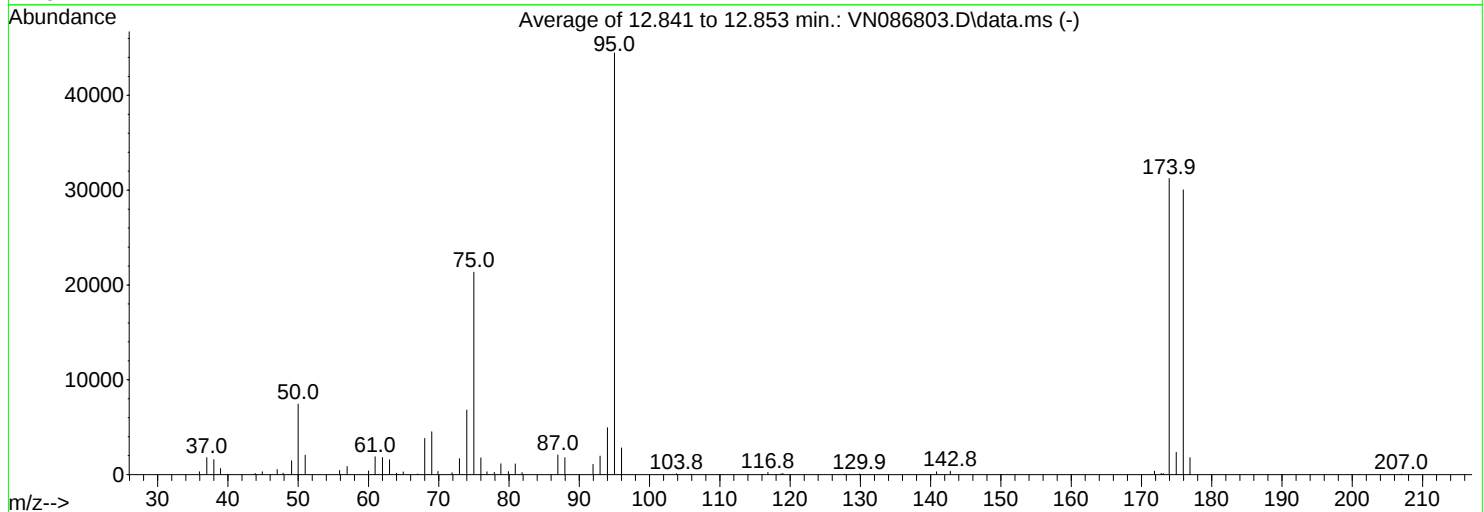


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN052925\
Data File : VN086803.D
Acq On : 29 May 2025 08:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052925W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri May 30 02:22:52 2025

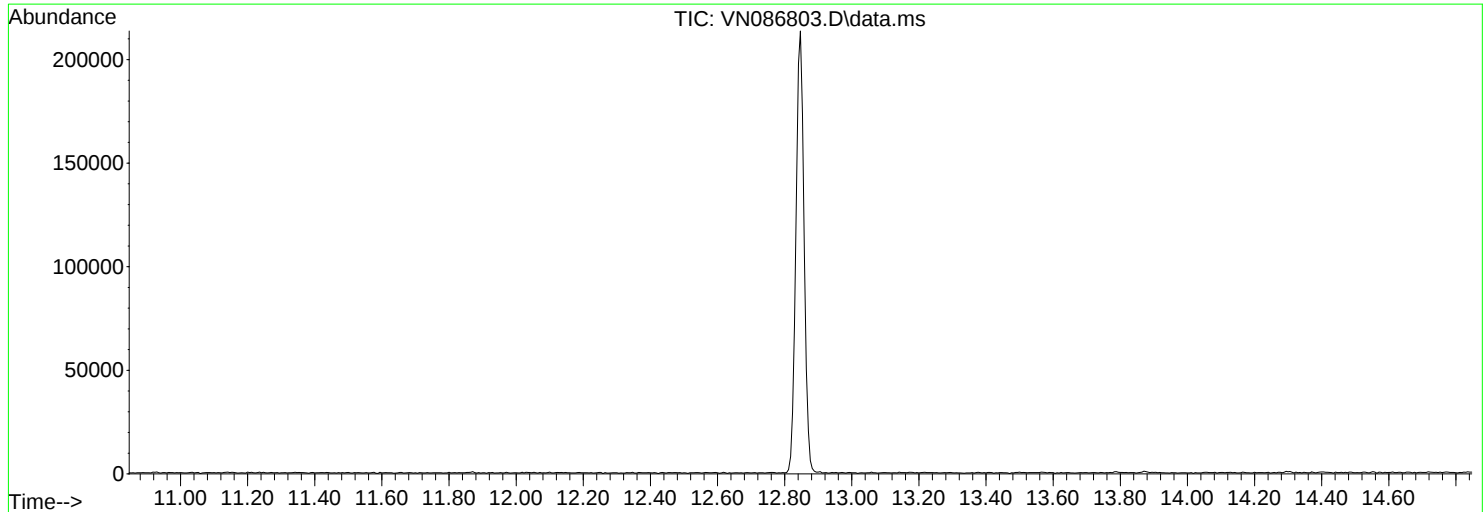

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7440	PASS
75	95	30	60	48.0	21341	PASS
95	95	100	100	100.0	44480	PASS
96	95	5	9	6.3	2819	PASS
173	174	0.00	2	0.5	141	PASS
174	95	50	100	70.2	31232	PASS
175	174	5	9	7.5	2339	PASS
176	174	95	101	96.2	30032	PASS
177	176	5	9	6.0	1791	PASS