

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN053019\
 Data File : VN055899.D
 Acq On : 30 May 2019 14:46
 Operator : JC/SP
 Sample : VN0530WBL02
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0530WBL02

Quant Time: May 31 05:07:33 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N052219W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Thu May 23 05:54:54 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.19	128	50358	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.58	114	270687	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.41	117	211758	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.02	65	100993	30.68	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	102.27%
60) 4-Bromofluorobenzene	12.40	95	74676	22.67	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	75.57%
63) Toluene-d8	10.09	98	308780	31.91	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	106.37%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN053019\
Data File : VN055899.D
Acq On : 30 May 2019 14:46
Operator : JC/SP
Sample : VN0530WBL02
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0530WBL02

Quant Time: May 31 05:07:33 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA N\METHODS\624N052219W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Thu May 23 05:54:54 2019
Response via : Initial Calibration

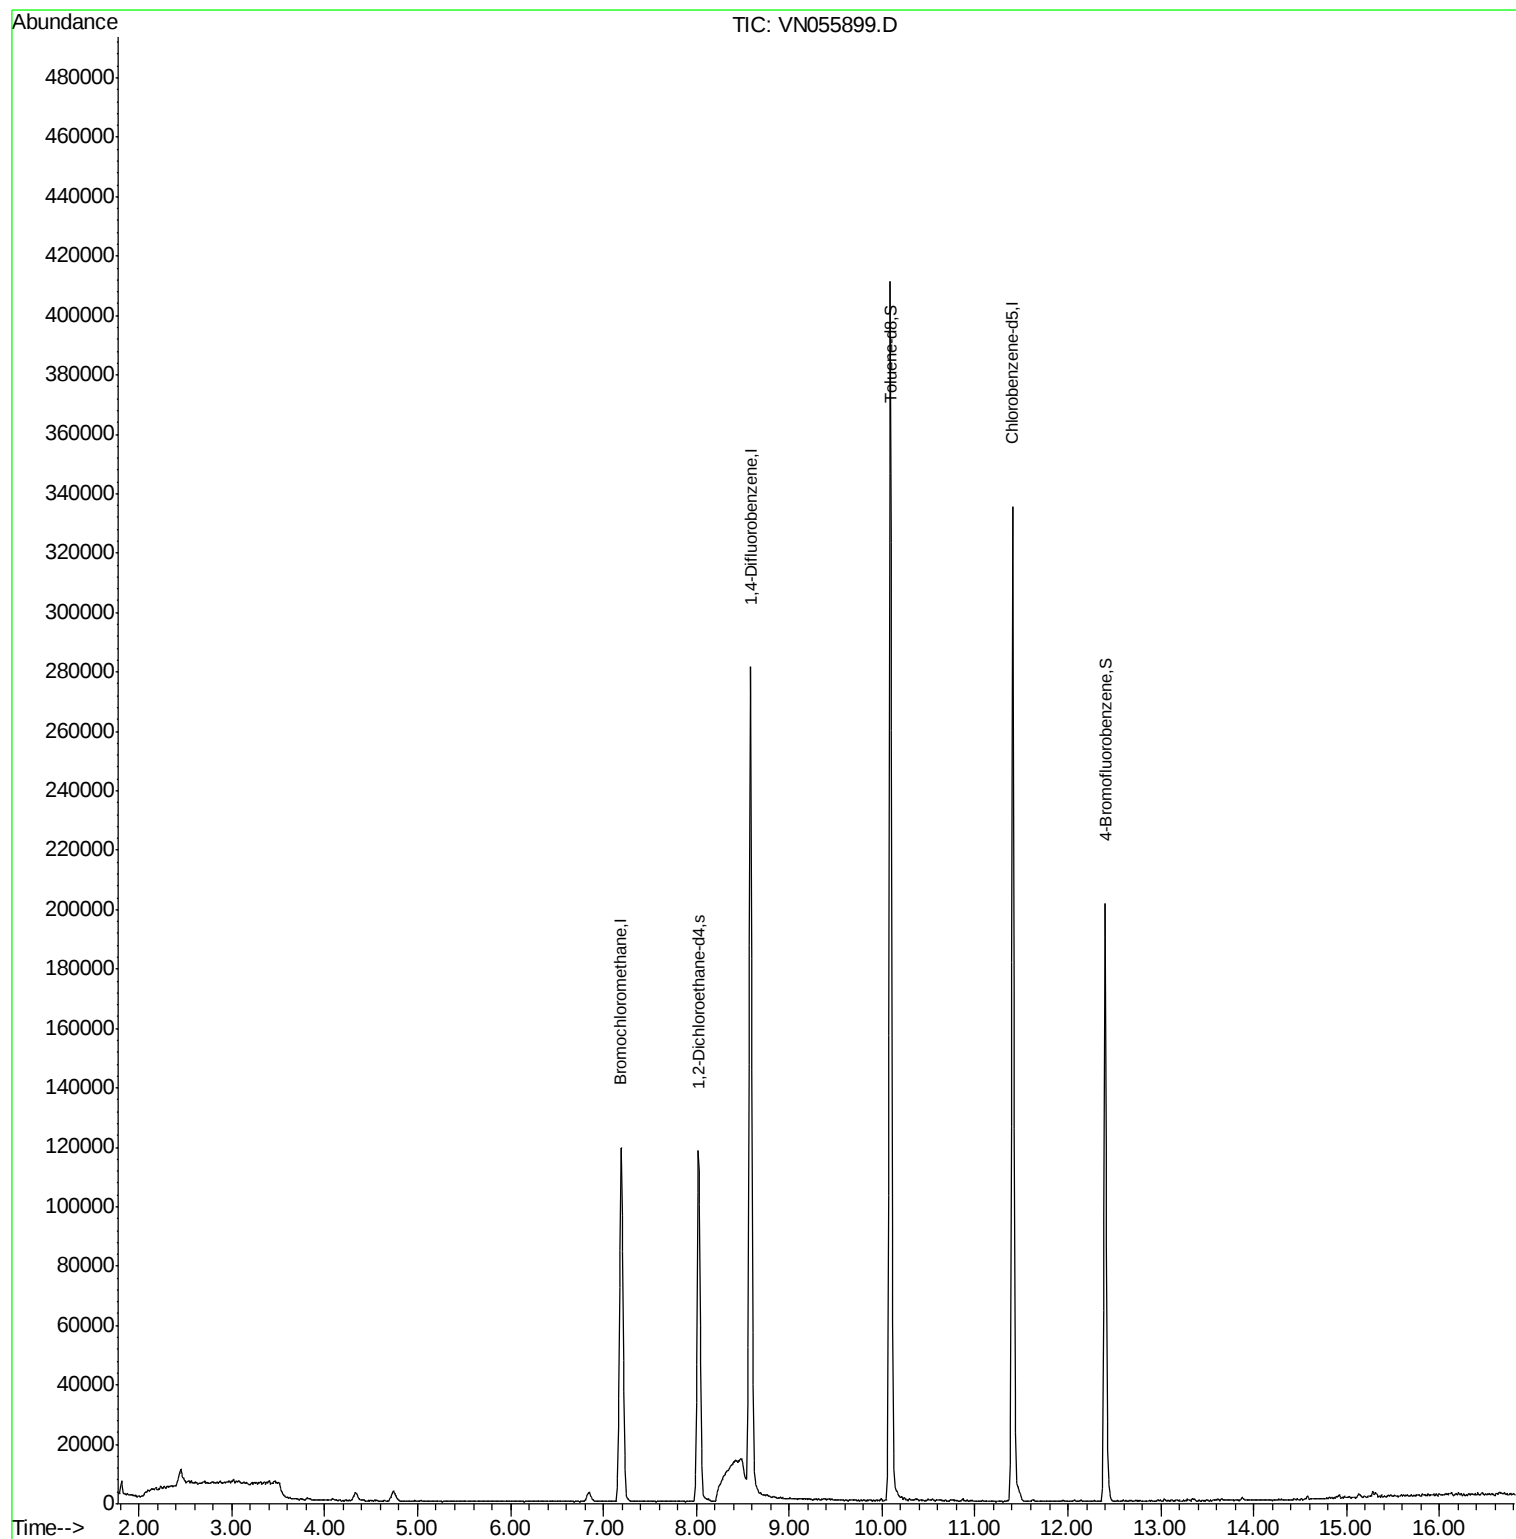

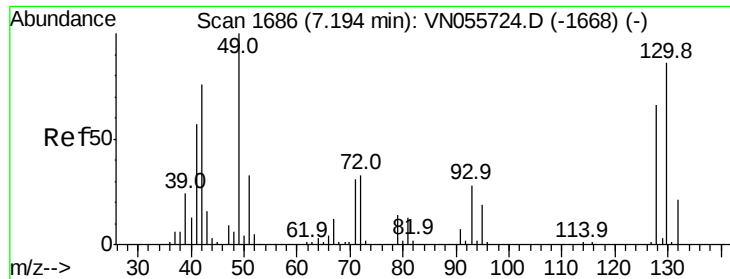

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.19 min Scan# 1685

Delta R.T. -0.00 min

Lab File: VN055899.D

Acq: 30 May 2019 14:46

Instrument :

MSVOA_N

ClientSampleId :

VN0530WBL02


Tot Ion:128 Resp: 50358

Ion Ratio Lower Upper

128 100

49 148.3 0.0 383.2




130 130.9 0.0 326.3

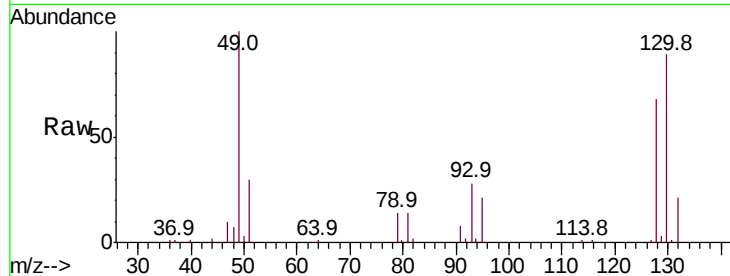

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VN0

Ion 130.00 (129.70 to 130.70): V

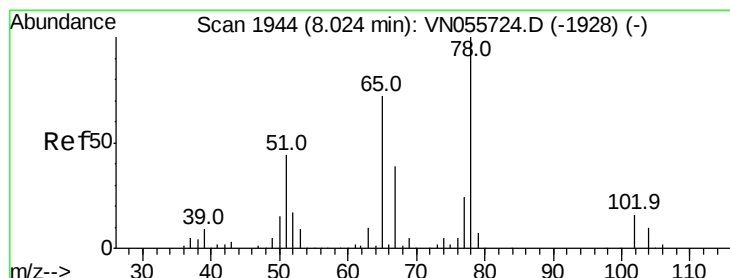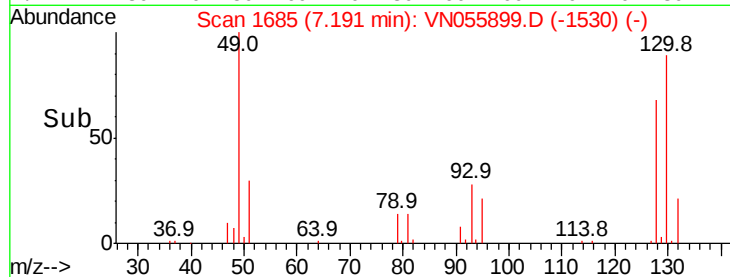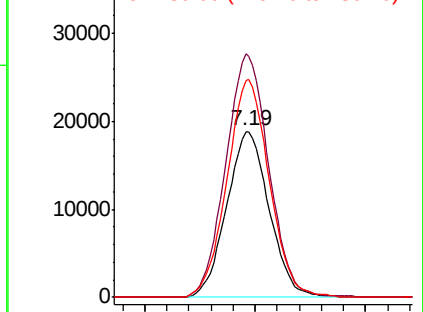

#27

1,2-Dichloroethane-d4

Concen: 30.682 ug/l

RT: 8.02 min Scan# 1944

Delta R.T. 0.00 min

Lab File: VN055899.D


Acq: 30 May 2019 14:46

Tgt Ion: 65 Resp: 100993

Ion Ratio Lower Upper



65 100


67 54.4 43.5 65.3

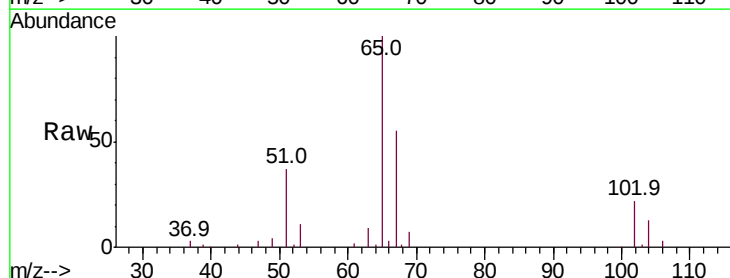

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0

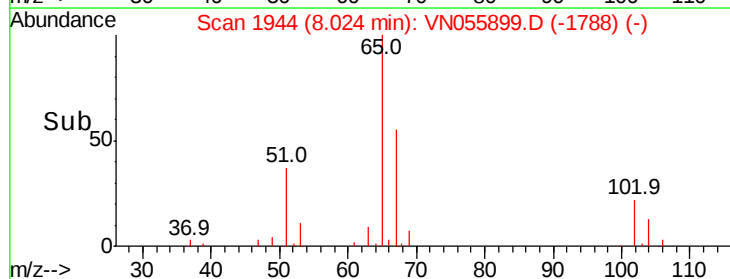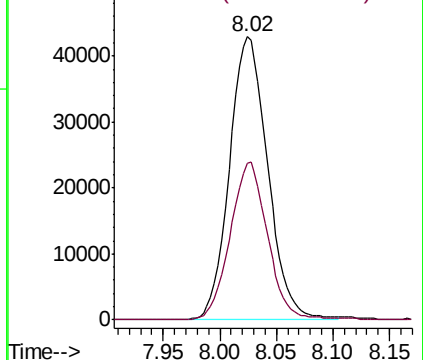


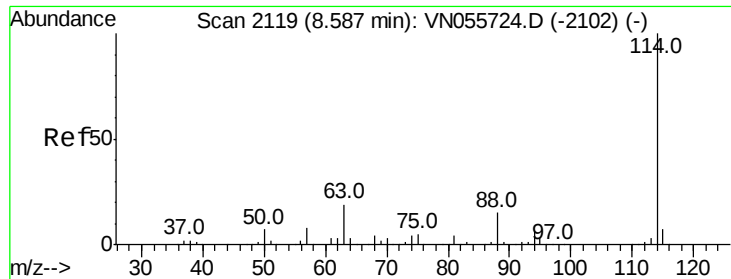




#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.58 min Scan# 2118
 Delta R.T. -0.00 min
 Lab File: VN055899.D
 Acq: 30 May 2019 14:46

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0530WBL02

Tot Ion:114 Resp: 270687
 Ion Ratio Lower Upper
 114 100
 63 19.3 15.6 23.4
 88 14.9 12.3 18.5

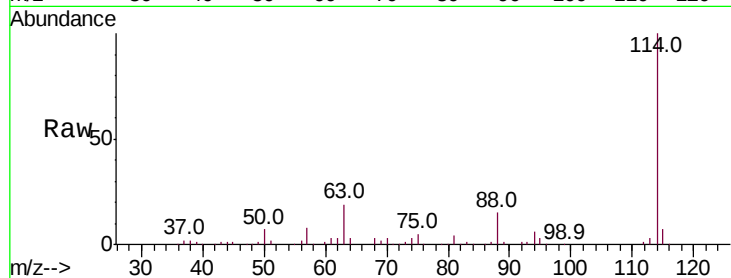


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 88.00 (87.70 to 88.70): VN

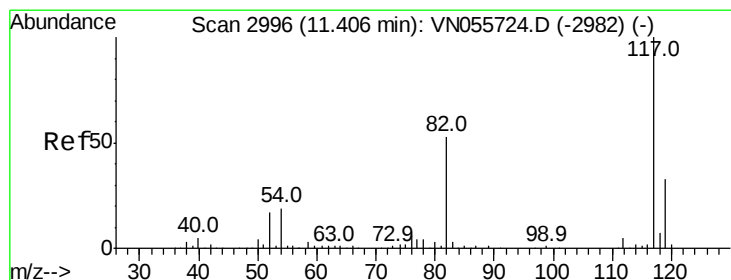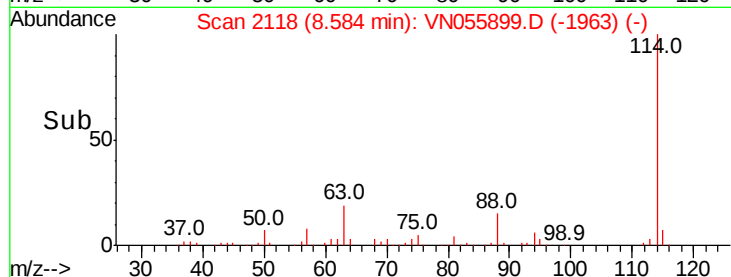
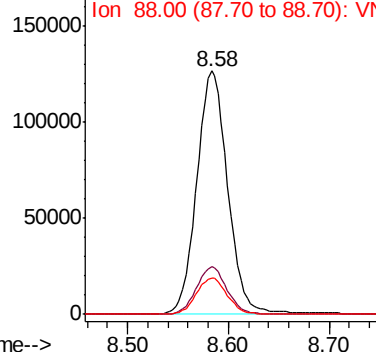



#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 11.41 min Scan# 2996
 Delta R.T. 0.00 min
 Lab File: VN055899.D
 Acq: 30 May 2019 14:46

Tgt Ion:117 Resp: 211758
 Ion Ratio Lower Upper
 117 100
 82 52.1 42.6 64.0
 119 32.1 25.9 38.9

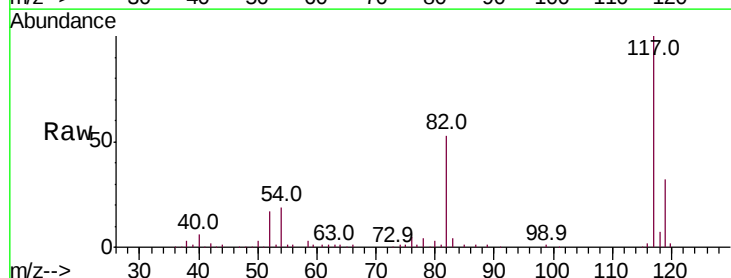

Abundance Ion 117.00 (116.70 to 117.70): V
 Ion 82.00 (81.70 to 82.70): VN
 Ion 119.00 (118.70 to 119.70): V



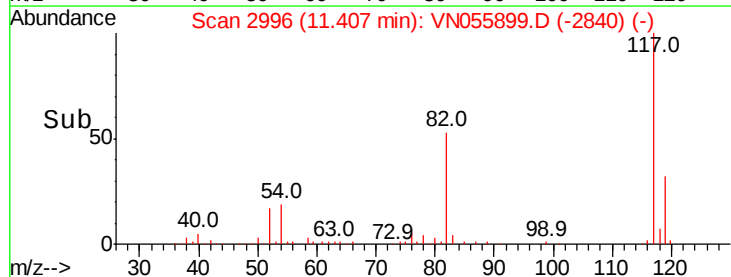
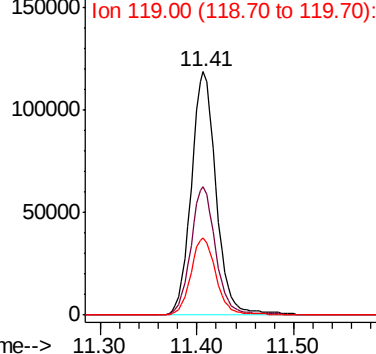


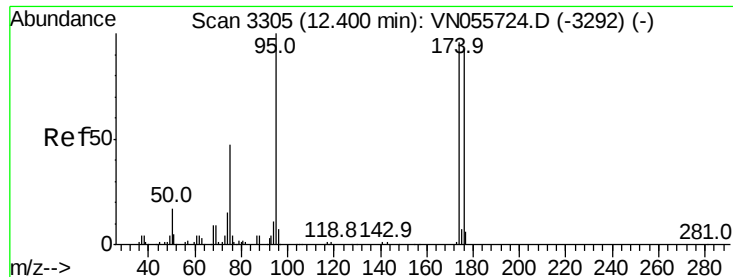

#60
4-Bromofluorobenzene
Concen: 22.669 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. 0.00 min
Lab File: VN055899.D
Acq: 30 May 2019 14:46

Instrument :
MSVOA_N
ClientSampleId :
VN0530WBL02

Tot Ion: 95 Resp: 74676
Ion Ratio Lower Upper
95 100
174 91.9 75.7 113.5
176 89.2 74.1 111.1

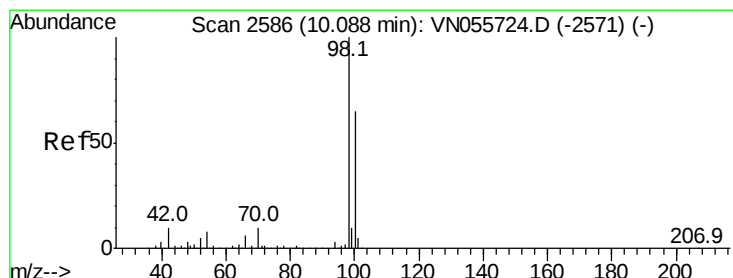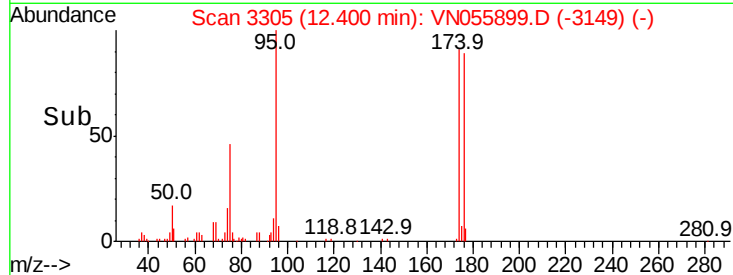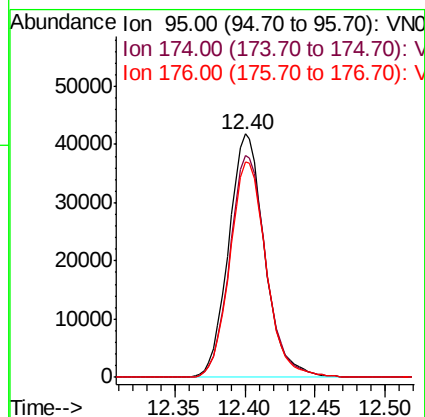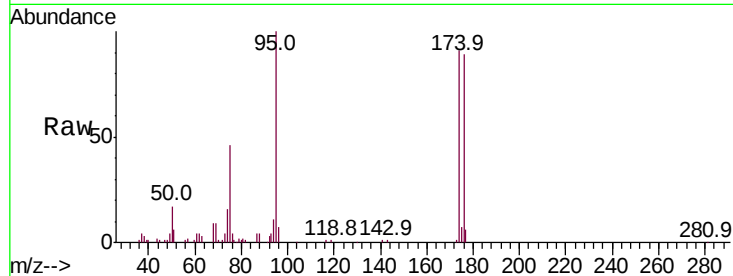

#63
Toluene-d8
Concen: 31.908 ug/l
RT: 10.09 min Scan# 2586
Delta R.T. 0.00 min
Lab File: VN055899.D
Acq: 30 May 2019 14:46

Tgt Ion: 98 Resp: 308780
Ion Ratio Lower Upper
98 100
100 63.7 51.6 77.4

