
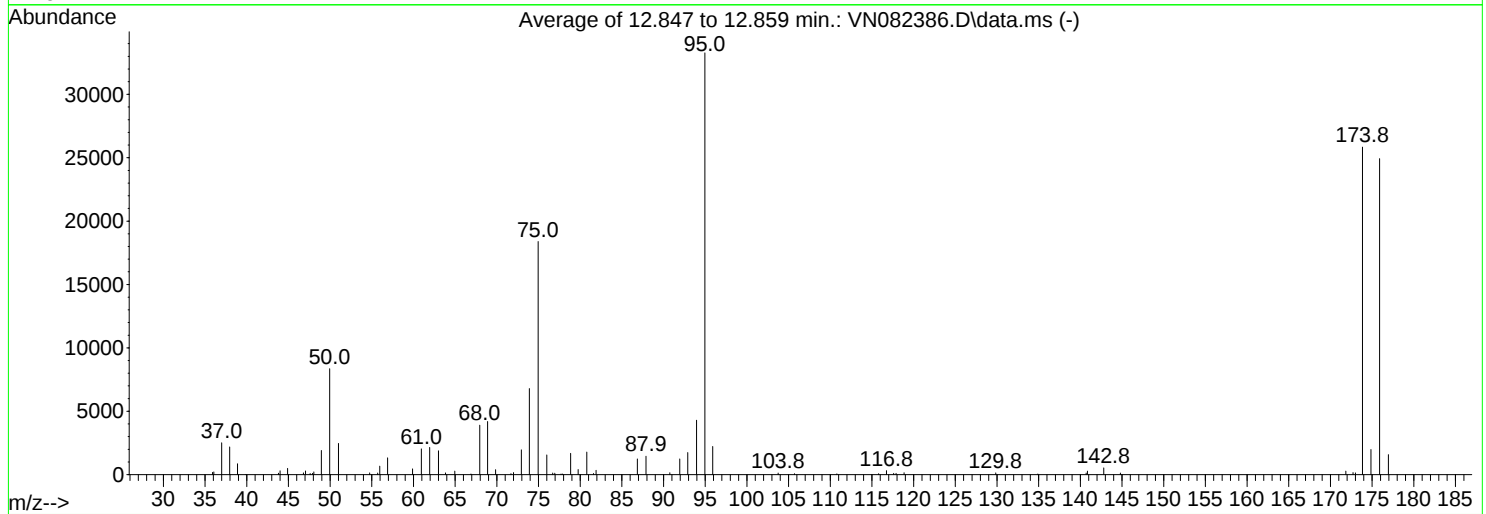


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053024\
Data File : VN082386.D
Acq On : 30 May 2024 11:09
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N051524W.M
Title : SW846 8260
Last Update : Thu May 16 05:21:06 2024

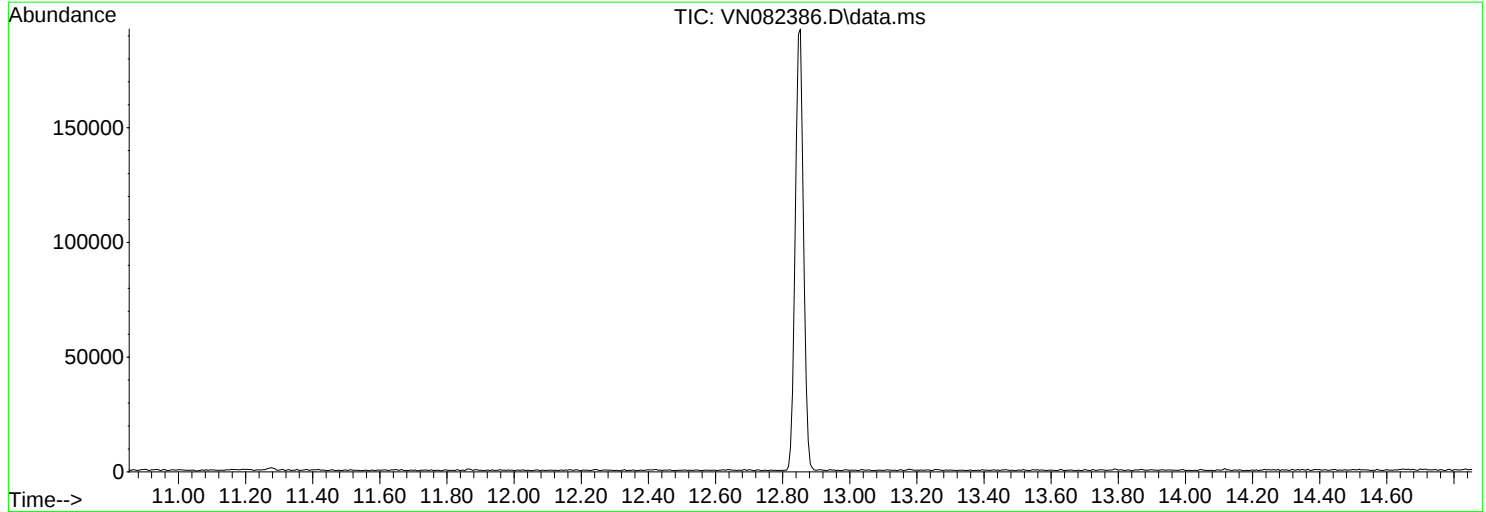

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	8362	PASS
75	95	30	60	55.3	18391	PASS
95	95	100	100	100.0	33275	PASS
96	95	5	9	6.7	2226	PASS
173	174	0.00	2	0.6	162	PASS
174	95	50	100	77.6	25837	PASS
175	174	5	9	7.7	1980	PASS
176	174	95	101	96.5	24931	PASS
177	176	5	9	6.3	1576	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	179	47.60	91	60.95	2034	72.95	196
36.05	220	47.90	100	61.95	2140	73.90	678
37.00	2514	48.05	214	63.00	1876	74.95	1839
37.95	2187	48.95	1913	63.85	141	76.00	155
38.90	860	49.95	8362	64.95	272	76.70	124
39.90	18	51.00	2466	66.90	52	76.95	118
43.80	108	54.75	139	67.95	3905	77.70	50
44.00	302	55.70	131	68.90	4188	77.90	50
44.90	499	55.95	675	69.85	390	78.85	1679
46.80	139	56.90	1323	71.70	82	79.75	410
47.05	288	59.90	452	72.00	164	80.80	1785

Average of 12.847 to 12.859 min.: VN082386.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
81.60	84	105.70	74	142.80	533		
81.90	346	110.80	69	144.80	124		
86.85	1238	115.80	79	171.85	283		
87.90	1455	116.75	314	172.70	162		
90.75	159	117.60	101	173.00	134		
91.95	1238	117.90	97	173.85	25837		
92.90	1740	118.85	159	174.85	1980		
93.95	4293	129.85	137	175.90	24931		
94.95	33275	134.90	52	176.95	1576		
95.90	2226	140.70	130				
103.75	125	140.85	282				

Instrument :

MSVOA_N

ClientSampleId :

BFB