
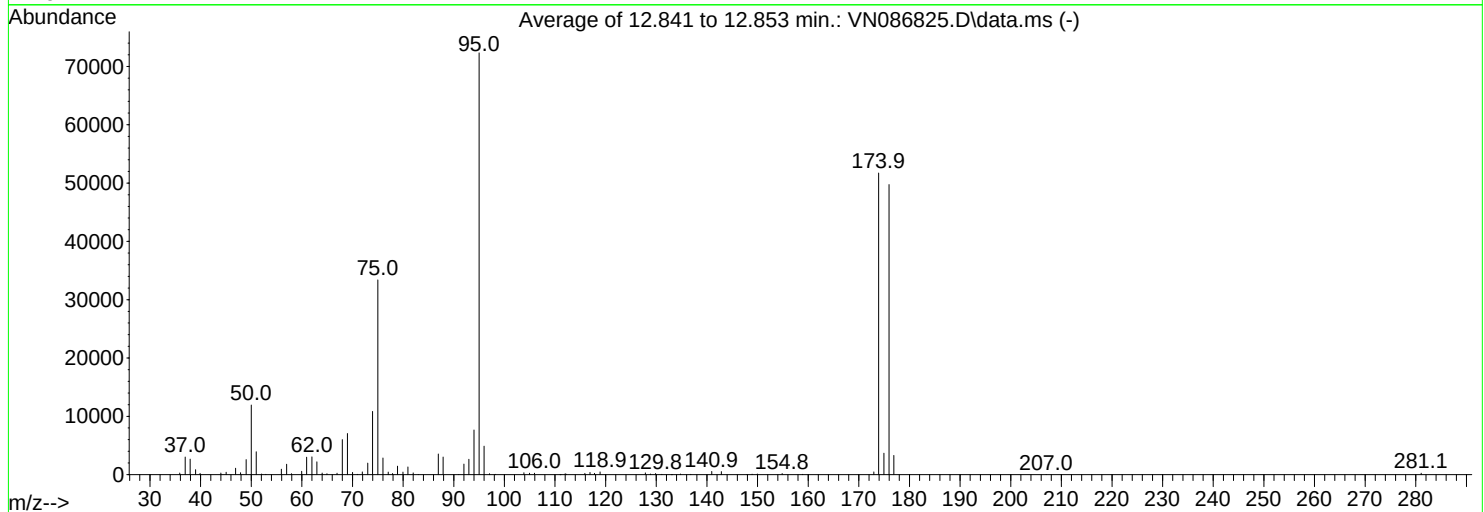


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN053025\
Data File : VN086825.D
Acq On : 30 May 2025 08:58
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N052925W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri May 30 02:22:52 2025

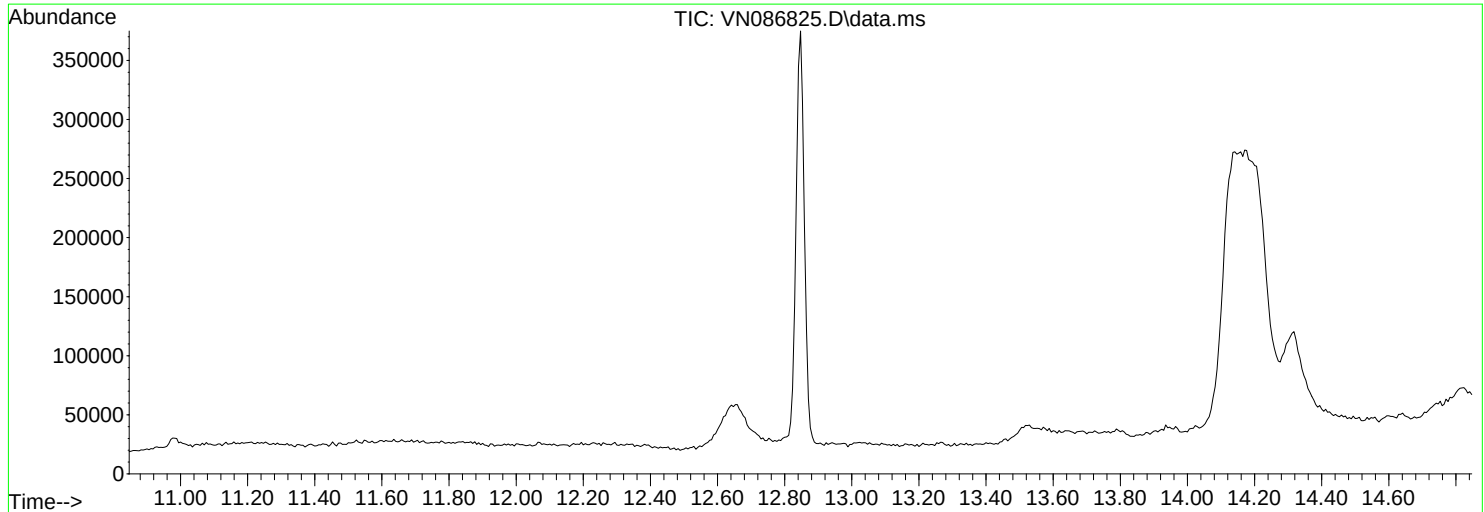

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1842

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	11932	PASS
75	95	30	60	46.2	33402	PASS
95	95	100	100	100.0	72333	PASS
96	95	5	9	6.7	4875	PASS
173	174	0.00	2	0.9	457	PASS
174	95	50	100	71.5	51712	PASS
175	174	5	9	7.1	3691	PASS
176	174	95	101	96.2	49749	PASS
177	176	5	9	6.6	3302	PASS