


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN053119\
 Data File : VN055906.D
 Acq On : 31 May 2019 8:21
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N052319W.M
 Title : SW846 8260
 Last Update : Fri May 24 06:41:54 2019

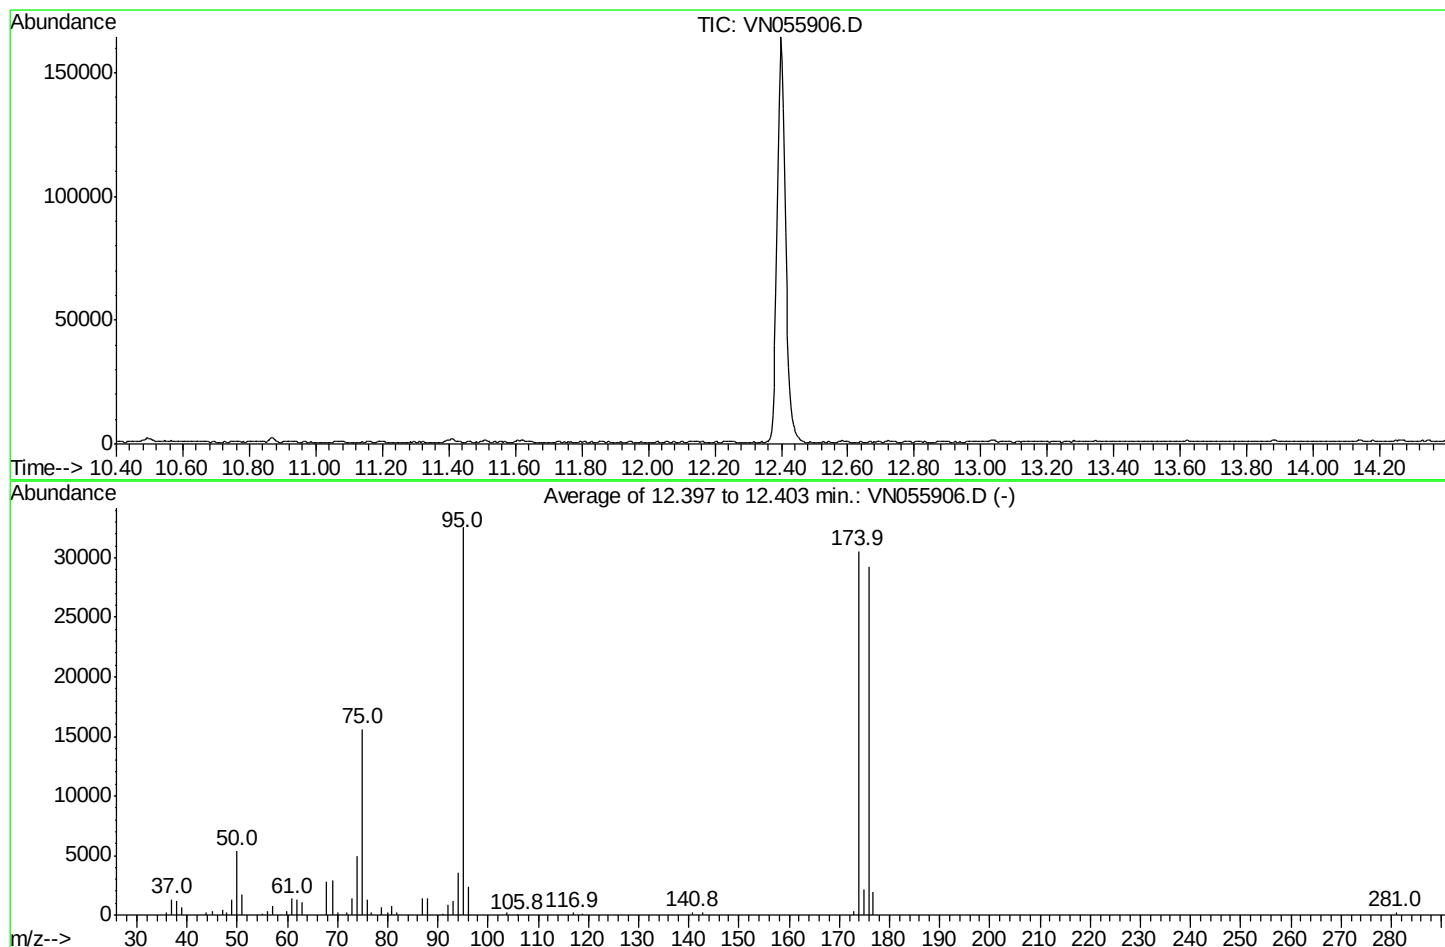

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	5409	PASS
75	95	30	60	47.9	15600	PASS
95	95	100	100	100.0	32560	PASS
96	95	5	9	7.2	2341	PASS
173	174	0.00	2	1.1	335	PASS
174	95	50	100	93.8	30541	PASS
175	174	5	9	7.2	2202	PASS
176	174	95	101	95.6	29205	PASS
177	176	5	9	6.6	1931	PASS